

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060220\
 Data File : BF120491.D
 Acq On : 2 Jun 2020 13:34
 Operator : JU/CG
 Sample : PB129235BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB129235BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.922	3	6	10	rVB	236551	267524	5.33%	0.748%
2	1.963	10	13	21	rBV	52032	69011	1.37%	0.193%
3	2.099	31	36	44	rVB	127988	157871	3.14%	0.442%
4	5.469	604	609	612	rBV	4260379	4292969	85.51%	12.007%
5	6.481	775	781	784	rBV	3885271	4326488	86.18%	12.101%
6	6.845	839	843	846	rBV	1300693	1053153	20.98%	2.946%
7	7.004	865	870	873	rBV	3939016	3740390	74.50%	10.461%
8	7.410	933	939	942	rBV	2626055	2919305	58.15%	8.165%
9	8.128	1056	1061	1064	rBV	1485752	1321665	26.33%	3.697%
10	9.204	1239	1244	1247	rBV	5200106	5020423	100.00%	14.041%
11	9.881	1355	1359	1362	rBV	1700217	1408536	28.06%	3.939%
12	10.669	1489	1493	1497	rBV	2919920	2849921	56.77%	7.971%
13	11.369	1608	1612	1615	rBV	1540061	1312778	26.15%	3.672%
14	12.957	1877	1882	1885	rBV	4621349	4603435	91.69%	12.875%
15	14.004	2056	2060	2064	rBV	1326461	1190848	23.72%	3.331%
16	15.468	2304	2309	2323	rVB	956337	1219948	24.30%	3.412%


Sum of corrected areas: 35754265

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060220\
Data File : BF120491.D
Acq On : 2 Jun 2020 13:34
Operator : JU/CG
Sample : PB129235BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129235BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

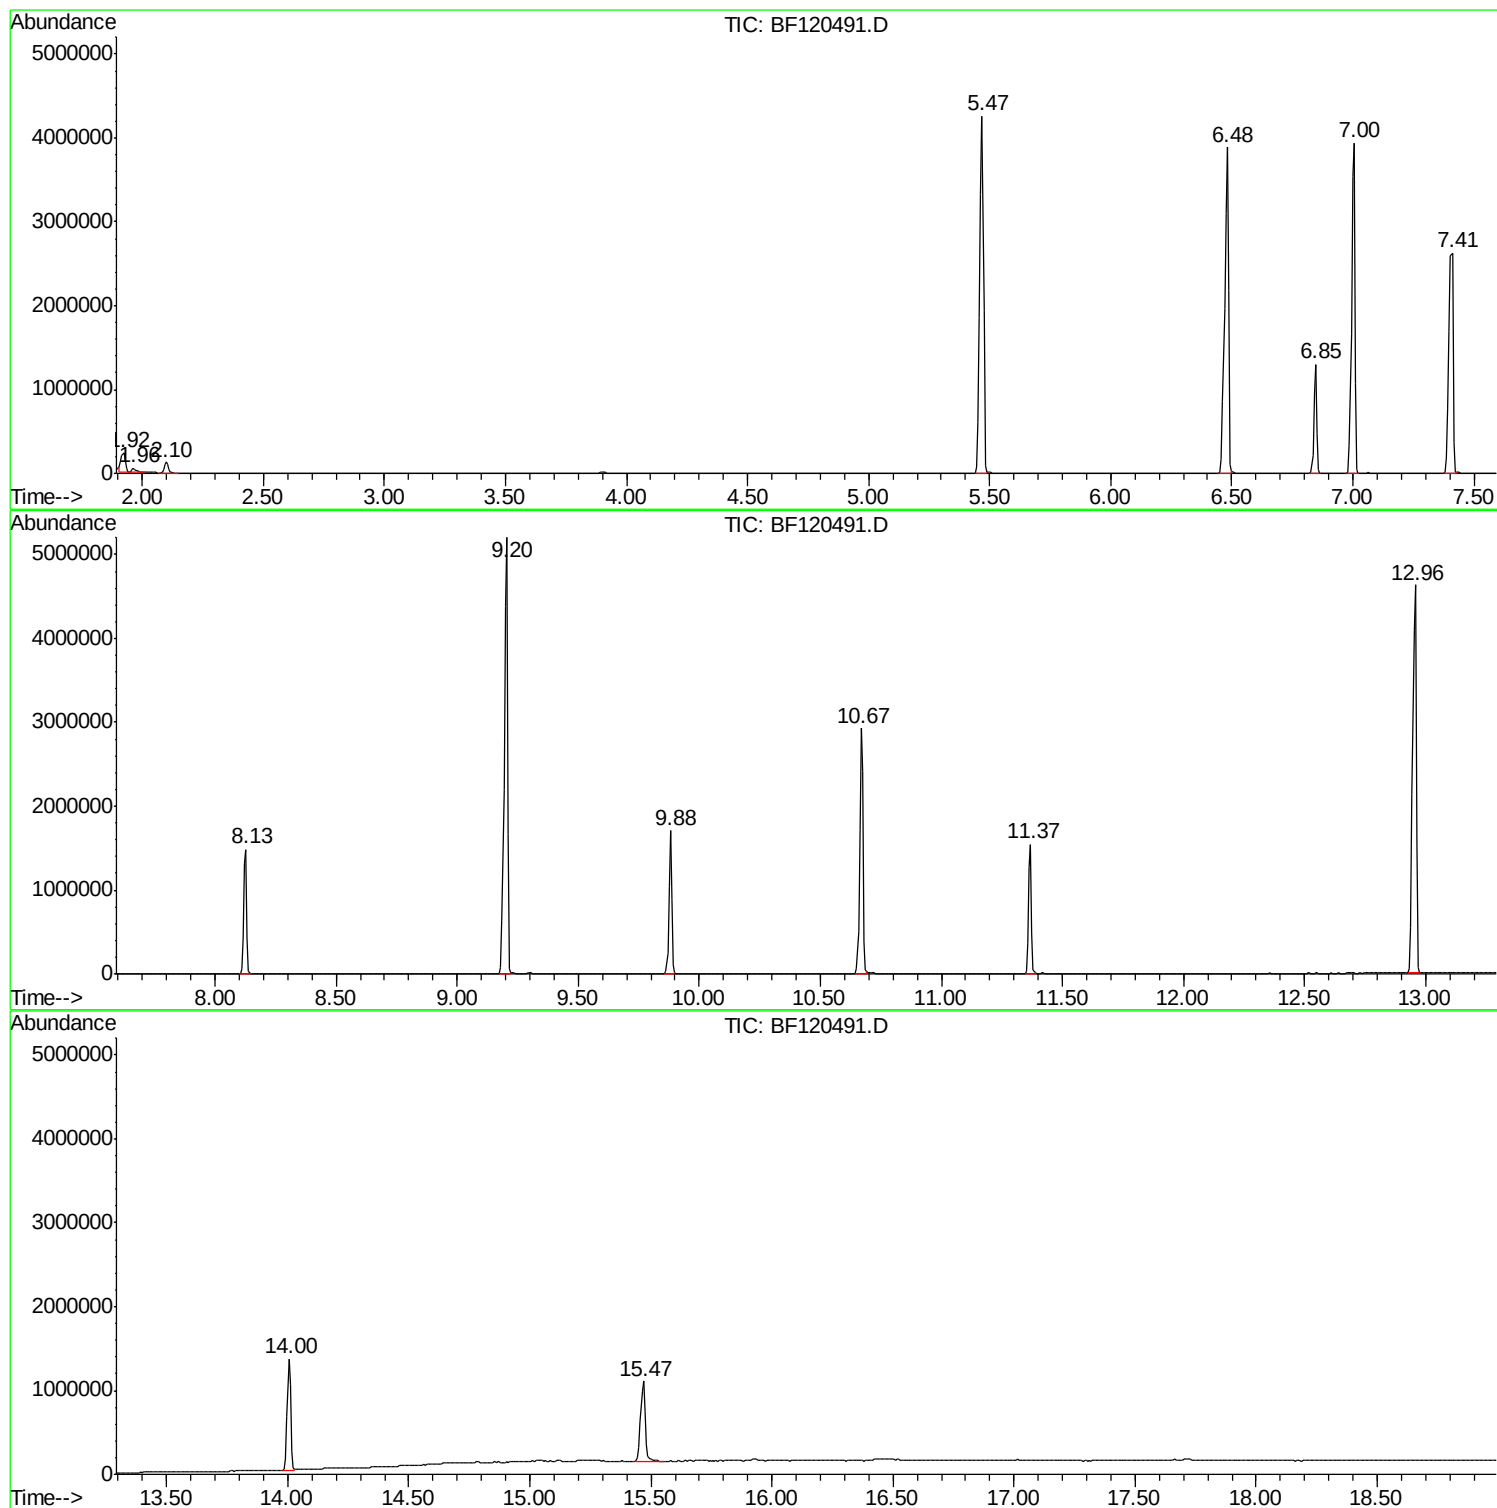

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060220\
Data File : BF120491.D
Acq On : 2 Jun 2020 13:34
Operator : JU/CG
Sample : PB129235BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129235BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.10	3.00 ng	157871	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	17
4		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	16
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	10

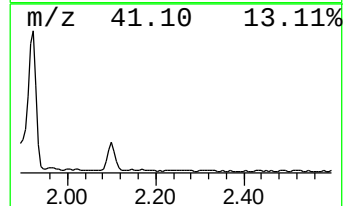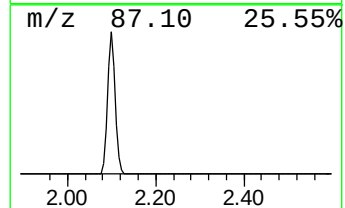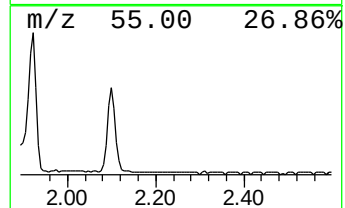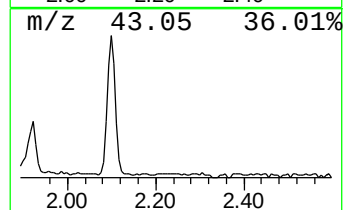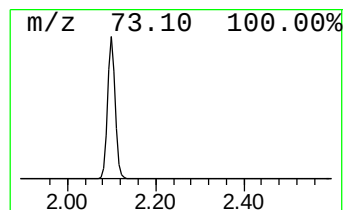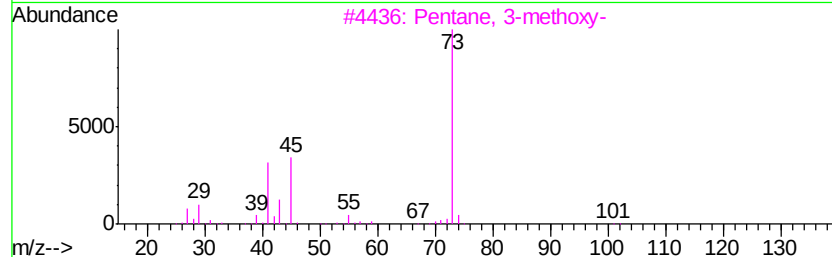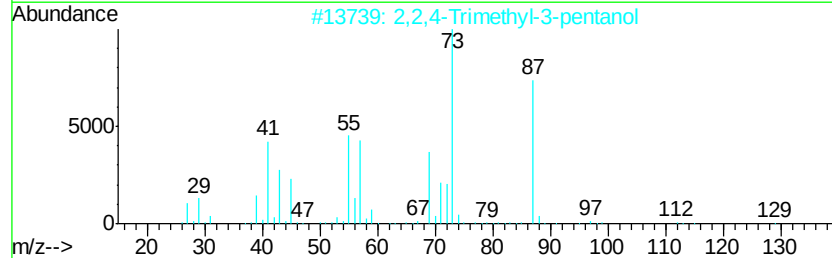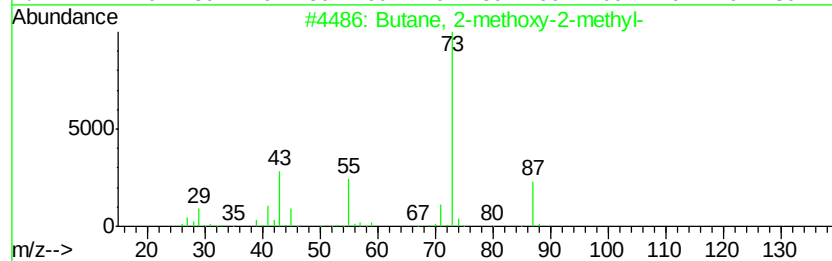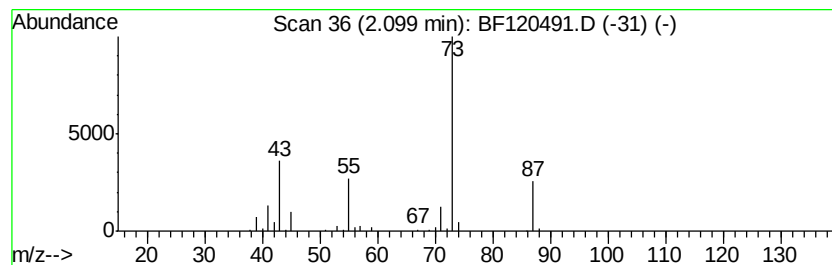

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060220\
Data File : BF120491.D
Acq On : 2 Jun 2020 13:34
Operator : JU/CG
Sample : PB129235BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129235BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.10	3.0	ng	157871	1	6.85	1053150	20.0