


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060220\
 Data File : BF120484.D
 Acq On : 2 Jun 2020 10:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 02 11:37:51 2020

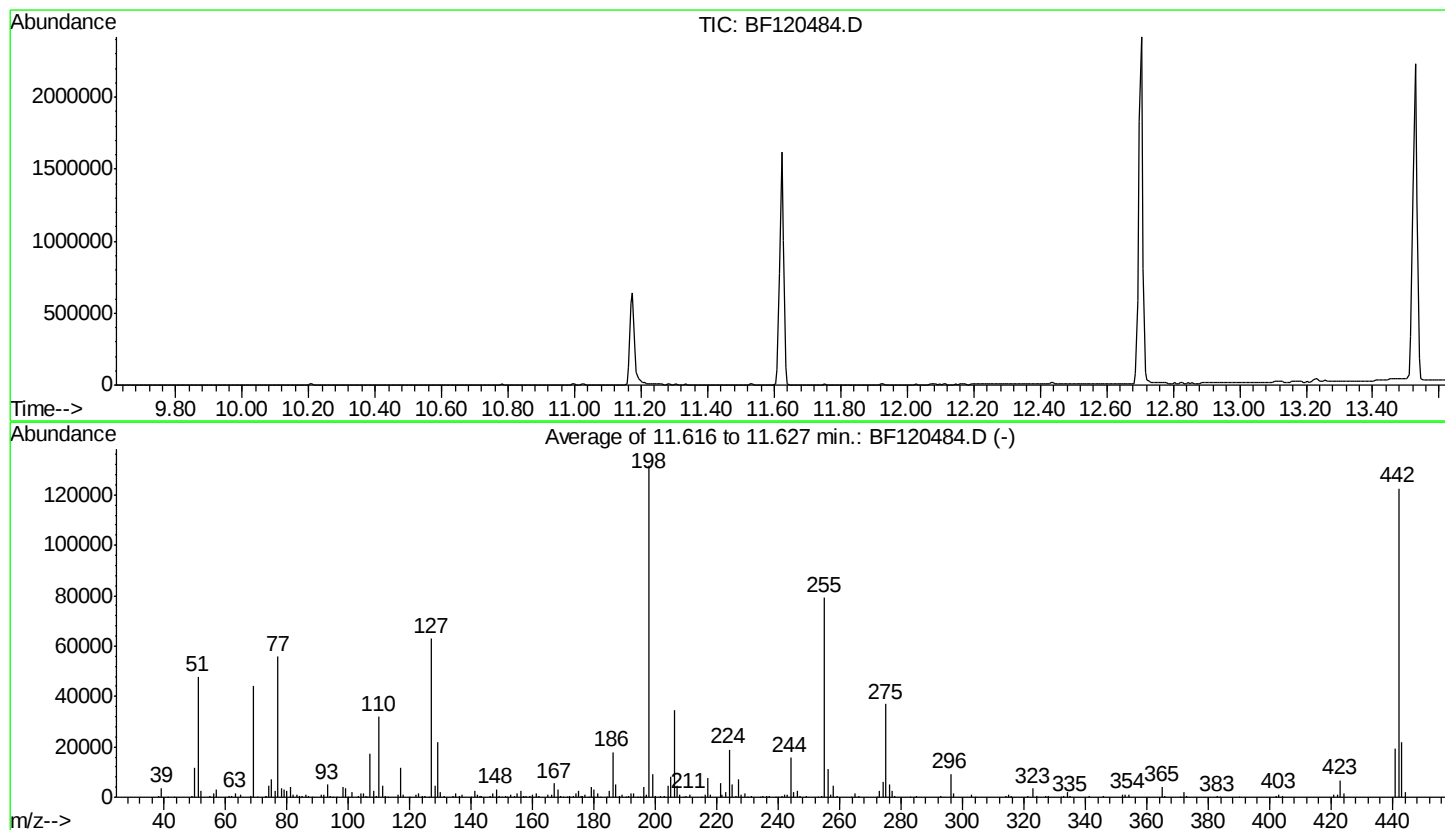

AutoFind: Scans 1654, 1655, 1656; Background Corrected with Scan 1649

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	47962	PASS
68	69	0.00	2	1.6	713	PASS
69	198	0.00	100	33.7	44405	PASS
70	69	0.00	2	0.3	147	PASS
127	198	10	80	47.8	62840	PASS
197	198	0.00	2	0.7	876	PASS
198	198	100	100	100.0	131602	PASS
199	198	5	9	7.0	9265	PASS
275	198	10	60	28.1	37016	PASS
365	198	1	100	3.3	4316	PASS
441	198	0.01	100	14.7	19399	PASS
442	198	50	100	93.2	122680	PASS
443	442	15	24	18.0	22036	PASS