

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
 Data File : BF128661.D
 Acq On : 03 Jun 2022 02:38
 Operator : CG\JU
 Sample : N2989-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P015-SS008-0006-01

Quant Time: Jun 03 03:28:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 17:07:23 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.822	152	79146	20.000	ng	0.00
21) Naphthalene-d8	8.104	136	292615	20.000	ng	0.00
39) Acenaphthene-d10	9.863	164	156293	20.000	ng	0.00
64) Phenanthrene-d10	11.351	188	271012	20.000	ng	# 0.00
76) Chrysene-d12	13.992	240	176973	20.000	ng	# 0.00
86) Perylene-d12	15.457	264	182064	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	383305	77.141	ng	0.00
7) Phenol-d6	6.486	99	480174	79.166	ng	-0.01
23) Nitrobenzene-d5	7.386	82	356199	56.676	ng	0.00
42) 2,4,6-Tribromophenol	10.657	330	137233	74.313	ng	0.00
45) 2-Fluorobiphenyl	9.186	172	664395	59.547	ng	0.00
79) Terphenyl-d14	12.939	244	583370	57.279	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	11.916	149	48961	3.218	ng	99
84) Bis(2-ethylhexyl)phtha...	13.980	149	37992	5.285	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
Data File : BF128661.D
Acq On : 03 Jun 2022 02:38
Operator : CG\JU
Sample : N2989-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P015-SS008-0006-01

Quant Time: Jun 03 03:28:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration



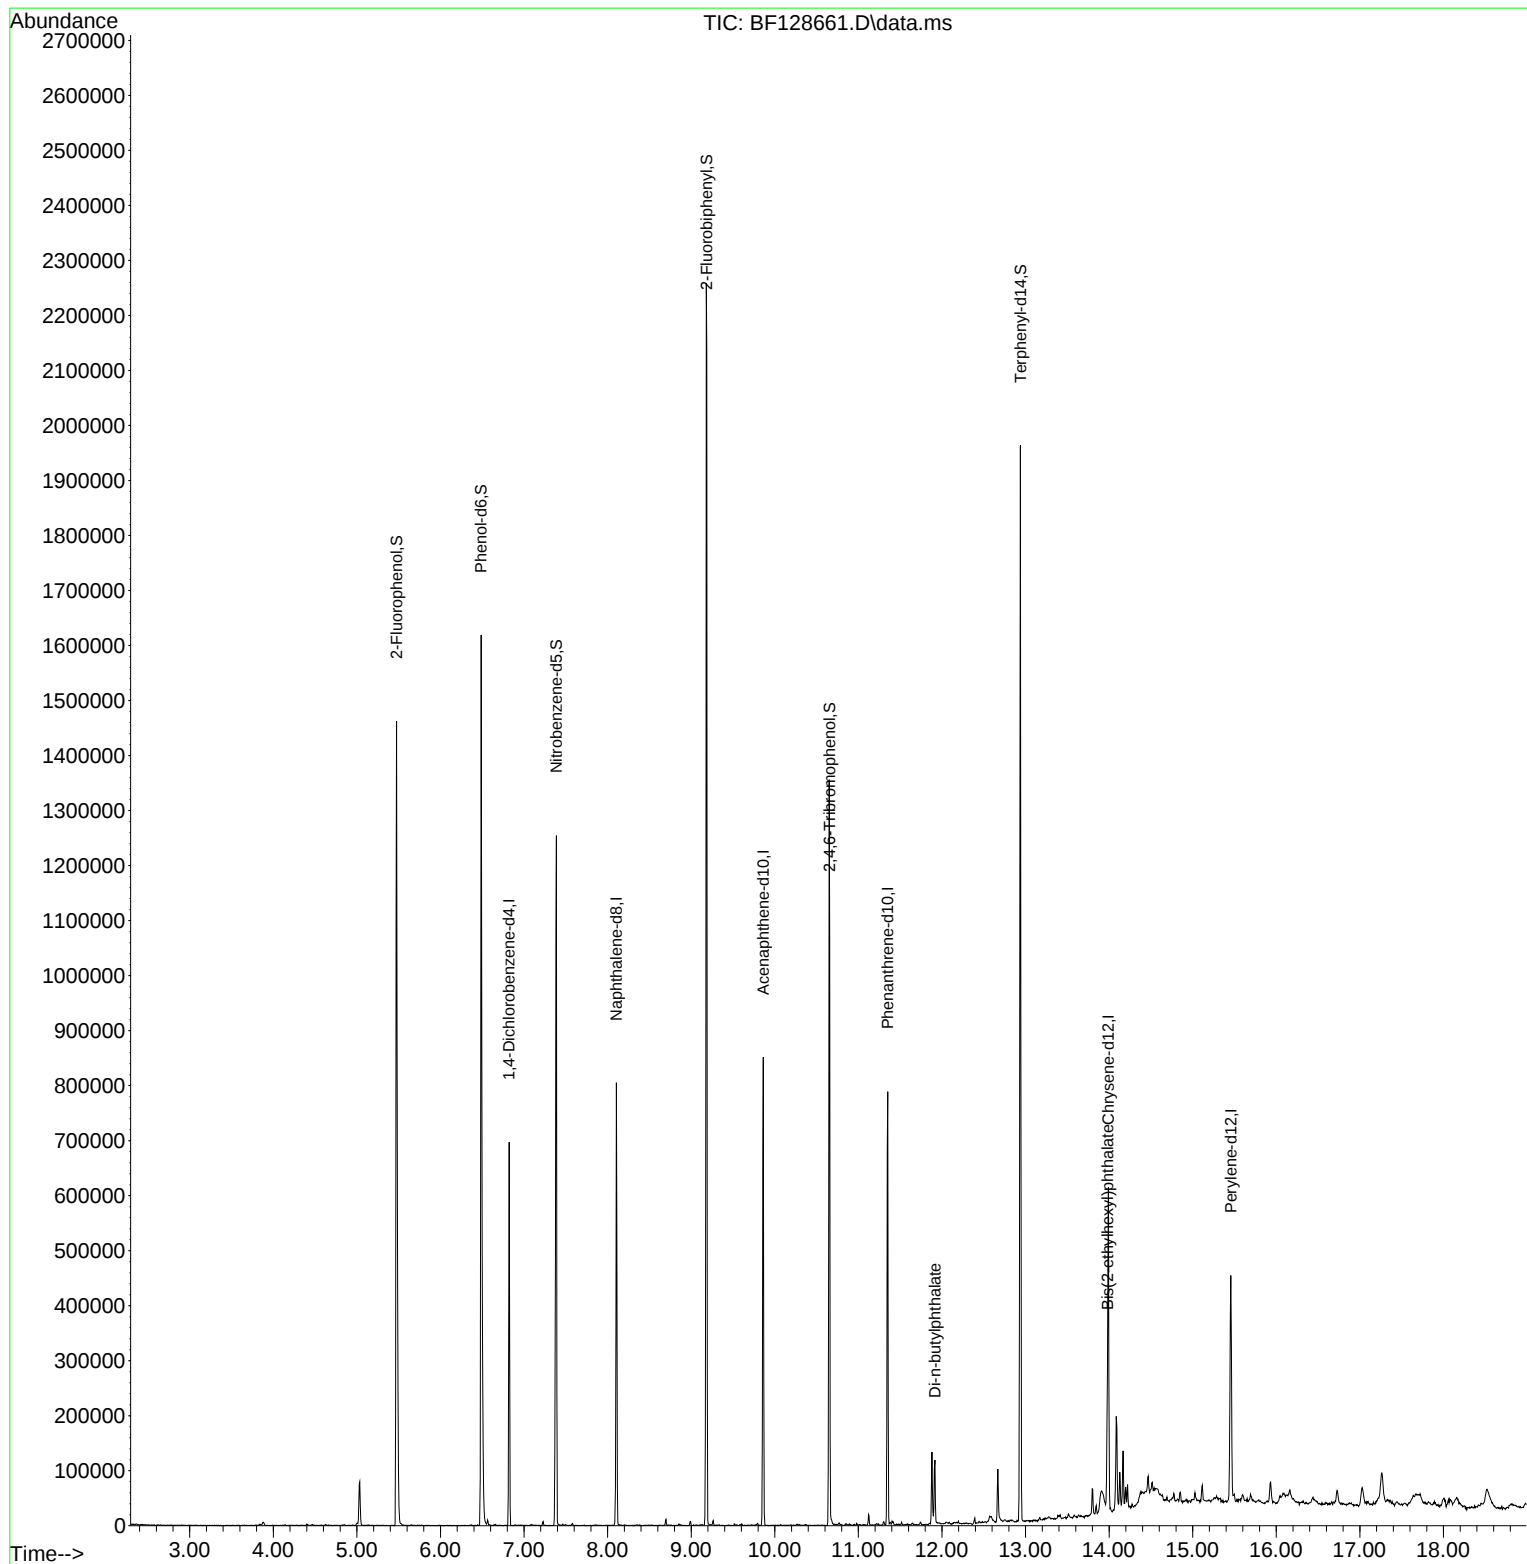


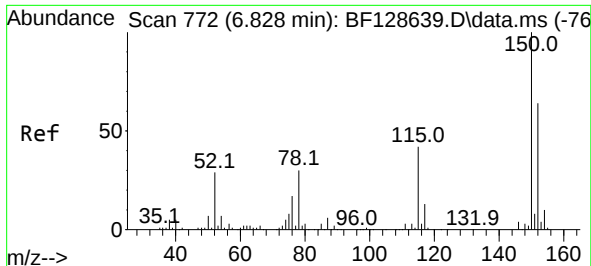

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.822 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38




Instrument :
BNA_F
ClientSampleId :
P015-SS008-0006-01

Tgt Ion:152 Resp: 79146
Ion Ratio Lower Upper
152 100
150 155.4 123.7 185.5
115 66.9 49.9 74.9

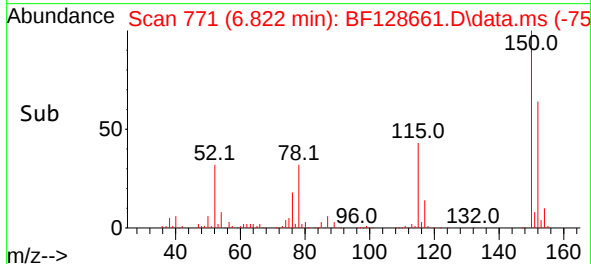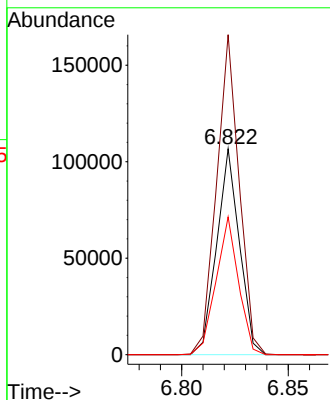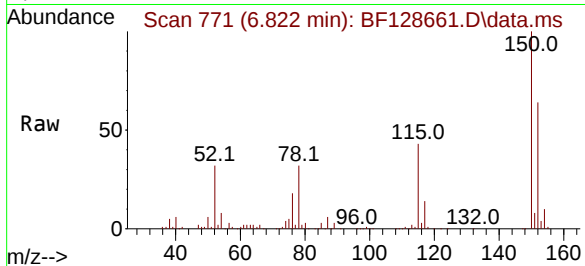

#5
2-Fluorophenol
Concen: 77.141 ng
RT: 5.475 min Scan# 542
Delta R.T. -0.000 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38

Tgt Ion:112 Resp: 383305
Ion Ratio Lower Upper
112 100
64 70.5 53.3 79.9
63 40.1 28.0 42.0

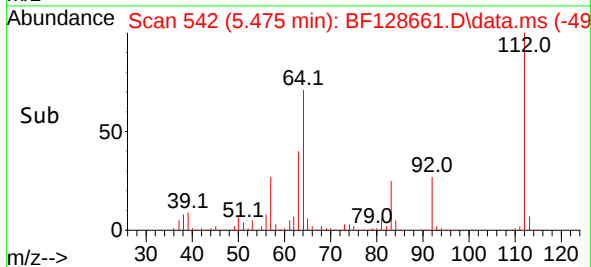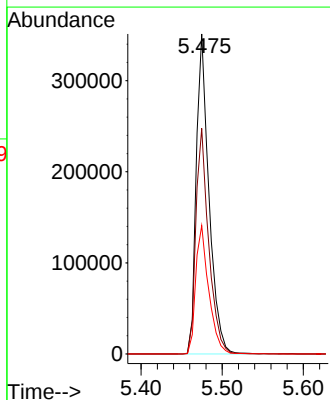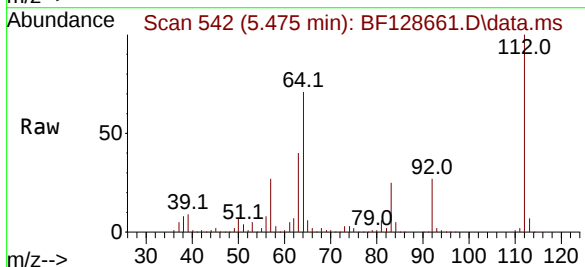



#7

Phenol-d6

Concen: 79.166 ng

RT: 6.486 min Scan# 716

Delta R.T. -0.012 min

Lab File: BF128661.D


Acq: 03 Jun 2022 02:38

Instrument :




BNA_F

ClientSampleId :

P015-SS008-0006-01

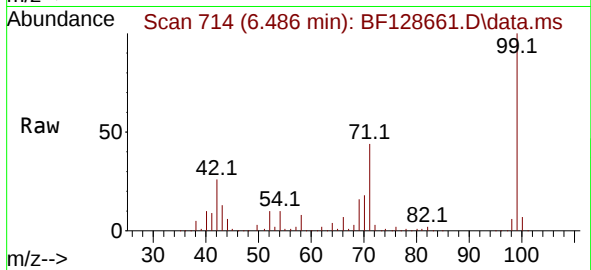

Tgt Ion:	99	Resp:	480174
Ion	Ratio	Lower	Upper
99	100		
42	25.8	17.3	25.9
71	44.3	28.9	43.3

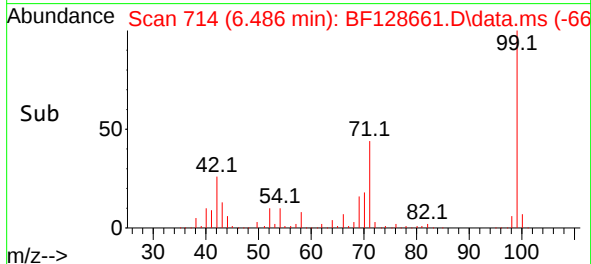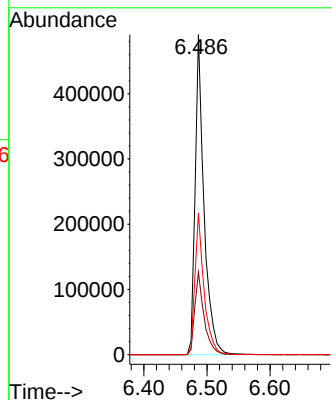

#21

Naphthalene-d8

Concen: 20.000 ng




RT: 8.104 min Scan# 989

Delta R.T. -0.006 min

Lab File: BF128661.D

Acq: 03 Jun 2022 02:38

Tgt Ion:	136	Resp:	292615
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.8	13.2
54	10.3	7.5	11.3
68	4.9	4.7	7.1

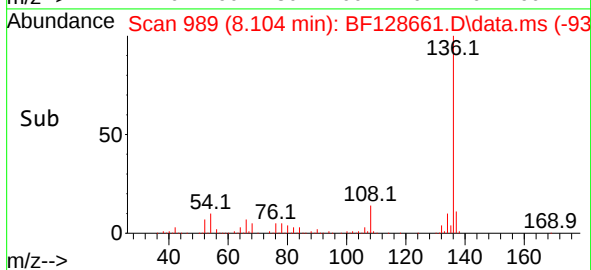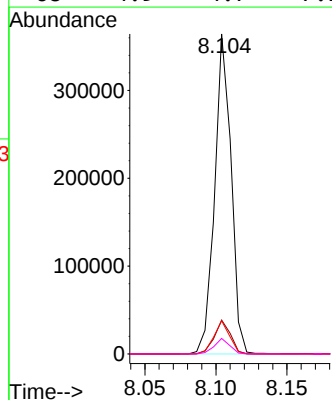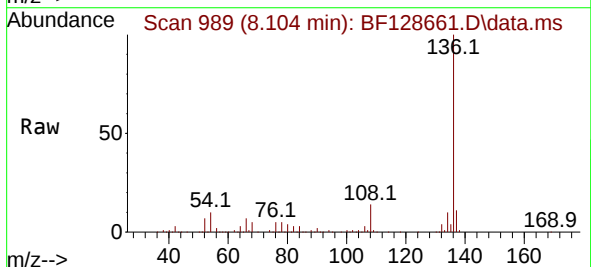



#23

Nitrobenzene-d5

Concen: 56.676 ng

RT: 7.386 min Scan# 8

Delta R.T. -0.006 min

Lab File: BF128661.D


Acq: 03 Jun 2022 02:38

Instrument :

BNA_F

ClientSampleId :

P015-SS008-0006-01






Tgt Ion: 82 Resp: 356199

Ion Ratio Lower Upper

82 100

128 41.1 34.0 51.0

54 64.2 46.9 70.3

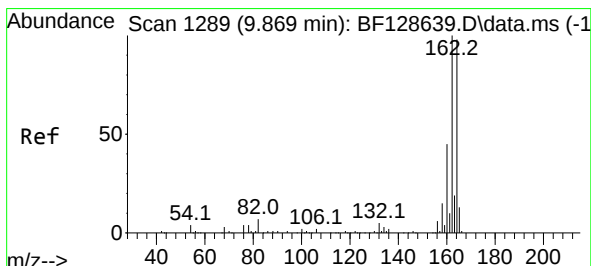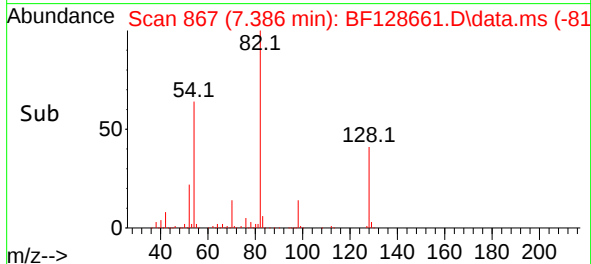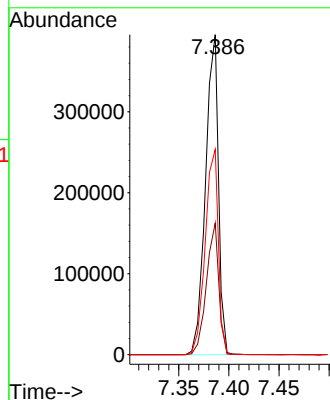

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.863 min Scan# 1288

Delta R.T. -0.006 min

Lab File: BF128661.D

Acq: 03 Jun 2022 02:38




Tgt Ion:164 Resp: 156293


Ion Ratio Lower Upper

164 100

162 104.3 79.5 119.3

160 46.9 34.2 51.4

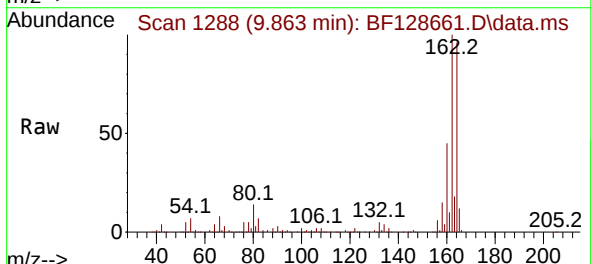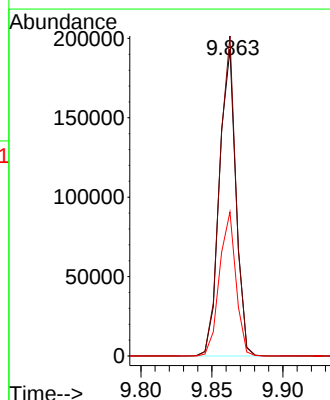



#42

2,4,6-Tribromophenol

Concen: 74.313 ng

RT: 10.657 min Scan# 1423

Delta R.T. -0.006 min

Lab File: BF128661.D


Acq: 03 Jun 2022 02:38

Instrument :

BNA_F

ClientSampleId :

P015-SS008-0006-01

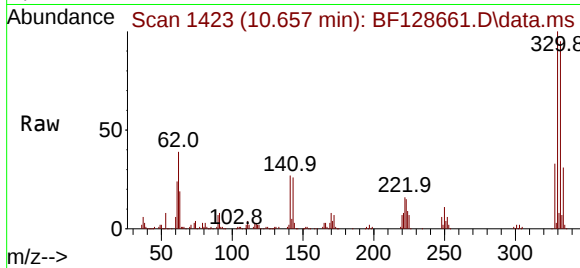




Tgt Ion:330 Resp: 137233

Ion Ratio Lower Upper

330 100

332 96.5 76.8 115.2

141 37.9 28.0 42.0

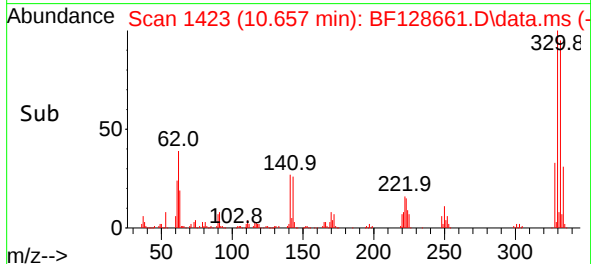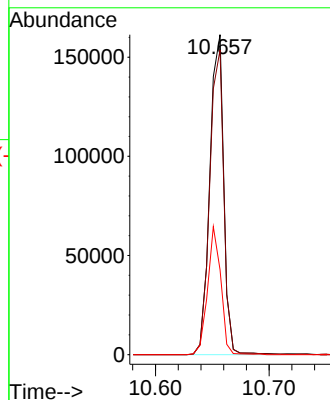

#45

2-Fluorobiphenyl

Concen: 59.547 ng

RT: 9.186 min Scan# 1173

Delta R.T. -0.006 min

Lab File: BF128661.D

Acq: 03 Jun 2022 02:38




Tgt Ion:172 Resp: 664395


Ion Ratio Lower Upper

172 100

171 35.0 28.8 43.2

170 23.3 19.8 29.8

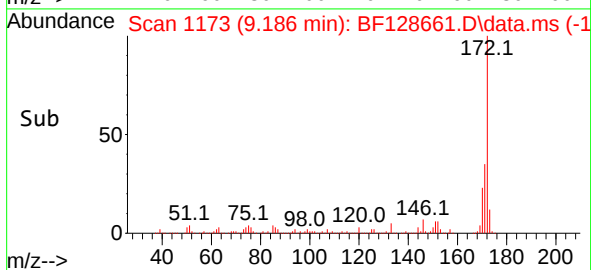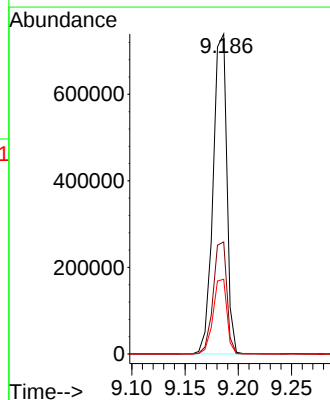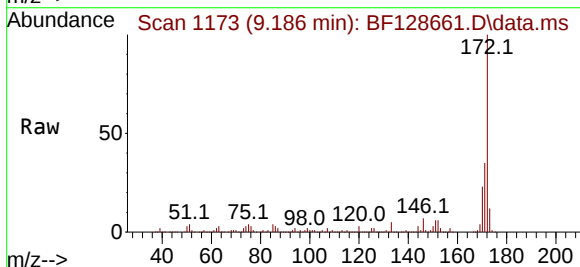



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.351 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF128661.D

Acq: 03 Jun 2022 02:38

Instrument :

BNA_F

ClientSampleId :

P015-SS008-0006-01





Tgt Ion:188 Resp: 271012

Ion Ratio Lower Upper

188 100

94 6.4 7.0 10.6#

80 6.7 7.6 11.4#

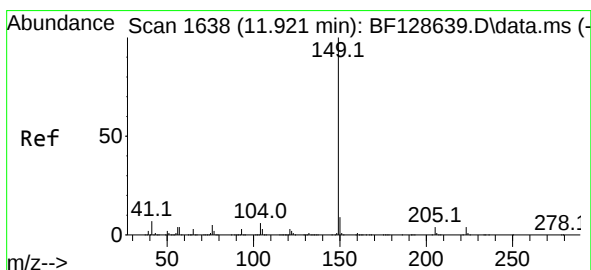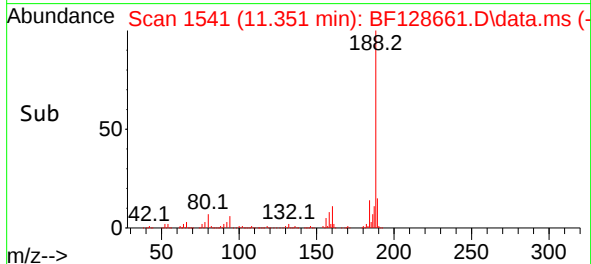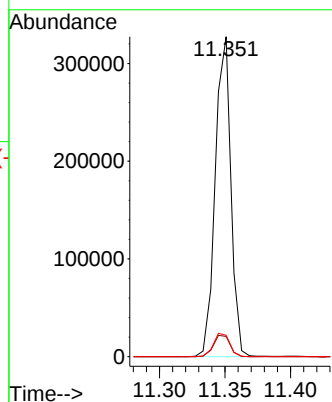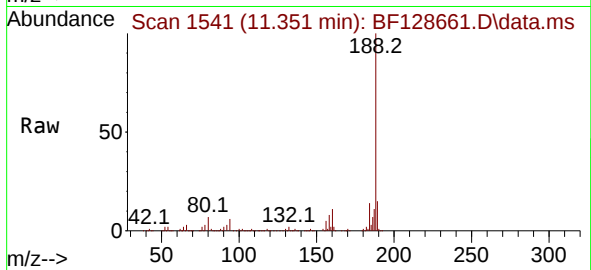

#74

Di-n-butylphthalate

Concen: 3.218 ng

RT: 11.916 min Scan# 1637

Delta R.T. -0.006 min

Lab File: BF128661.D

Acq: 03 Jun 2022 02:38




Tgt Ion:149 Resp: 48961


Ion Ratio Lower Upper

149 100

150 9.7 7.5 11.3


104 5.7 4.4 6.6

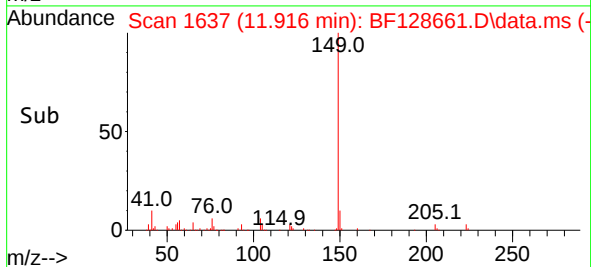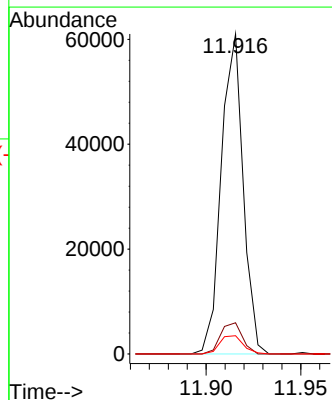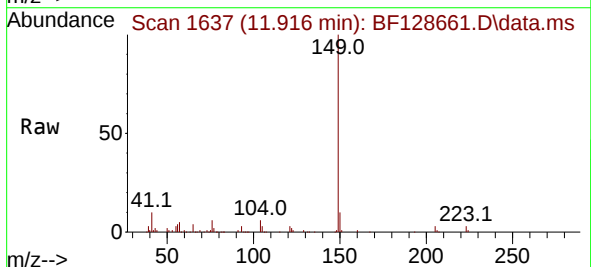



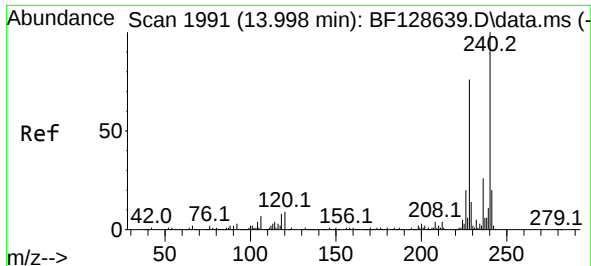


#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.992 min Scan# 1990
Delta R.T. -0.006 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38

Instrument :
BNA_F
ClientSampleId :
P015-SS008-0006-01







Tgt Ion:240 Resp: 176973
Ion Ratio Lower Upper
240 100
120 7.3 8.9 13.3#
236 26.2 20.8 31.2

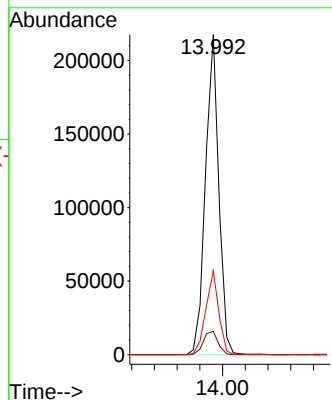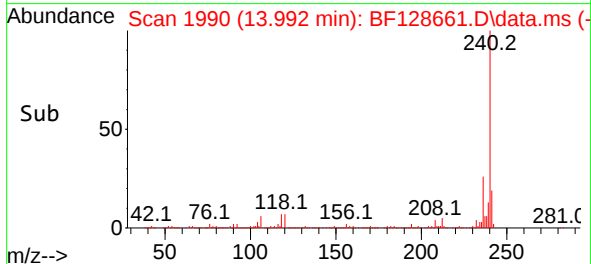

#79
Terphenyl-d14
Concen: 57.279 ng
RT: 12.939 min Scan# 1811
Delta R.T. -0.006 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38

Tgt Ion:244 Resp: 583370
Ion Ratio Lower Upper
244 100
212 7.8 6.1 9.1
122 8.7 8.8 13.2#


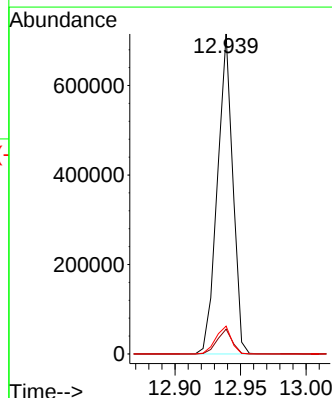
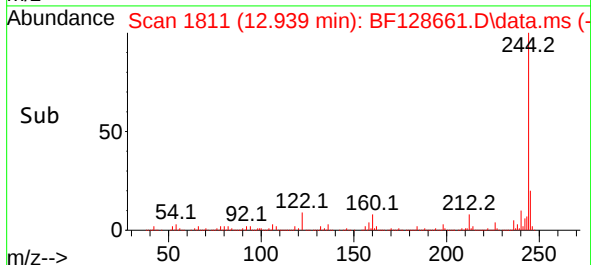
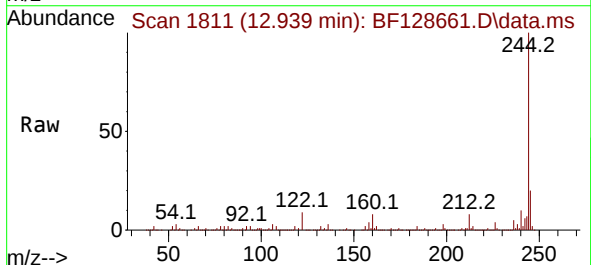




#84
Bis(2-ethylhexyl)phthalate
Concen: 5.285 ng
RT: 13.980 min Scan# 1988
Delta R.T. -0.000 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38

Instrument :
BNA_F
ClientSampleId :
P015-SS008-0006-01

Tgt Ion:149 Resp: 37992
Ion Ratio Lower Upper
149 100
167 25.0 21.0 31.4
279 4.0 3.1 4.7

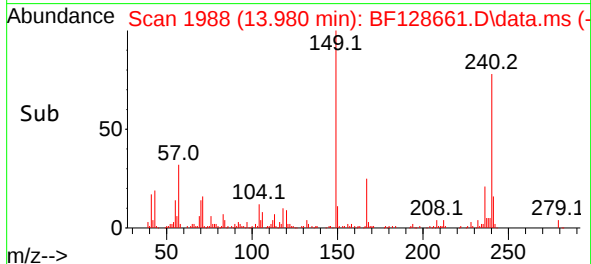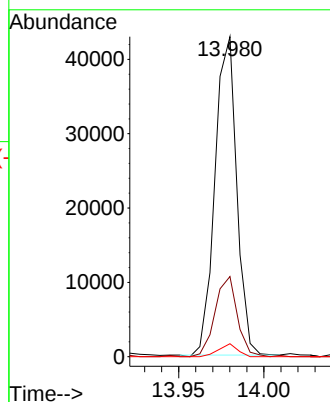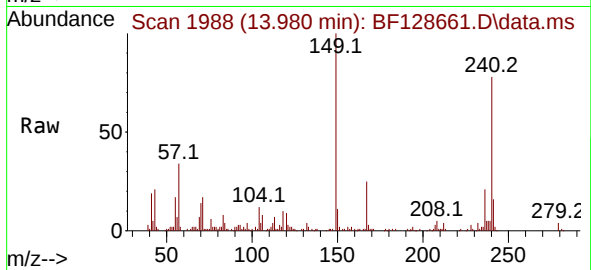

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.457 min Scan# 2239
Delta R.T. -0.005 min
Lab File: BF128661.D
Acq: 03 Jun 2022 02:38

Tgt Ion:264 Resp: 182064
Ion Ratio Lower Upper
264 100
260 24.1 18.4 27.6
265 22.2 17.2 25.8

