


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
 Data File : BF128635.D
 Acq On : 02 Jun 2022 10:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 17:07:23 2022

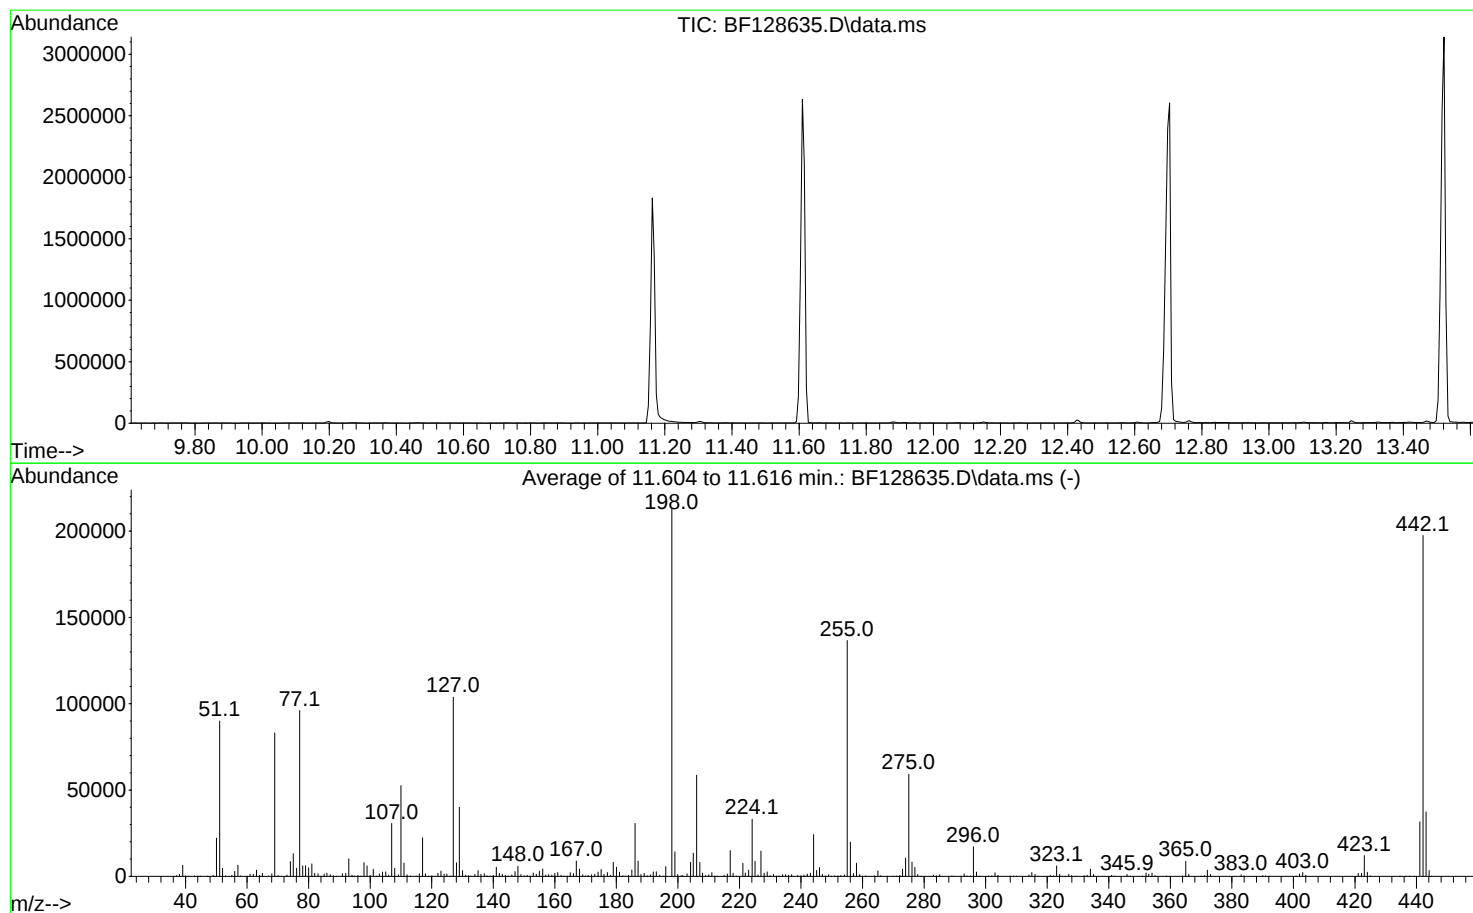

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	89965	PASS
68	69	0.00	2	1.8	1531	PASS
69	198	0.00	100	39.0	83181	PASS
70	69	0.00	2	0.6	478	PASS
127	198	10	80	48.7	103843	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	213104	PASS
199	198	5	9	6.6	14162	PASS
275	198	10	60	27.7	59107	PASS
365	198	1	100	4.1	8705	PASS
441	198	0.01	100	14.8	31625	PASS
442	442	50	100	100.0	197485	PASS
443	442	15	24	18.9	37374	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_F	<u>BF128635.D</u>
Compound Name	Response	Retention Time
DDT	524896	13.52
DDD	512	13.21
DDE	188	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
700	525596	0.13

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
Data File : BF128635.D
Acq On : 02 Jun 2022 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 13:25:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 13:18:43 2022
Response via : Initial Calibration

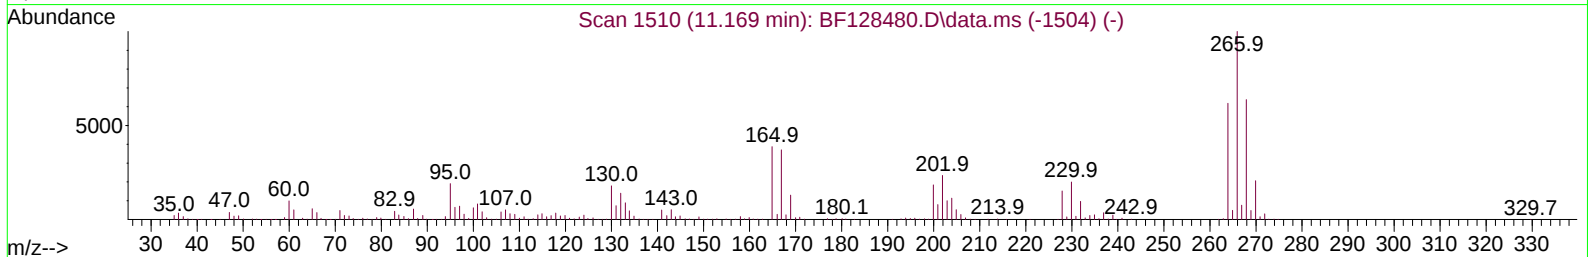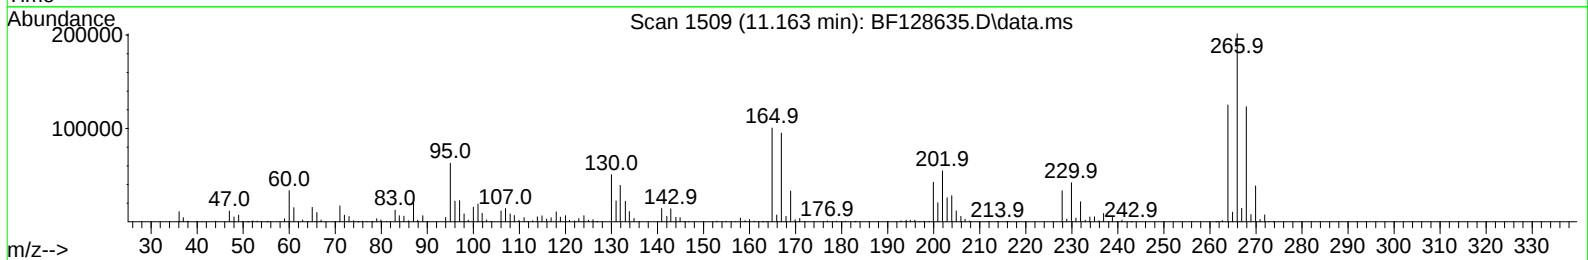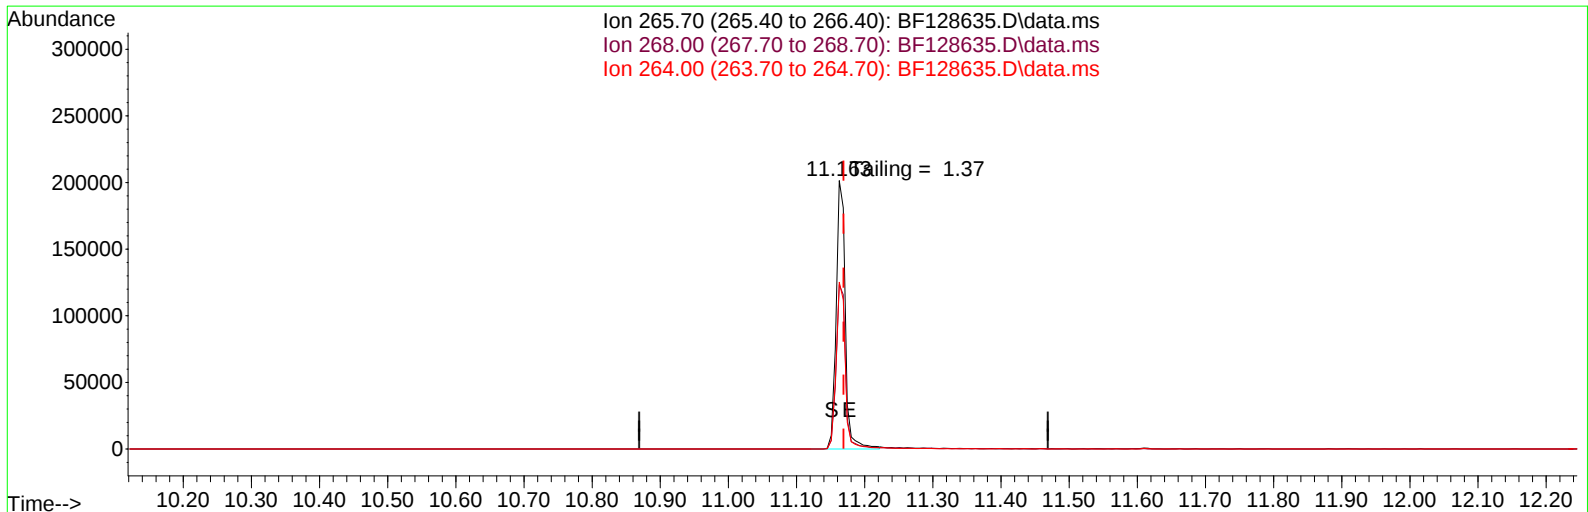

TIC: BF128635.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 22438.39 ng




response 189395

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	61.26
264.00	61.80	62.14
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\  
Data File : BF128635.D  
Acq On    : 02 Jun 2022  10:08  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 02 13:25:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 13:18:43 2022
Response via : Initial Calibration

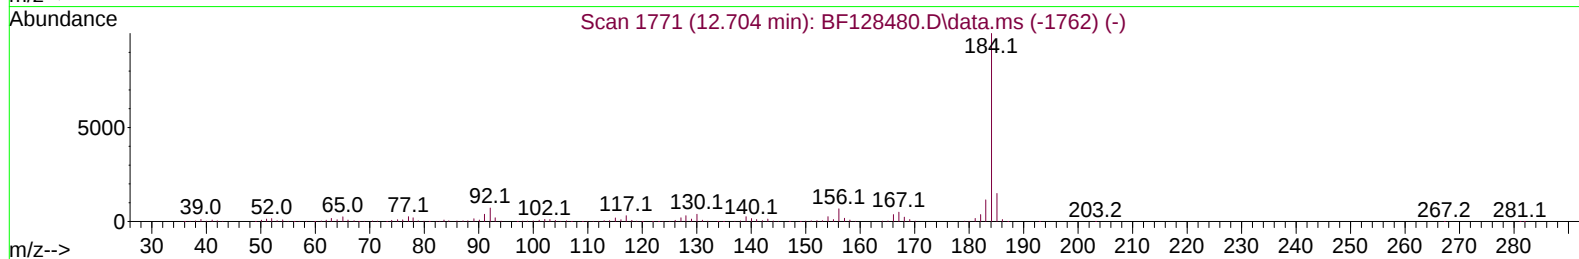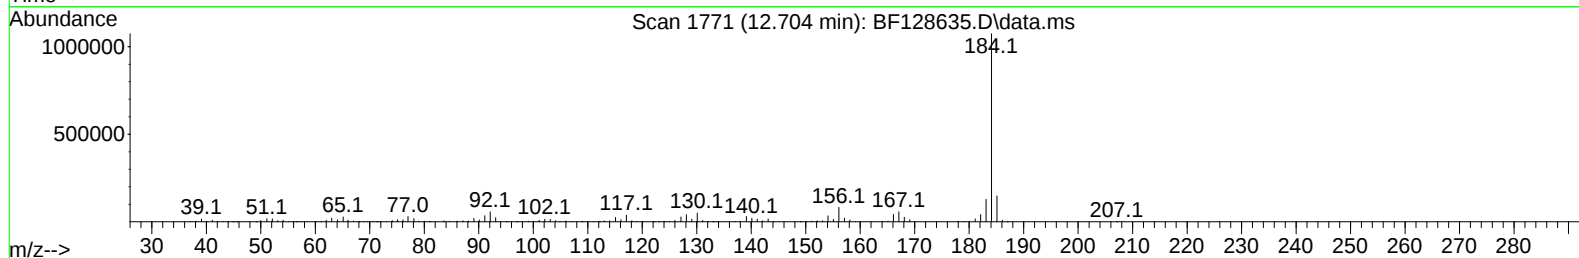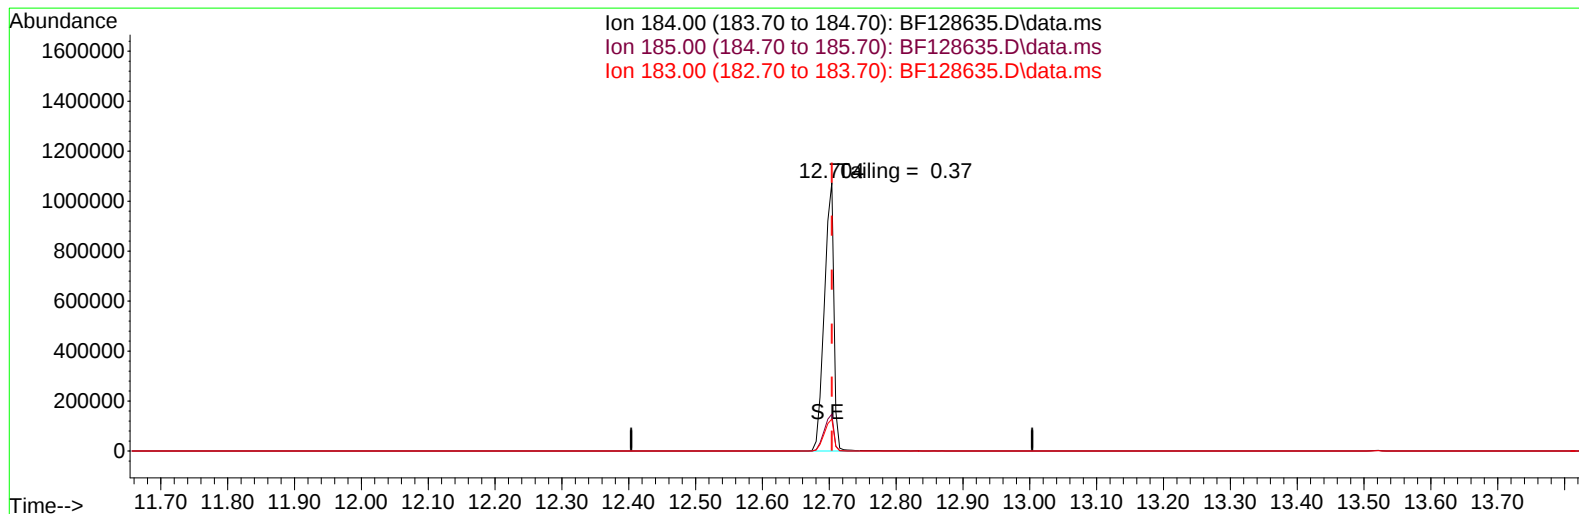

TIC: BF128635.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response **1061751**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.70
183.00	11.60	11.92
0.00	0.00	0.00