


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
 Data File : BF128645.D
 Acq On : 02 Jun 2022 18:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 17:07:23 2022

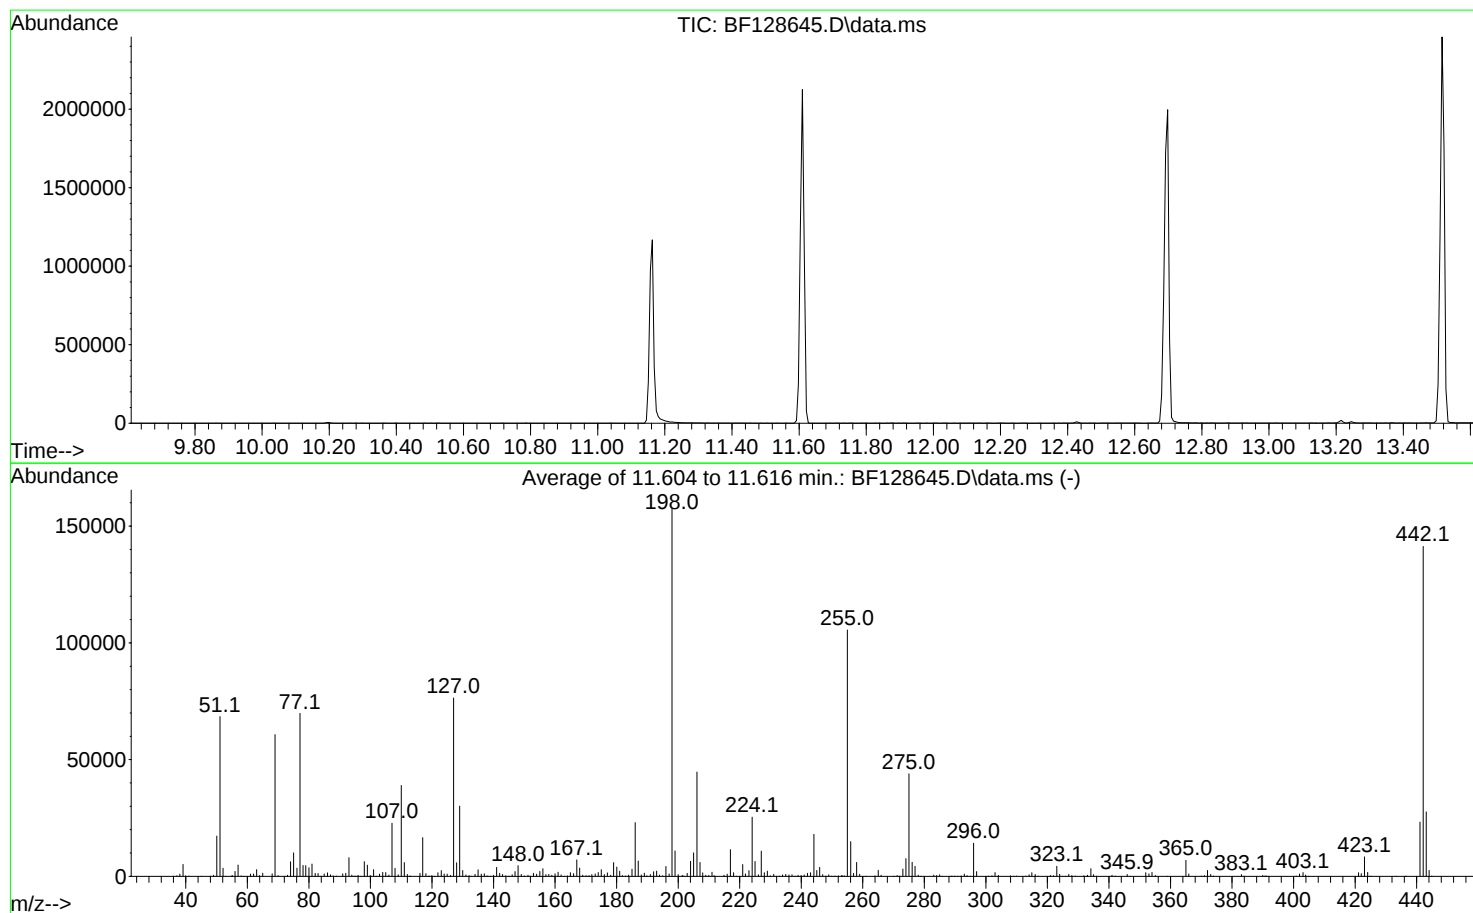

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	68461	PASS
68	69	0.00	2	1.8	1117	PASS
69	198	0.00	100	38.6	60755	PASS
70	69	0.00	2	0.5	314	PASS
127	198	10	80	48.5	76389	PASS
197	198	0.00	2	0.7	1040	PASS
198	198	100	100	100.0	157560	PASS
199	198	5	9	6.9	10883	PASS
275	198	10	60	27.9	43901	PASS
365	198	1	100	4.4	6879	PASS
441	198	0.01	100	14.7	23223	PASS
442	442	50	100	100.0	141325	PASS
443	442	15	24	19.6	27653	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
6/2/2022	BNA_F	<u>BF128645.D</u>
Compound Name	Response	Retention Time
DDT	391052	13.515
DDD	4795	13.215
DDE	358	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5153	396205	1.30

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
Data File : BF128645.D
Acq On : 02 Jun 2022 18:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 03 05:17:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

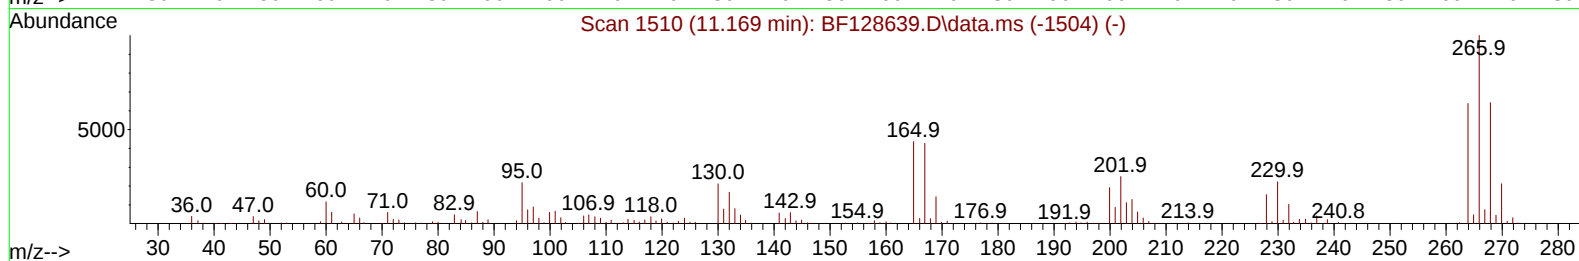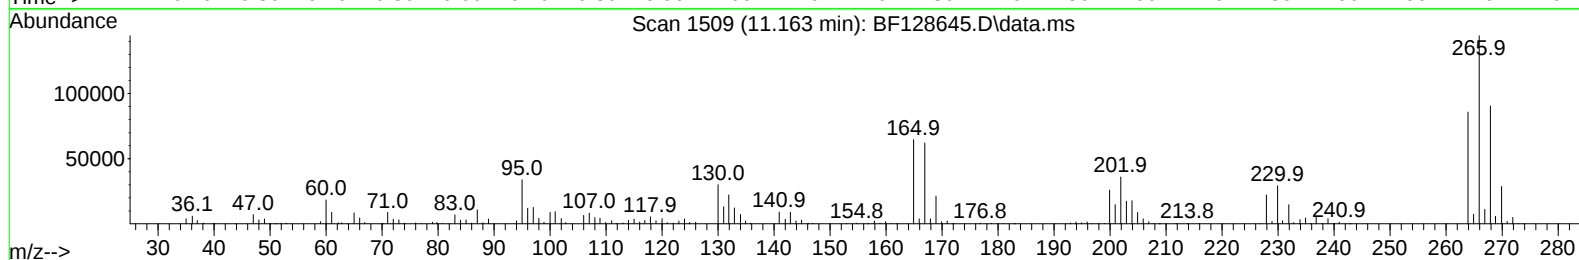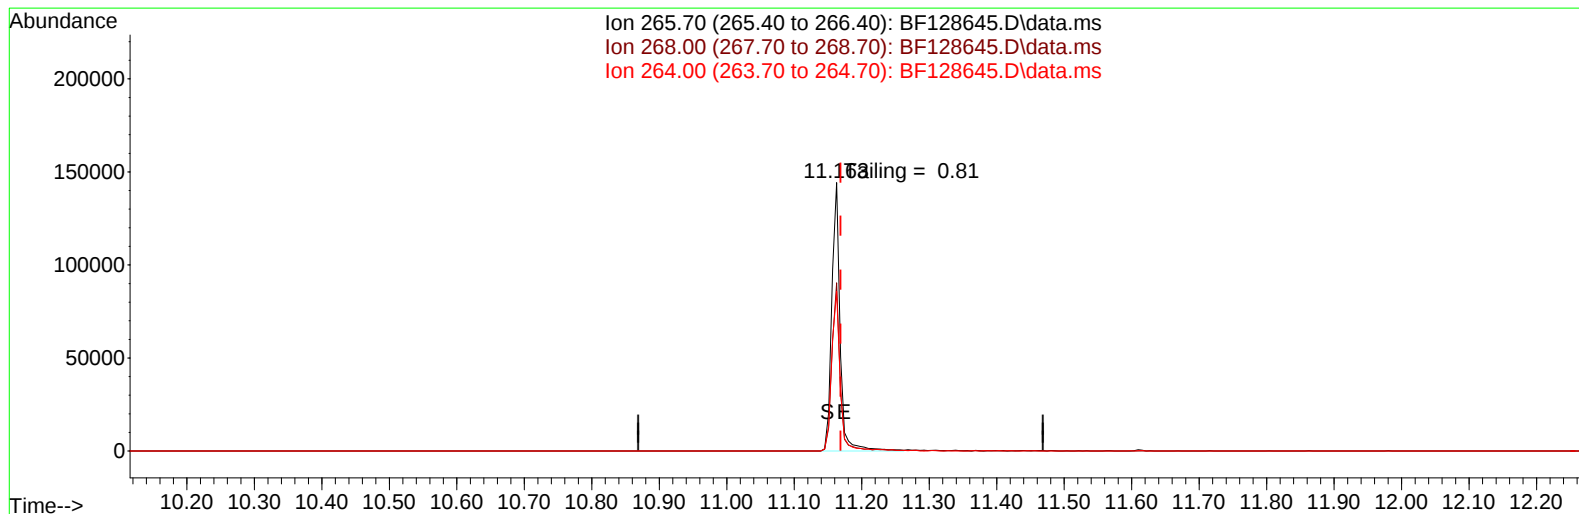

TIC: BF128645.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 28970.40 ng




response 123222

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.69
264.00	61.80	59.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060222\
Data File : BF128645.D
Acq On : 02 Jun 2022 18:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 03 05:17:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 17:07:23 2022
Response via : Initial Calibration

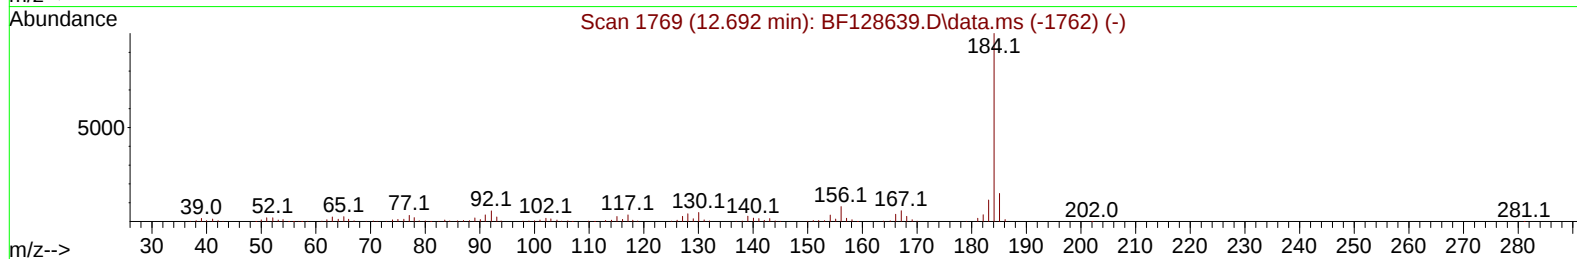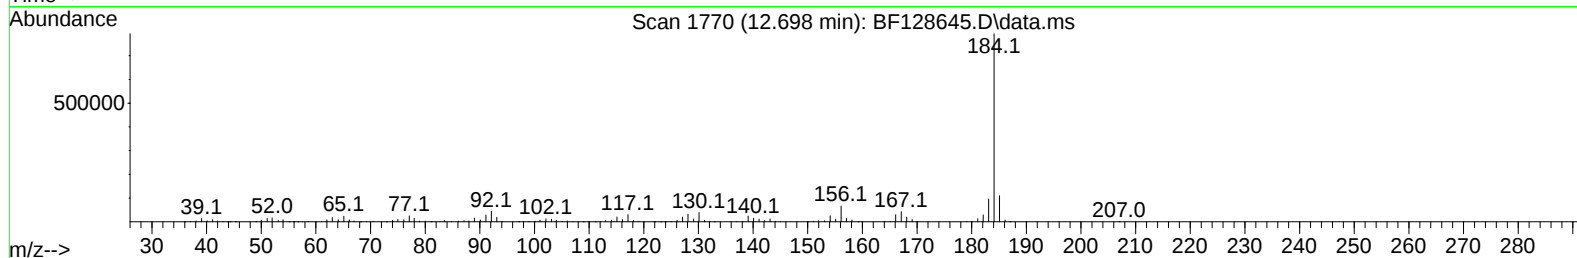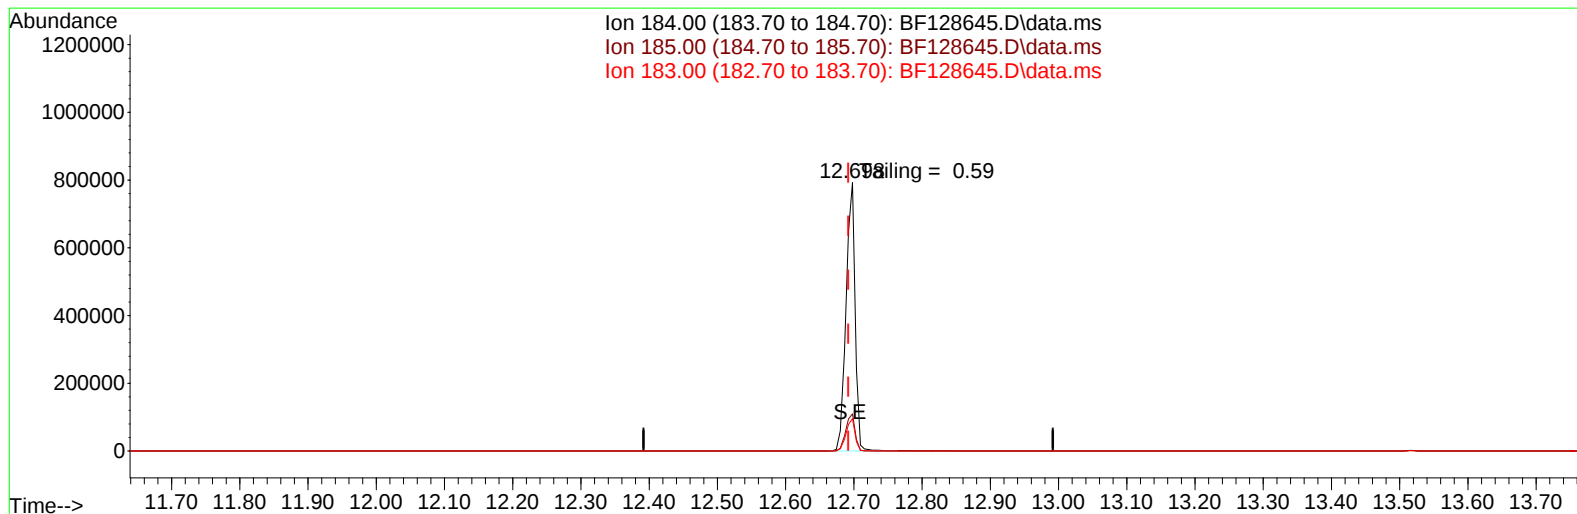

TIC: BF128645.D\data.ms

(77) Benzidine

12.698min (+ 0.006) 0.00 ng

response 733828

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.87
183.00	11.60	12.07
0.00	0.00	0.00