
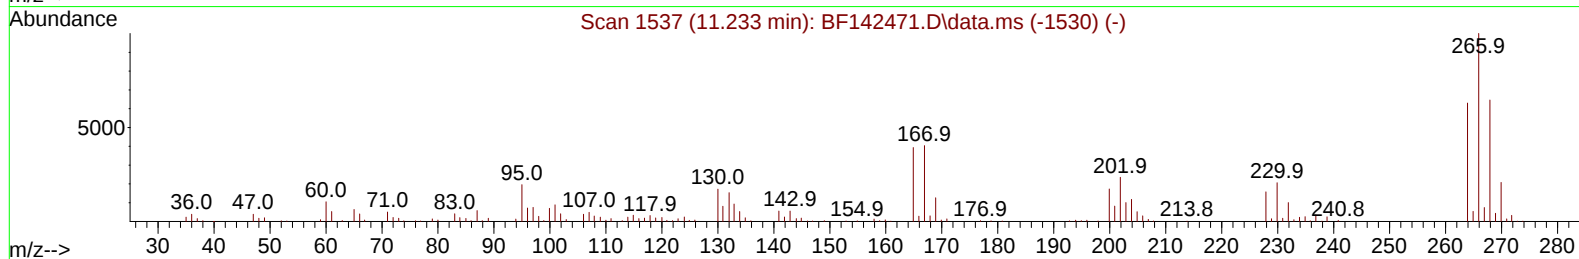
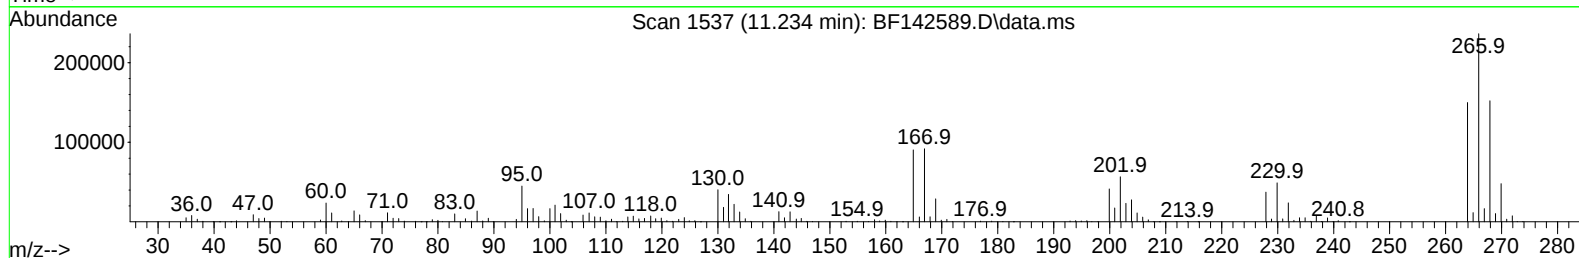


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060225\
Data File : BF142589.D
Acq On : 02 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 12:45:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

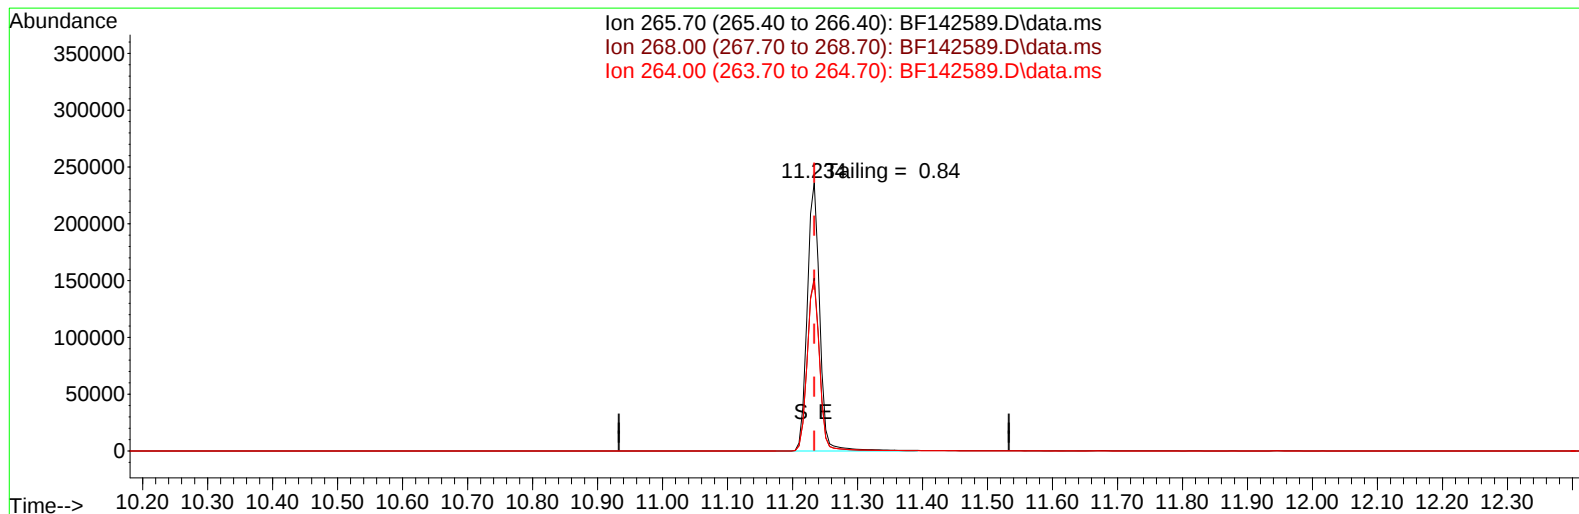

TIC: BF142589.D\data.ms

(70) Pentachlorophenol (C)




11.234min (+ 0.000) 81847.51 ng m

response 317877

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.41
264.00	63.00	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060225\
Data File : BF142589.D
Acq On : 02 Jun 2025 11:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 02 12:45:30 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

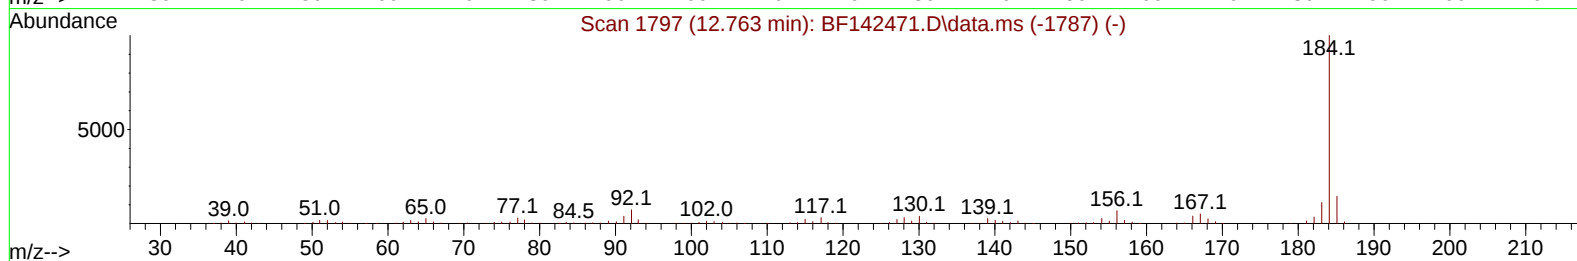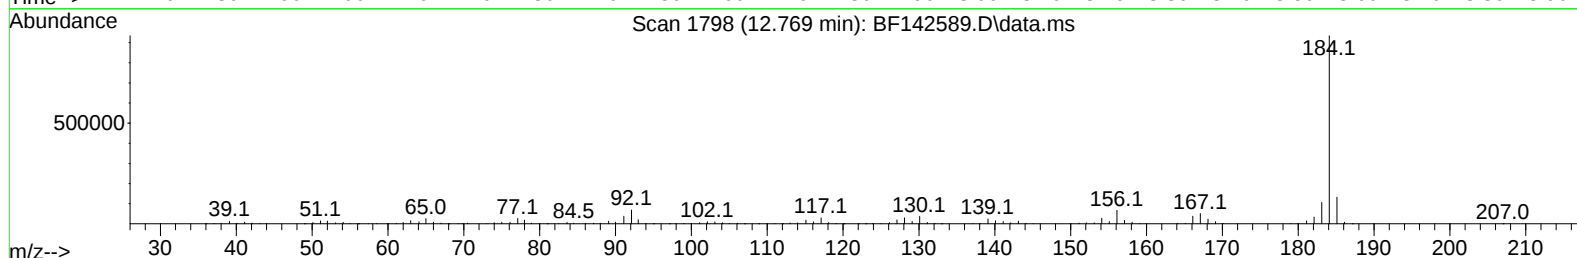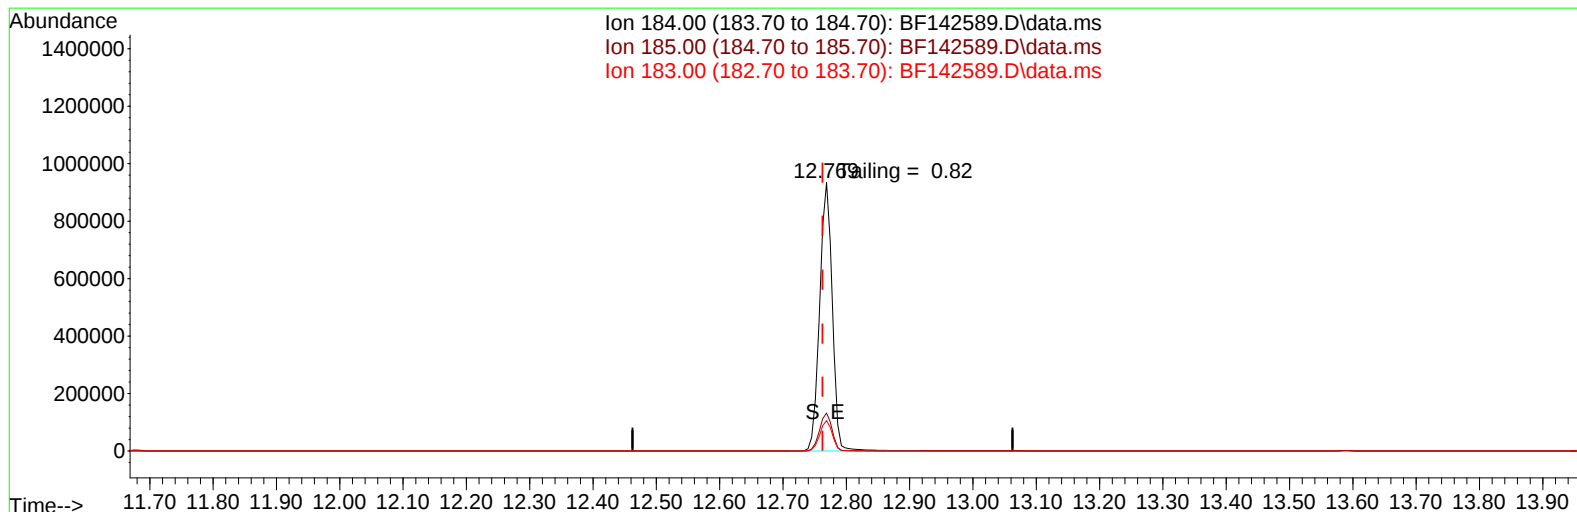

TIC: BF142589.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 63416.49 ng

response 1295595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.12
183.00	11.20	11.33
0.00	0.00	0.00