



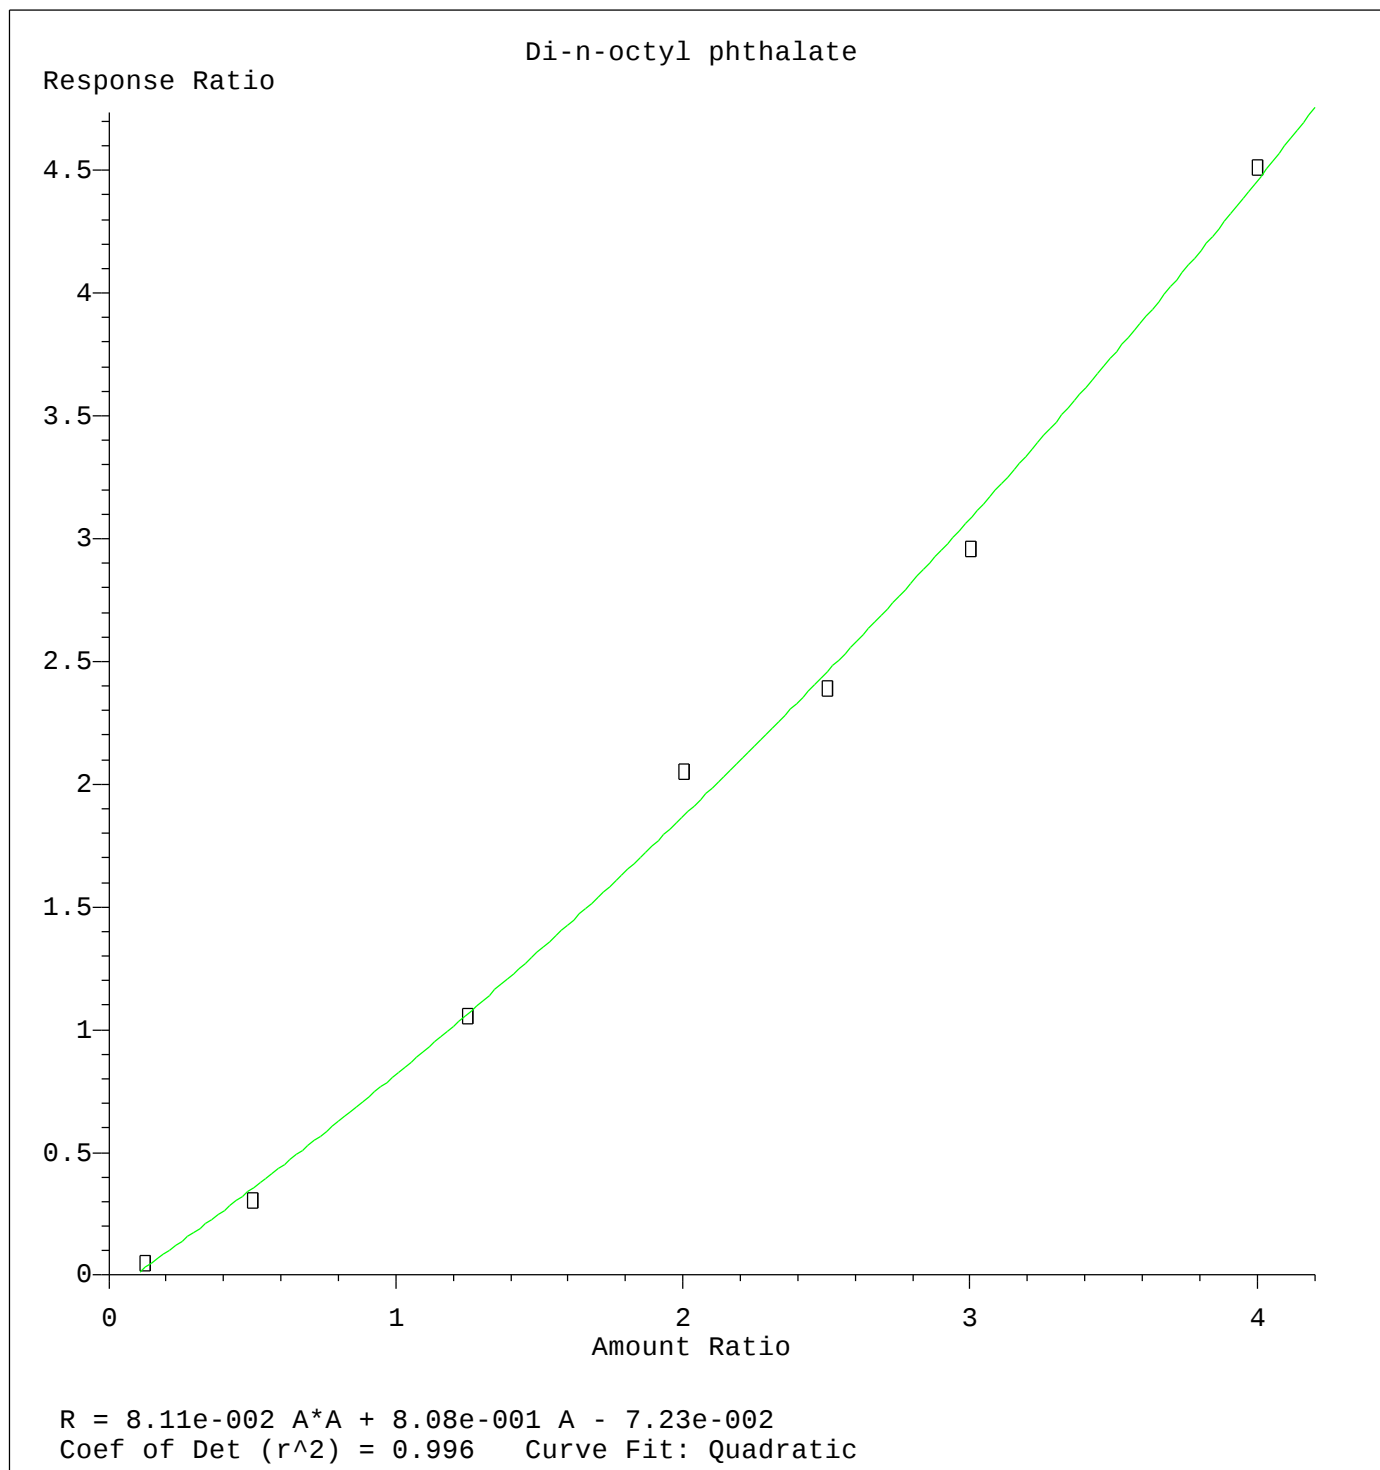

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015


2-Fluorophenol

Response Ratio

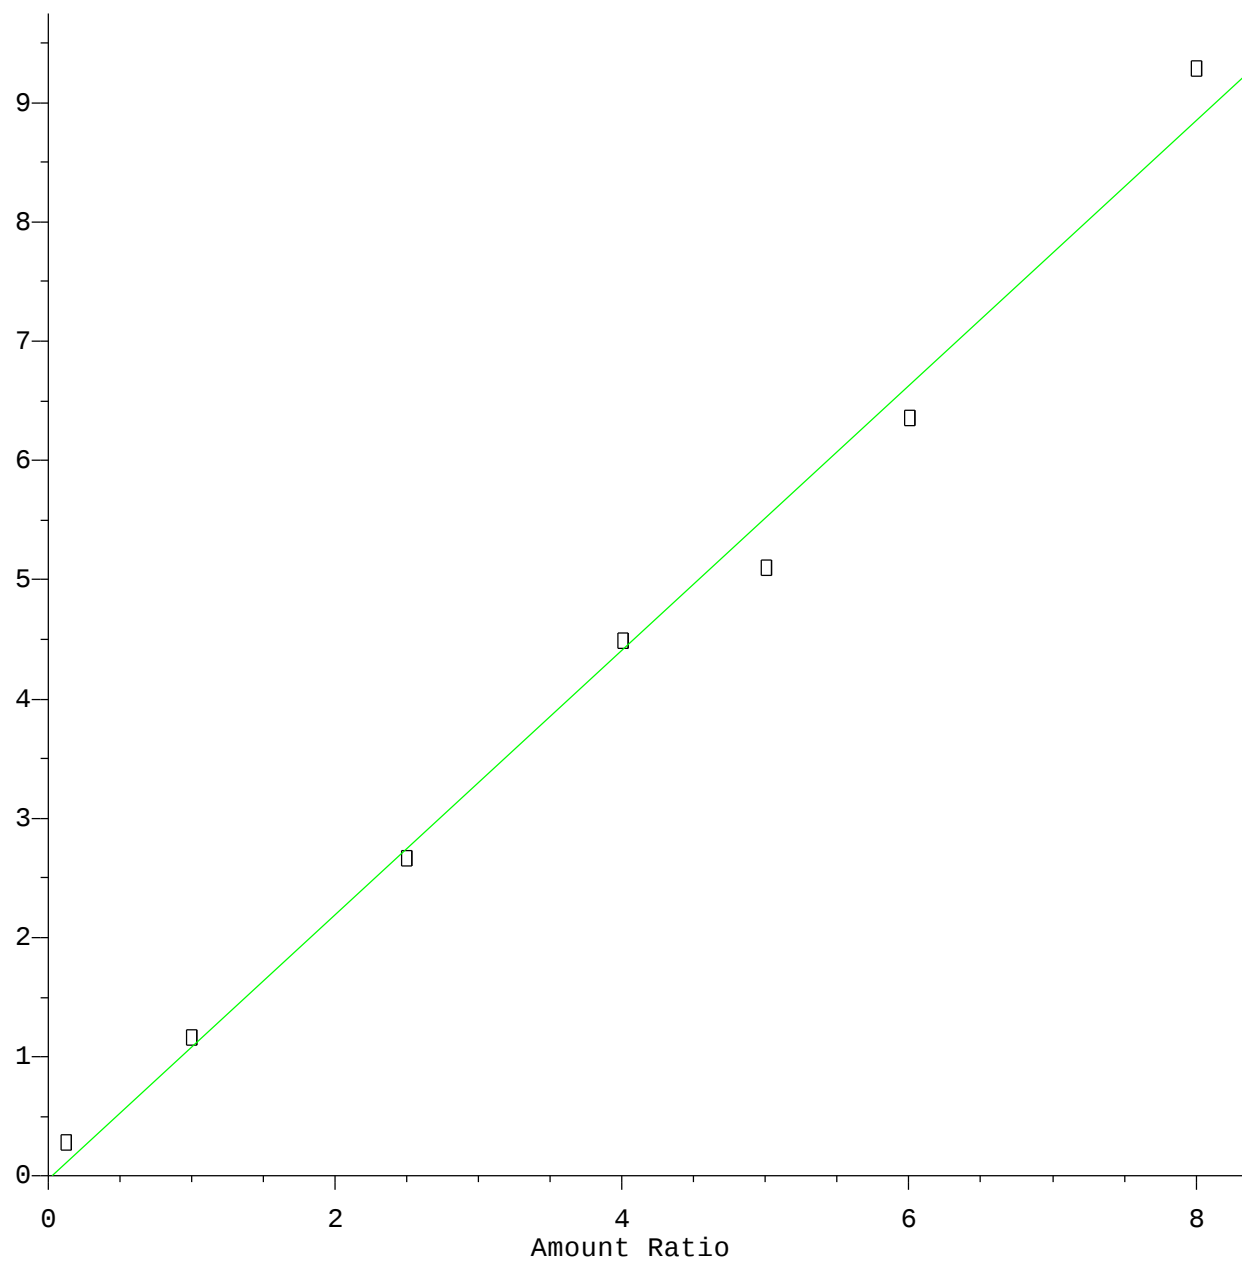


Resp Ratio = $1.11 \times 10^0 \times \text{Amt} - 3.13 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

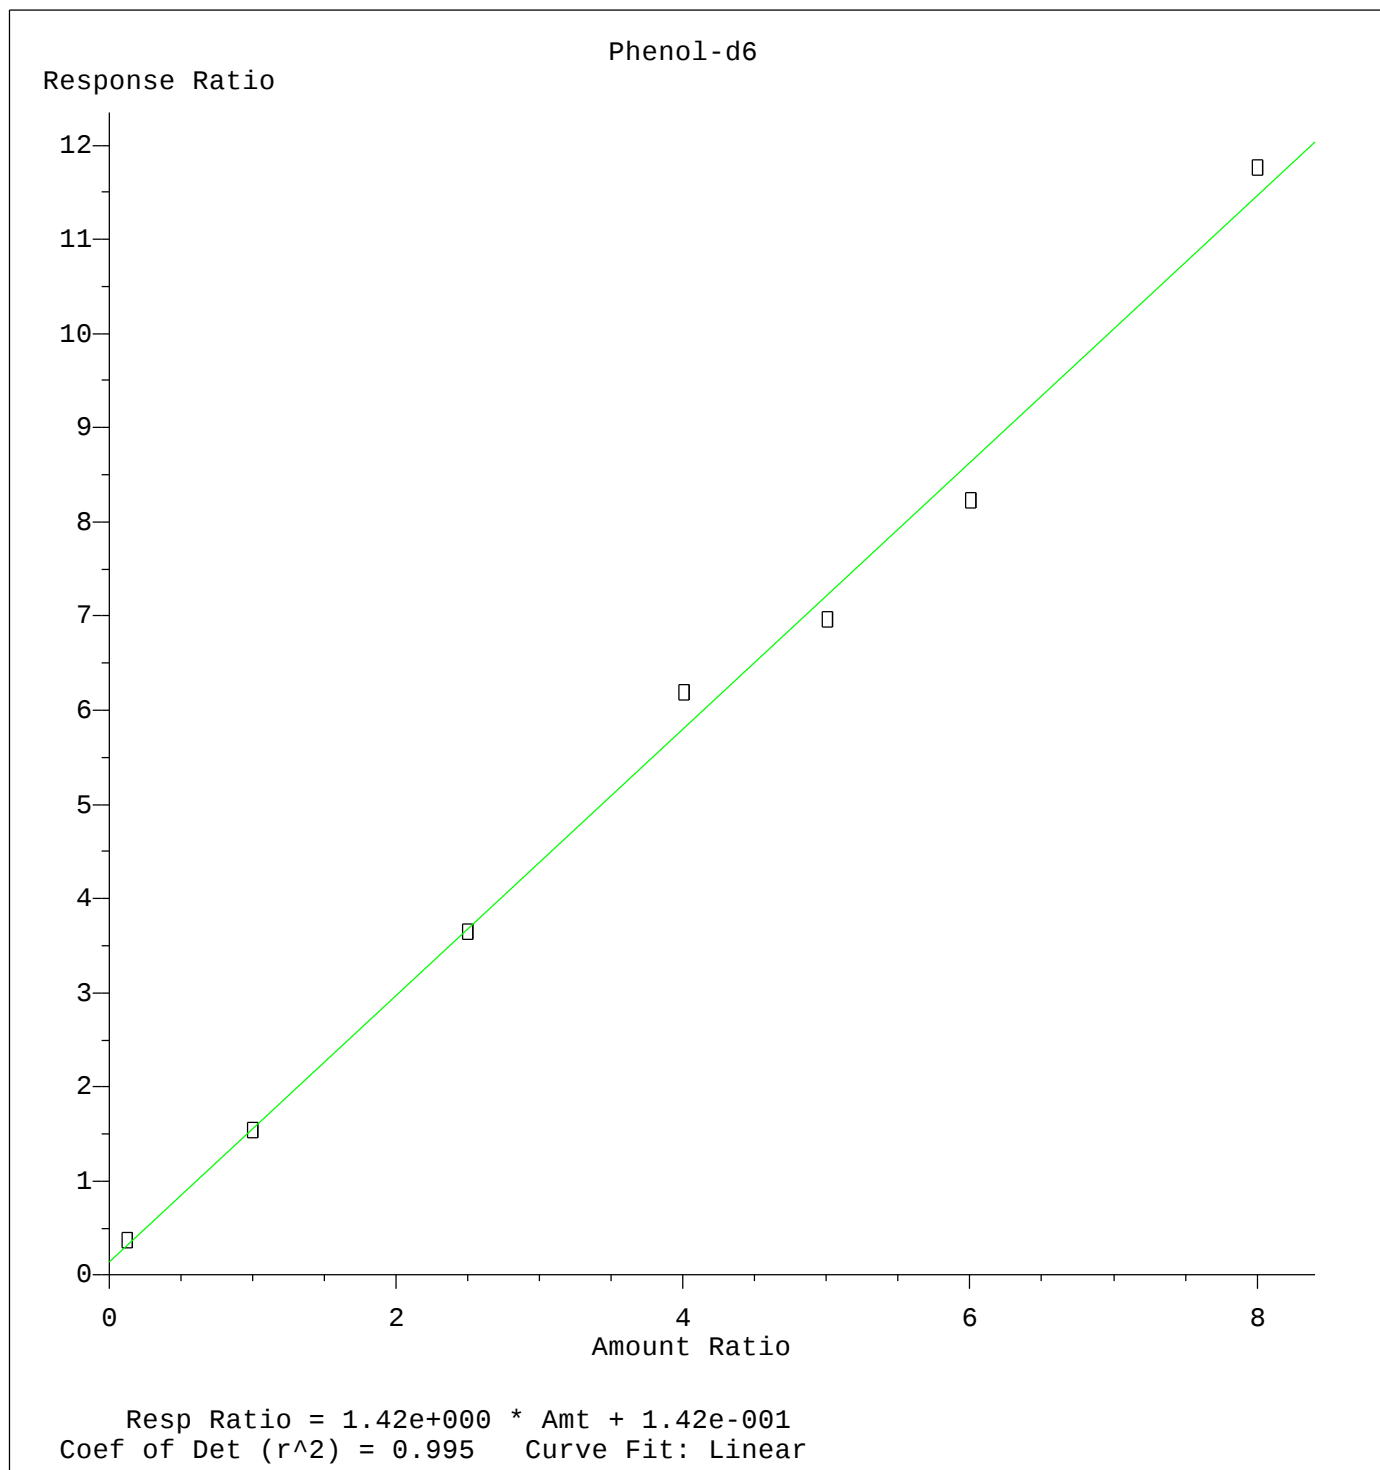

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

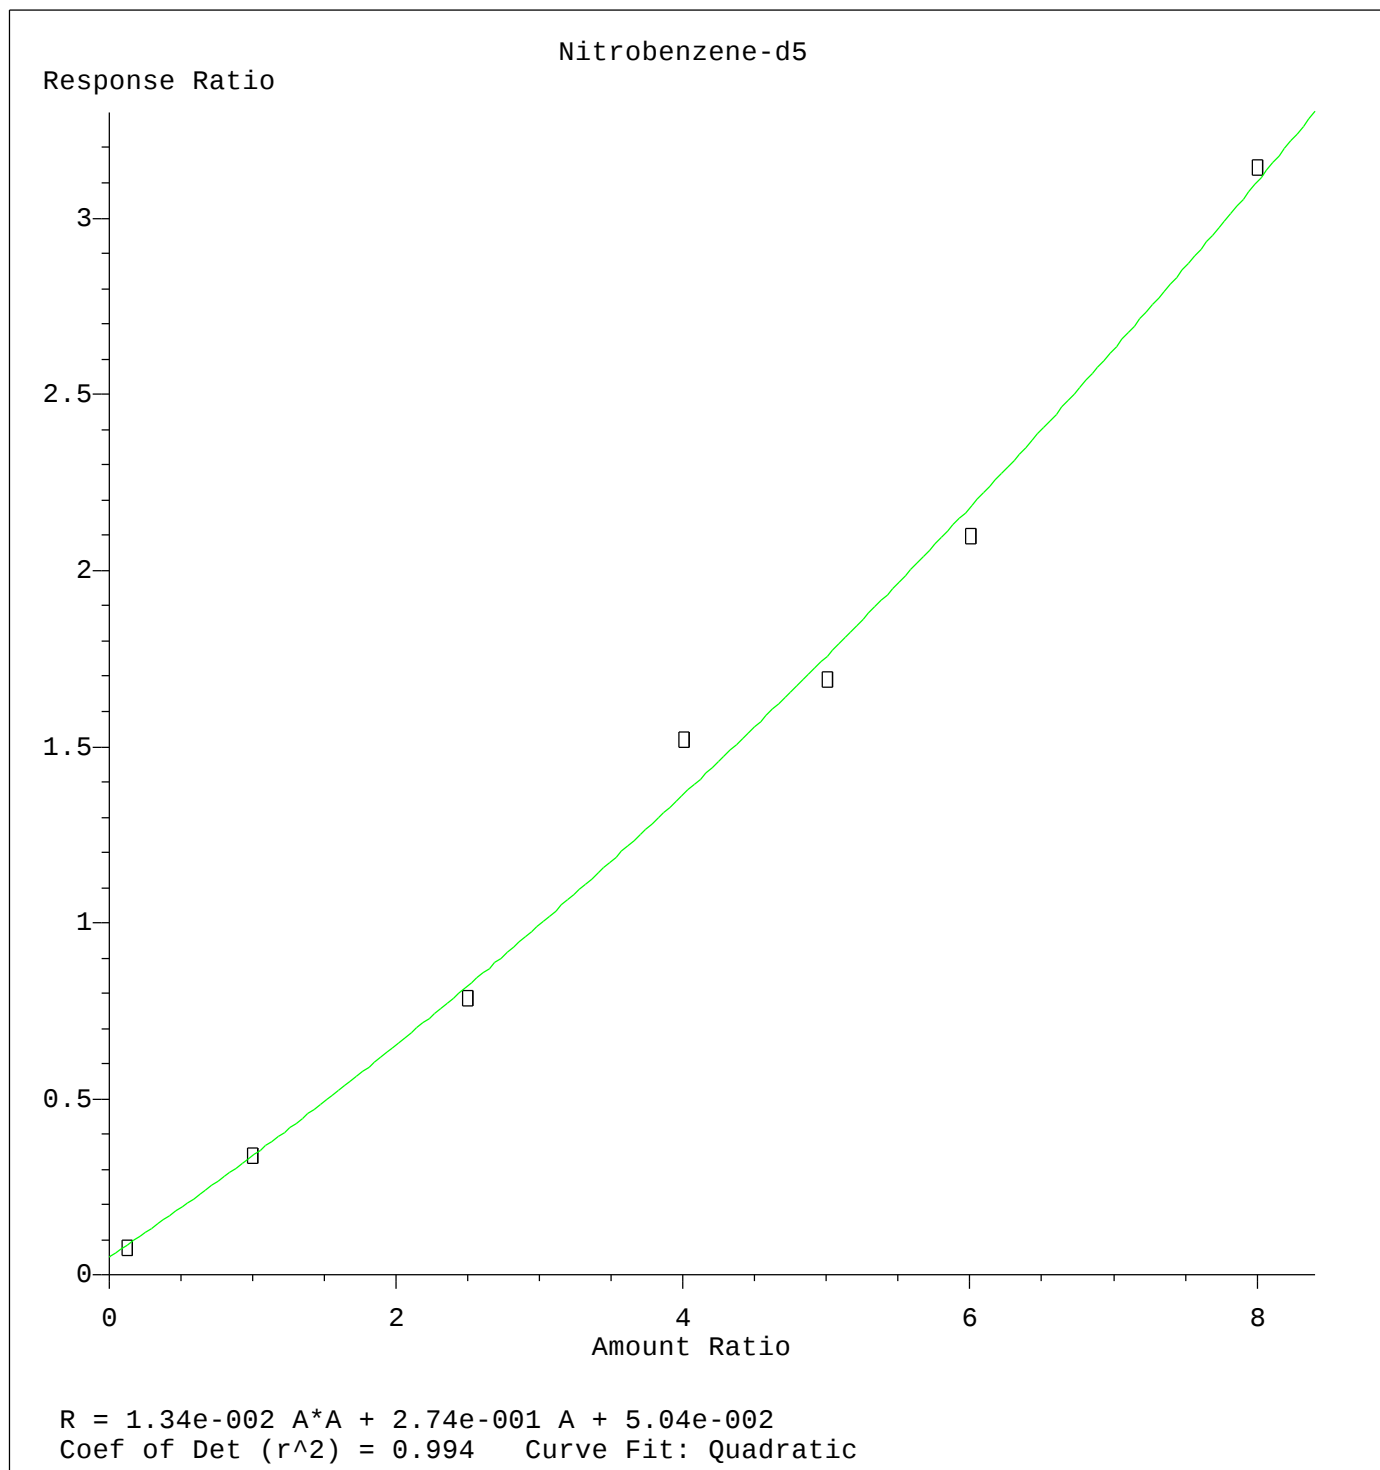


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

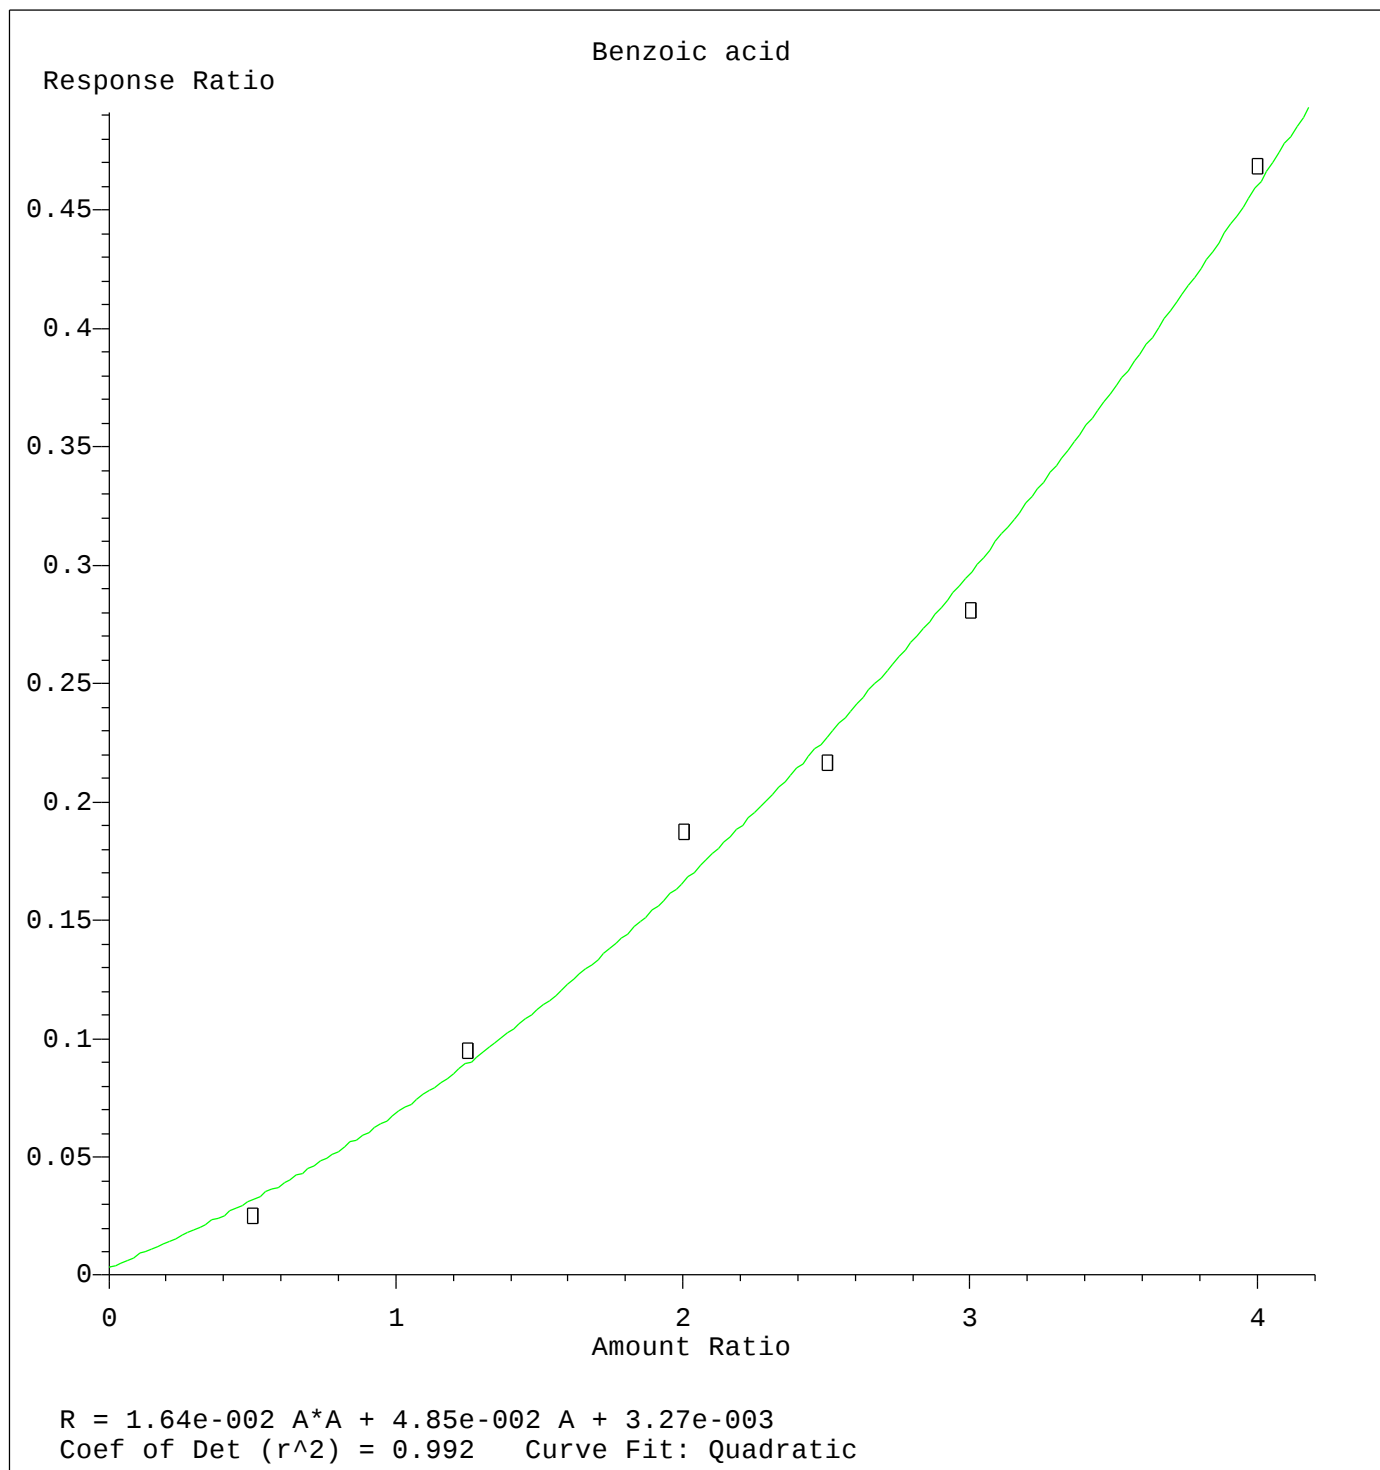

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

2-Fluorobiphenyl

Response Ratio

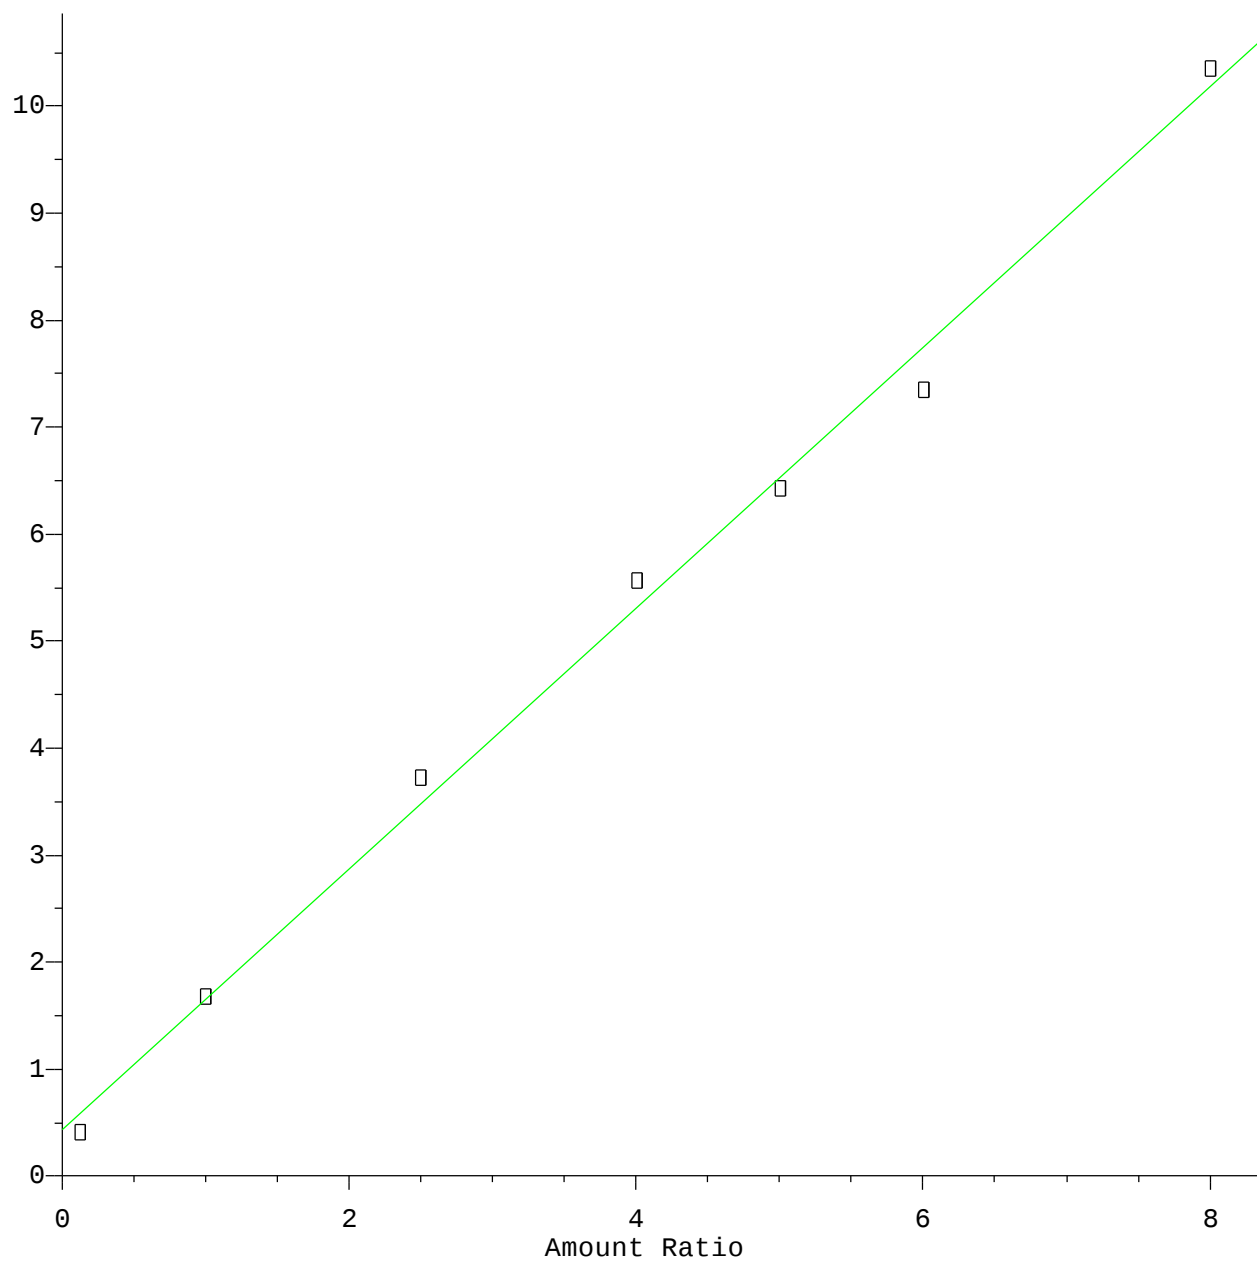


Resp Ratio = 1.22e+000 * Amt + 4.34e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

2,4-Dinitrotoluene


Response Ratio

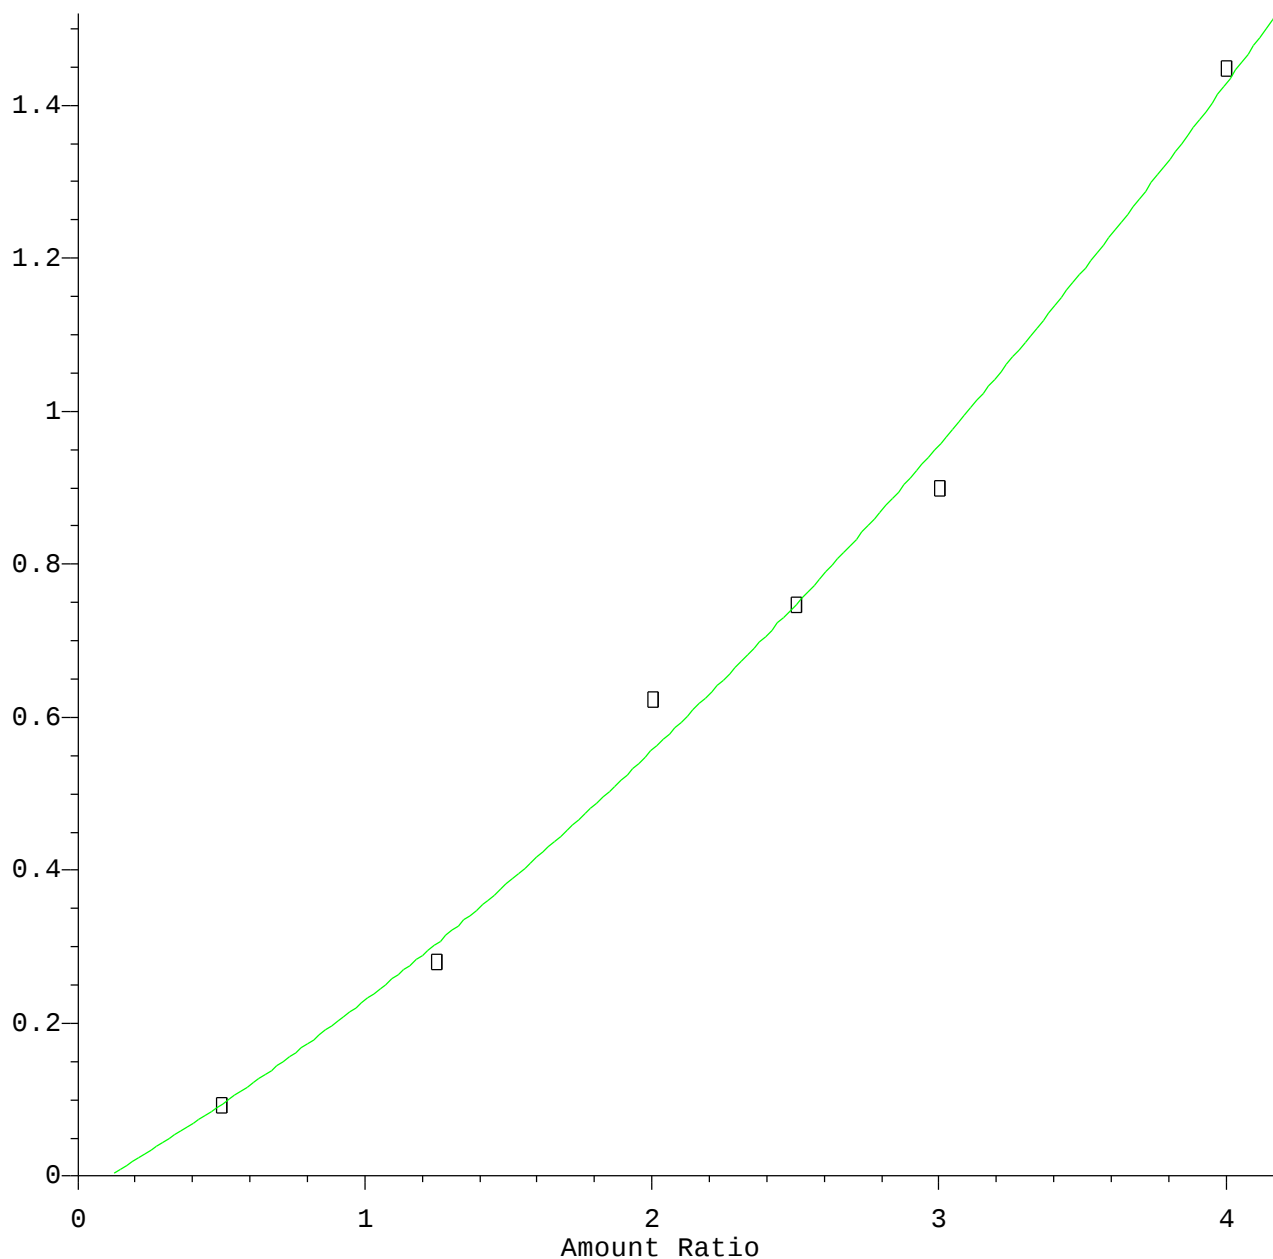

$R = 3.64e-002 A^2 + 2.18e-001 A - 2.45e-002$
Coef of Det (r^2) = 0.993 Curve Fit: Quadratic


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

4,6-Dinitro-2-methylphenol

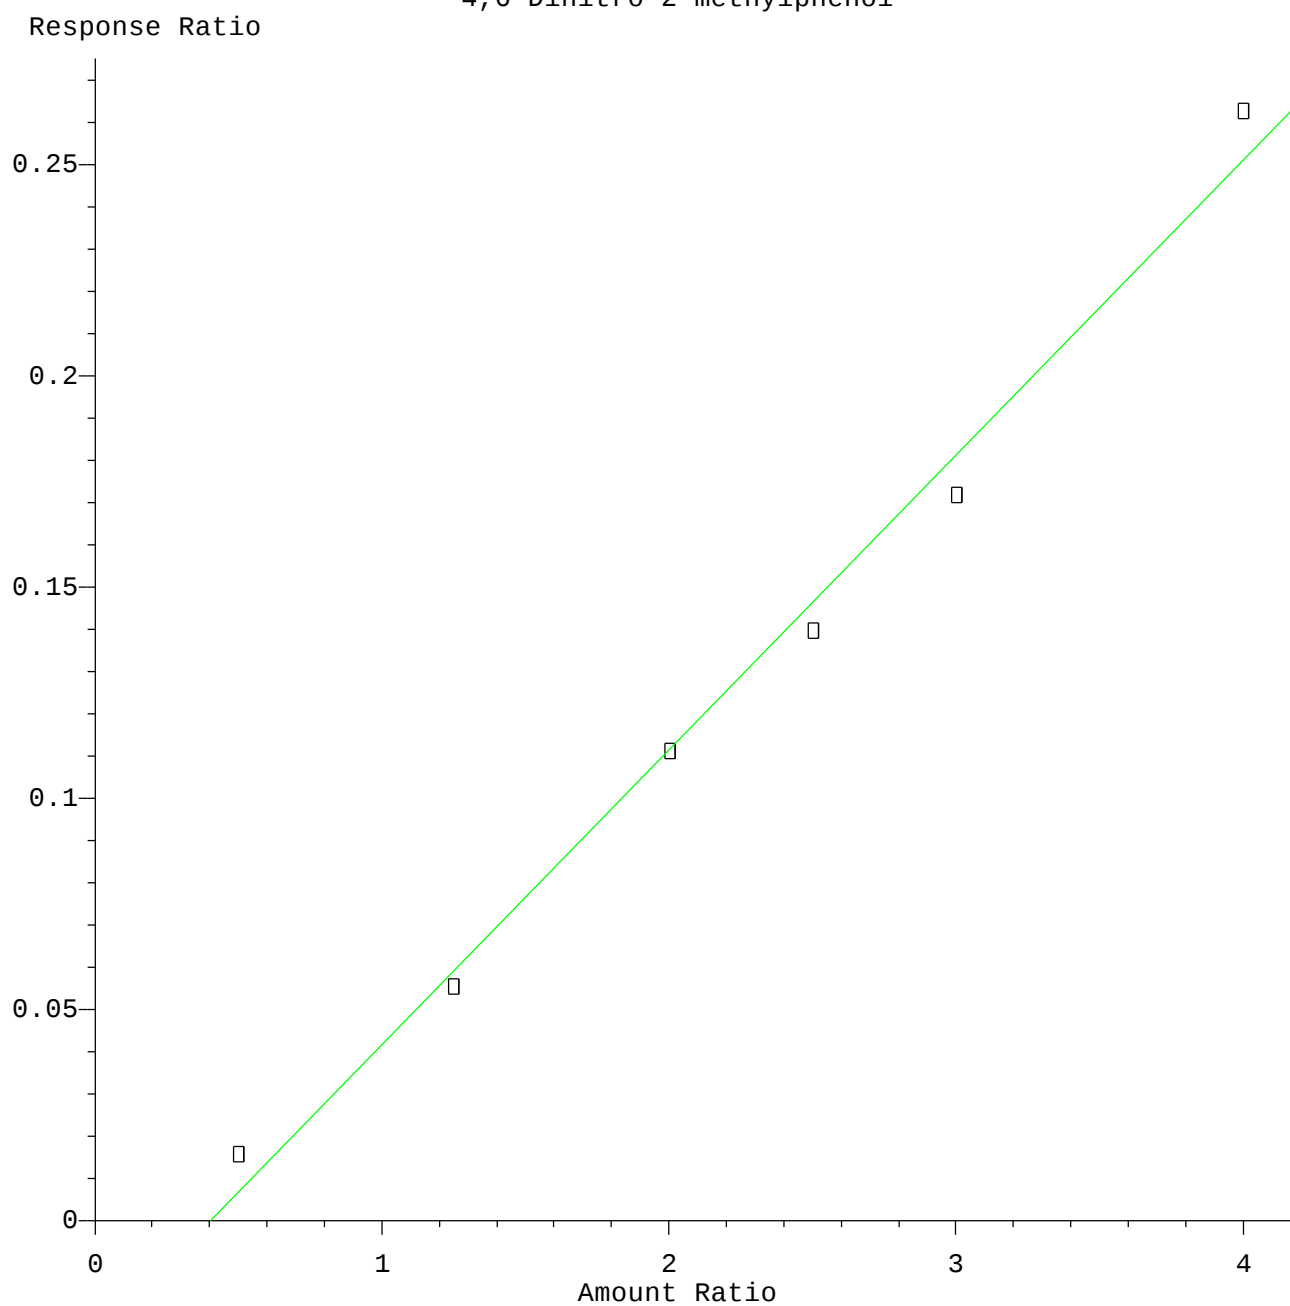


Resp Ratio = $6.97 \times 10^{-2} \times \text{Amt} - 2.79 \times 10^{-2}$
Coef of Det (r^2) = 0.990 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

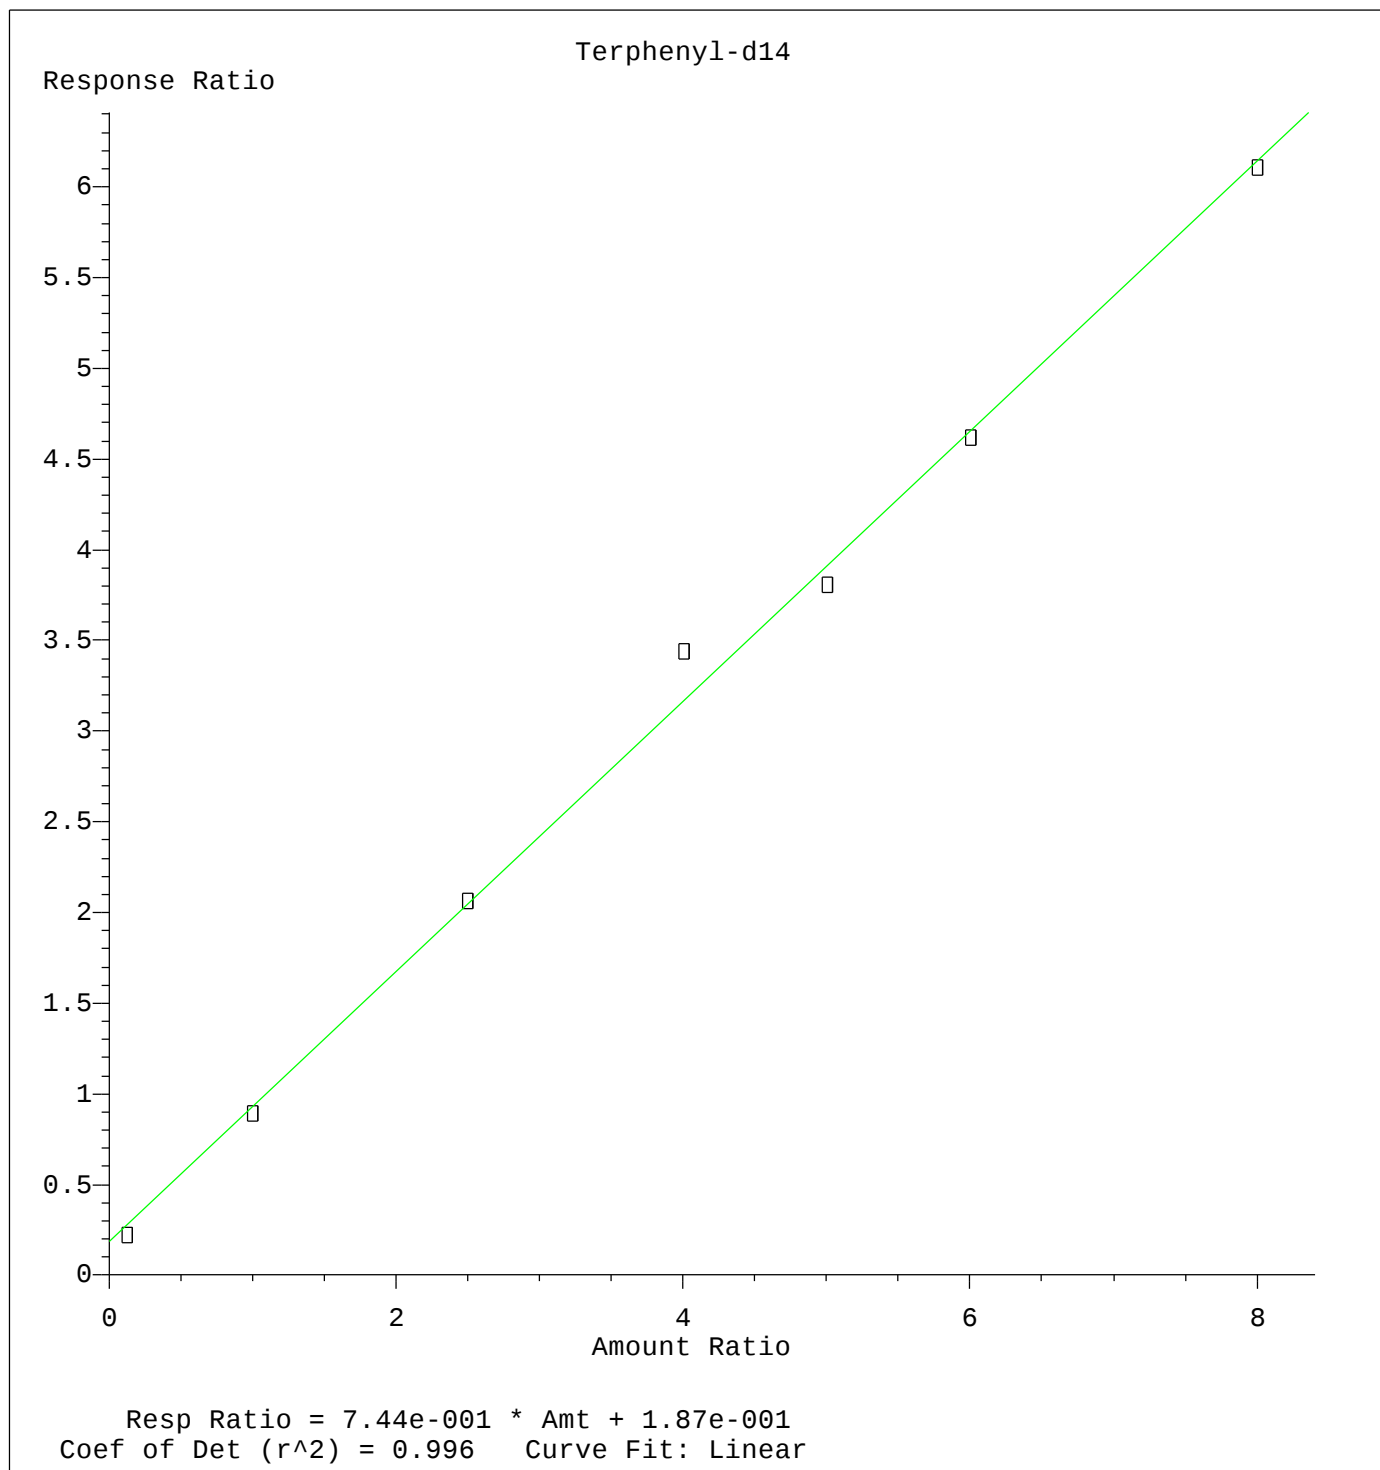


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

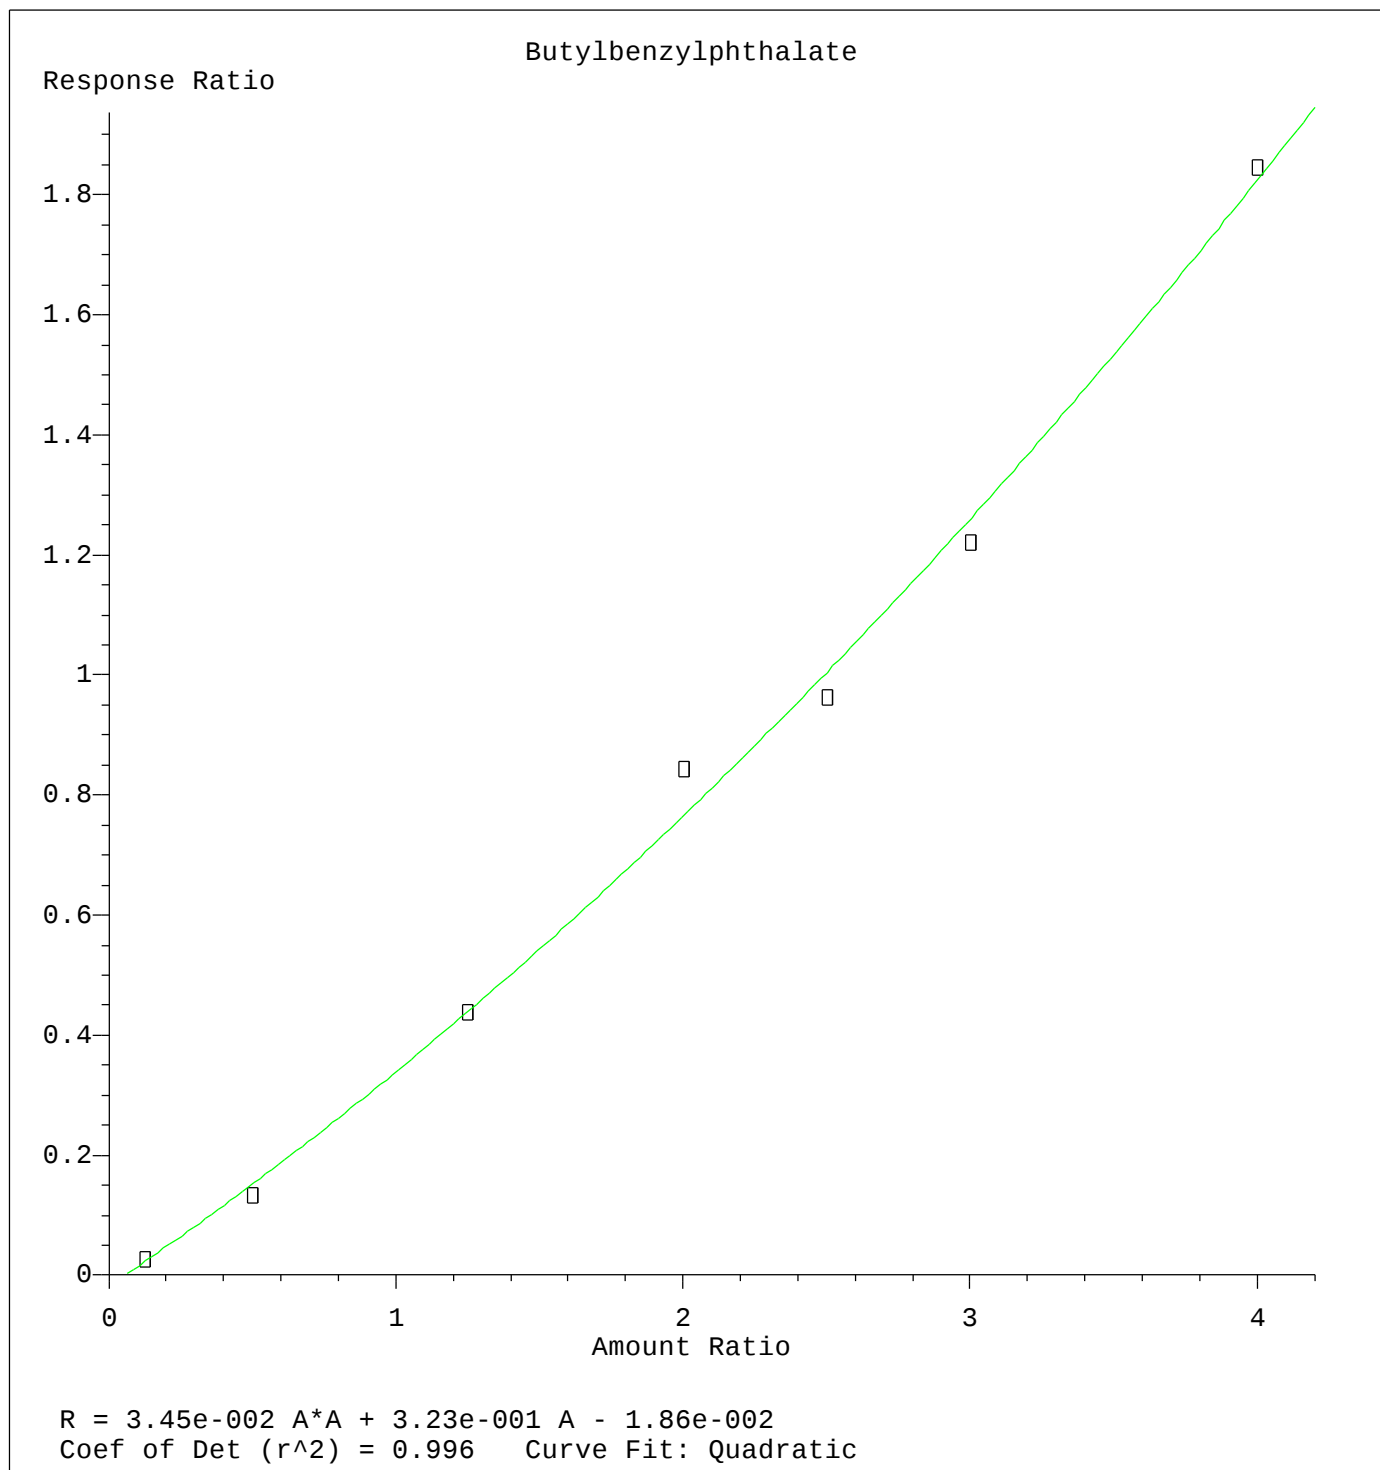

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015

Bis(2-ethylhexyl)phthalate

Response Ratio

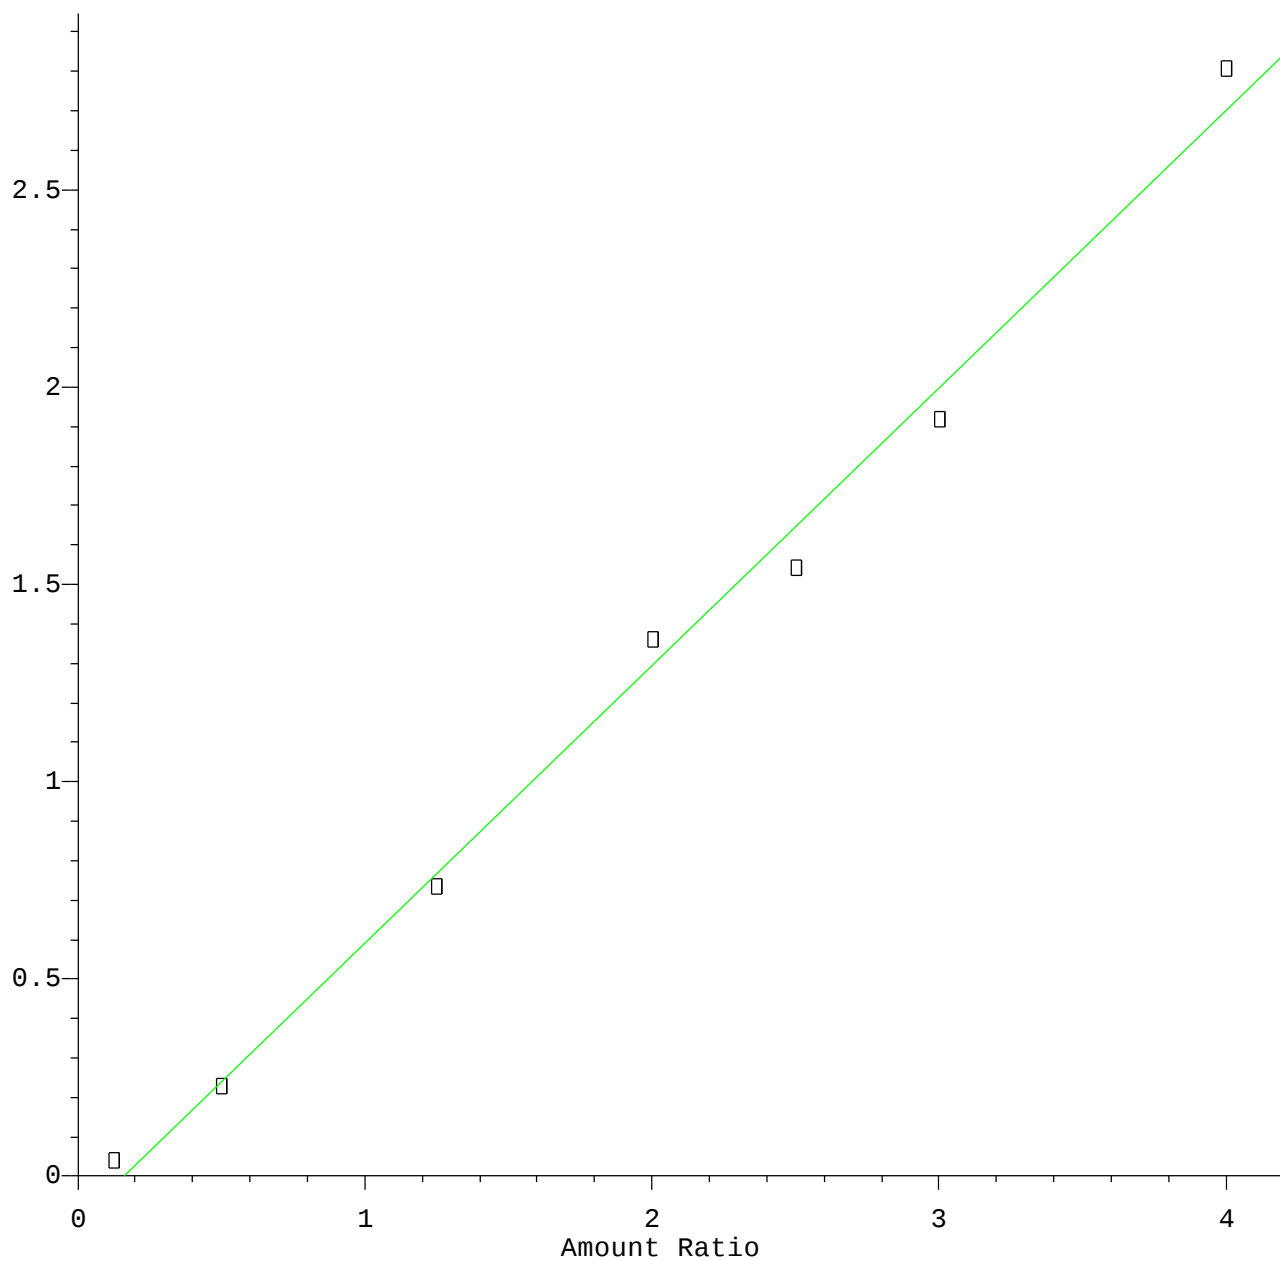

Resp Ratio = $7.03e-001 * \text{Amt} - 1.13e-001$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Calibration Table Last Updated: Fri Jun 05 10:52:02 2015