
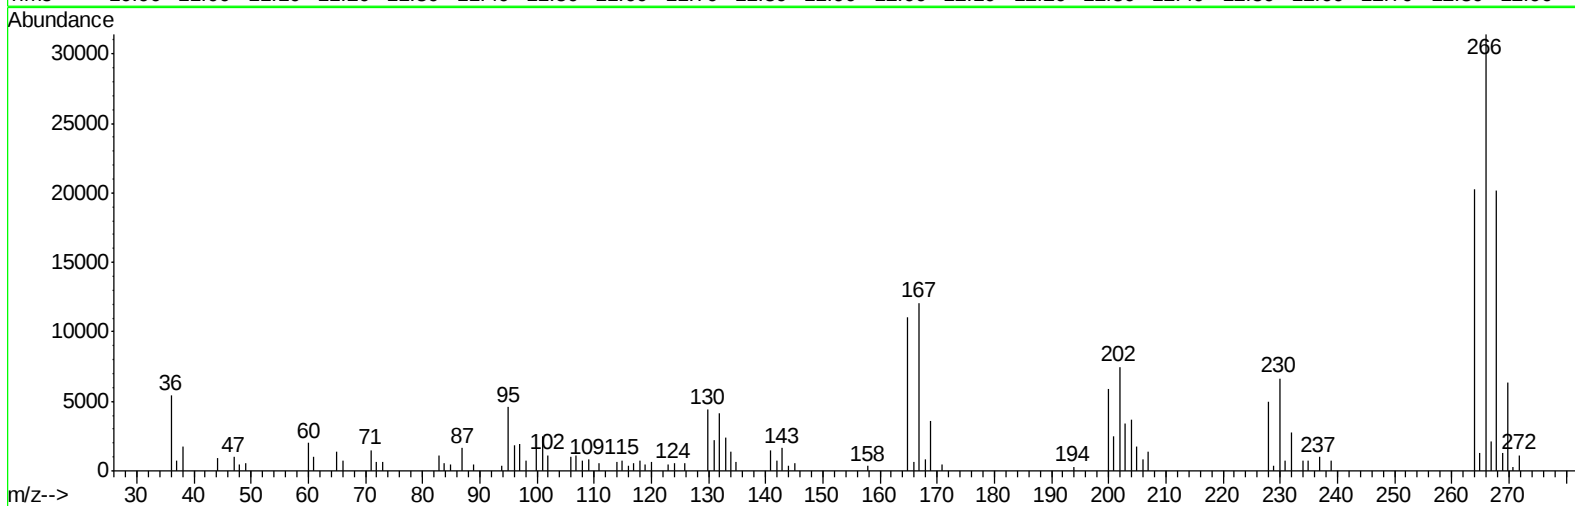


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079652.D
Acq On : 3 Jun 2015 9:41
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:20:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 03 15:20:47 2015
Response via : Initial Calibration

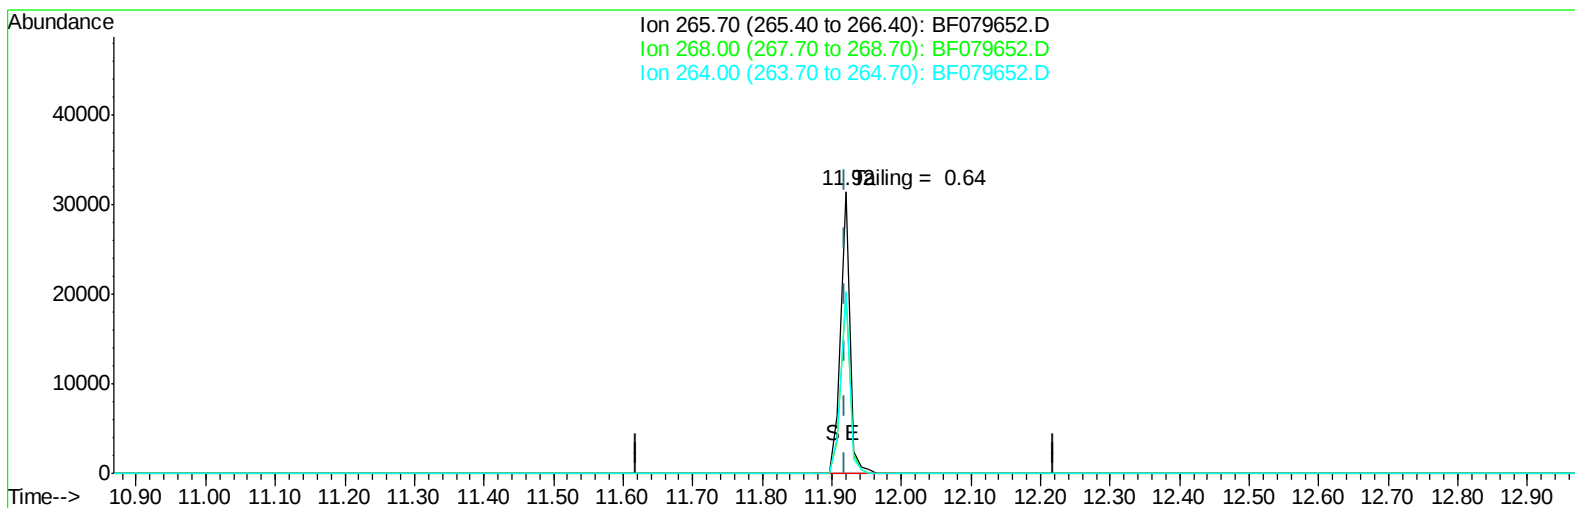

TIC: BF079652.D

(69) Pentachlorophenol (C)



11.919min (+0.000) 0.00ng

response 28339

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	64.09
264.00	60.70	64.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079652.D
Acq On : 3 Jun 2015 9:41
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:20:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 03 15:20:47 2015
Response via : Initial Calibration

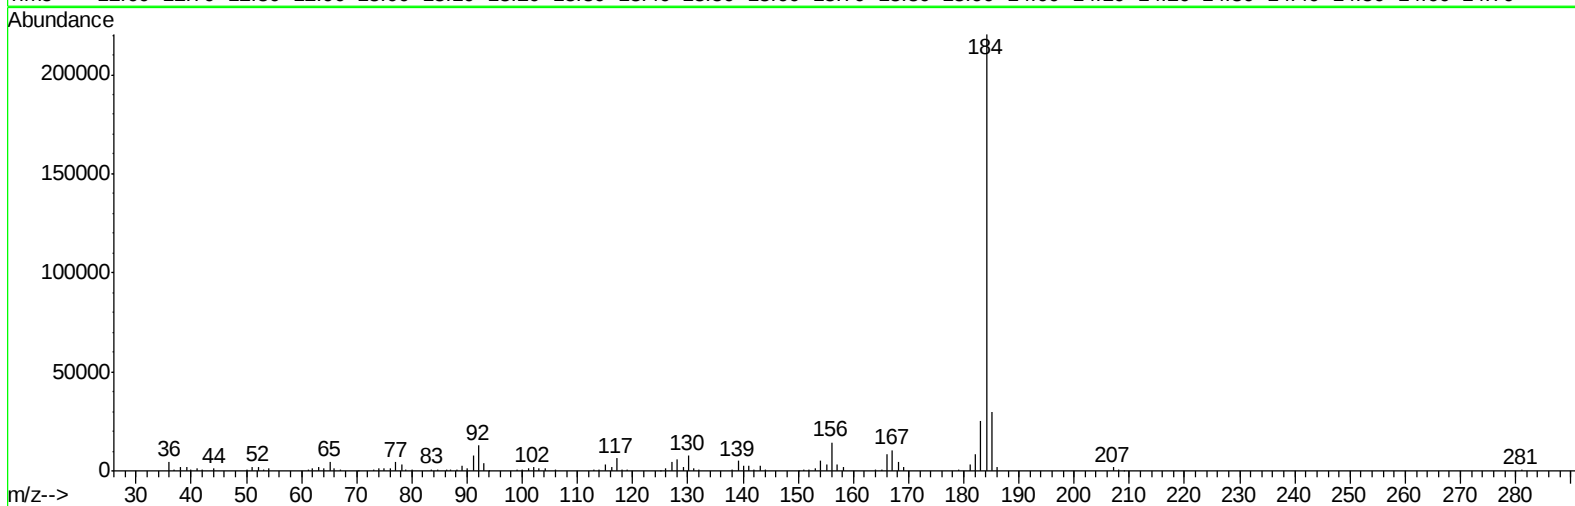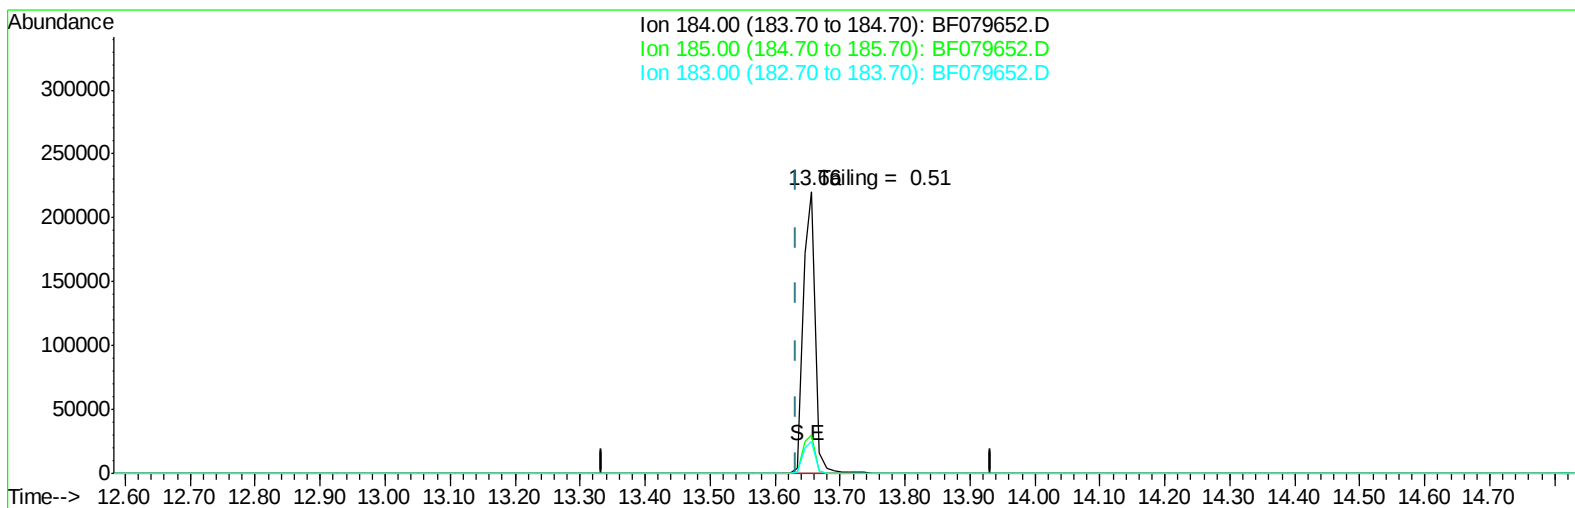

TIC: BF079652.D

(76) Benzidine

13.657min (+0.023) 0.00ng

response 291001

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.59
183.00	11.50	11.32
0.00	0.00	0.00