
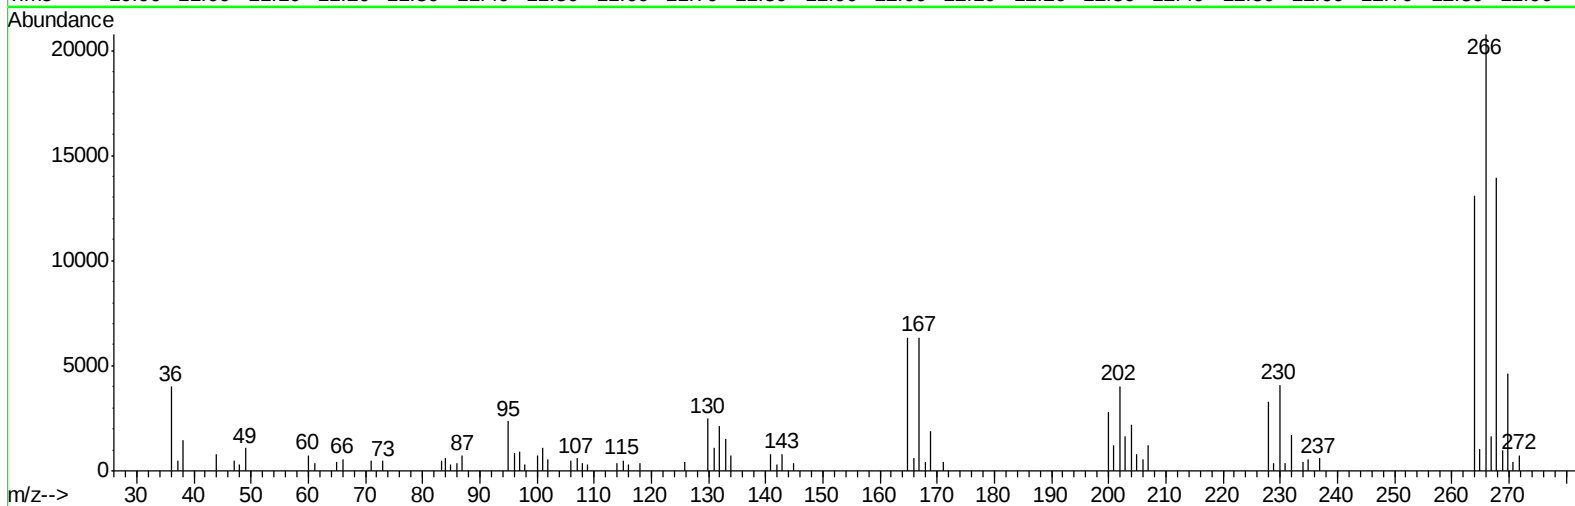


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060315\  
Data File : BF079675.D  
Acq On : 3 Jun 2015 22:43  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:22:36 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060315.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 03 15:20:47 2015  
Response via : Initial Calibration

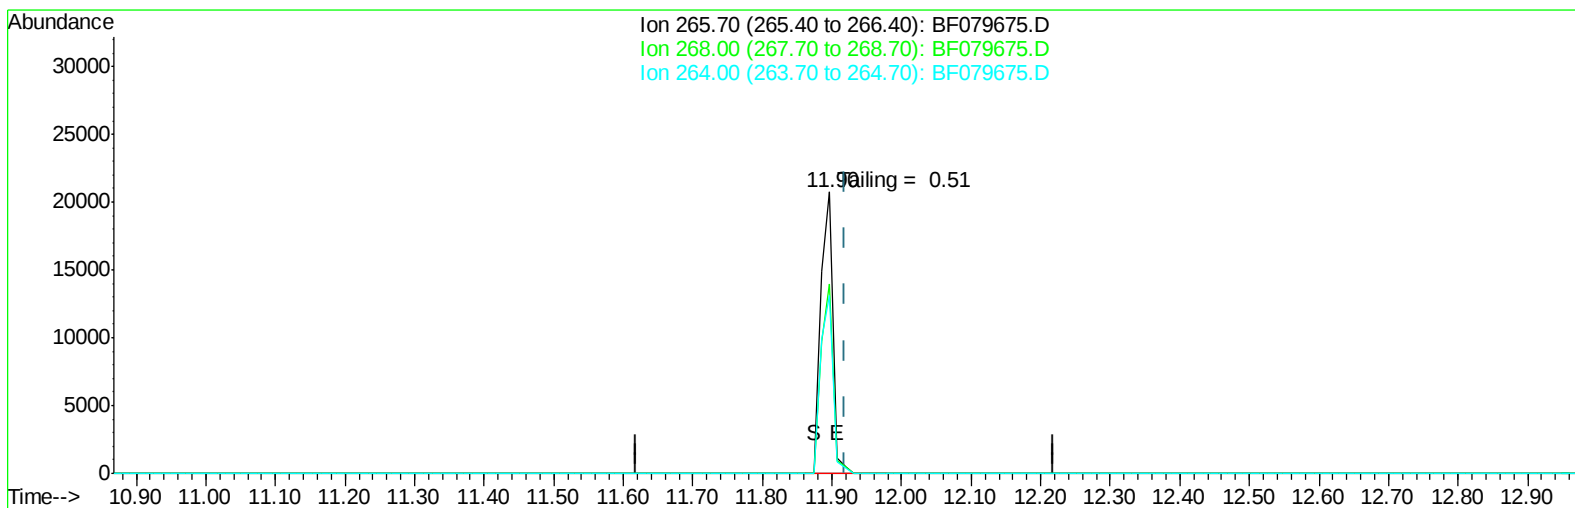

TIC: BF079675.D

(69) Pentachlorophenol (C)



11.896min (-0.023) 0.00ng

response 25596

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.70 | 67.24 |
| 264.00 | 60.70 | 62.99 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF060315\  
Data File : BF079675.D  
Acq On : 3 Jun 2015 22:43  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 06:22:36 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF060315.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 03 15:20:47 2015  
Response via : Initial Calibration

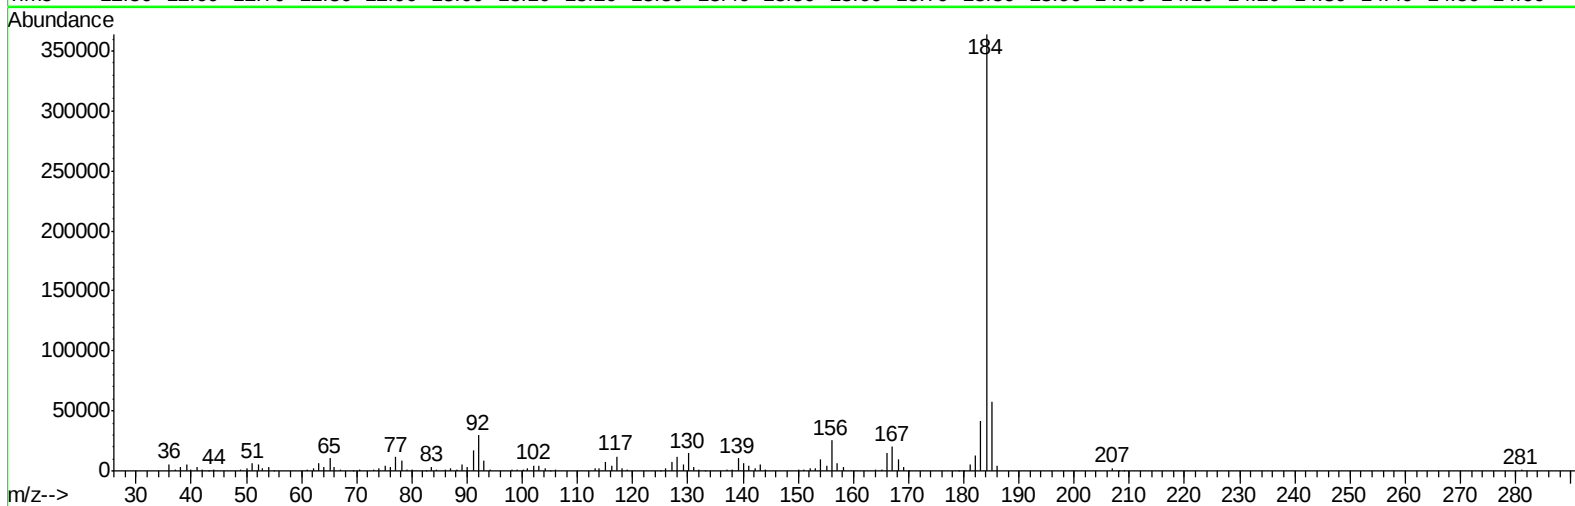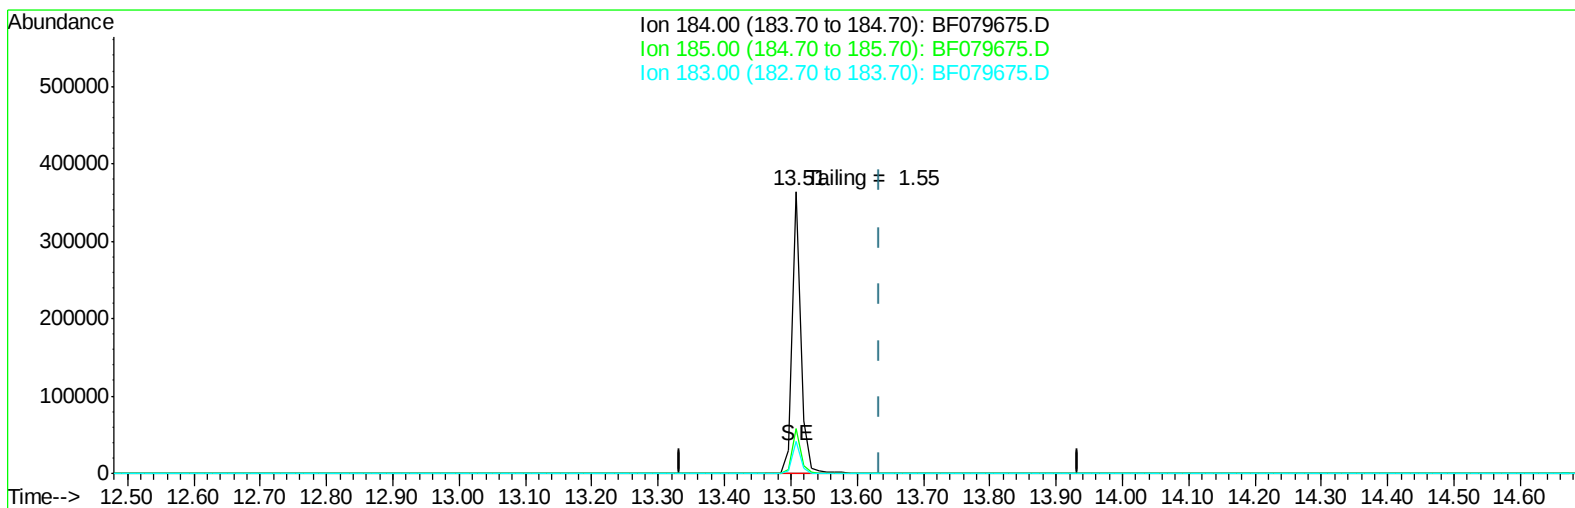

TIC: BF079675.D

(76) Benzidine

13.508min (-0.126) 0.00ng

response 327259

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.70 | 15.88 |
| 183.00 | 11.50 | 11.37 |
| 0.00   | 0.00  | 0.00  |