

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
 Data File : BF079662.D
 Acq On : 3 Jun 2015 14:34
 Operator : TP/IZ
 Sample : G2446-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 T-550

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.507	26	28	97	rVB3	1320051	21067363	100.00%	67.562%
2	2.455	109	111	128	rVV	1524786	3591659	17.05%	11.518%
3	2.684	128	131	134	rVB	259630	377208	1.79%	1.210%
4	2.936	150	153	156	rVB	717225	1037885	4.93%	3.328%
5	7.519	552	554	556	rBV	605995	484142	2.30%	1.553%
6	8.810	665	667	669	rBV	803805	652076	3.10%	2.091%
7	9.885	760	761	763	rVB	390720	287130	1.36%	0.921%
8	10.593	821	823	825	rVB	668811	726870	3.45%	2.331%
9	12.114	953	956	958	rBV	884790	808266	3.84%	2.592%
10	13.851	1106	1108	1111	rBV	378627	451466	2.14%	1.448%
11	15.188	1223	1225	1228	rBV	658307	880139	4.18%	2.823%
12	17.211	1398	1402	1411	rBV	463086	817968	3.88%	2.623%


Sum of corrected areas: 31182172

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079662.D
Acq On : 3 Jun 2015 14:34
Operator : TP/IZ
Sample : G2446-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-550

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

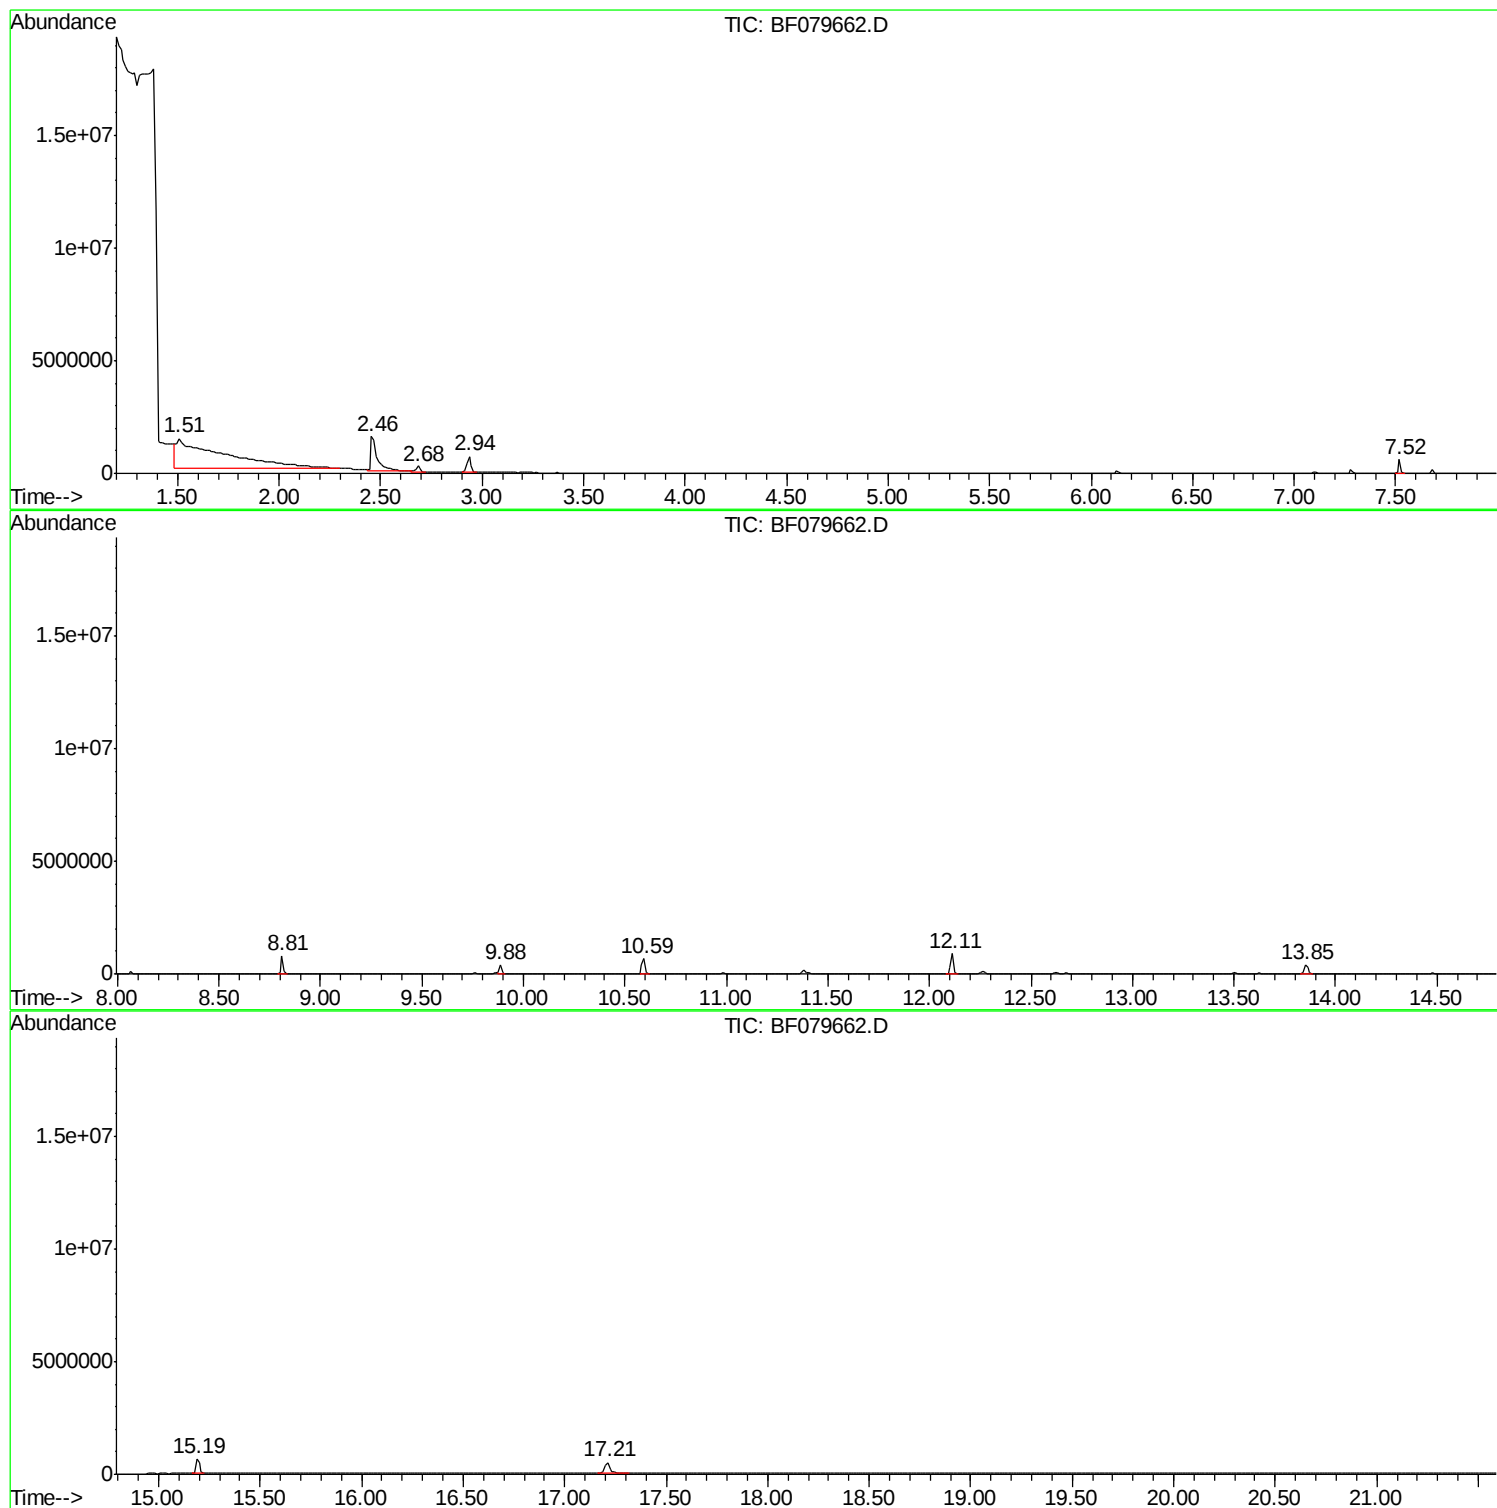

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079662.D
Acq On : 3 Jun 2015 14:34
Operator : TP/IZ
Sample : G2446-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-550










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, 1,2-dichloro-, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.51	870.30 ng	21067400	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	97
2		Ethene, 1,2-dichloro-, (E)-	96	C2H2Cl2	000156-60-5	95
3		1,2-Dichloroethylene	96	C2H2Cl2	000540-59-0	91
4		Ethene, 1,1-dichloro-	96	C2H2Cl2	000075-35-4	90
5		Chloromethylmethyl sulfide	96	C2H5ClS	002373-51-5	46

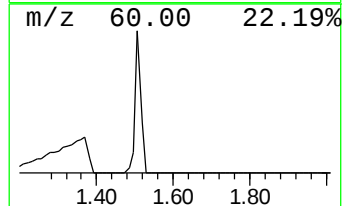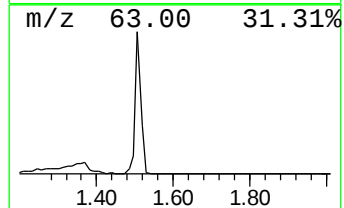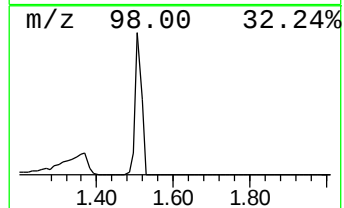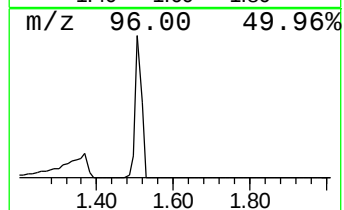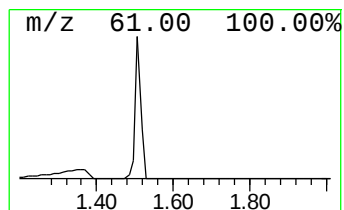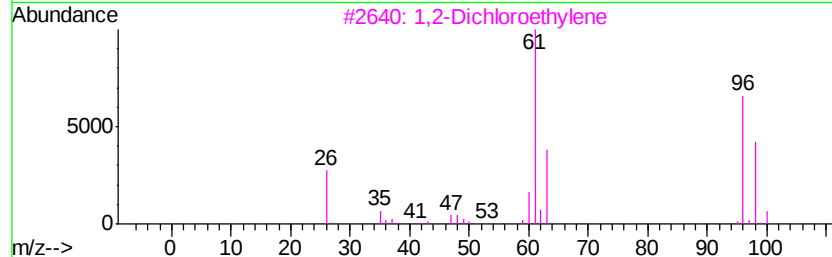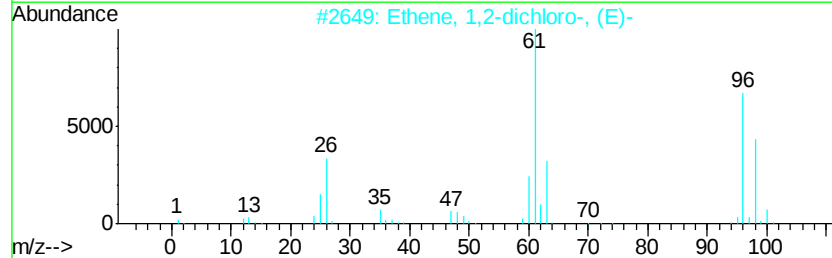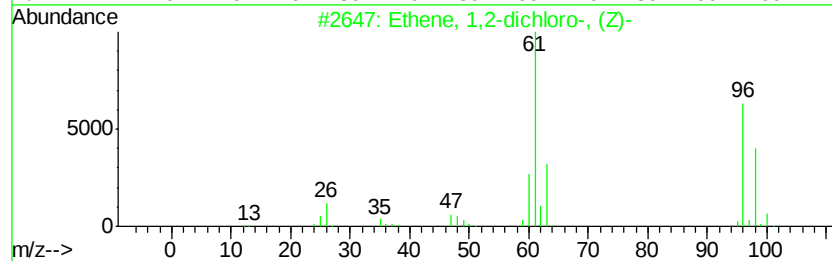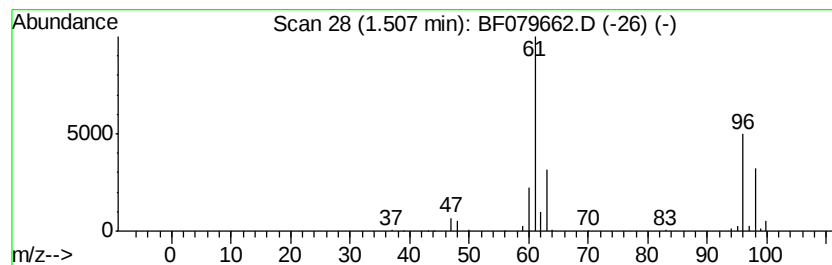

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079662.D
Acq On : 3 Jun 2015 14:34
Operator : TP/IZ
Sample : G2446-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-550










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.94	42.88 ng	1037890	1,4-Dichlorobenzene-d4	7.52

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3		3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	37
4		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
5		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

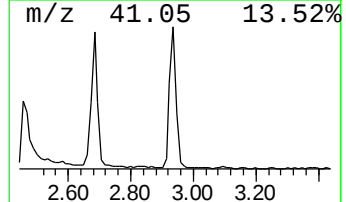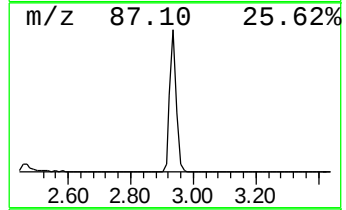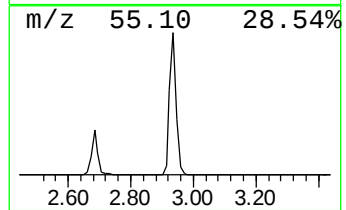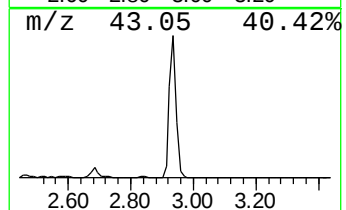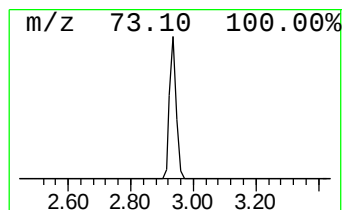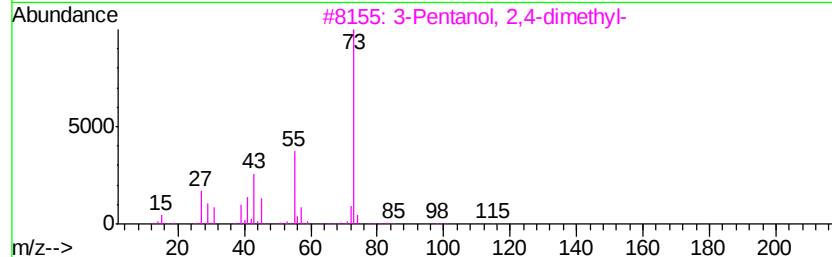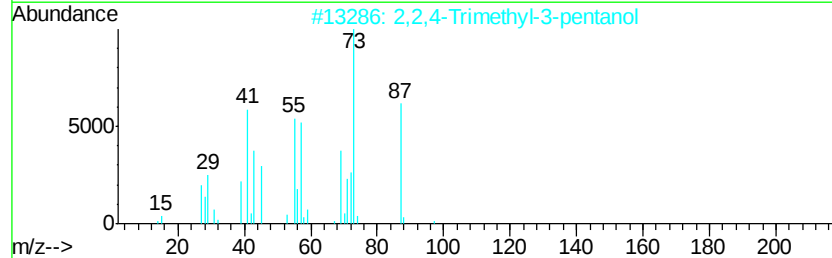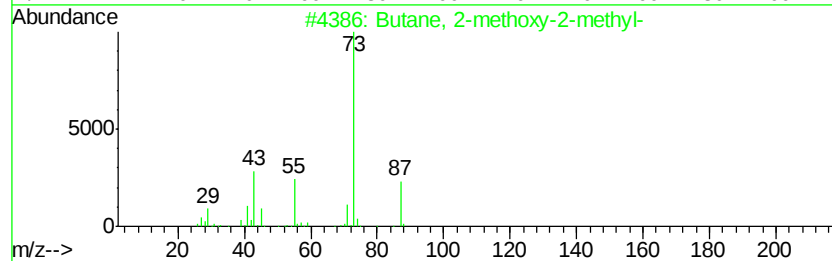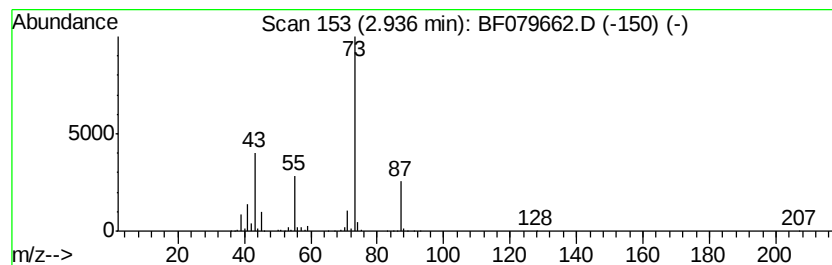

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079662.D
Acq On : 3 Jun 2015 14:34
Operator : TP/IZ
Sample : G2446-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
T-550

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, 1,2-dichl...	1.51	870.3	ng	21067400	1	7.52	484142	20.0
Butane, 2-methoxy...	2.94	42.9	ng	1037890	1	7.52	484142	20.0