

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
 Data File : BF079669.D
 Acq On : 3 Jun 2015 18:43
 Operator : TP/IZ
 Sample : G2452-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-052915

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.393	17	18	20	rVB	17416056	12920592	100.00%	33.048%
2	2.261	93	94	109	rVB	347188	827321	6.40%	2.116%
3	2.456	109	111	127	rVV	1335401	2539320	19.65%	6.495%
4	2.684	127	131	135	rVB	156023	358568	2.78%	0.917%
5	2.947	151	154	158	rVB	844767	1228020	9.50%	3.141%
6	5.747	397	399	402	rBV	156179	222269	1.72%	0.569%
7	6.136	430	433	435	rBV	2001726	1956070	15.14%	5.003%
8	7.107	516	518	520	rBV	2293960	1907414	14.76%	4.879%
9	7.279	531	533	536	rBV	1773922	2095949	16.22%	5.361%
10	7.519	552	554	556	rVB	657840	531342	4.11%	1.359%
11	7.679	566	568	570	rBV	2173665	1745781	13.51%	4.465%
12	8.068	600	602	604	rBV	1045806	1113877	8.62%	2.849%
13	8.810	665	667	670	rVB	853757	708460	5.48%	1.812%
14	9.885	759	761	764	rVB	3051064	2647472	20.49%	6.772%
15	10.594	821	823	825	rBV	802792	830090	6.42%	2.123%
16	11.382	890	892	895	rBV2	1270957	1322612	10.24%	3.383%
17	12.114	954	956	959	rBV	928685	892648	6.91%	2.283%
18	13.885	1108	1111	1114	rBV	3481122	3270248	25.31%	8.365%
19	15.245	1228	1230	1233	rBV	883196	1016838	7.87%	2.601%
20	17.291	1406	1409	1419	rVB	583624	961342	7.44%	2.459%


Sum of corrected areas: 39096233

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data File : BF079669.D
Acq On : 3 Jun 2015 18:43
Operator : TP/IZ
Sample : G2452-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-052915

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

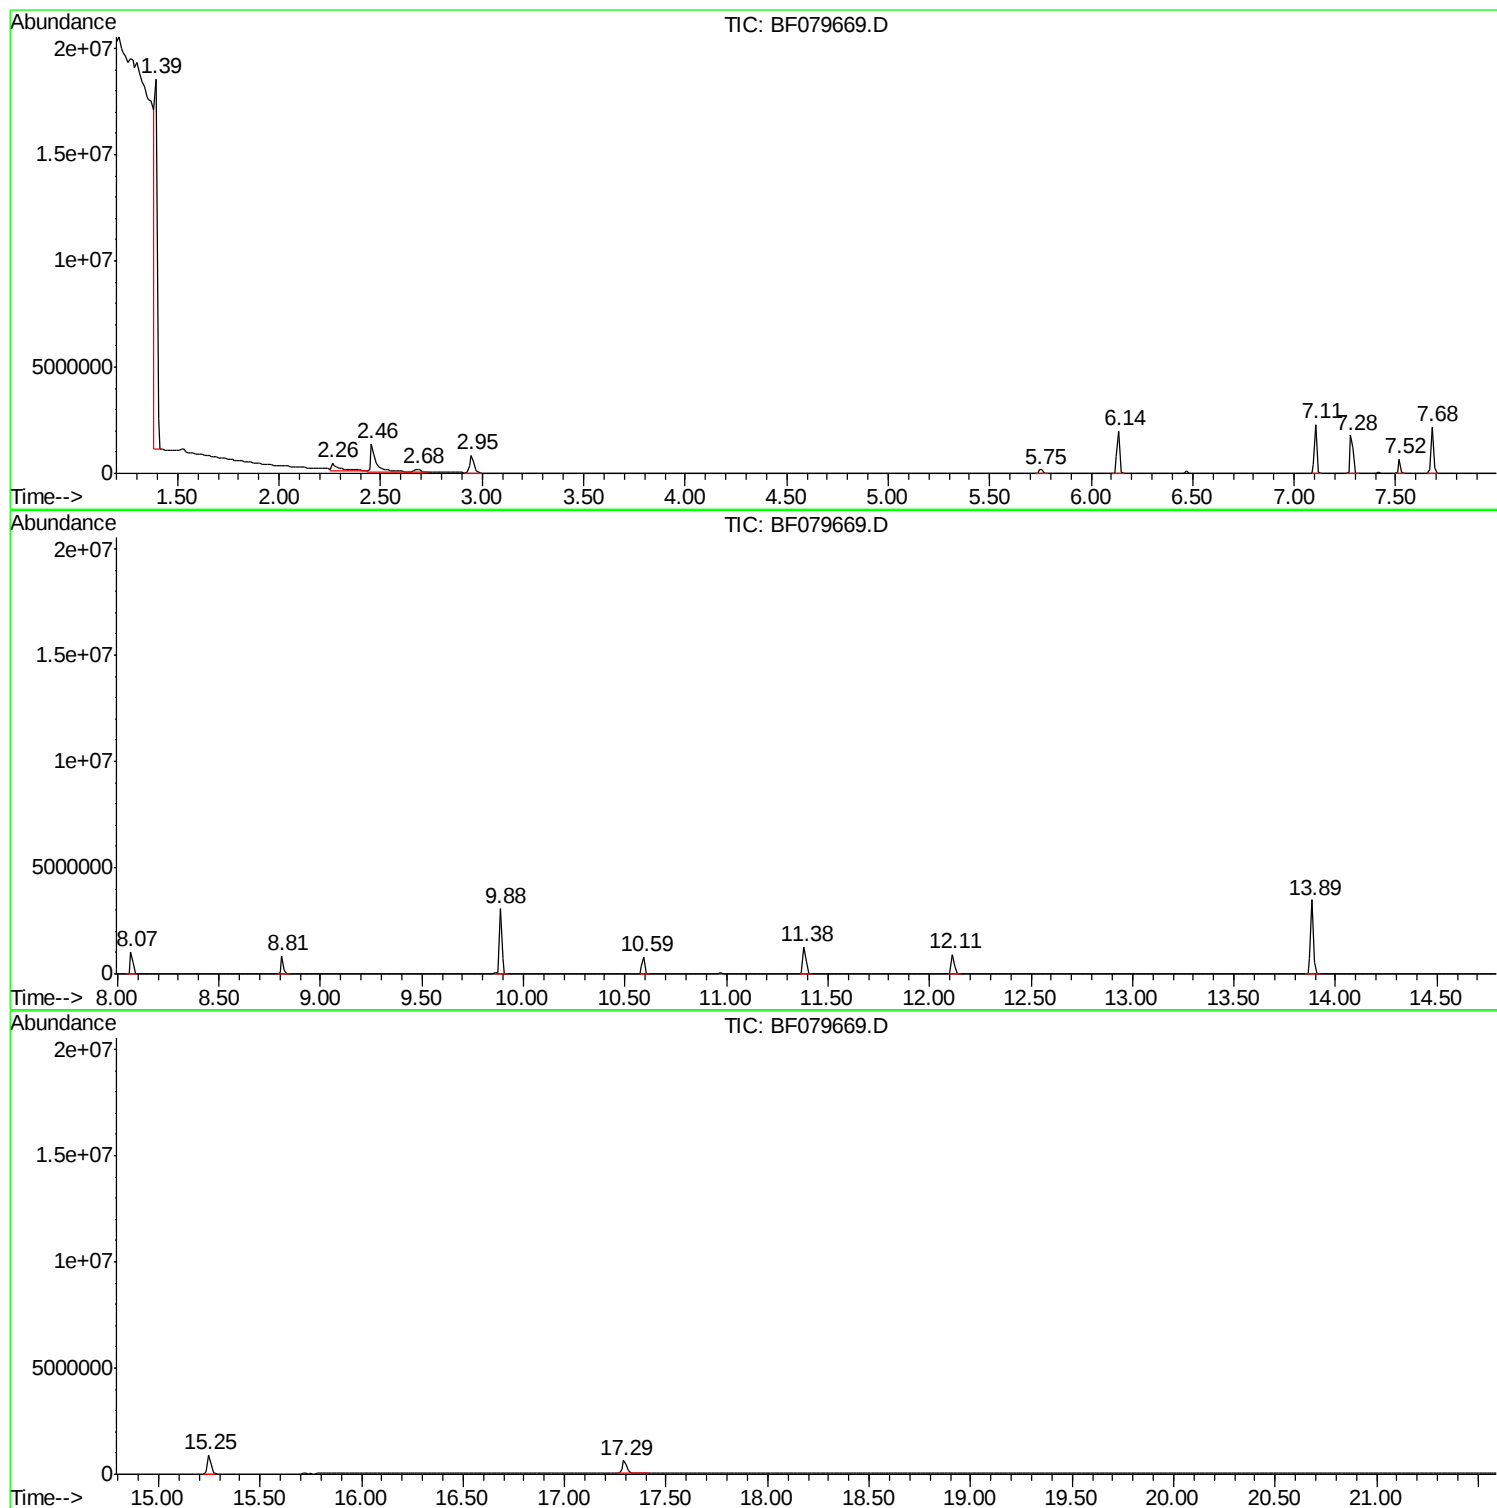

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
Data_File : BF079669.D
Acq_On : 3_Jun_2015_ 18:433
Operator : TP/IZZ
Sample : G2452-011
Misc :
ALS_Vial : 18_ Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
WC-052915

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
