


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
 Data File : BF079652.D
 Acq On : 3 Jun 2015 9:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 03 15:20:47 2015

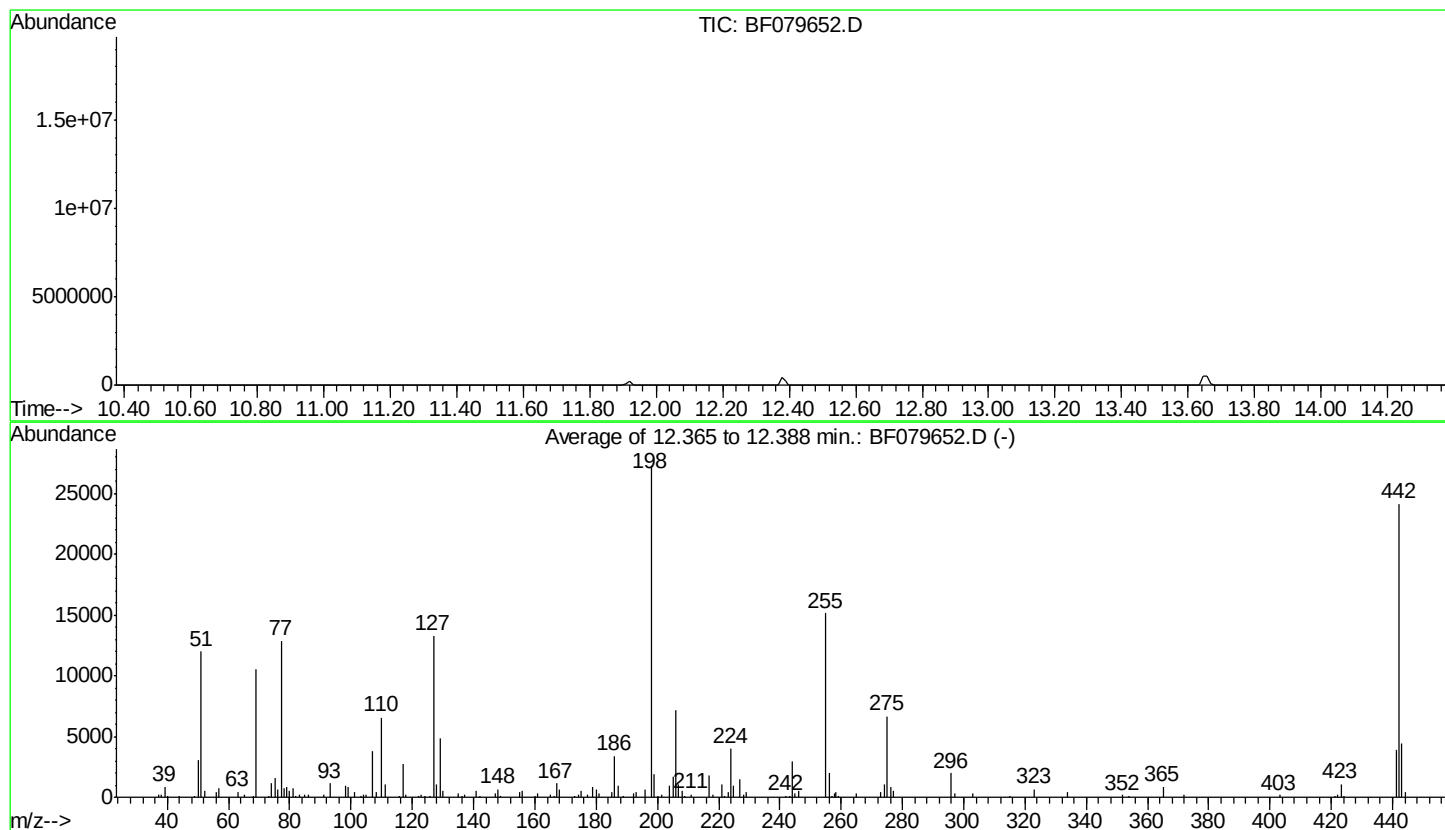

AutoFind: Scans 978, 979, 980; Background Corrected with Scan 975

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	12015	PASS
68	69	0.00	2	1.1	115	PASS
69	198	0.00	100	38.6	10548	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	13316	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27314	PASS
199	198	5	9	6.9	1883	PASS
275	198	10	60	24.4	6668	PASS
365	198	1	100	3.2	871	PASS
441	442	0.01	24	16.0	3858	PASS
442	198	50	100	88.4	24147	PASS
443	442	15	24	18.3	4410	PASS