


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060315\
 Data File : BF079675.D
 Acq On : 3 Jun 2015 22:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 03 15:20:47 2015

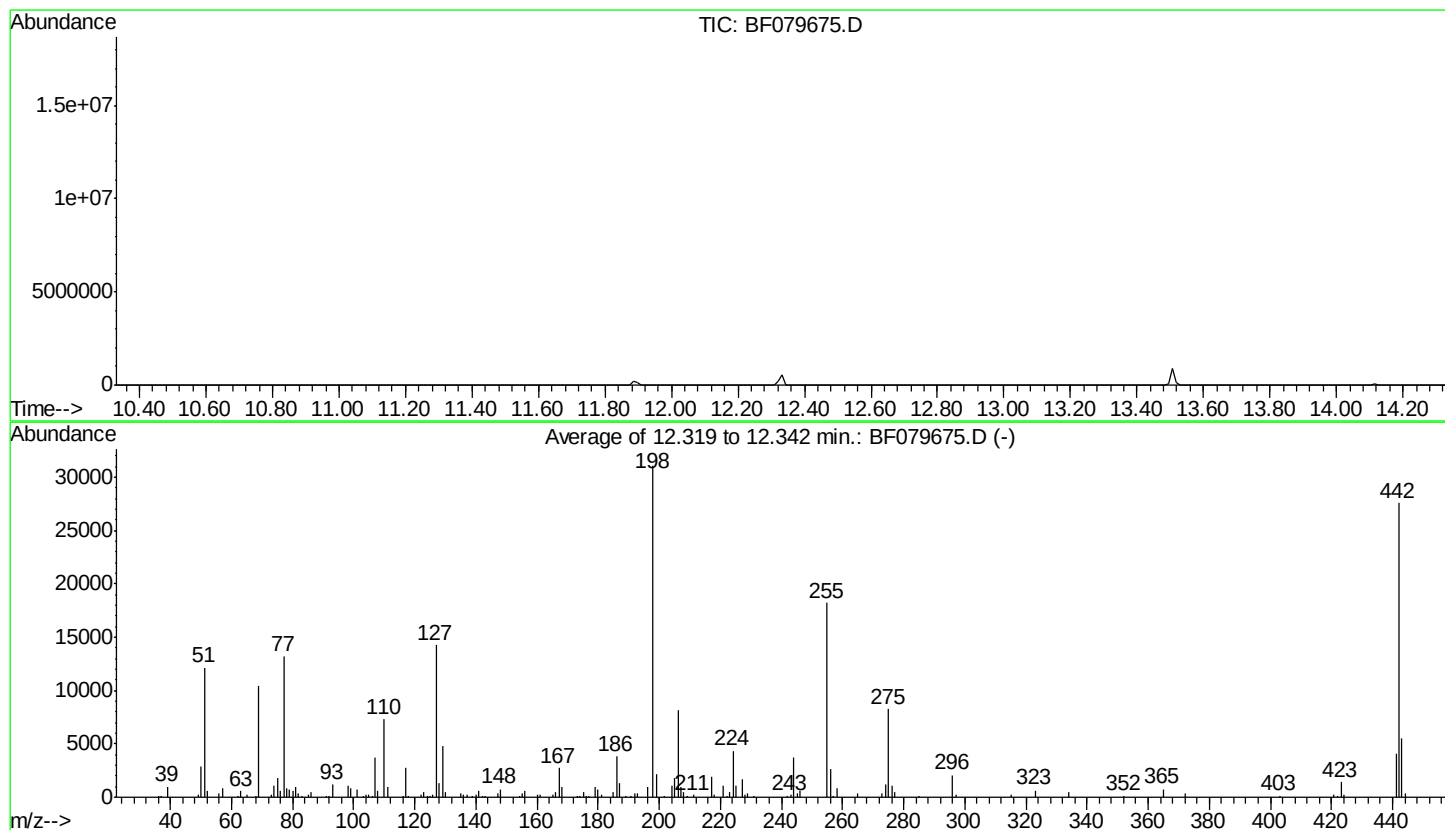

AutoFind: Scans 974, 975, 976; Background Corrected with Scan 971

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	12162	PASS
68	69	0.00	2	1.3	131	PASS
69	198	0.00	100	33.5	10418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	14243	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31098	PASS
199	198	5	9	6.8	2115	PASS
275	198	10	60	26.5	8231	PASS
365	198	1	100	2.4	761	PASS
441	442	0.01	24	14.9	4122	PASS
442	198	50	100	88.7	27599	PASS
443	442	15	24	19.8	5466	PASS