
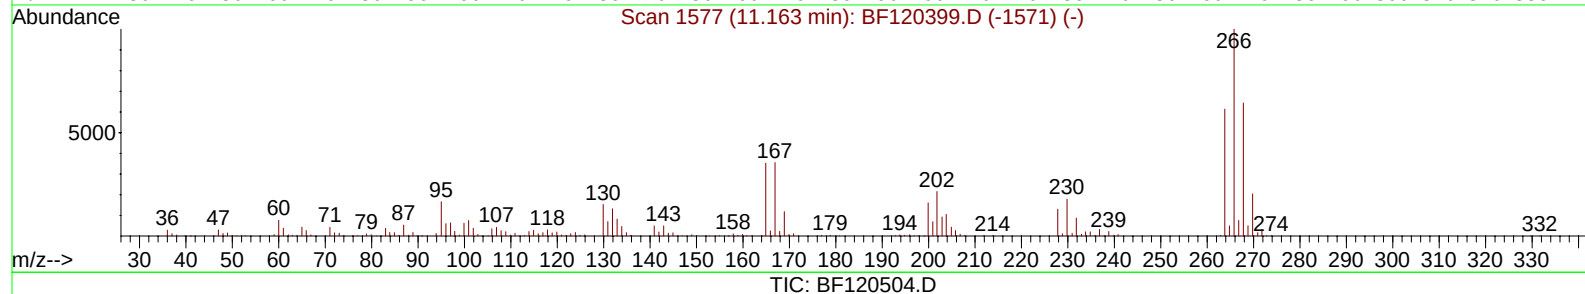
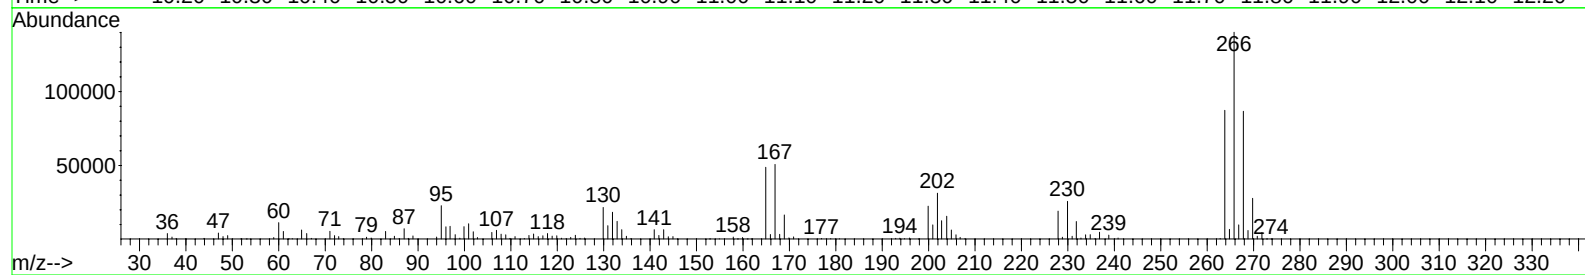


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060320\
Data File : BF120504.D
Acq On : 3 Jun 2020 12:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 17:10:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 03 14:26:17 2020
Response via : Initial Calibration

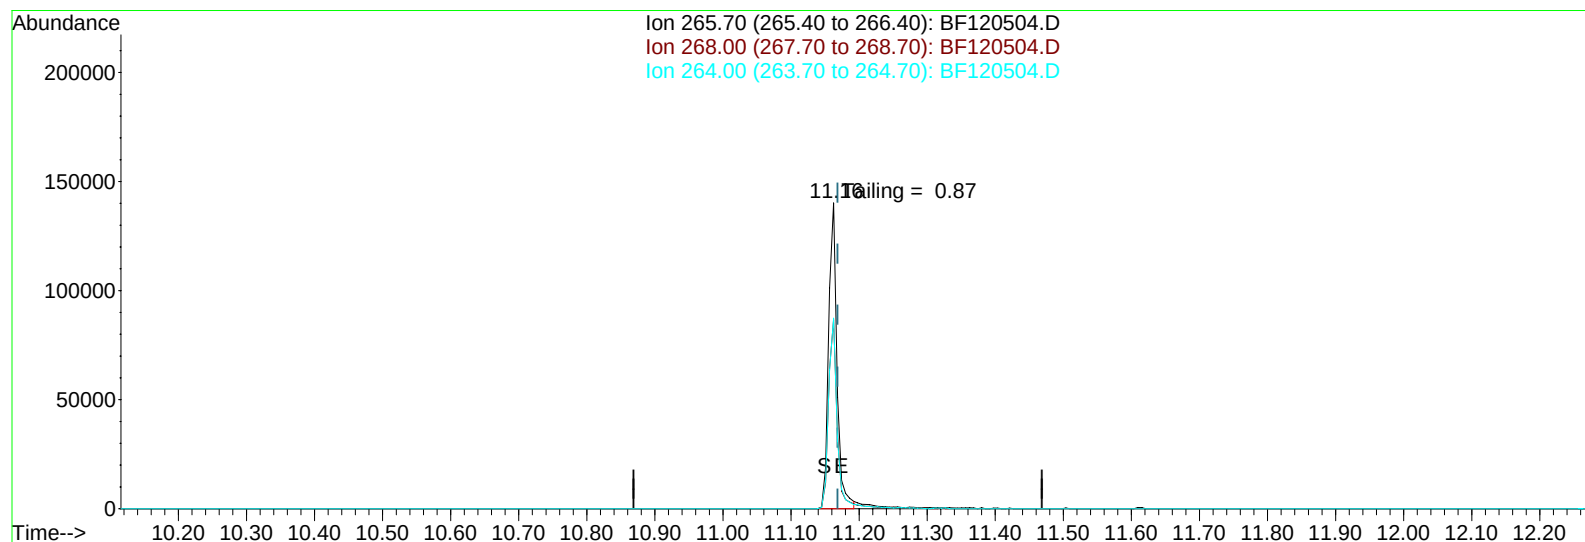

(70) Pentachlorophenol (C)




11.163min (-0.006) 33820.89ng

response 126037

Ion	Exp%	Act%
265.70	100	100
268.00	64.80	61.86
264.00	63.80	62.34
0.00	0.00	0.00

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060320\  
Data File   : BF120504.D  
Acq On      : 3 Jun 2020 12:04  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 03 17:10:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 03 14:26:17 2020
Response via : Initial Calibration

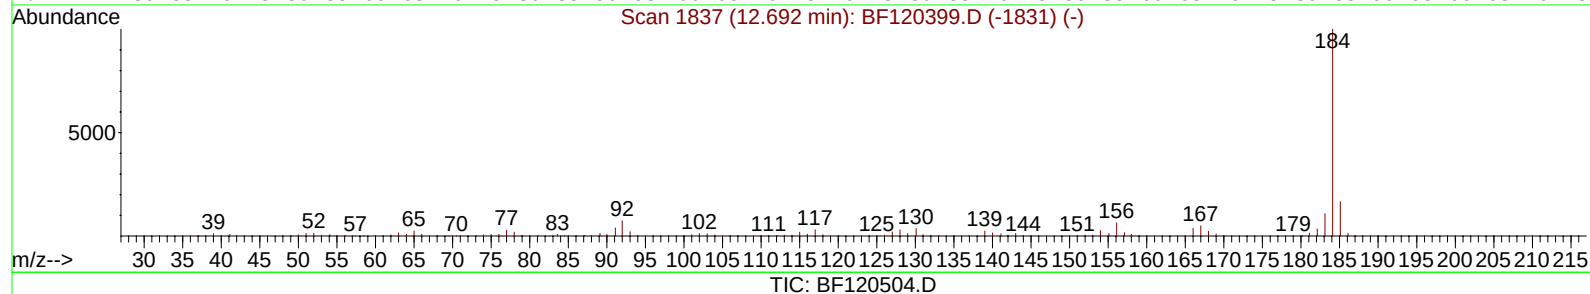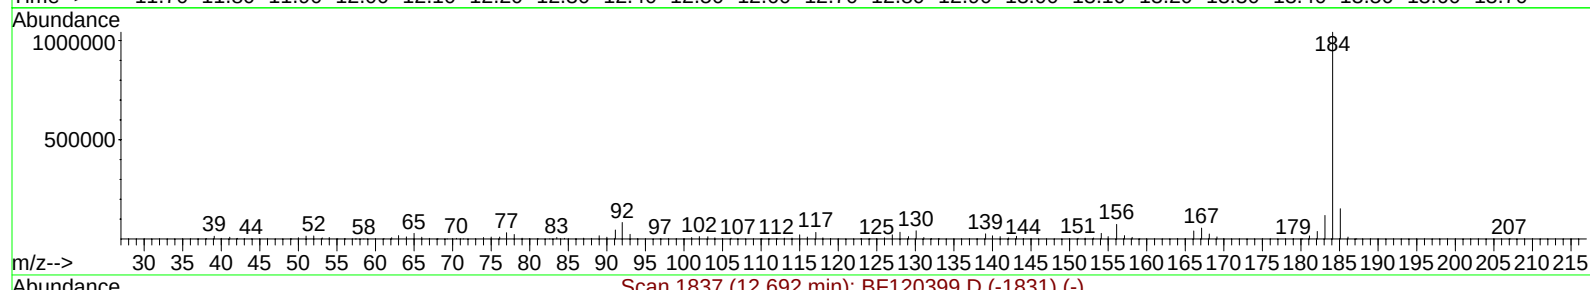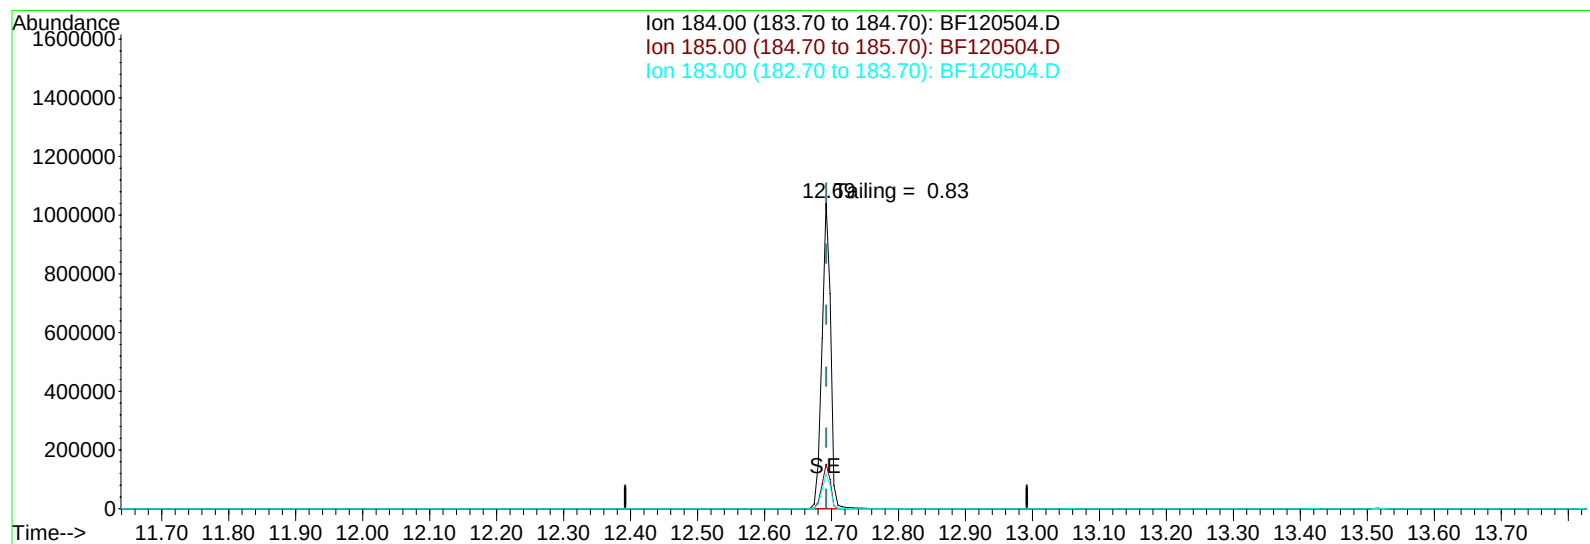

(77) Benzidine

12.692min (-0.000) 0.00ng

response 936527

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.62
183.00	11.40	11.41
0.00	0.00	0.00