


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060320\
 Data File : BF120504.D
 Acq On : 3 Jun 2020 12:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 03 14:26:17 2020

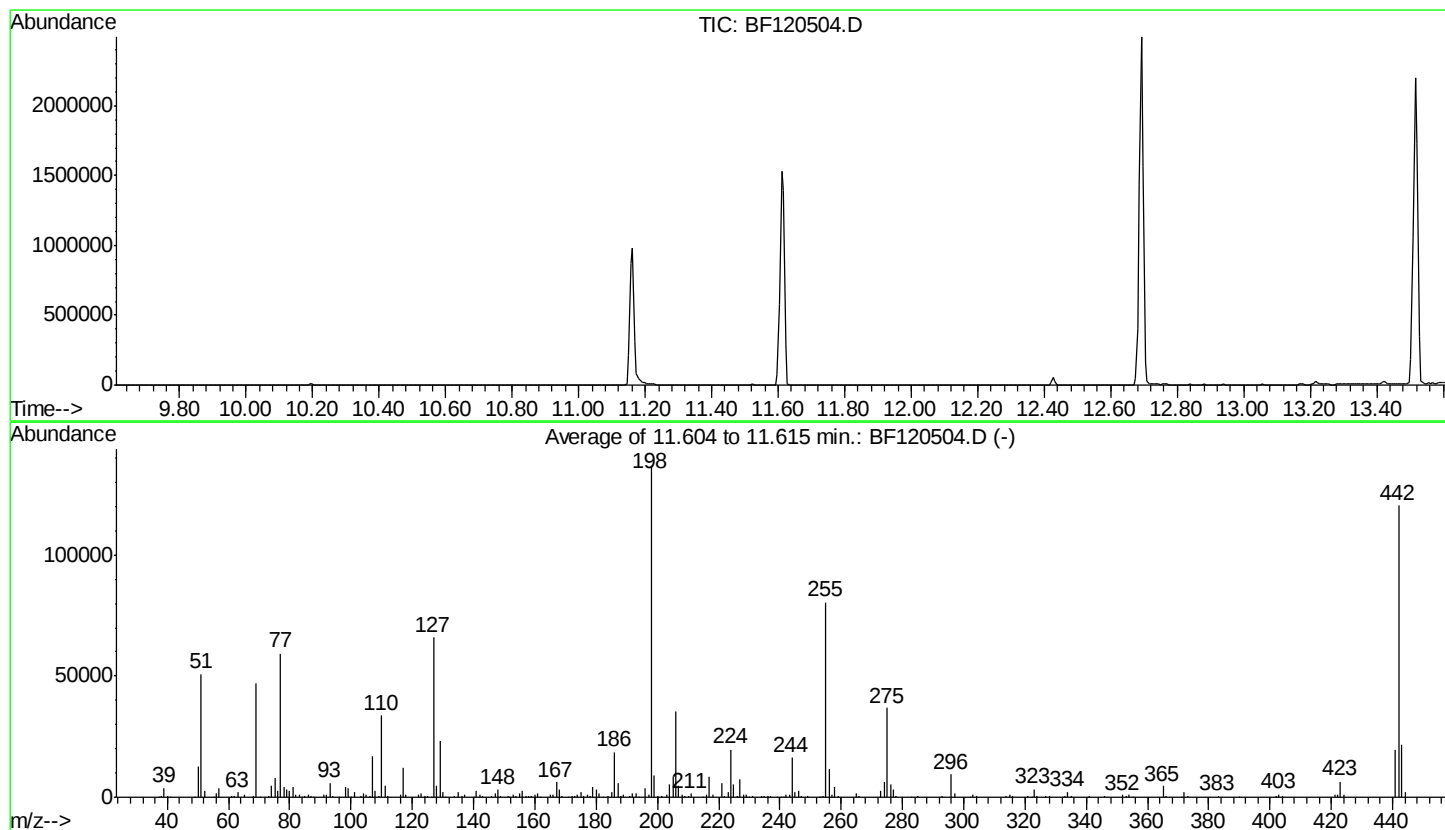

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	50805	PASS
68	69	0.00	2	1.7	785	PASS
69	198	0.00	100	34.2	46856	PASS
70	69	0.00	2	0.3	155	PASS
127	198	10	80	48.1	65885	PASS
197	198	0.00	2	0.6	852	PASS
198	198	100	100	100.0	136872	PASS
199	198	5	9	6.7	9193	PASS
275	198	10	60	27.0	36888	PASS
365	198	1	100	3.3	4518	PASS
441	198	0.01	100	14.1	19332	PASS
442	198	50	100	87.9	120304	PASS
443	442	15	24	18.2	21942	PASS