


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060321\
 Data File : BF124118.D
 Acq On : 3 Jun 2021 13:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 04 09:56:24 2021

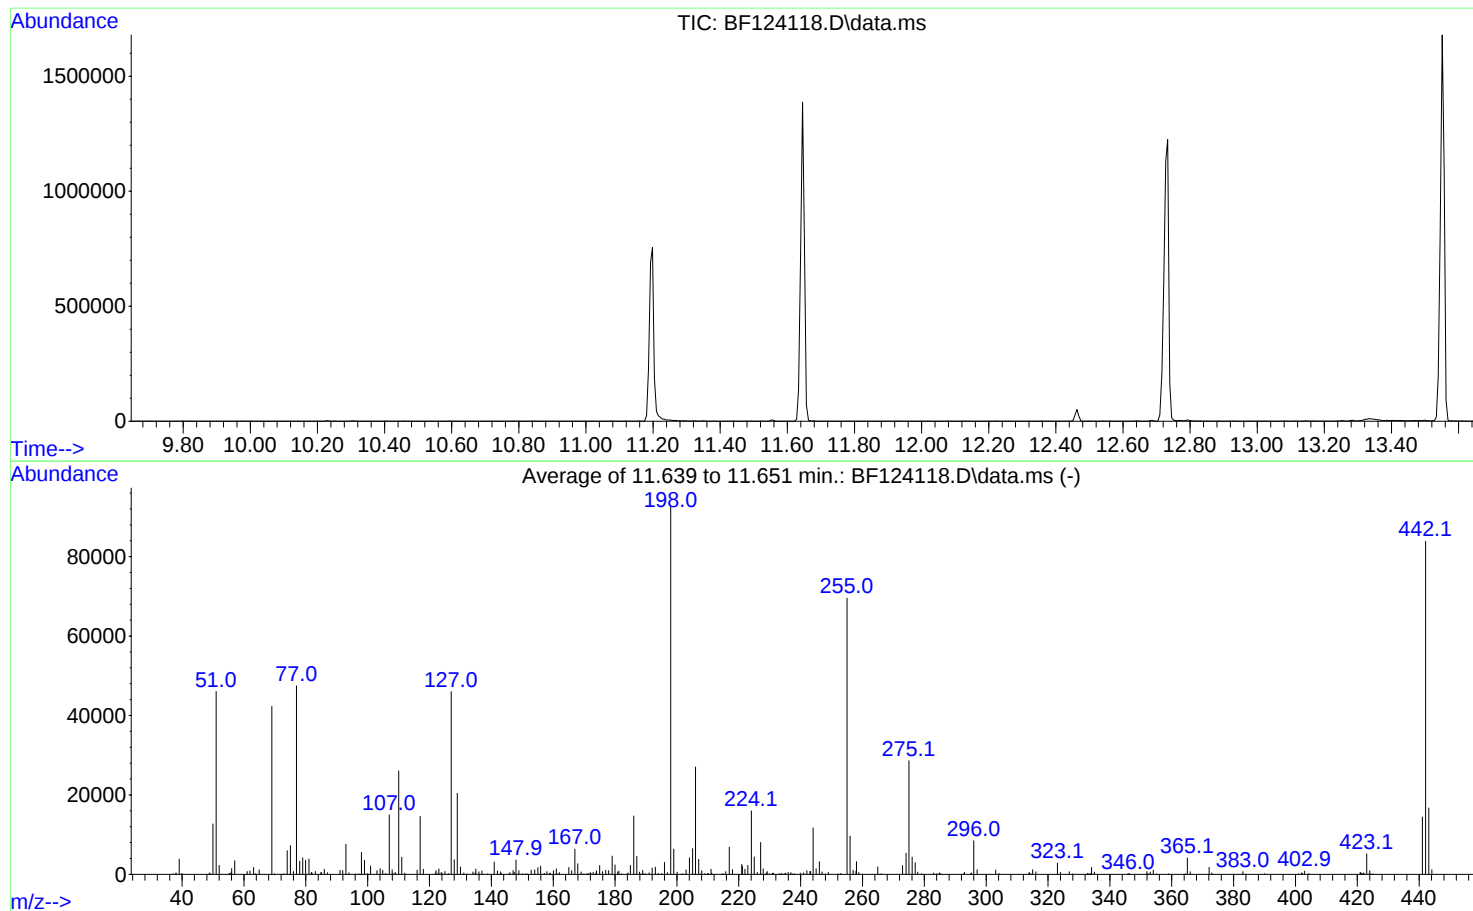




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.7	46032	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.7	42293	PASS
70	69	0.00	2	0.3	143	PASS
127	198	10	80	49.7	46019	PASS
197	198	0.00	2	0.5	460	PASS
198	198	100	100	100.0	92613	PASS
199	198	5	9	6.9	6361	PASS
275	198	10	60	30.9	28613	PASS
365	198	1	100	4.5	4167	PASS
441	198	0.01	100	15.6	14405	PASS
442	442	50	100	100.0	83861	PASS
443	442	15	24	20.0	16734	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060321\
 Data File : BF124118.D
 Acq On : 3 Jun 2021 13:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jun 03 13:45:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 27 13:12:25 2021
 Response via : Initial Calibration

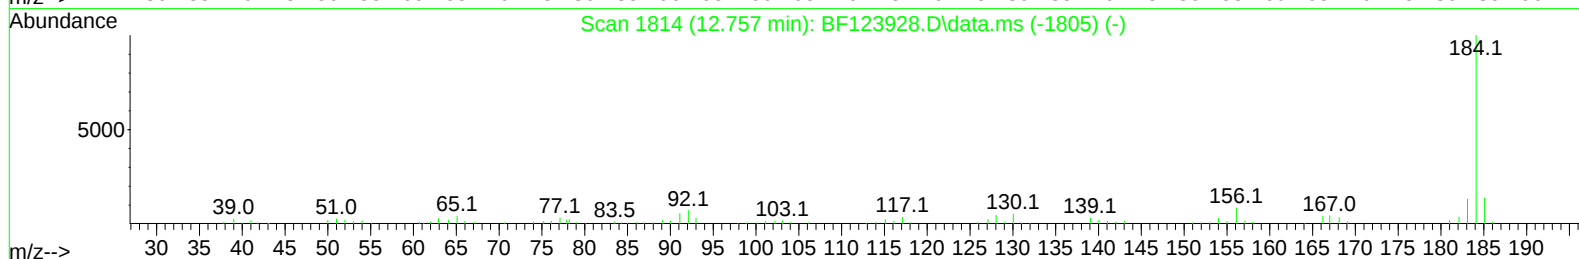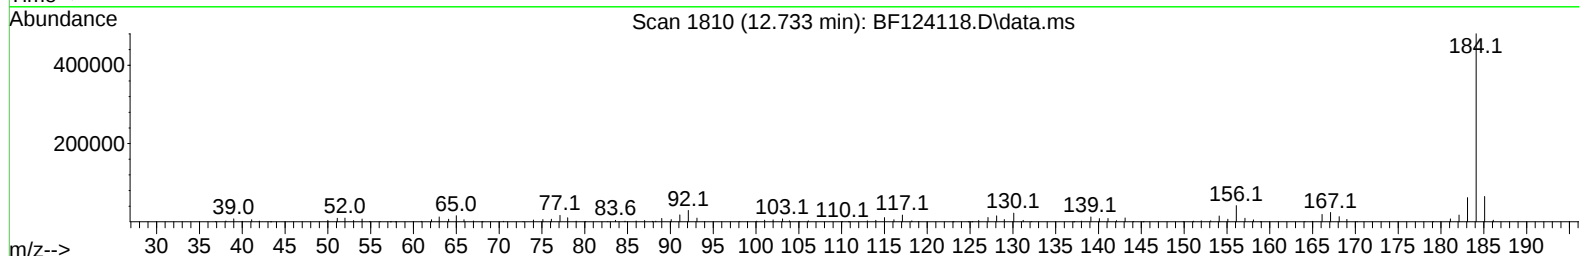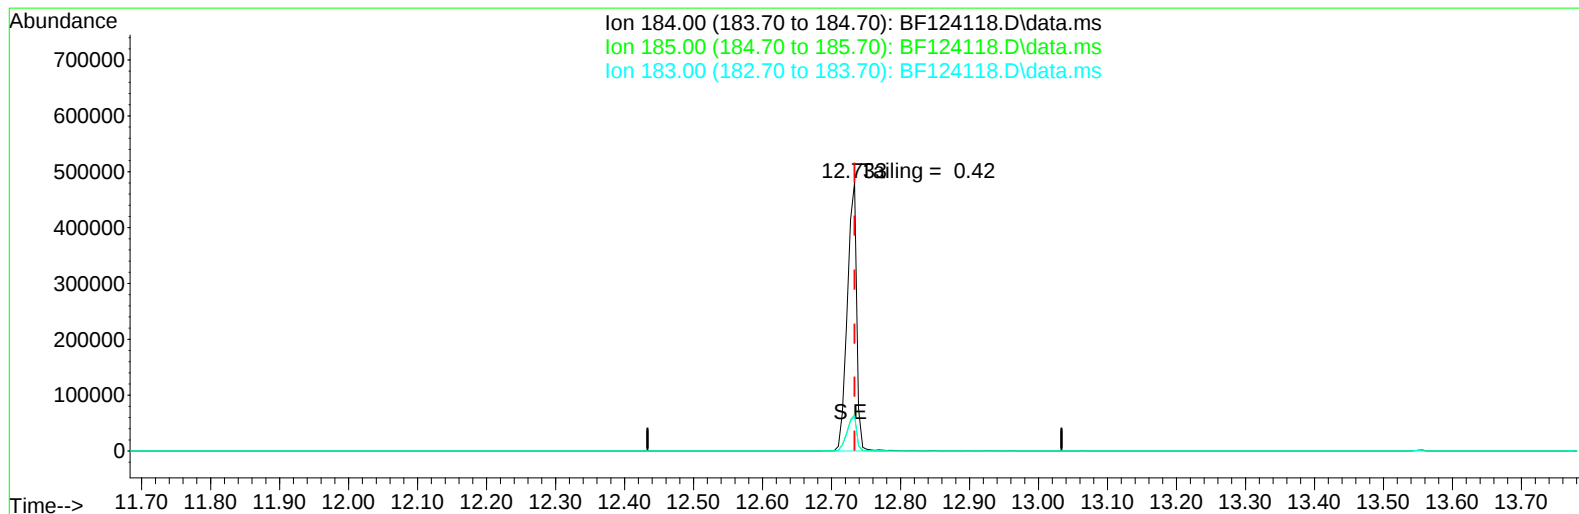

TIC: BF124118.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 0.00 ng




response 452486

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.48
183.00	9.80	12.95#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060321\
Data File : BF124118.D
Acq On : 3 Jun 2021 13:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 03 13:45:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 27 13:12:25 2021
Response via : Initial Calibration

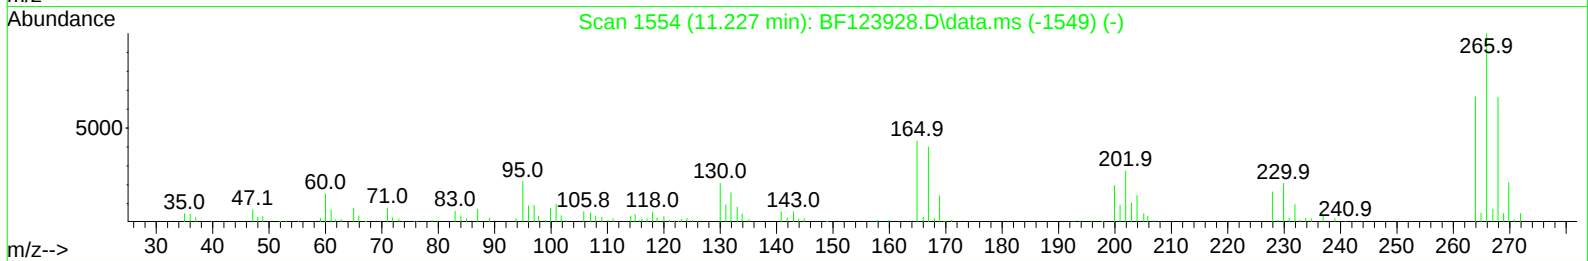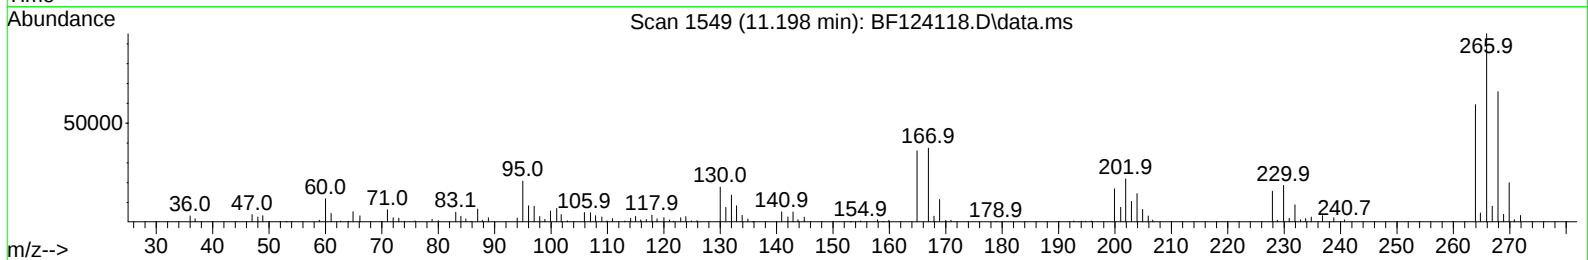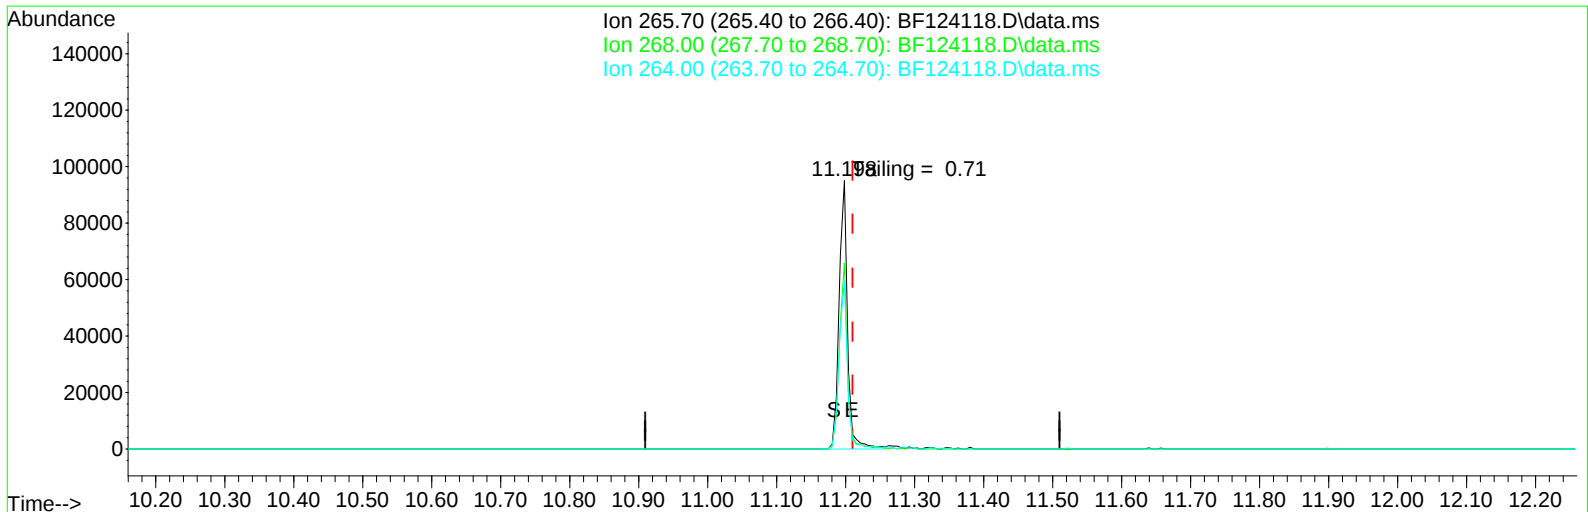

TIC: BF124118.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.012) 12484.33 ng

response 80681

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	69.26
264.00	65.70	62.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2021	BNA_F	<u>BF124118.D</u>
Compound Name	Response	Retention Time
DDT	248625	13.55
DDD	675	13.25
DDE	0	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
675	249300	0.27