
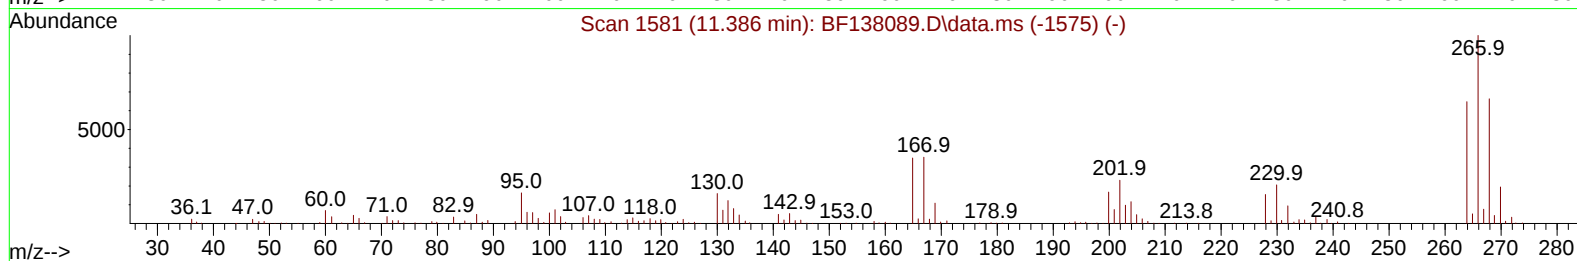
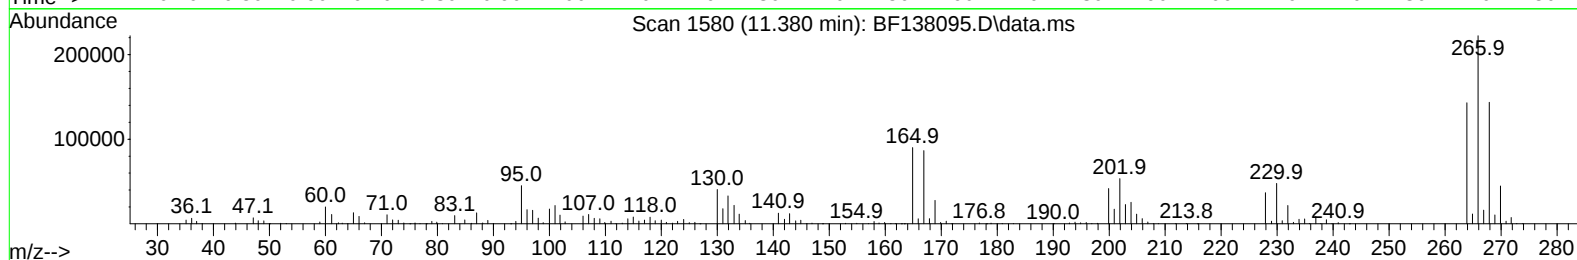


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060324\
Data File : BF138095.D
Acq On : 03 Jun 2024 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 12:06:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF053124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

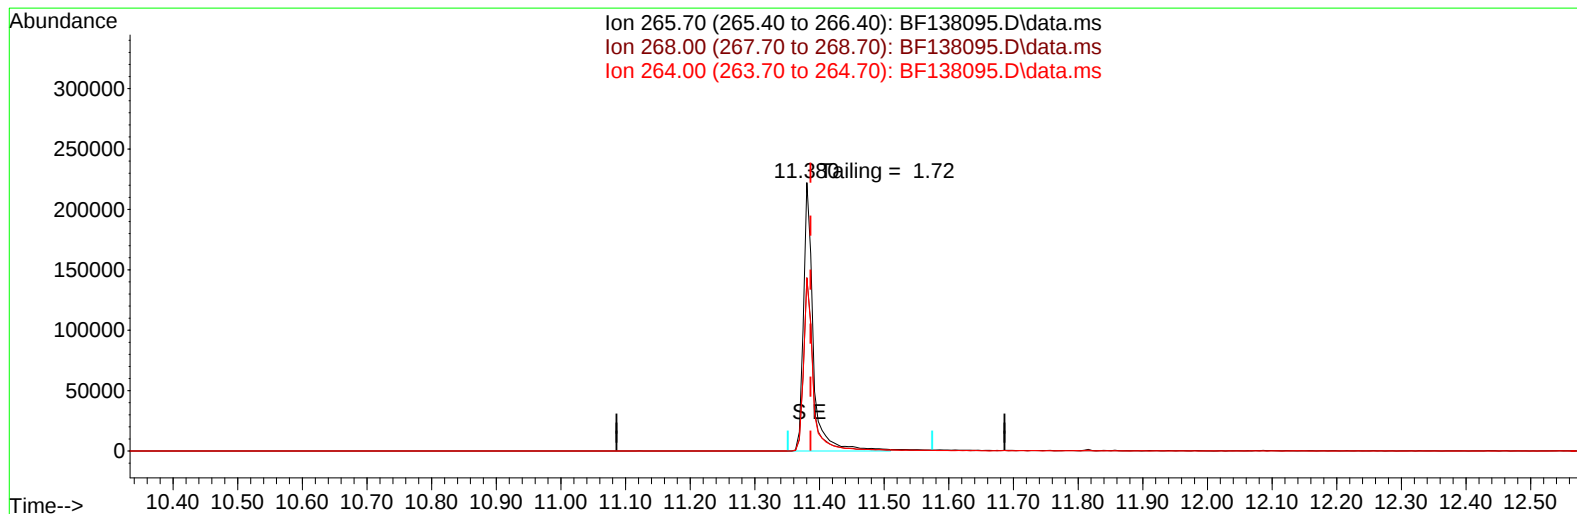

TIC: BF138095.D\data.ms

(70) Pentachlorophenol (C)




11.380min (-0.006) 78986.05 ng

response 237532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.60
264.00	64.80	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060324\
Data File : BF138095.D
Acq On : 03 Jun 2024 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 12:06:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF053124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

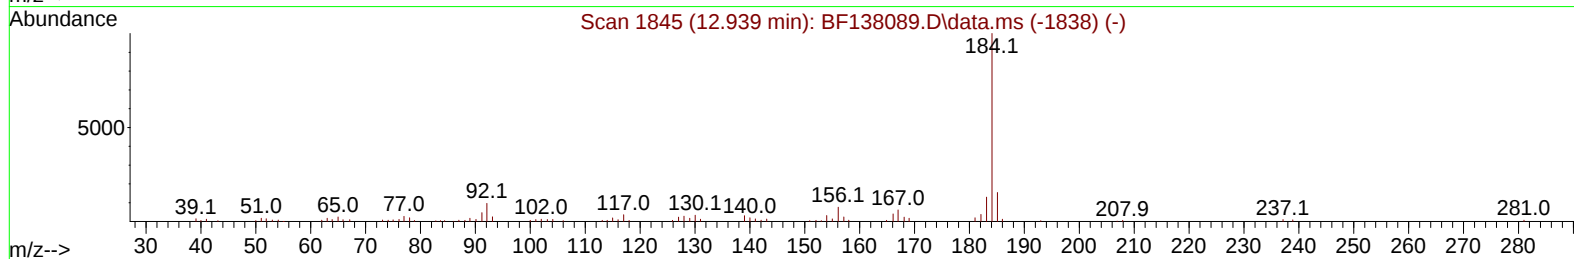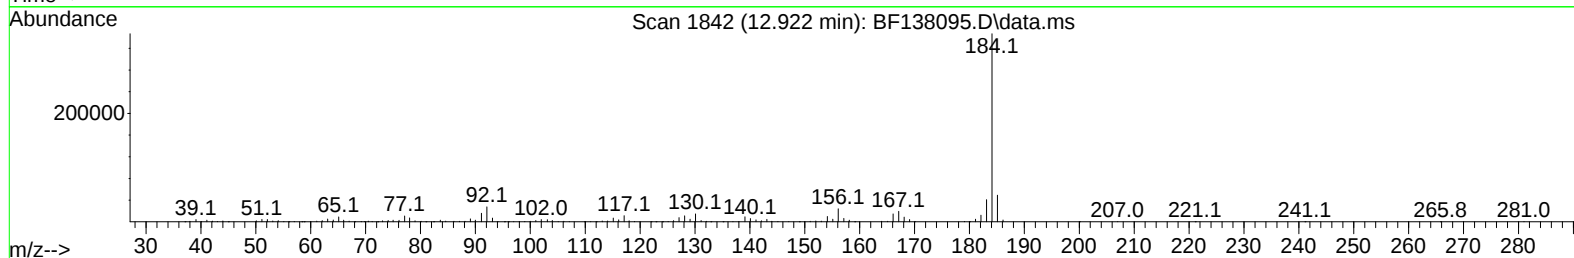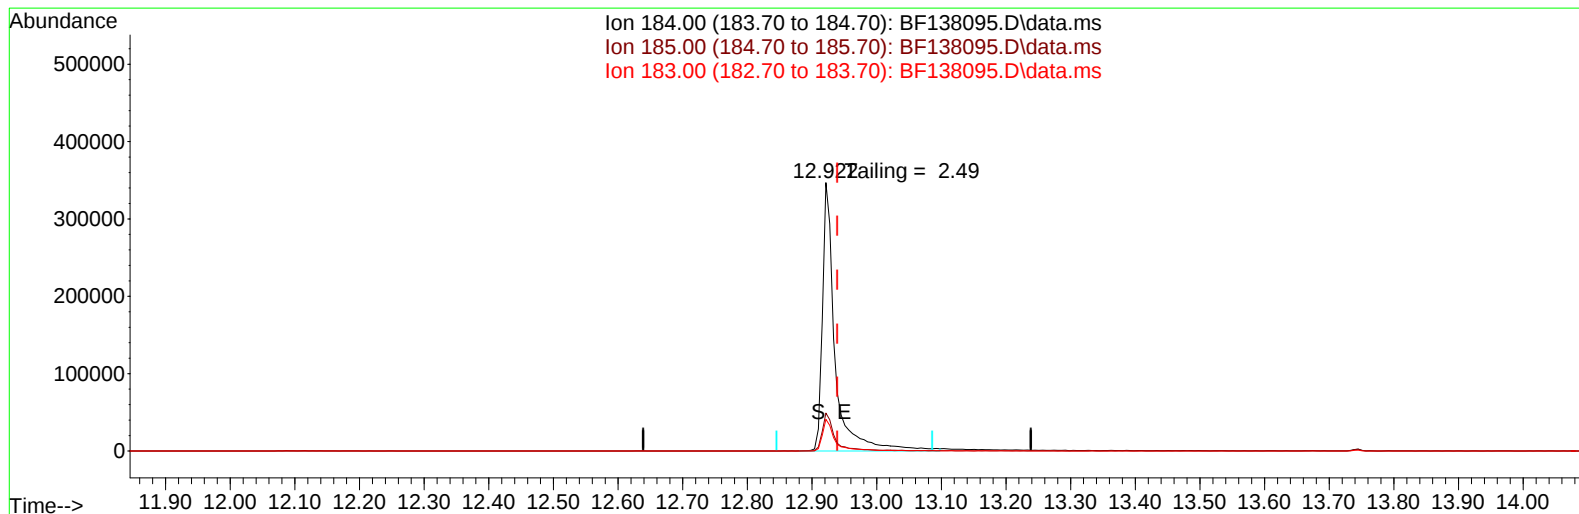

TIC: BF138095.D\data.ms

(77) Benzidine

12.922min (-0.017) -20.00 ng

response 475976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	12.80	11.83
0.00	0.00	0.00