


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060324\
Data File : BF138095.D
Acq On : 03 Jun 2024 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF053124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 01 01:21:05 2024

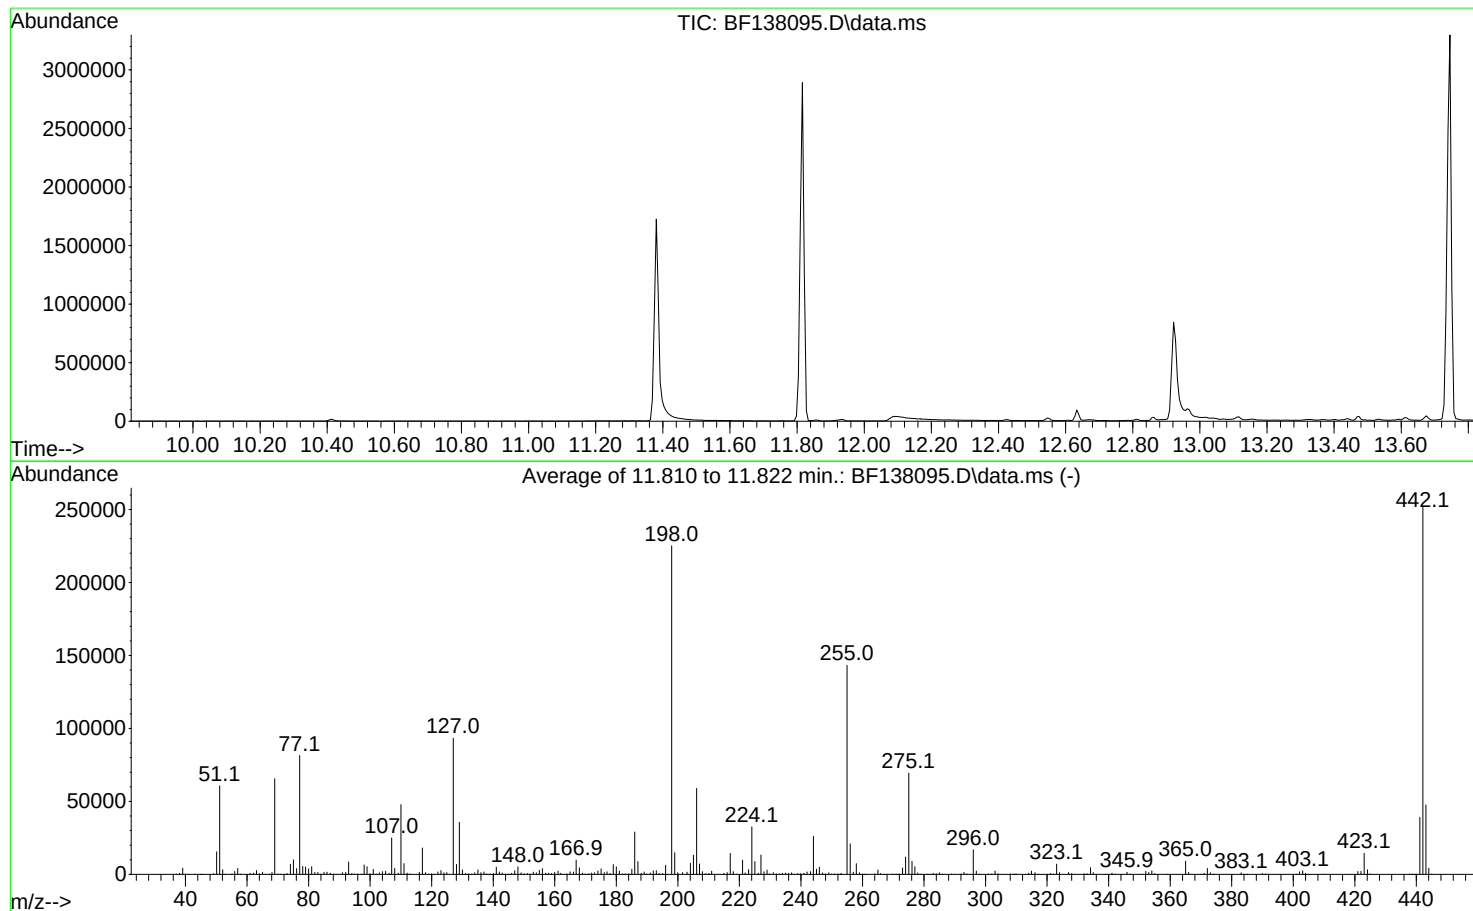




AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	60675	PASS
68	69	0.00	2	2.0	1287	PASS
69	198	0.00	100	29.1	65619	PASS
70	69	0.00	2	0.5	342	PASS
127	198	10	80	41.5	93347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	225144	PASS
199	198	5	9	6.6	14791	PASS
275	198	10	60	30.8	69360	PASS
365	198	1	100	4.1	9138	PASS
441	198	0.01	100	17.3	39008	PASS
442	442	50	100	100.0	252077	PASS
443	442	15	24	18.9	47643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060324\
Data File : BF138095.D
Acq On : 03 Jun 2024 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 03 12:06:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF053124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

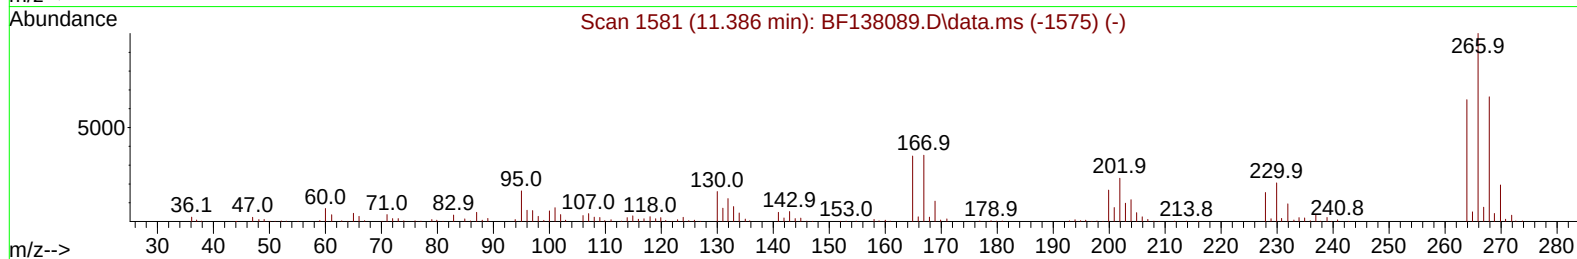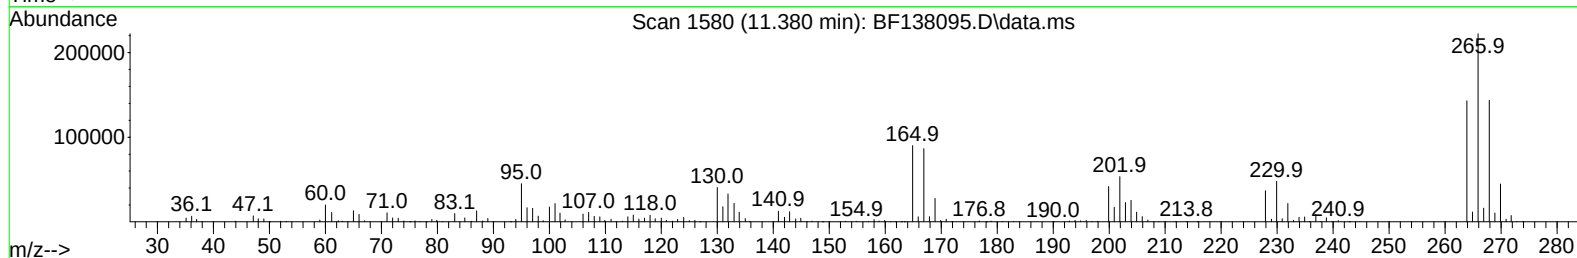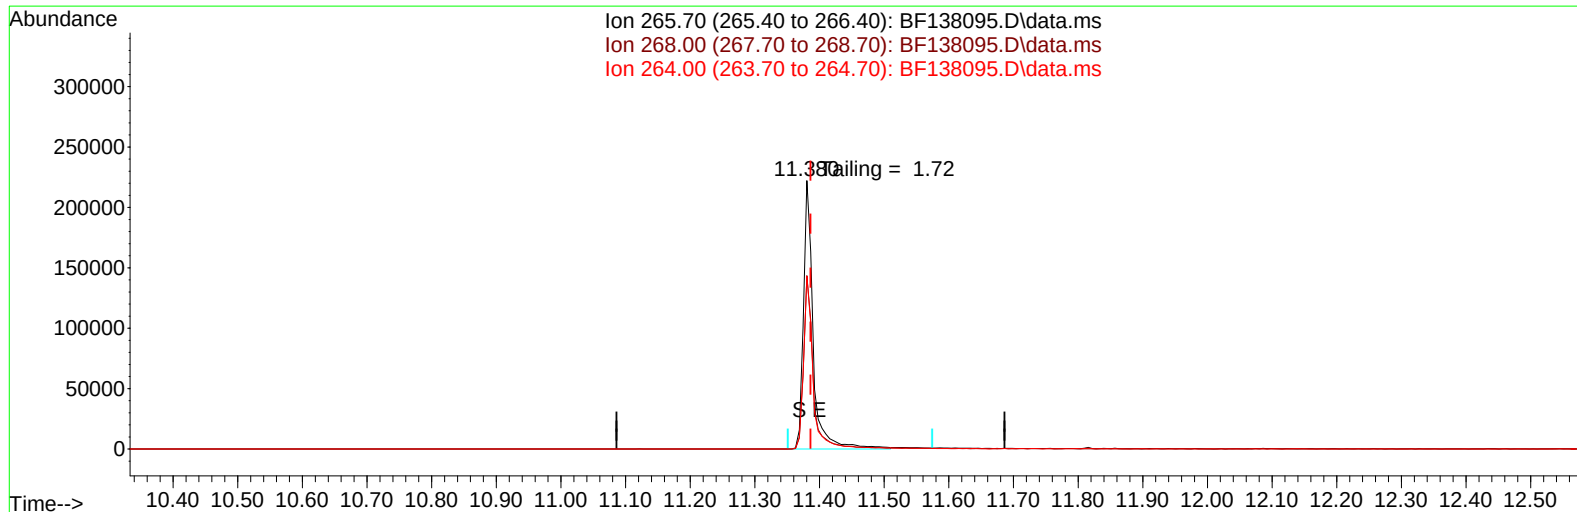

TIC: BF138095.D\data.ms

(70) Pentachlorophenol (C)

11.380min (-0.006) 78986.05 ng




response 237532

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.60
264.00	64.80	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060324\
Data File : BF138095.D
Acq On : 03 Jun 2024 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 03 12:06:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF053124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

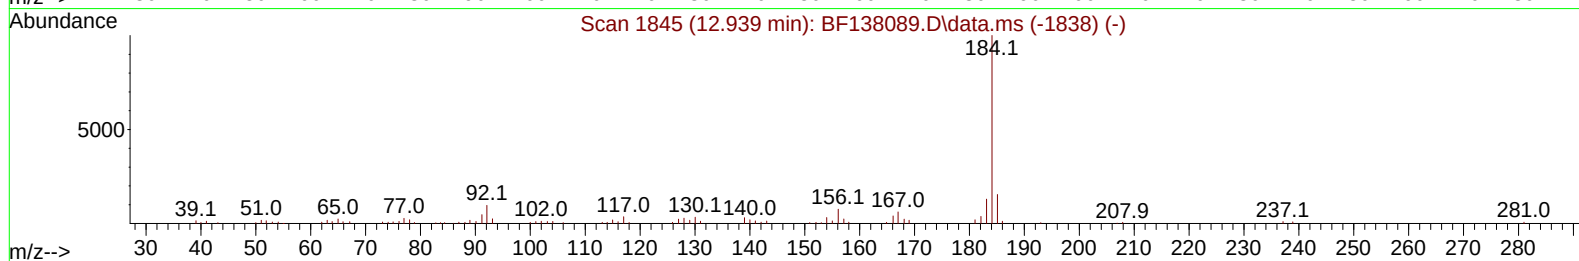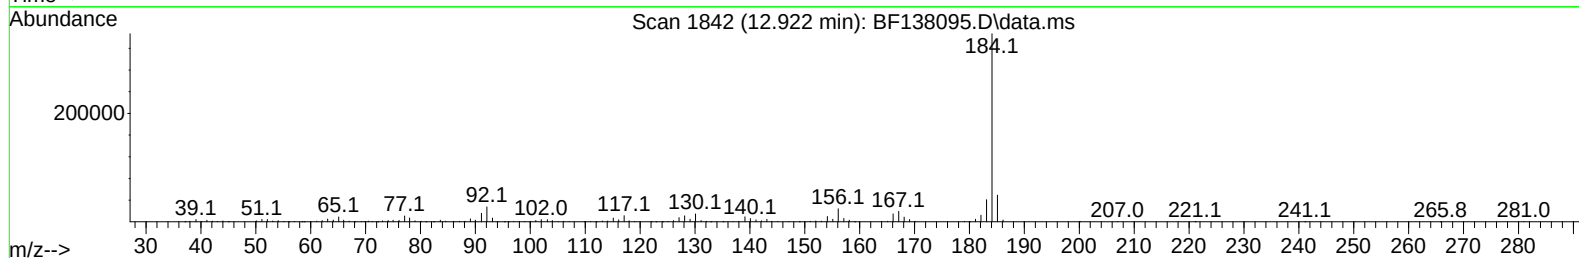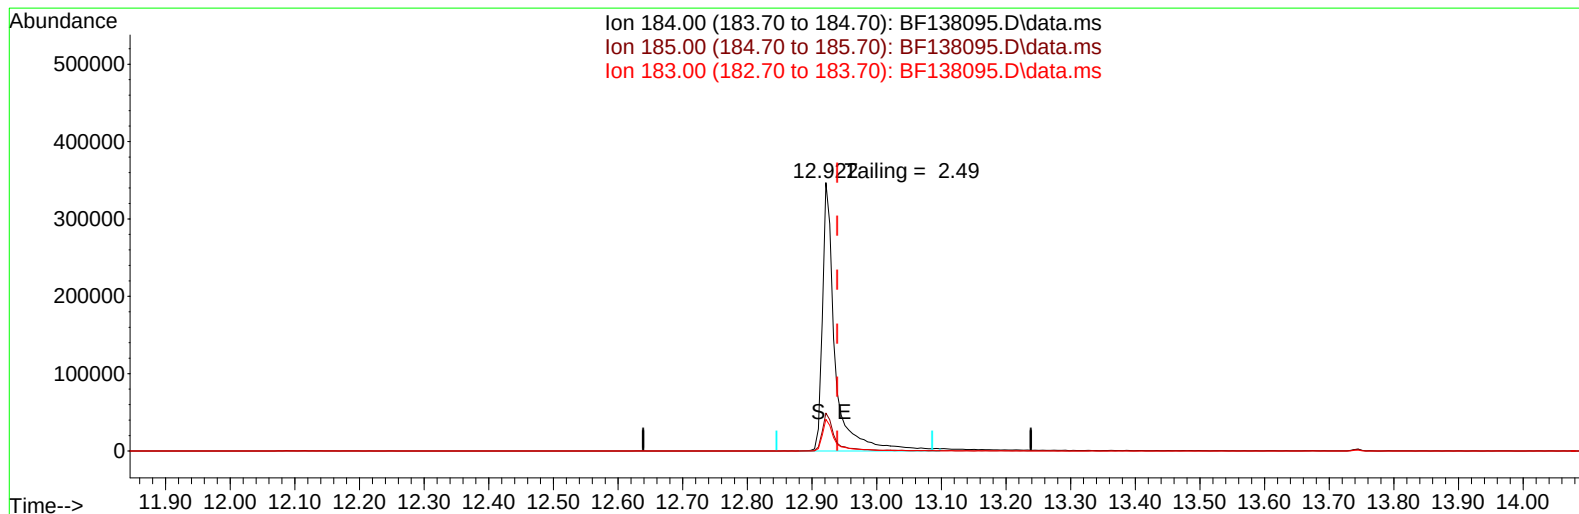

TIC: BF138095.D\data.ms

(77) Benzidine

12.922min (-0.017) -20.00 ng

response 475976

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.16
183.00	12.80	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2024	BNA_F	<u>BF138095.D</u>
Compound Name	Response	Retention Time
DDT	592883	13.745
DDD	9580	13.474
DDE	399	13.104
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9979	602862	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP