

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060415\
 Data File : BF079708.D
 Acq On : 4 Jun 2015 18:09
 Operator : TP/IZ
 Sample : PB83779BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83779BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.513	112	116	118	rVB	7896321	12858434	100.00%	33.317%
2	6.124	430	432	435	rBV	2606695	2439371	18.97%	6.321%
3	7.096	515	517	520	rBV	2291223	2389492	18.58%	6.191%
4	7.279	530	533	535	rBV	2325790	2671433	20.78%	6.922%
5	7.507	551	553	555	rBV	758153	610718	4.75%	1.582%
6	7.667	565	567	569	rBV	2595692	2114994	16.45%	5.480%
7	8.056	599	601	604	rBV	1027254	1354611	10.53%	3.510%
8	8.799	664	666	668	rBV	999580	805771	6.27%	2.088%
9	9.873	758	760	762	rBV	4138974	3310845	25.75%	8.579%
10	10.571	819	821	824	rBV	790109	897350	6.98%	2.325%
11	11.371	888	891	893	rBV	1826982	1734055	13.49%	4.493%
12	12.079	951	953	956	rBV	1145546	1018479	7.92%	2.639%
13	13.737	1095	1098	1100	rBV	4041477	4168780	32.42%	10.802%
14	14.971	1203	1206	1208	rBV	826266	1149286	8.94%	2.978%
15	16.880	1370	1373	1381	rBV	710661	1070110	8.32%	2.773%


Sum of corrected areas: 38593729

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060415\
Data File : BF079708.D
Acq On : 4 Jun 2015 18:09
Operator : TP/IZ
Sample : PB83779BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83779BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

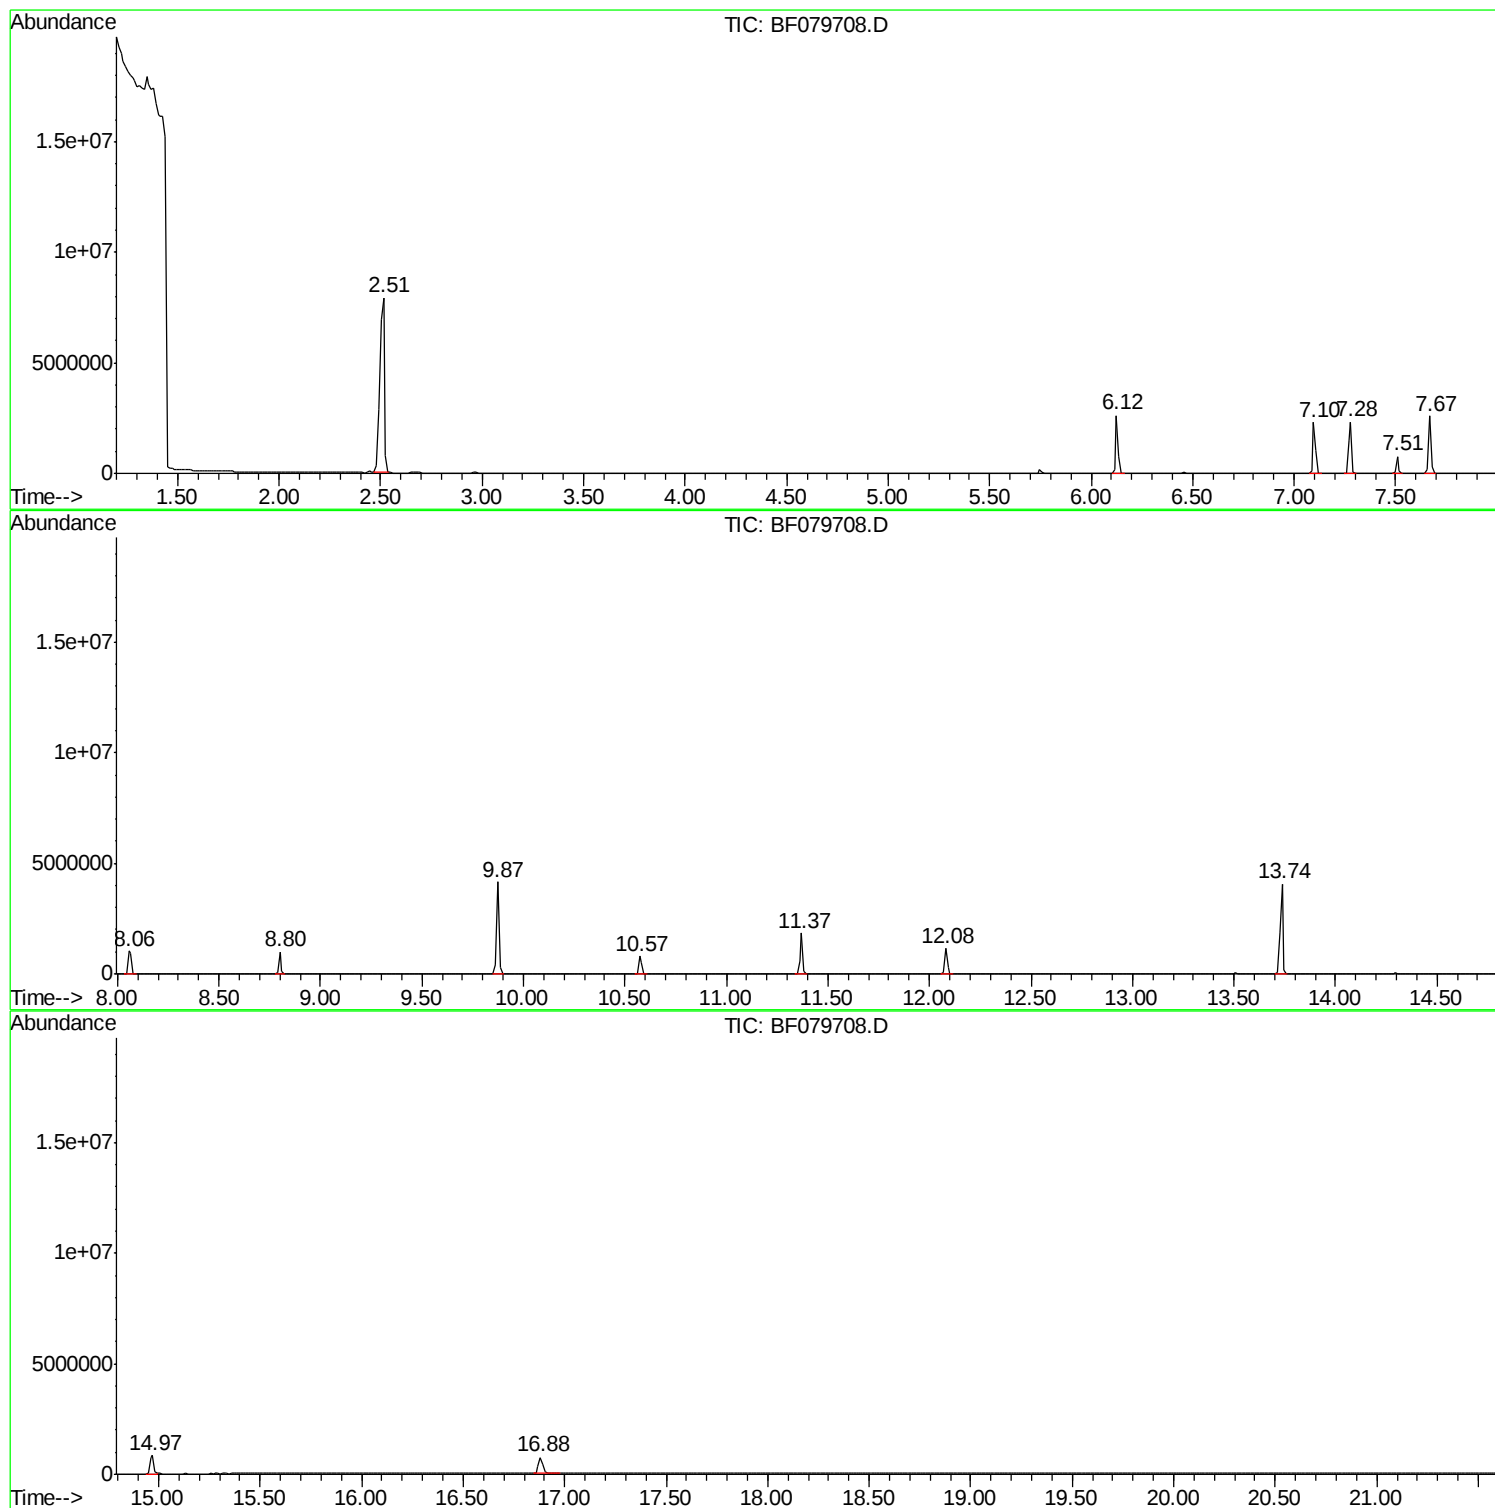

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060415\
Data File : BF079708.D
Acq On : 4 Jun 2015 18:09
Operator : TP/IZ
Sample : PB83779BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83779BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.51 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.51	421.09 ng	12858400	1,4-Dichlorobenzene-d4	7.51

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2,2-dimethoxy-	104	C5H12O2	000077-76-9	40
2		1,3-Diaminoguanidine	89	CH7N5	004364-78-7	9
3		1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	9
4		N-Ethylformamide	73	C3H7NO	000627-45-2	9
5		2-Butanone, 3-methoxy-3-methyl-	116	C6H12O2	036687-98-6	9

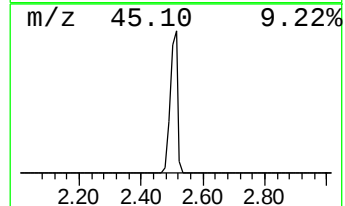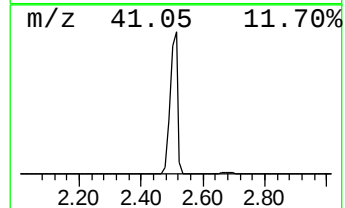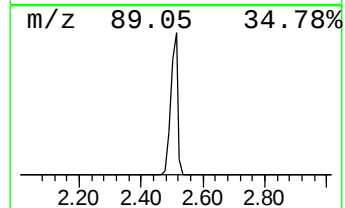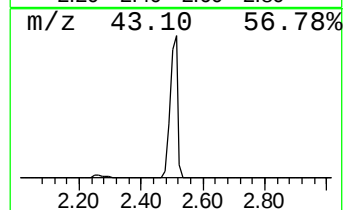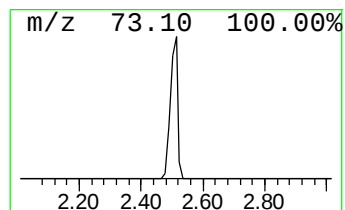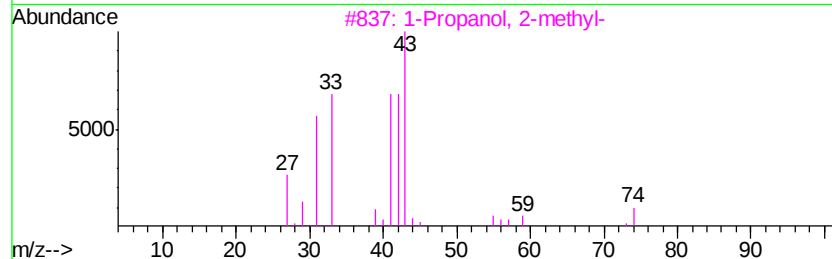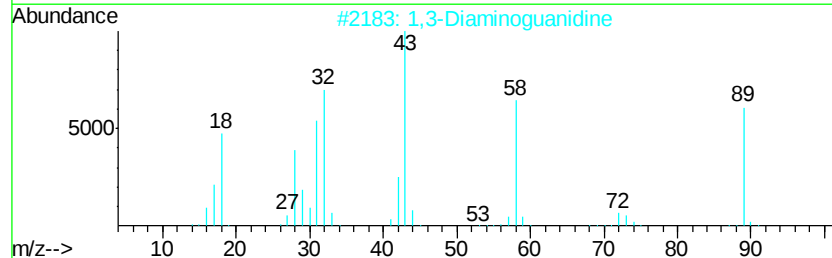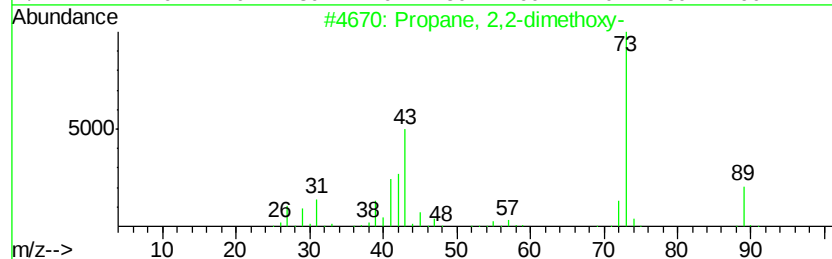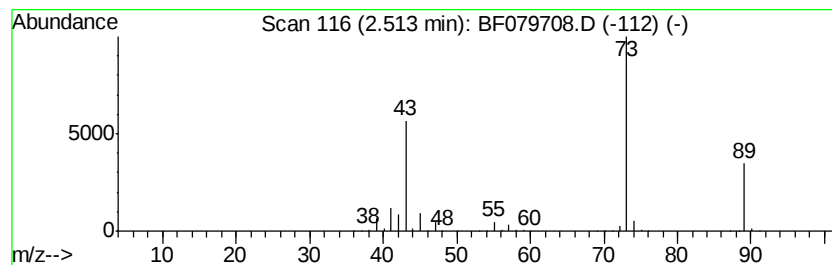

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060415\
Data File : BF079708.D
Acq On : 4 Jun 2015 18:09
Operator : TP/IZ
Sample : PB83779BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83779BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.28 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.28	87.49 ng	2671430	1,4-Dichlorobenzene-d4	7.51

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

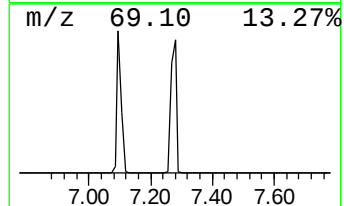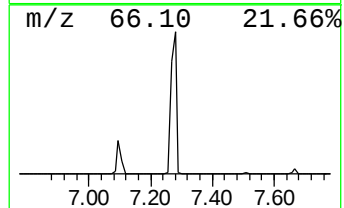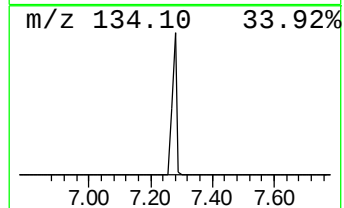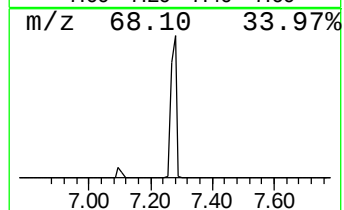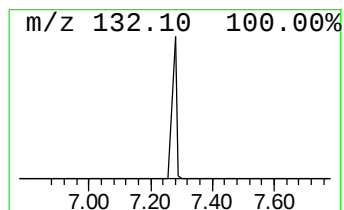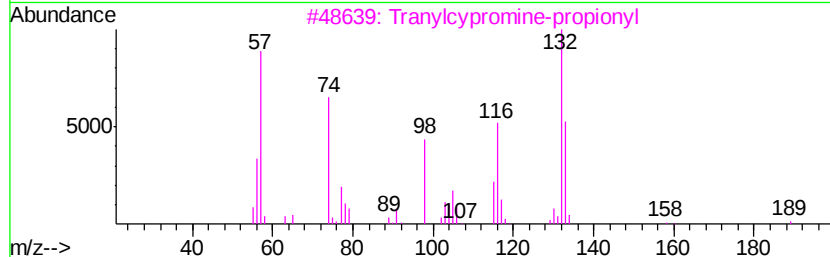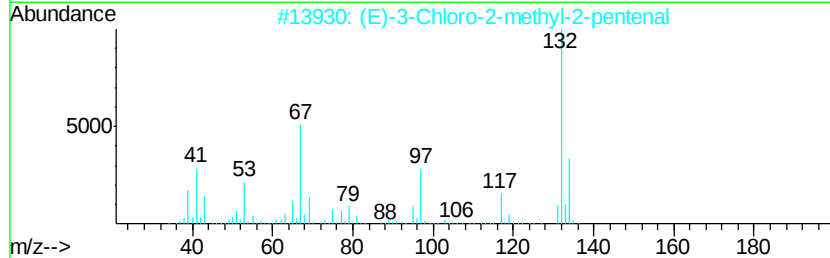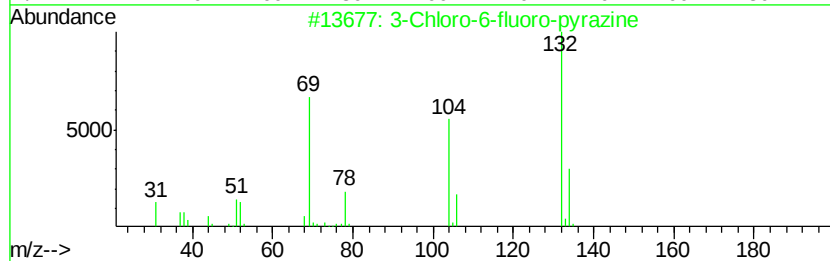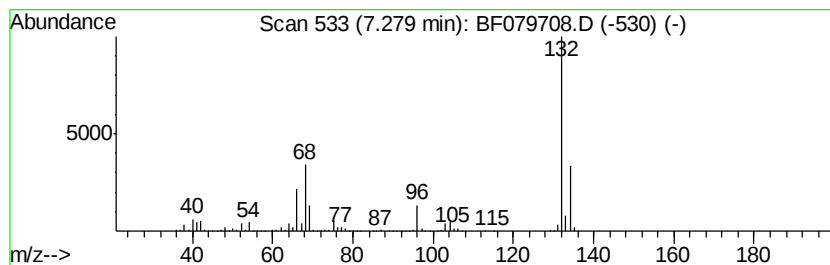

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060415\
Data File : BF079708.D
Acq On : 4 Jun 2015 18:09
Operator : TP/IZ
Sample : PB83779BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83779BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.51	2.51	421.1	ng	12858400	1	7.51	610718	20.0
unknown7.28	7.28	87.5	ng	2671430	1	7.51	610718	20.0