


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060415\
 Data File : BF079699.D
 Acq On : 4 Jun 2015 12:43
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 19:33:57 2015

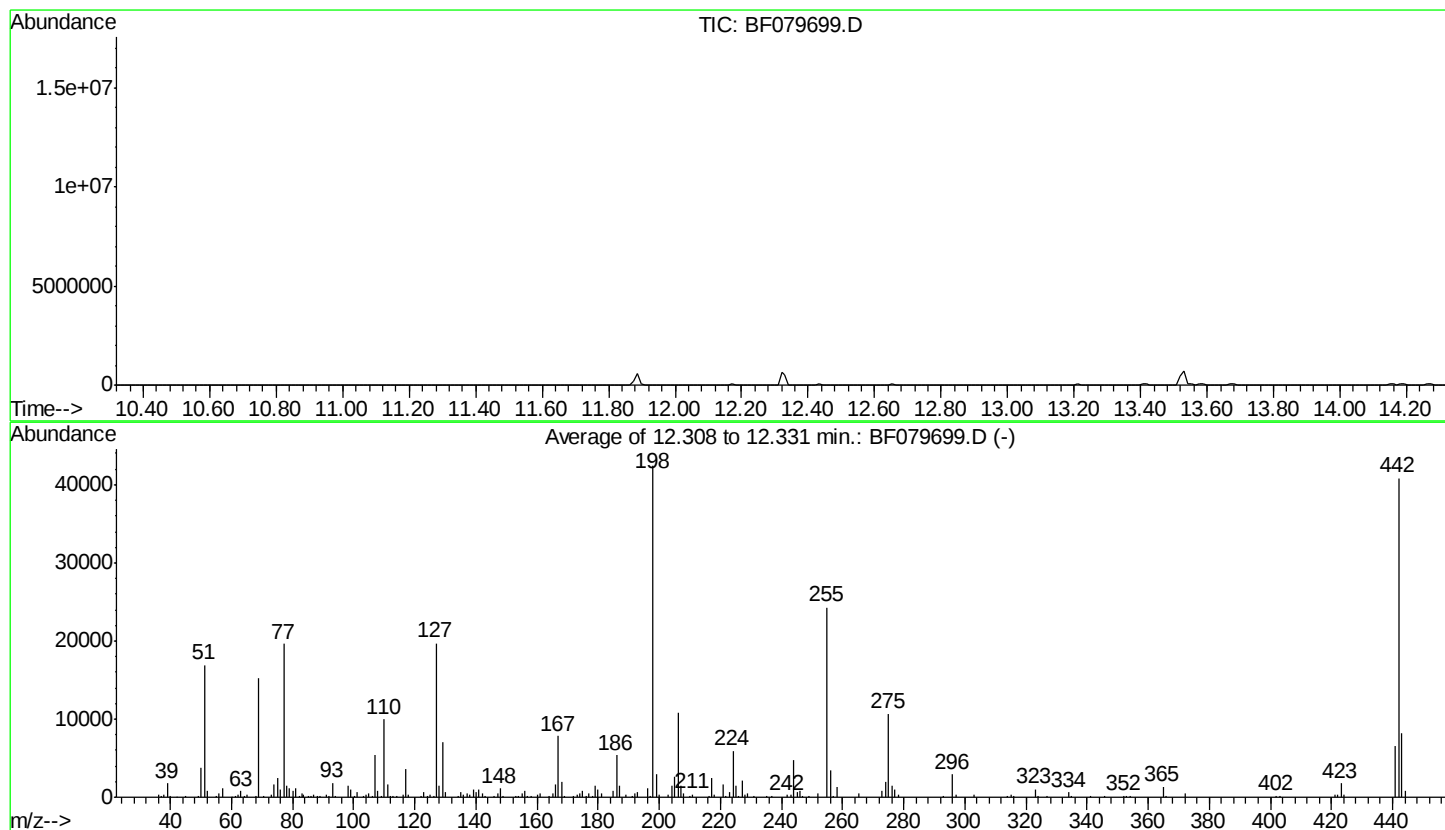

AutoFind: Scans 973, 974, 975; Background Corrected with Scan 970

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	16957	PASS
68	69	0.00	2	1.5	236	PASS
69	198	0.00	100	36.0	15262	PASS
70	69	0.00	2	1.1	174	PASS
127	198	10	80	46.3	19669	PASS
197	198	0.00	2	0.4	179	PASS
198	198	100	100	100.0	42446	PASS
199	198	5	9	7.0	2974	PASS
275	198	10	60	25.2	10691	PASS
365	198	1	100	3.2	1370	PASS
441	442	0.01	24	15.8	6479	PASS
442	198	50	100	96.3	40884	PASS
443	442	15	24	20.0	8178	PASS