


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060415\
 Data File : BF079719.D
 Acq On : 5 Jun 2015 00:51
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 19:33:57 2015

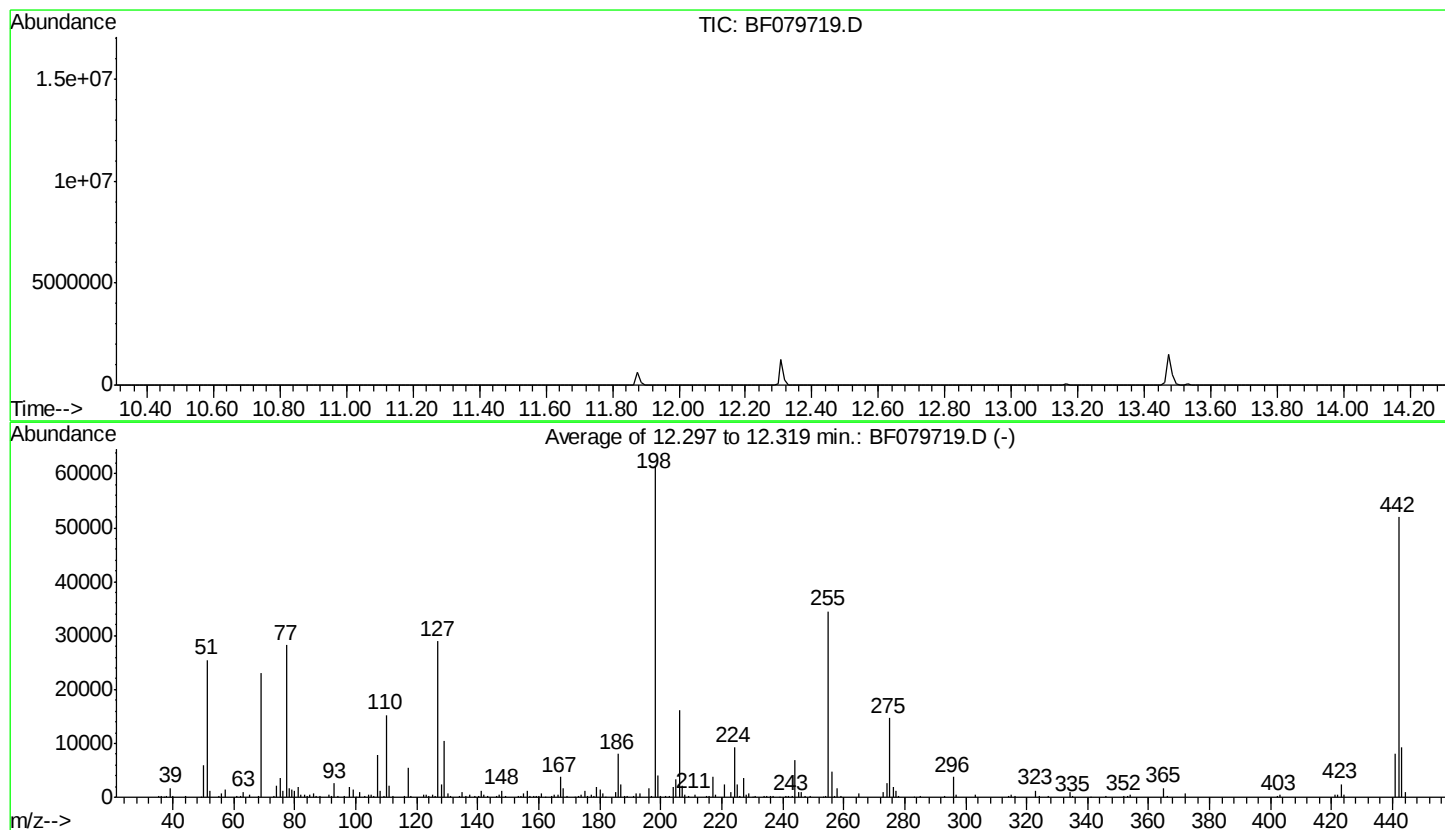

AutoFind: Scans 972, 973, 974; Background Corrected with Scan 969

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	25468	PASS
68	69	0.00	2	1.5	347	PASS
69	198	0.00	100	37.6	23124	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	28922	PASS
197	198	0.00	2	0.5	284	PASS
198	198	100	100	100.0	61525	PASS
199	198	5	9	6.7	4096	PASS
275	198	10	60	23.8	14669	PASS
365	198	1	100	2.9	1777	PASS
441	442	0.01	24	15.7	8149	PASS
442	198	50	100	84.5	52008	PASS
443	442	15	24	17.8	9238	PASS