

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060416\
 Data File : BF087682.D
 Acq On : 5 Jun 2016 1:38
 Operator : UM/SJ
 Sample : H3359-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OM-SPS-002-160531

Quant Time: Jun 05 04:41:35 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	132535	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	546829	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	254084	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	501931	20.00	ng	0.00
75) Chrysene-d12	14.01	240	407649	20.00	ng	-0.01
86) Perylene-d12	15.44	264	308706	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	665225	81.13	ng	0.00
7) Phenol-d6	6.48	99	896840	87.21	ng	-0.01
23) Nitrobenzene-d5	7.42	82	538642	56.99	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	226493	88.80	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	929336	49.49	ng	-0.01
78) Terphenyl-d14	12.97	244	925333	55.39	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.42	70	68694	10.70	ng	# 78
49) Dimethylphthalate	9.61	163	128868	6.98	ng	98
56) 2,4-Dinitrotoluene	9.90	165	32975	6.16	ng	# 38
64) 4,6-Dinitro-2-methylphenol	10.68	198	396	2.15	ng	# 1
66) 4-Bromophenyl-phenylether	10.68	248	14203	2.85	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060416\
Data File : BF087682.D
Acq On : 5 Jun 2016 1:38
Operator : UM/SJ
Sample : H3359-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OM-SPS-002-160531

Quant Time: Jun 05 04:41:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

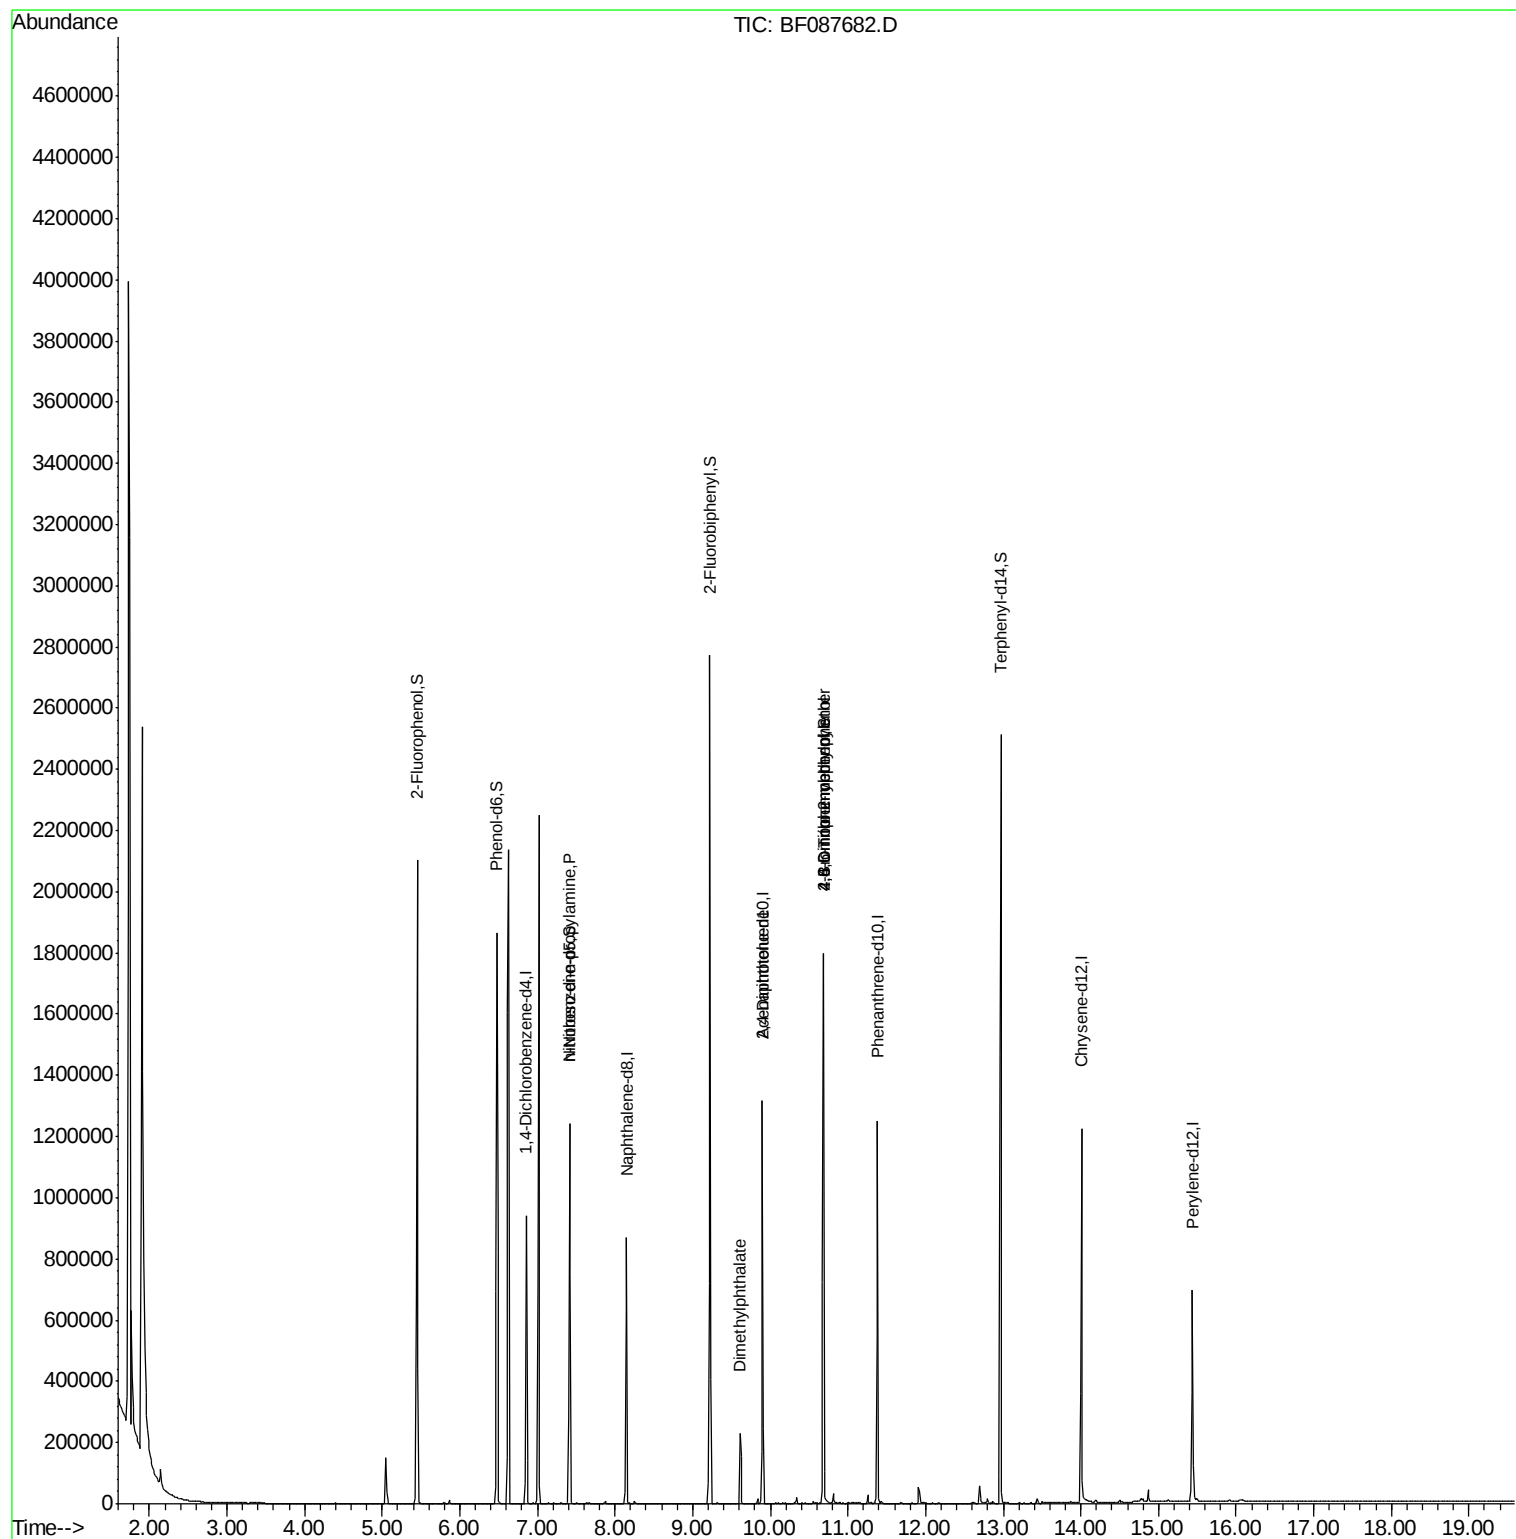

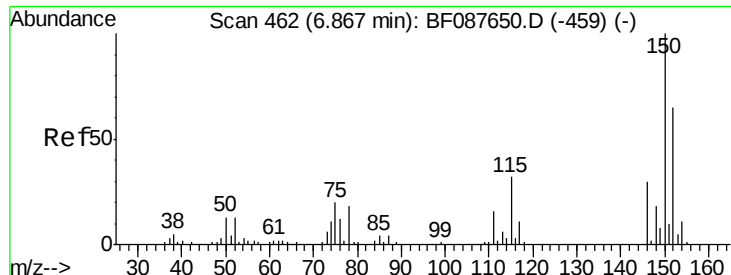

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 461

Delta R.T. -0.01 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tgt Ion:152 Resp: 132535

Ion Ratio Lower Upper

152 100

150 156.1 123.8 185.6




115 63.5 39.6 59.4#

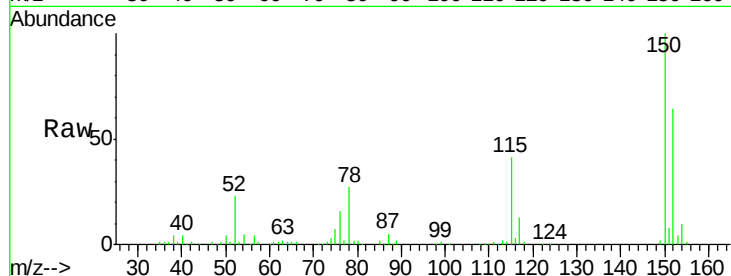

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

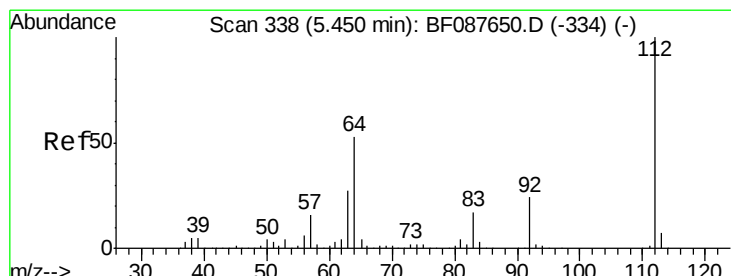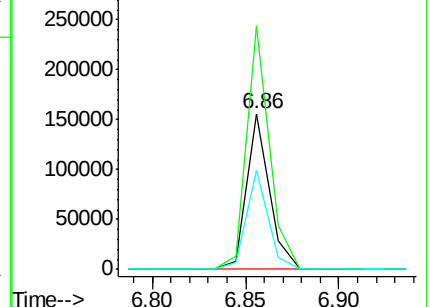

#5

2-Fluorophenol

Concen: 81.13 ng

RT: 5.45 min Scan# 338

Delta R.T. 0.00 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Tgt Ion:112 Resp: 665225

Ion Ratio Lower Upper

112 100

64 60.1 42.2 63.2



63 31.2 21.8 32.8

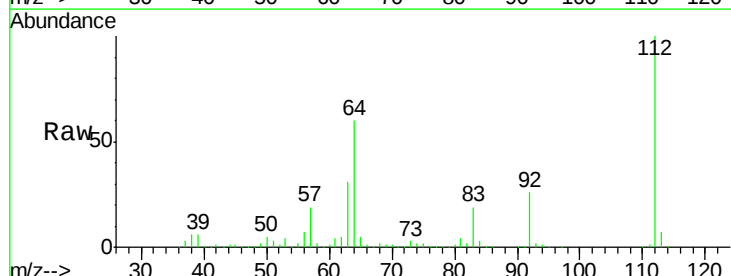


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

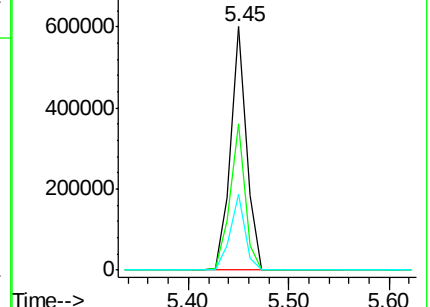

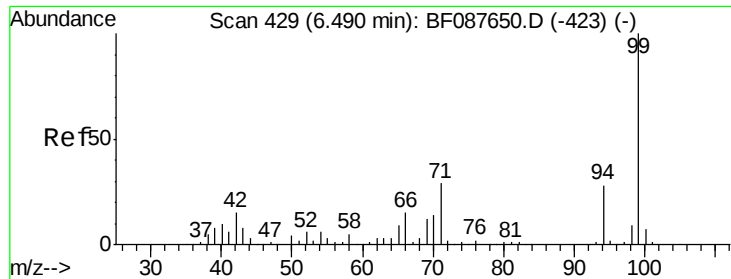

#7

Phenol-d6

Concen: 87.21 ng

RT: 6.48 min Scan# 428

Delta R.T. -0.01 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tgt Ion: 99 Resp: 896840

Ion Ratio Lower Upper

99 100

42 18.2 12.2 18.2




71 33.4 23.4 35.0

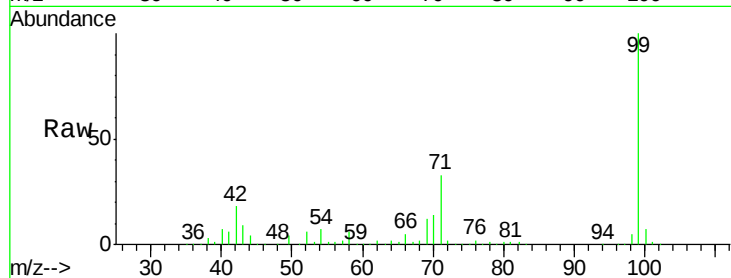

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

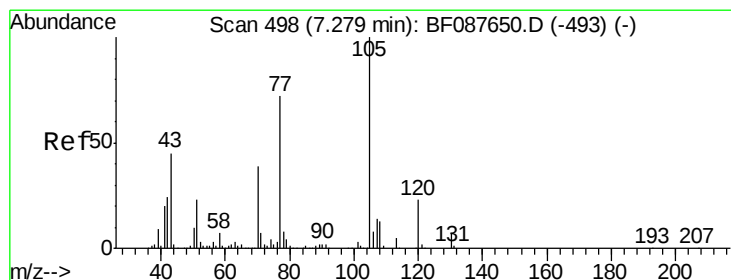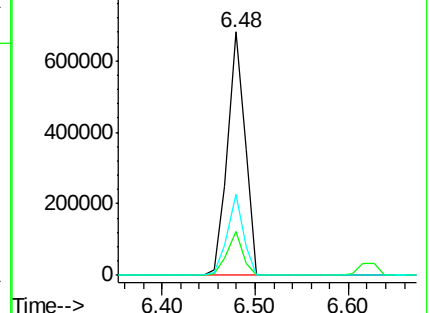

#19

n-Nitroso-di-n-propylamine

Concen: 10.70 ng

RT: 7.42 min Scan# 510

Delta R.T. 0.14 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Tgt Ion: 70 Resp: 68694


Ion Ratio Lower Upper

70 100

42 49.3 49.6 74.4#

101 0.0 7.1 10.7#

130 2.1 15.4 23.2#


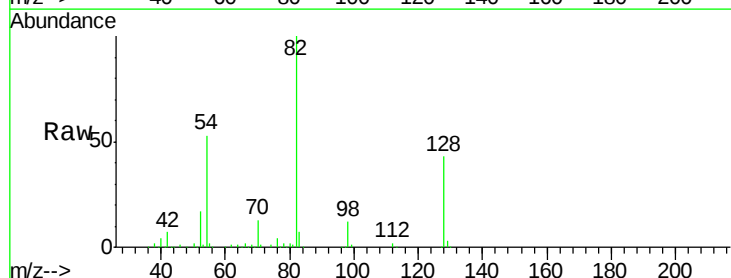



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

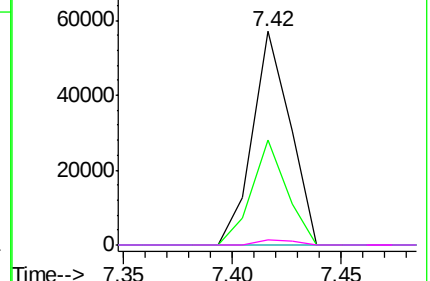



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 574

Delta R.T. -0.00 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531

Tgt Ion:136 Resp: 546829


Ion Ratio Lower Upper

136 100

137 10.6 9.1 13.7

54 5.5 6.6 10.0#

68 4.5 5.1 7.7#



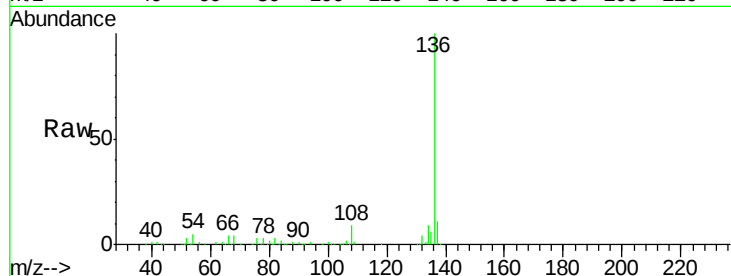


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

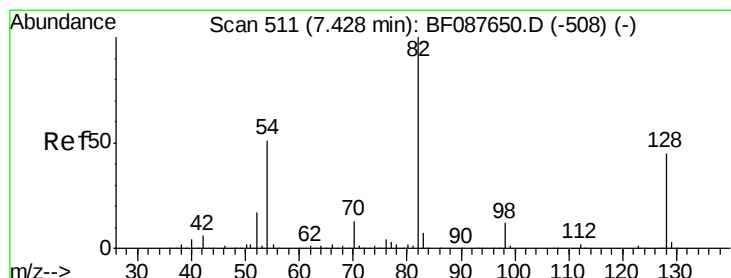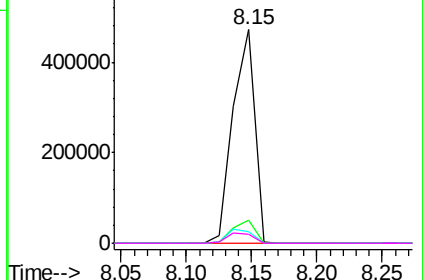

#23

Nitrobenzene-d5

Concen: 56.99 ng

RT: 7.42 min Scan# 510

Delta R.T. -0.01 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Tgt Ion: 82 Resp: 538642

Ion Ratio Lower Upper

82 100

128 42.8 35.9 53.9



54 52.7 40.9 61.3

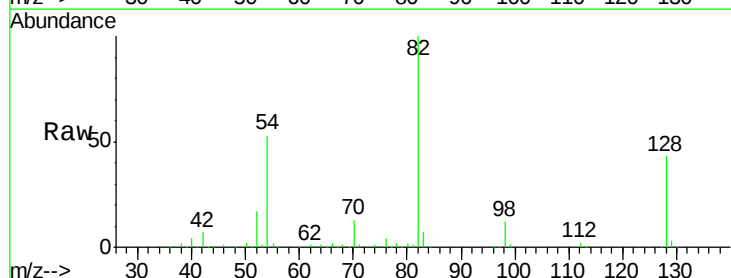


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

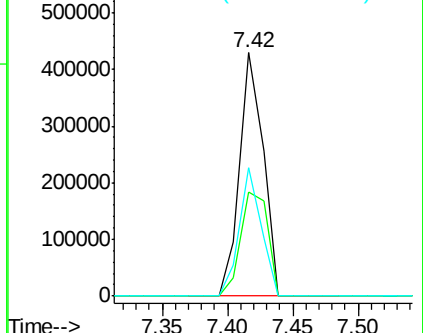

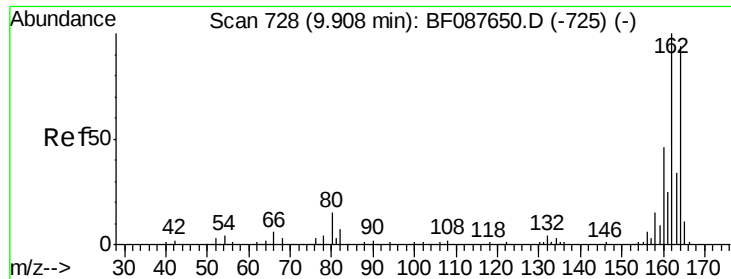

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.90 min Scan# 727

Delta R.T. -0.01 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tgt Ion:164 Resp: 254084

Ion Ratio Lower Upper

164 100

162 104.9 85.4 128.2




160 47.0 39.5 59.3

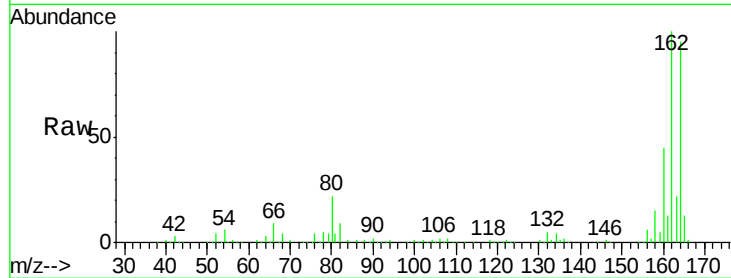

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

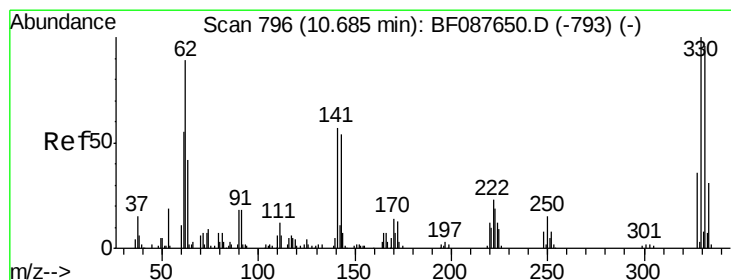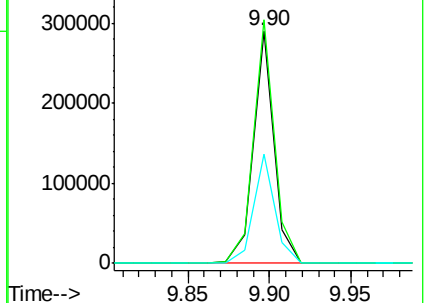

#41

2,4,6-Tribromophenol

Concen: 88.80 ng

RT: 10.68 min Scan# 796

Delta R.T. -0.00 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Tgt Ion:330 Resp: 226493

Ion Ratio Lower Upper

330 100

332 95.3 0.0 0.0#



141 39.4 0.0 0.0#

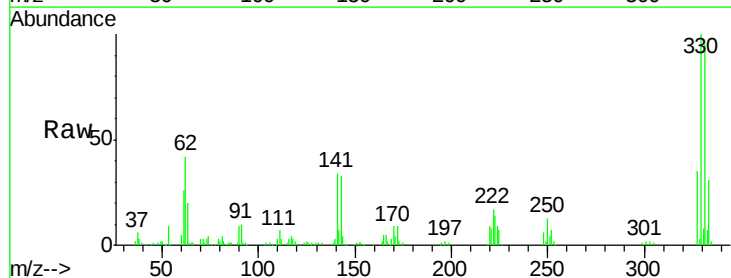


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



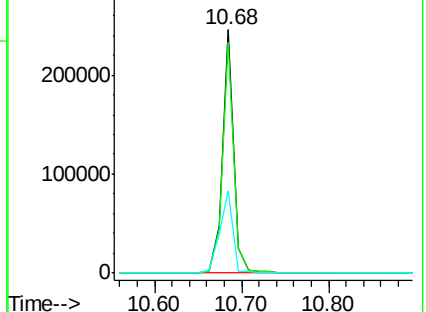



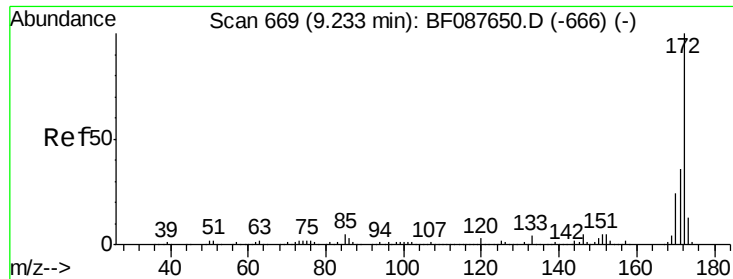

#44
 2-Fluorobiphenyl
 Concen: 49.49 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087682.D
 Acq: 5 Jun 2016 1:38




Instrument :
 BNA_F
 ClientSampleId :
 OM-SPS-002-160531


Tgt Ion:172 Resp: 929336
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.6 43.0
 170 24.0 19.2 28.8

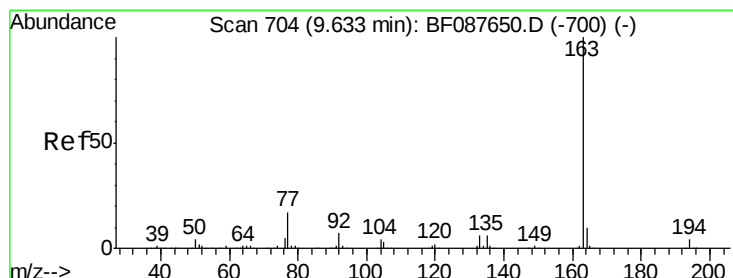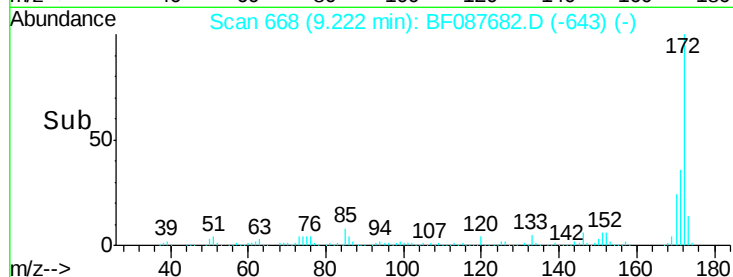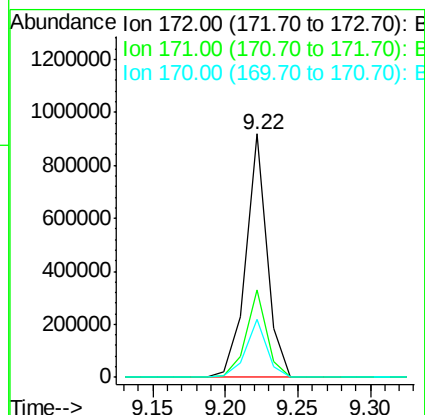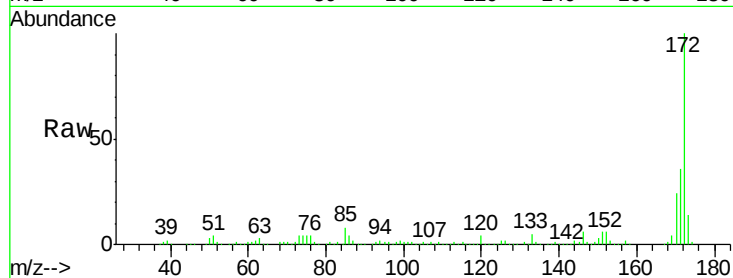

#49
 Dimethylphthalate
 Concen: 6.98 ng
 RT: 9.61 min Scan# 702
 Delta R.T. -0.02 min
 Lab File: BF087682.D
 Acq: 5 Jun 2016 1:38

Tgt Ion:163 Resp: 128868
 Ion Ratio Lower Upper
 163 100
 194 3.0 2.8 4.2
 164 11.0 8.3 12.5

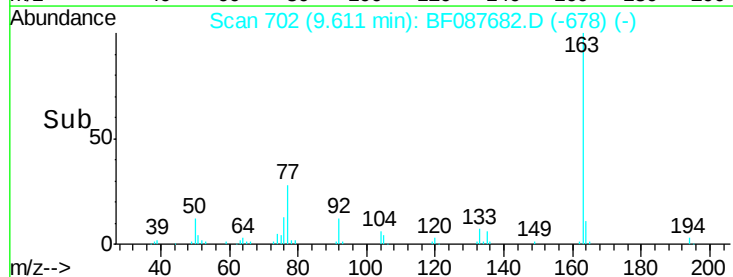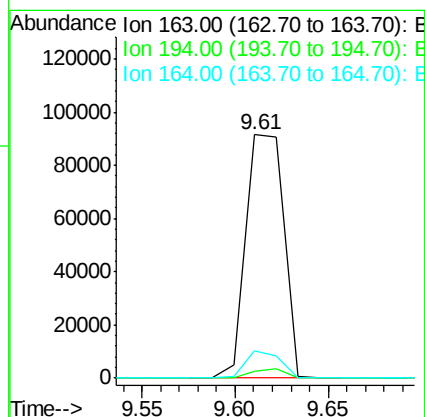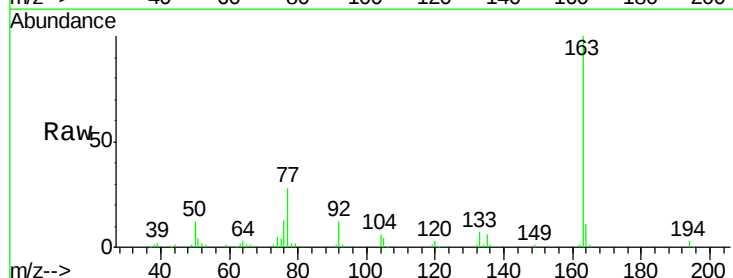

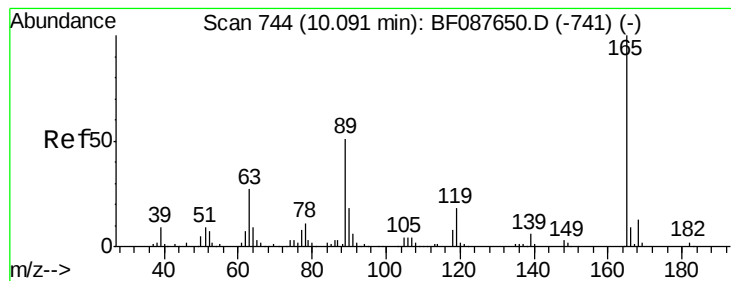

#56

2,4-Dinitrotoluene

Concen: 6.16 ng

RT: 9.90 min Scan# 727

Delta R.T. -0.19 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531

Tgt Ion:	165	Resp:	32975
Ion Ratio	Lower	Upper	
165	100		
63	1.1	22.0	33.0#
89	1.5	41.1	61.7#
182	0.0	2.0	3.0#



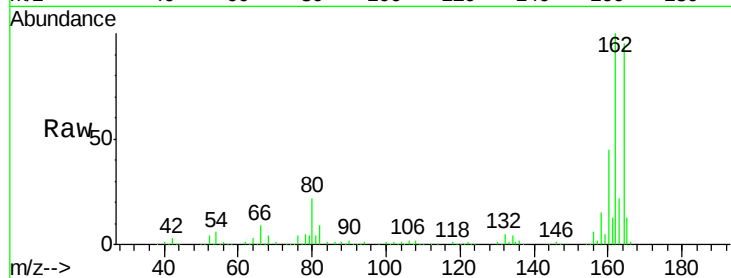


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E

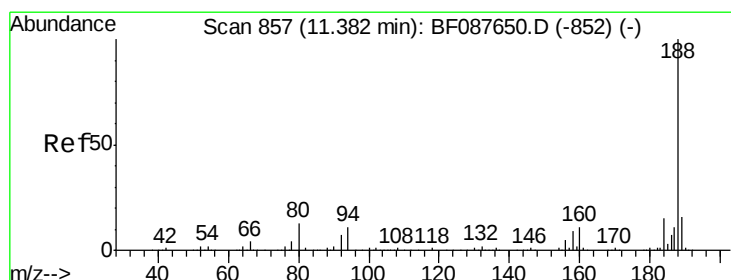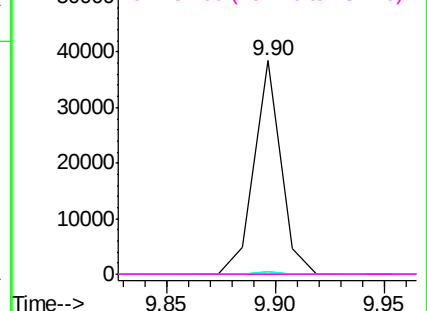

#63

Phenanthrene-d10

Concen: 20.00 ng


RT: 11.38 min Scan# 857

Delta R.T. -0.00 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38



Tgt Ion:	188	Resp:	501931
Ion Ratio	Lower	Upper	
188	100		
94	8.3	9.0	13.6#
80	8.4	10.0	15.0#

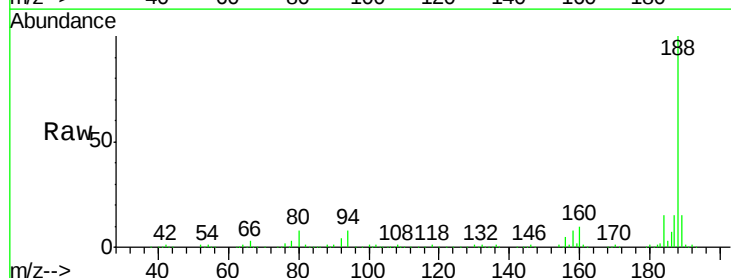


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

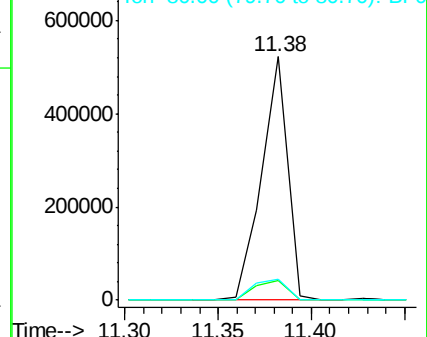

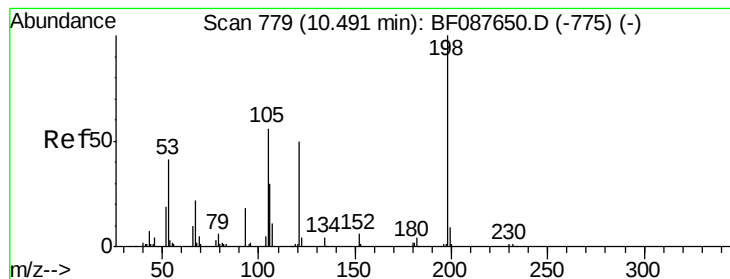

#64

4,6-Dinitro-2-methylphenol

Concen: 2.15 ng

RT: 10.68 min Scan# 796

Delta R.T. 0.19 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tgt Ion:198 Resp: 396

Ion Ratio Lower Upper

198 100

51 137.3 39.6 79.6#




105 192.5 36.6 76.6#

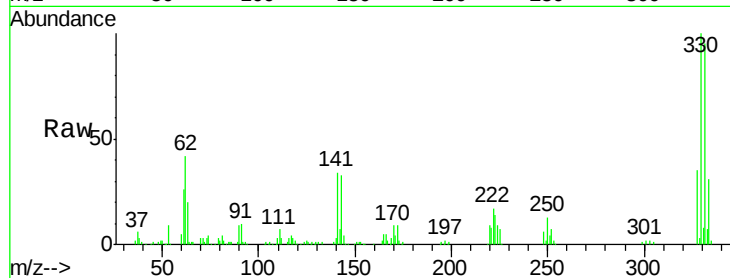

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF0

Ion 105.00 (104.70 to 105.70): E

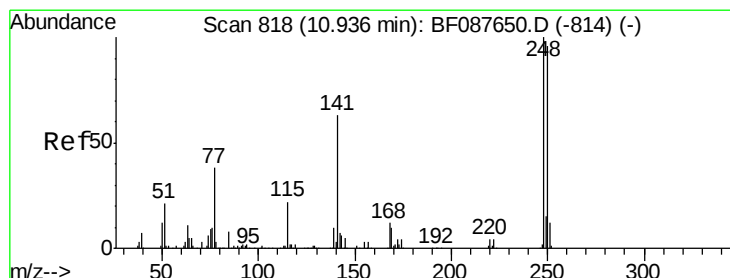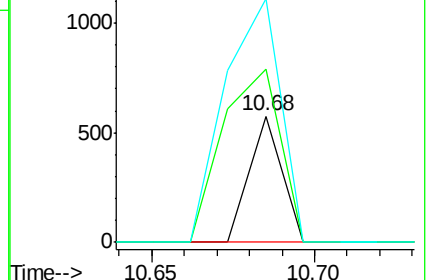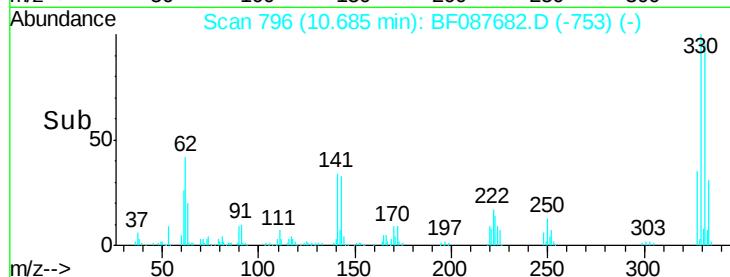

#66

4-Bromophenyl-phenylether

Concen: 2.85 ng

RT: 10.68 min Scan# 796

Delta R.T. -0.25 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Tgt Ion:248 Resp: 14203

Ion Ratio Lower Upper

248 100

250 200.7 77.1 115.7#



141 536.4 50.6 76.0#

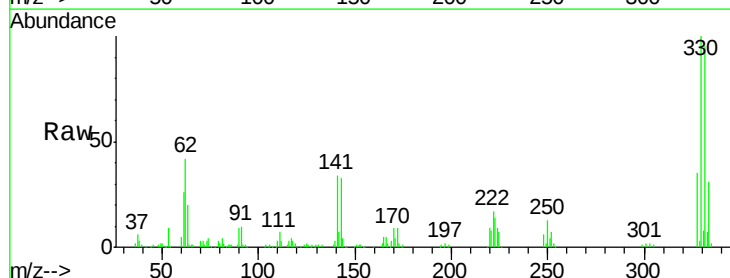


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

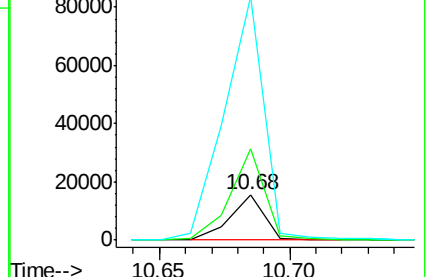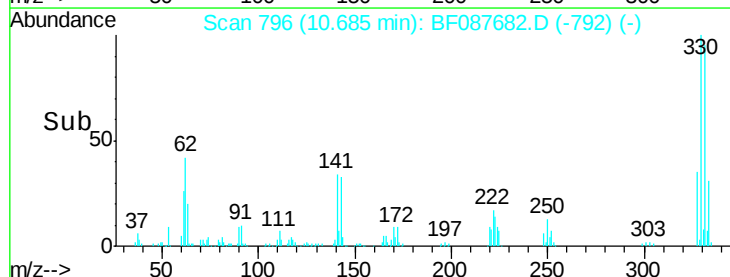

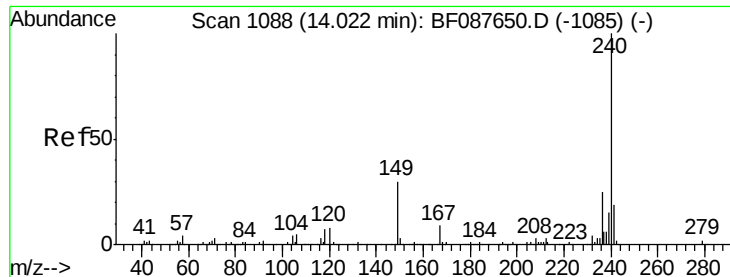

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1087

Delta R.T. -0.01 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tgt Ion:240 Resp: 407649

Ion Ratio Lower Upper

240 100

120 12.0 6.8 10.2#




236 25.8 20.2 30.2

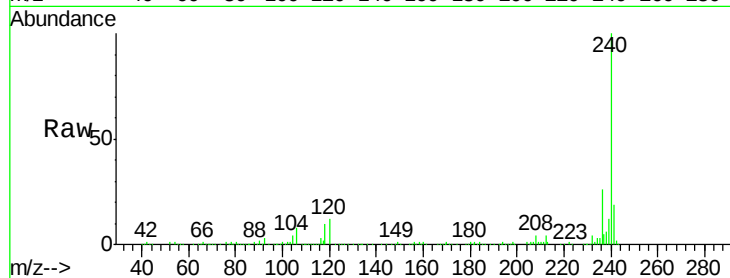

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

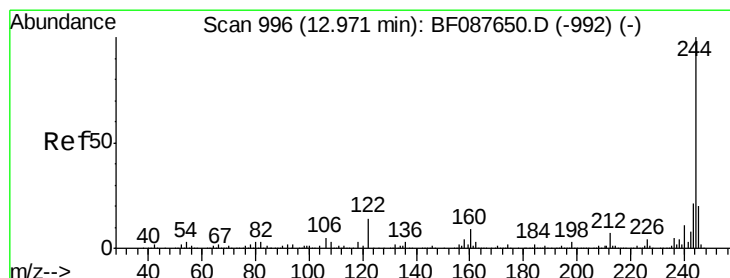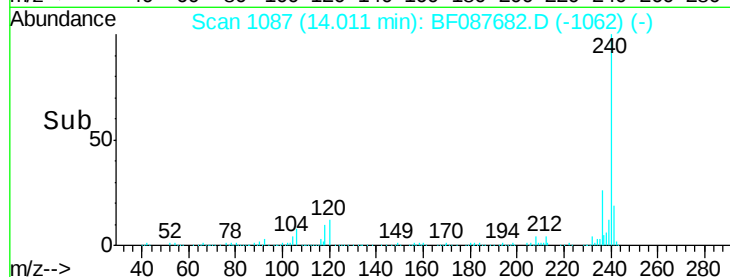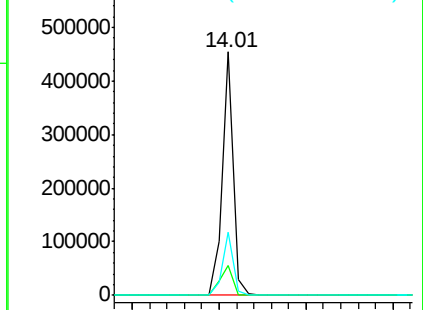

#78

Terphenyl-d14

Concen: 55.39 ng

RT: 12.97 min Scan# 996

Delta R.T. 0.00 min

Lab File: BF087682.D

Acq: 5 Jun 2016 1:38


Tgt Ion:244 Resp: 925333

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0



122 10.8 11.2 16.8#

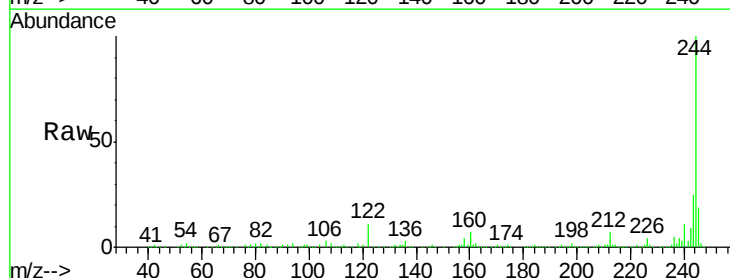


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

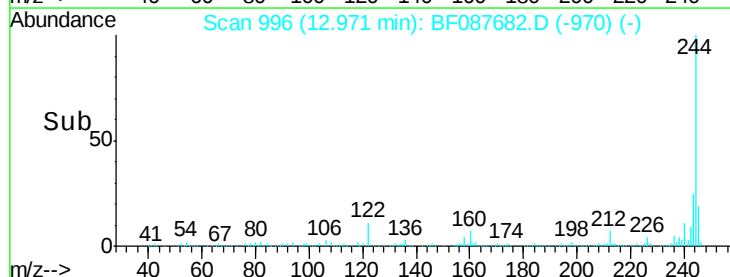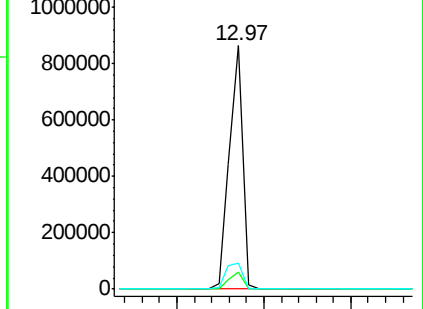


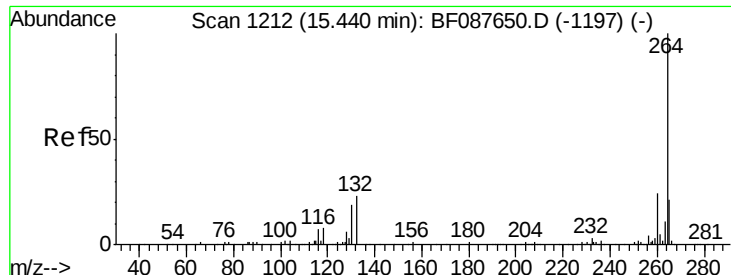

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.44 min Scan# 1212
Delta R.T. -0.00 min
Lab File: BF087682.D
Acq: 5 Jun 2016 1:38

Instrument :
BNA_F
ClientSampleId :
OM-SPS-002-160531

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.2	28.8
265	21.4	16.9	25.3

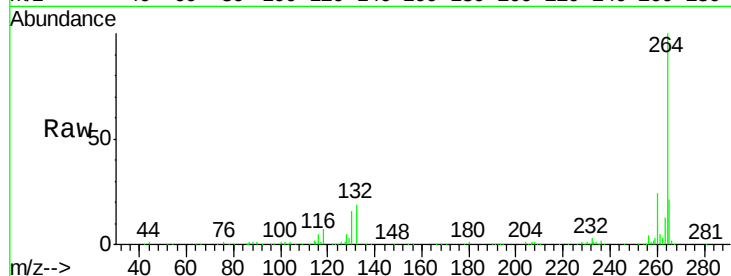

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

