

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060416\
 Data File : BF087667.D
 Acq On : 4 Jun 2016 15:44
 Operator : UM/SJ
 Sample : PB91074TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB91074TB

Quant Time: Jun 05 01:30:11 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	120184	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	499855	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	225652	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	454067	20.00	ng	0.00
75) Chrysene-d12	14.01	240	372883	20.00	ng	-0.01
86) Perylene-d12	15.44	264	289122	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	776140	104.38	ng	0.01
7) Phenol-d6	6.49	99	1114962	119.57	ng	0.00
23) Nitrobenzene-d5	7.42	82	597915	69.21	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	232700	102.73	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1077746	69.12	ng	-0.01
78) Terphenyl-d14	12.97	244	1006203	65.85	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060416\
Data File : BF087667.D
Acq On : 4 Jun 2016 15:44
Operator : UM/SJ
Sample : PB91074TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB91074TB

Quant Time: Jun 05 01:30:11 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

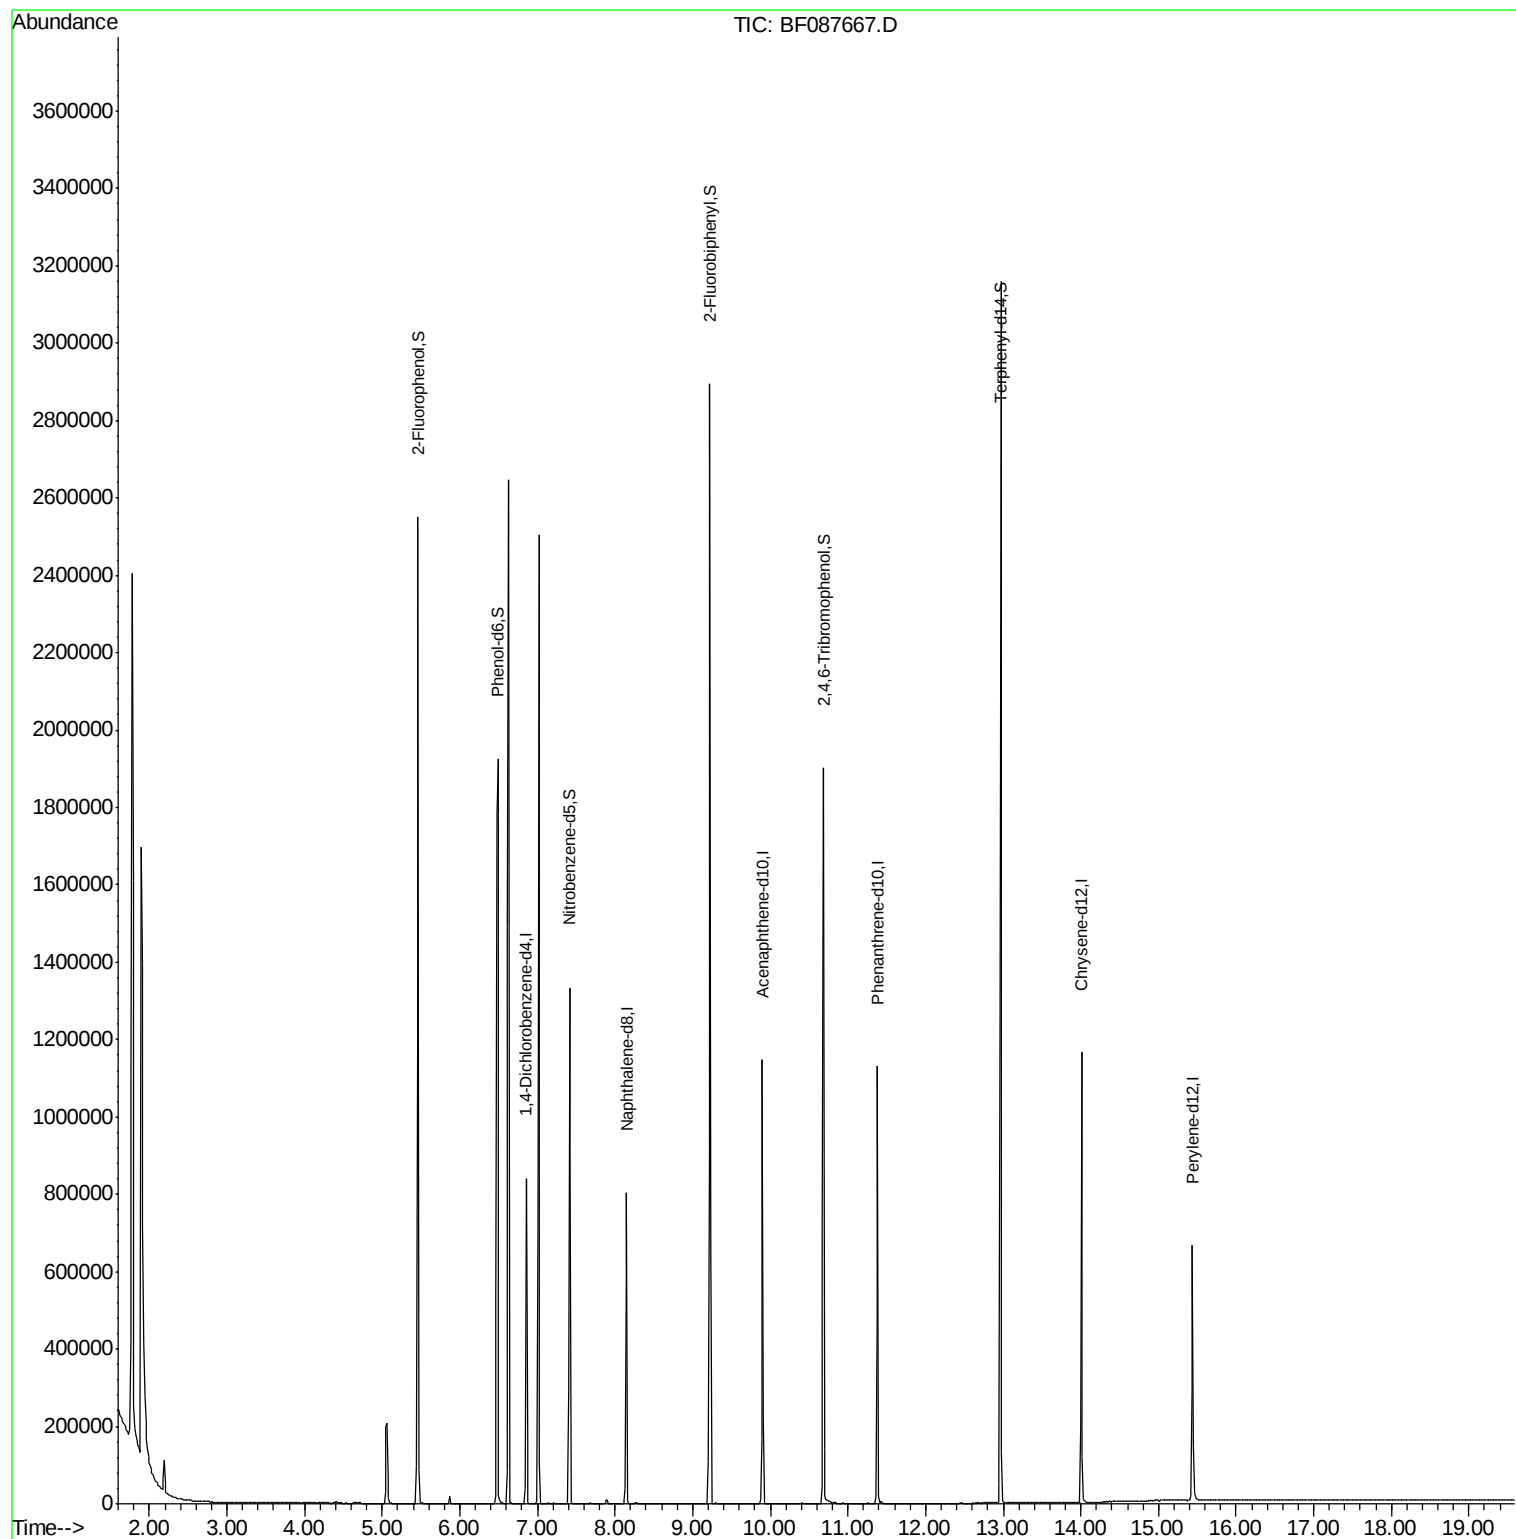

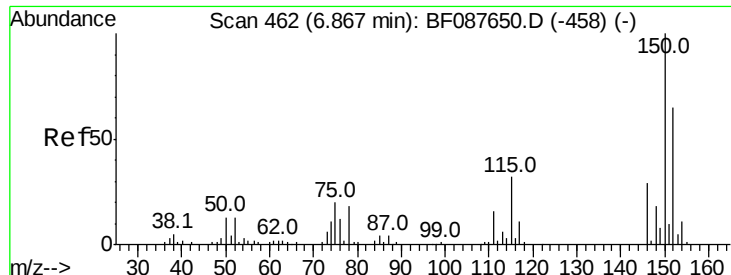

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 461

Delta R.T. -0.01 min

Lab File: BF087667.D

Acq: 4 Jun 2016 15:44

Instrument :

BNA_F

ClientSampleId :

PB91074TB


Tot Ion:152 Resp: 120184

Ion Ratio Lower Upper

152 100

150 157.6 123.8 185.6




115 64.9 39.6 59.4#

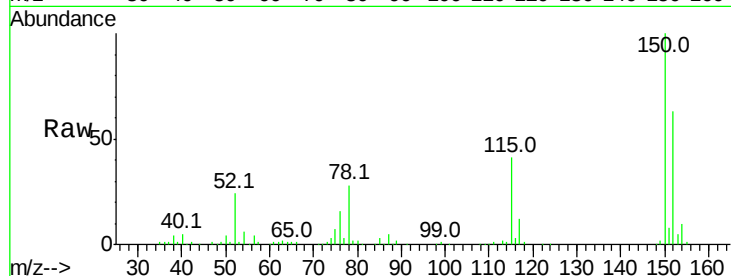

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

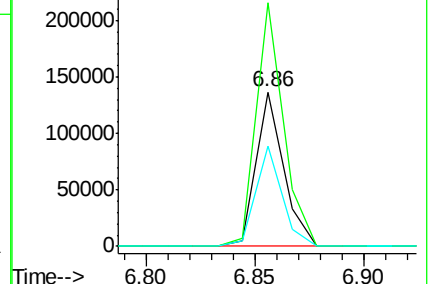

#5

2-Fluorophenol

Concen: 104.38 ng

RT: 5.46 min Scan# 339

Delta R.T. 0.01 min

Lab File: BF087667.D

Acq: 4 Jun 2016 15:44


Tgt Ion:112 Resp: 776140

Ion Ratio Lower Upper

112 100

64 57.3 42.2 63.2



63 30.7 21.8 32.8




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

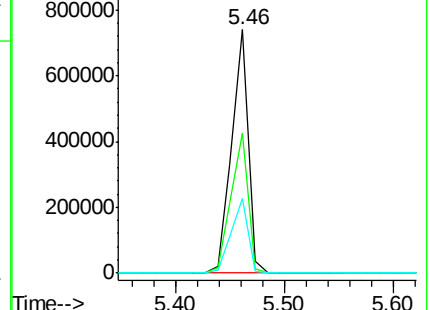

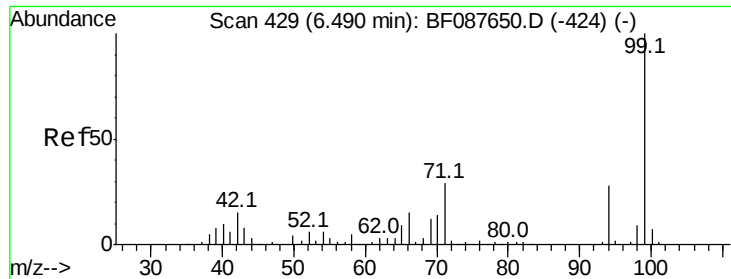

#7

Phenol-d6

Concen: 119.57 ng

RT: 6.49 min Scan# 429

Delta R.T. -0.00 min

Lab File: BF087667.D

Acq: 4 Jun 2016 15:44

Instrument :

BNA_F

ClientSampleId :

PB91074TB


Tot Ion: 99 Resp: 1114962

Ion Ratio Lower Upper

99 100

42 13.3 12.2 18.2




71 28.9 23.4 35.0

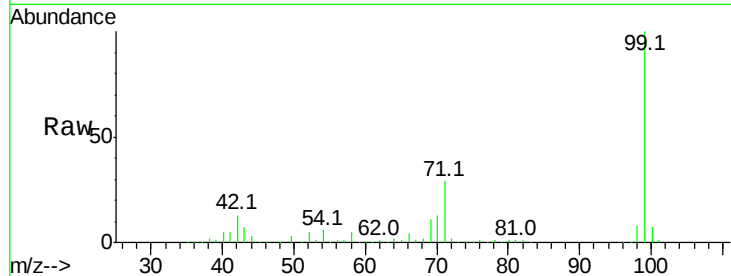

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

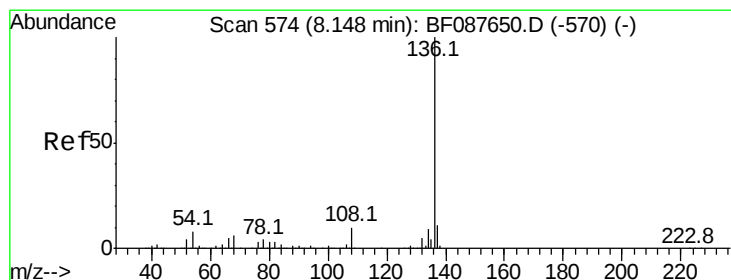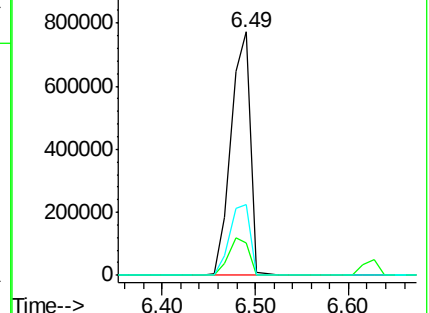

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 574

Delta R.T. -0.00 min

Lab File: BF087667.D

Acq: 4 Jun 2016 15:44

Tgt Ion: 136 Resp: 499855


Ion Ratio Lower Upper

136 100

137 10.6 9.1 13.7

54 5.9 6.6 10.0#

68 4.6 5.1 7.7#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

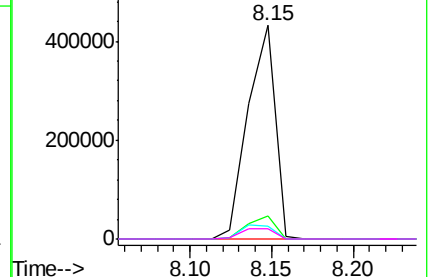


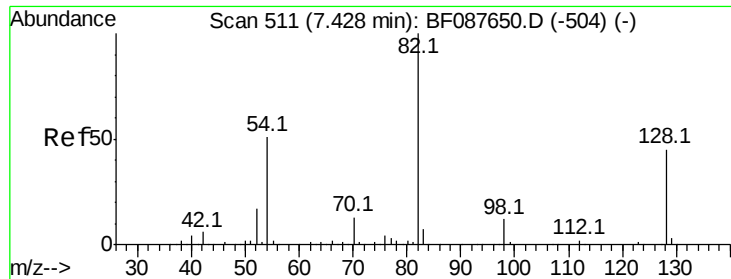




#23
 Nitrobenzene-d5
 Concen: 69.21 ng
 RT: 7.42 min Scan# 510
 Delta R.T. -0.01 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Instrument :
 BNA_F
 ClientSampleId :
 PB91074TB

Tot Ion	Ratio	Lower	Upper
82	100		
128	43.8	35.9	53.9
54	52.4	40.9	61.3

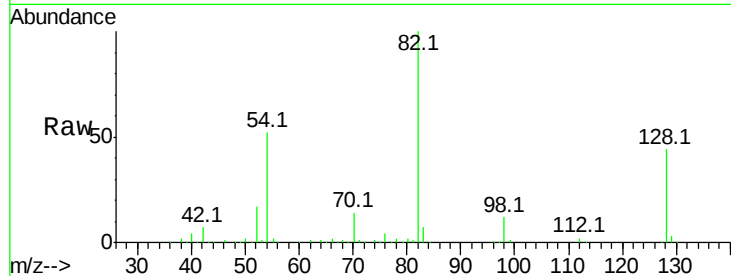


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0


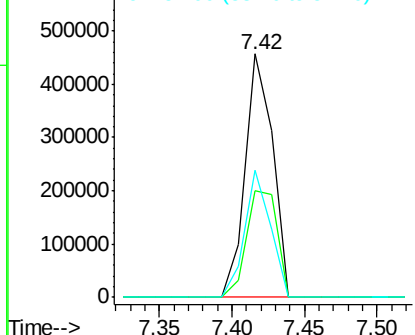



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 727
 Delta R.T. -0.01 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.6	85.4	128.2
160	47.4	39.5	59.3



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

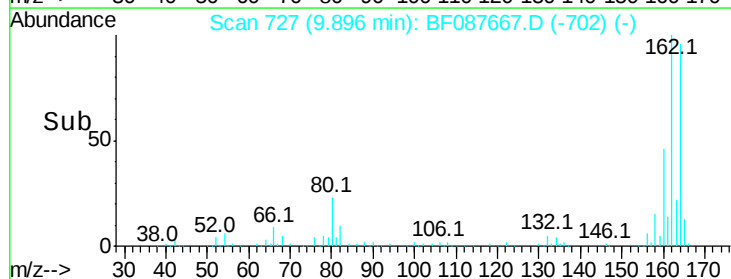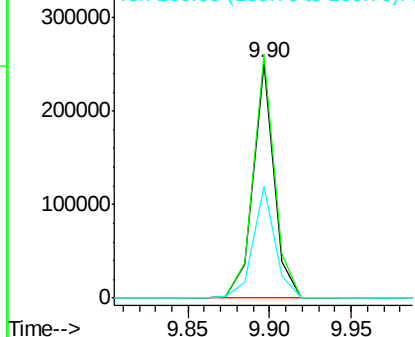


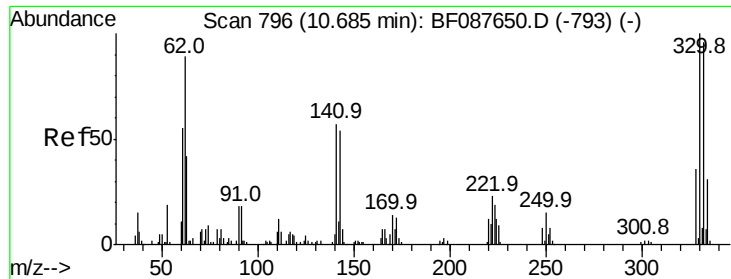




#41
 2,4,6-Tribromophenol
 Concen: 102.73 ng
 RT: 10.68 min Scan# 796
 Delta R.T. -0.00 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Instrument :
 BNA_F
 ClientSampleId :
 PB91074TB

Tot Ion:330 Resp: 232700
 Ion Ratio Lower Upper
 330 100
 332 94.5 0.0 0.0#
 141 40.8 0.0 0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

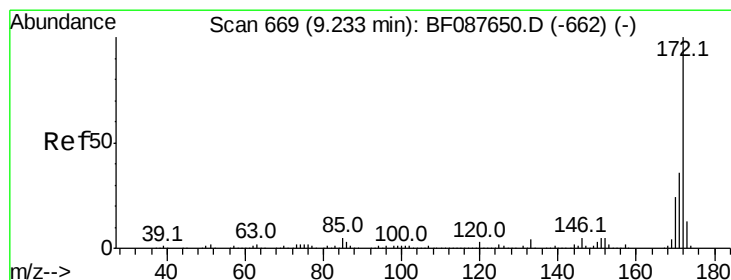
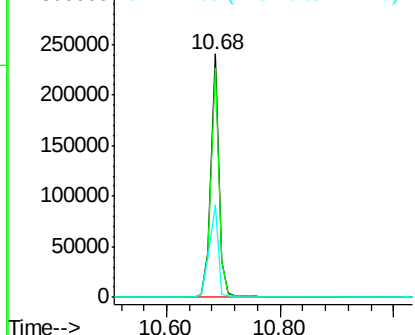



#44
 2-Fluorobiphenyl
 Concen: 69.12 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Tgt Ion:172 Resp: 1077746
 Ion Ratio Lower Upper
 172 100
 171 35.9 28.6 43.0
 170 24.1 19.2 28.8

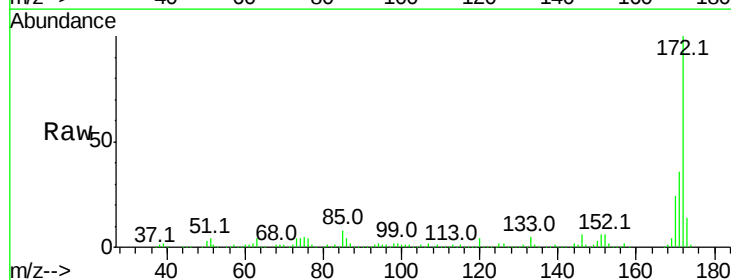

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

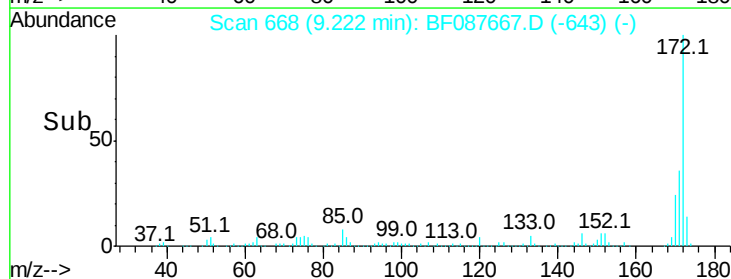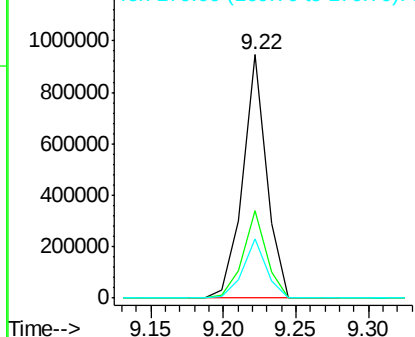







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.38 min Scan# 857
Delta R.T. -0.00 min
Lab File: BF087667.D
Acq: 4 Jun 2016 15:44

Instrument :
BNA_F
ClientSampleId :
PB91074TB

Tot Ion:188 Resp: 454067
Ion Ratio Lower Upper
188 100
94 7.9 9.0 13.6#
80 8.1 10.0 15.0#

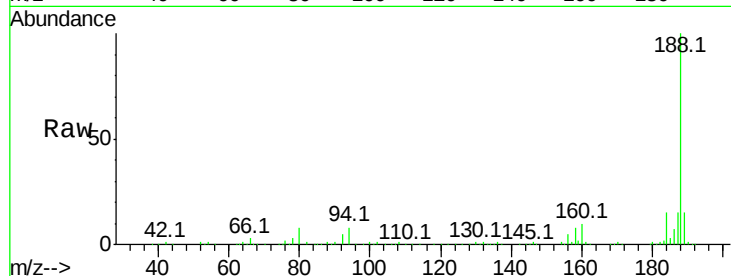


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


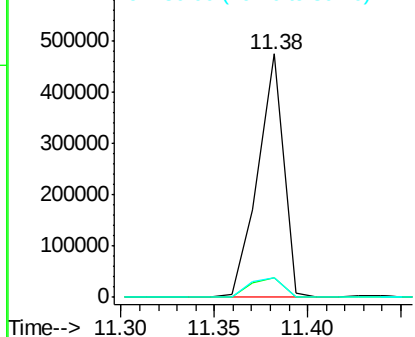



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.01 min Scan# 1087
Delta R.T. -0.01 min
Lab File: BF087667.D
Acq: 4 Jun 2016 15:44

Tgt Ion:240 Resp: 372883
Ion Ratio Lower Upper
240 100
120 13.8 6.8 10.2#
236 25.9 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

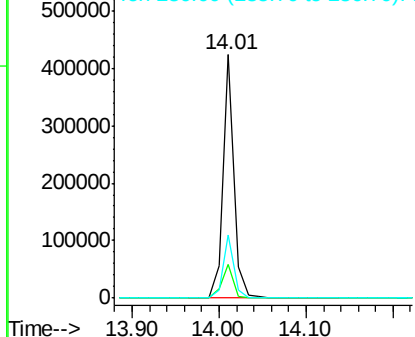







#78
 Terphenyl-d14
 Concen: 65.85 ng
 RT: 12.97 min Scan# 996
 Delta R.T. 0.00 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Instrument :
 BNA_F
 ClientSampleId :
 PB91074TB

Tot Ion:244 Resp: 1006203
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.0 9.0
 122 13.3 11.2 16.8

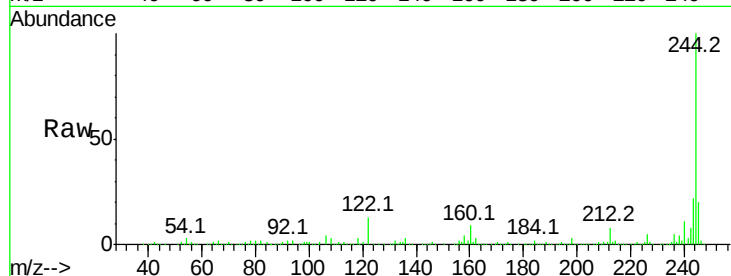


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

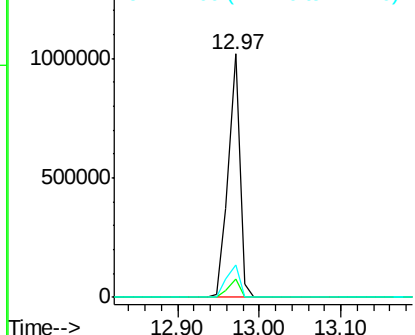

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.44 min Scan# 1212
 Delta R.T. -0.00 min
 Lab File: BF087667.D
 Acq: 4 Jun 2016 15:44

Tgt Ion:264 Resp: 289122
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.2 28.8
 265 21.7 16.9 25.3



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

