

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060416\
 Data File : BF087677.D
 Acq On : 4 Jun 2016 20:48
 Operator : UM/SJ
 Sample : H3359-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OM-SPS-002-160531

Quant Time: Jun 05 01:51:48 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	131764	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	535624	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	243735	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	489115	20.00	ng	0.00
75) Chrysene-d12	14.01	240	395060	20.00	ng	-0.01
86) Perylene-d12	15.44	264	310503	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	687473	84.33	ng	0.00
7) Phenol-d6	6.48	99	904599	88.48	ng	-0.01
23) Nitrobenzene-d5	7.42	82	535757	57.87	ng	-0.01
41) 2,4,6-Tribromophenol	10.68	330	228068	93.22	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	899311	50.01	ng	-0.01
78) Terphenyl-d14	12.97	244	913739	56.44	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.61	163	129613	7.31	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060416\
Data File : BF087677.D
Acq On : 4 Jun 2016 20:48
Operator : UM/SJ
Sample : H3359-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OM-SPS-002-160531

Quant Time: Jun 05 01:51:48 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

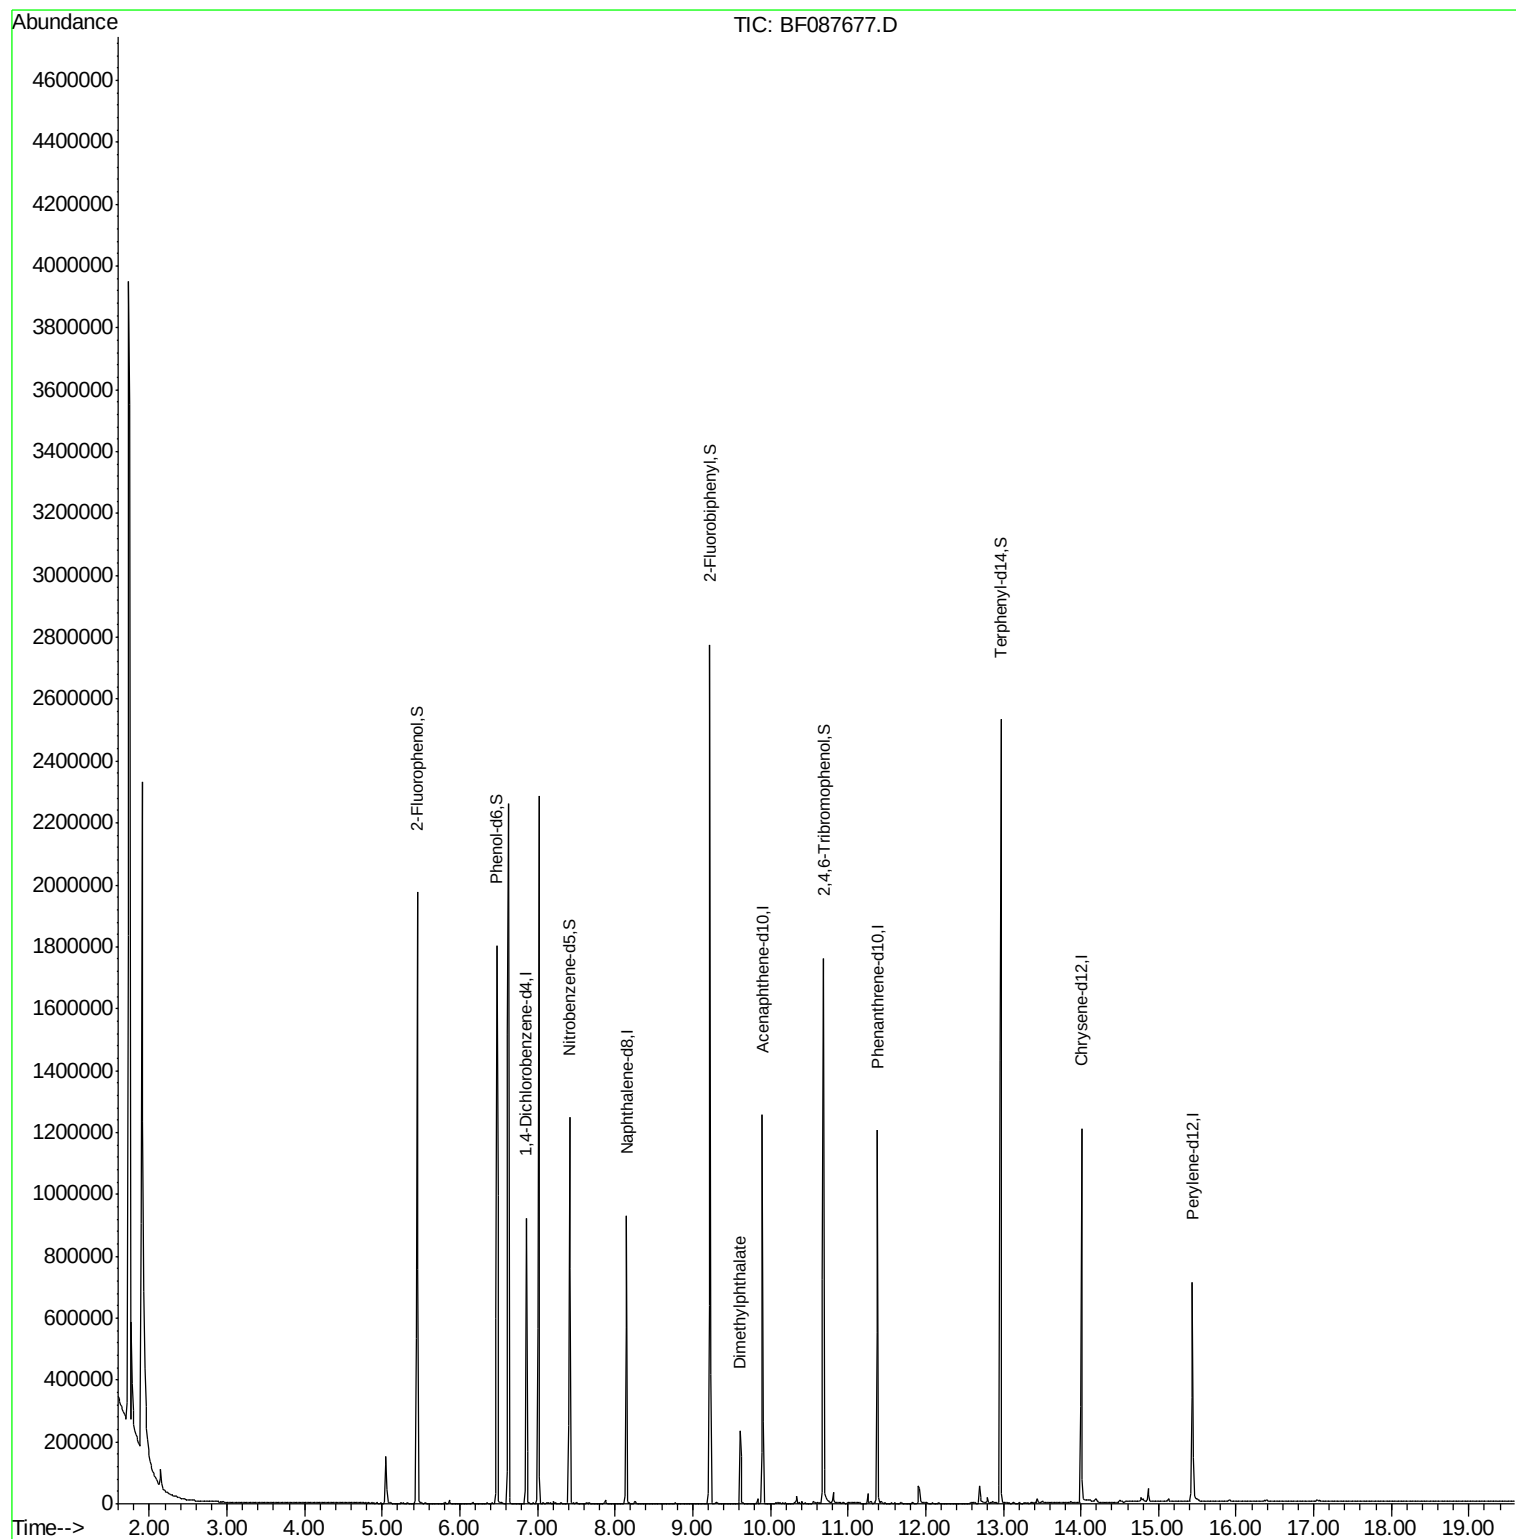

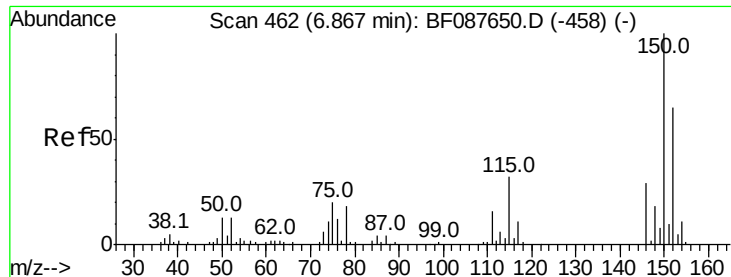

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 461

Delta R.T. -0.01 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tot Ion:152 Resp: 131764

Ion Ratio Lower Upper

152 100

150 158.5 123.8 185.6




115 64.3 39.6 59.4#

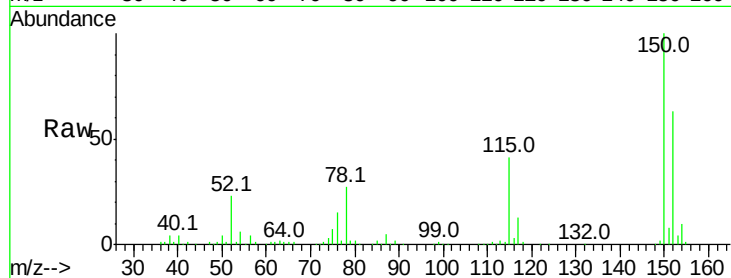

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

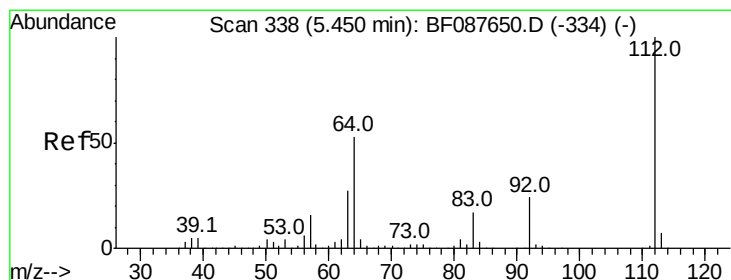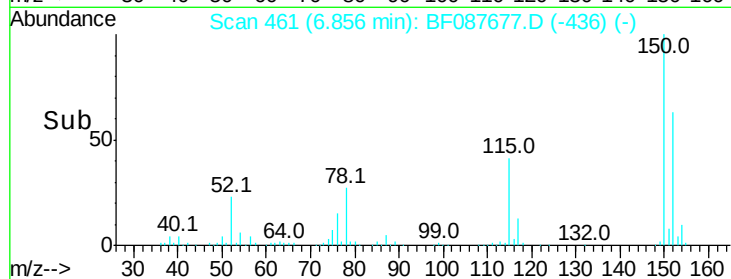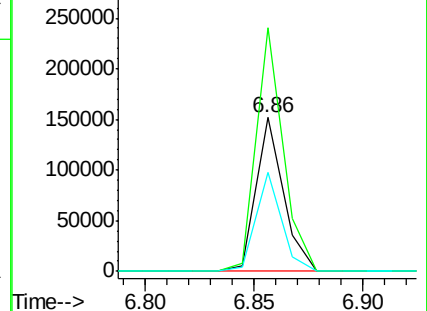

#5

2-Fluorophenol

Concen: 84.33 ng

RT: 5.45 min Scan# 338

Delta R.T. 0.00 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48


Tgt Ion:112 Resp: 687473

Ion Ratio Lower Upper

112 100

64 60.1 42.2 63.2



63 31.5 21.8 32.8

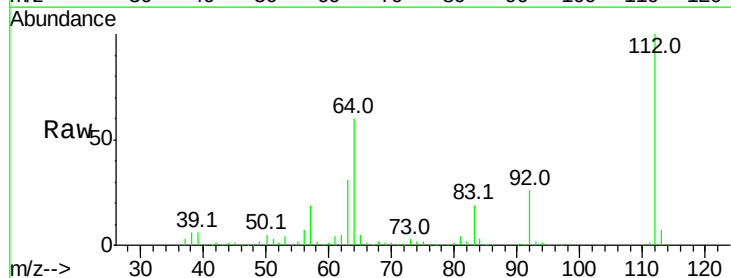


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

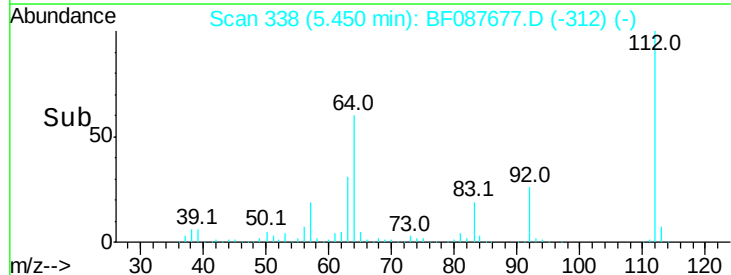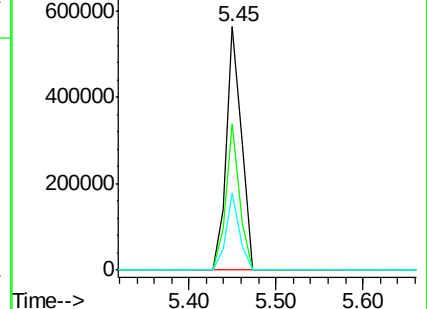

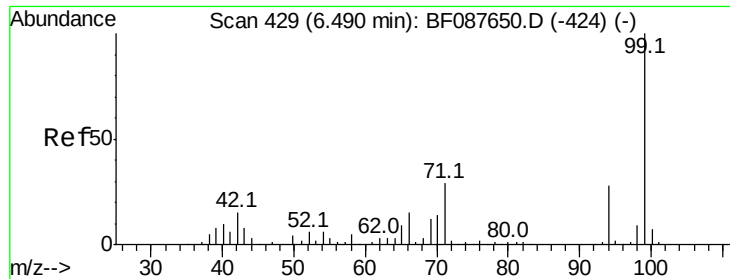

#7

Phenol-d6

Concen: 88.48 ng

RT: 6.48 min Scan# 428

Delta R.T. -0.01 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tot Ion: 99 Resp: 904599

Ion Ratio Lower Upper

99 100

42 18.7 12.2 18.2#




71 33.8 23.4 35.0

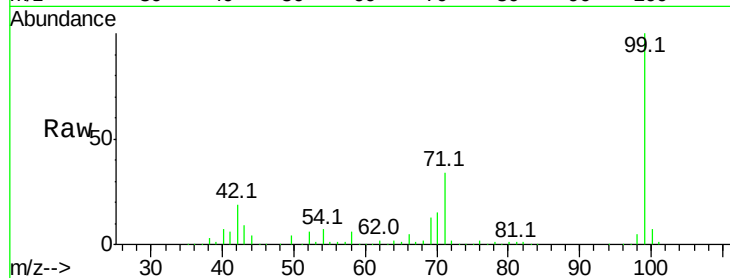

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

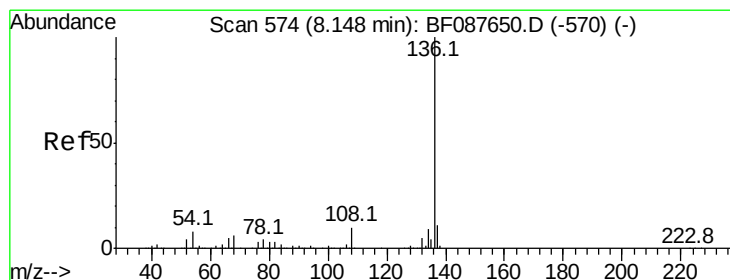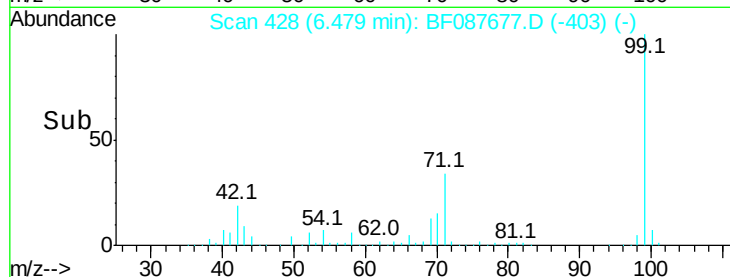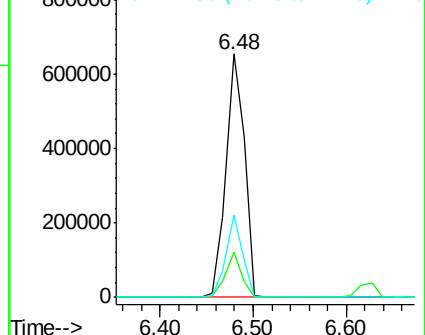

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 574

Delta R.T. 0.00 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48

Tgt Ion: 136 Resp: 535624


Ion Ratio Lower Upper

136 100

137 10.7 9.1 13.7

54 6.1 6.6 10.0#

68 5.0 5.1 7.7#


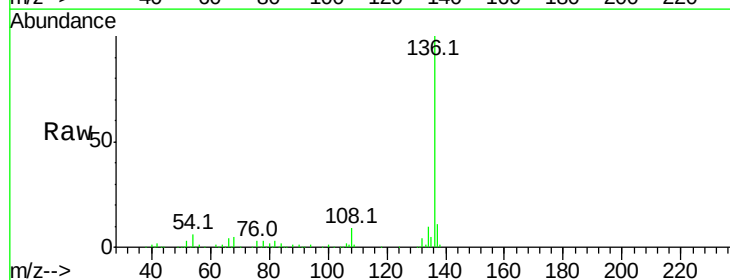



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

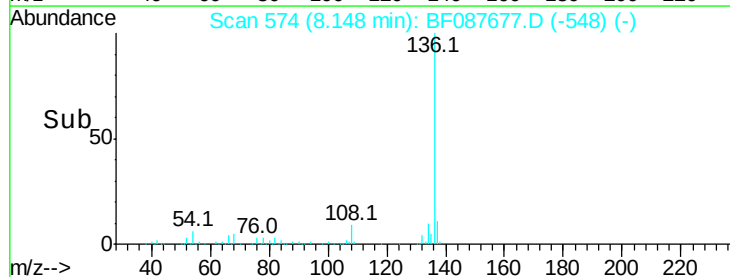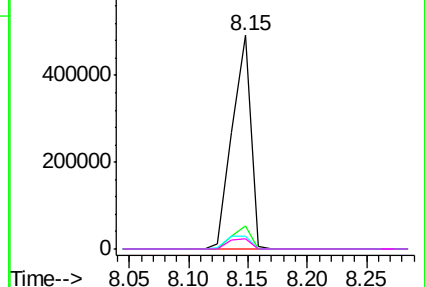


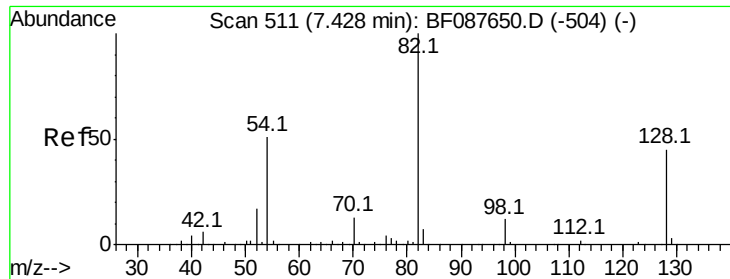




#23
 Nitrobenzene-d5
 Concen: 57.87 ng
 RT: 7.42 min Scan# 510
 Delta R.T. -0.01 min
 Lab File: BF087677.D
 Acq: 4 Jun 2016 20:48

Instrument :
 BNA_F
 ClientSampleId :
 OM-SPS-002-160531

Tot Ion	Ratio	Lower	Upper
82	100		
128	43.7	35.9	53.9
54	52.2	40.9	61.3

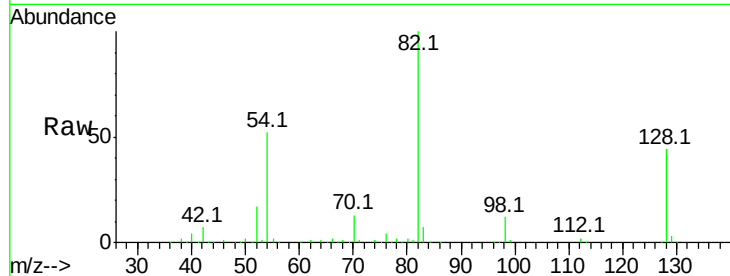


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

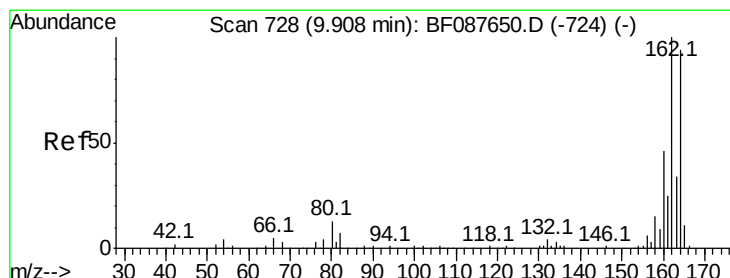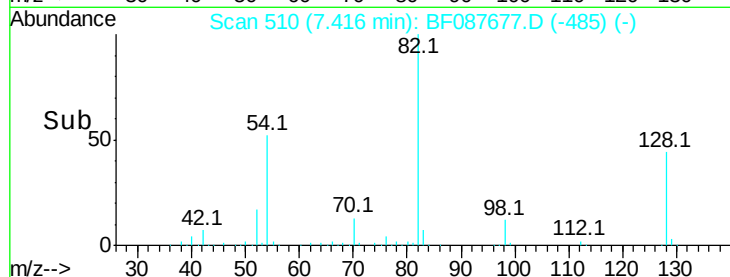
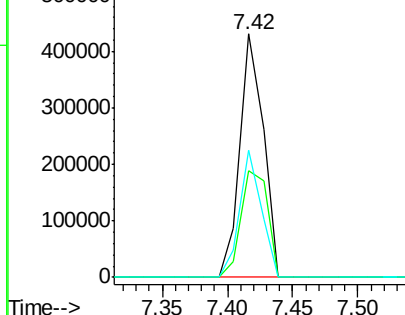



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 727
 Delta R.T. -0.01 min
 Lab File: BF087677.D
 Acq: 4 Jun 2016 20:48

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.4	85.4	128.2
160	46.6	39.5	59.3

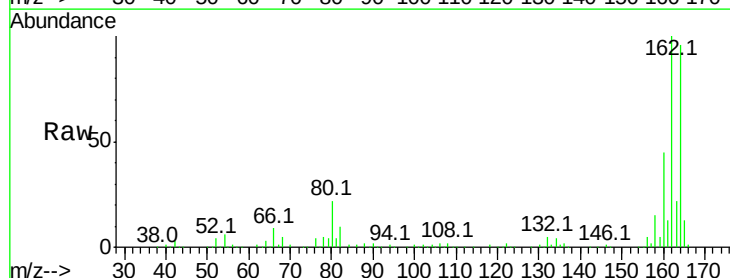

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

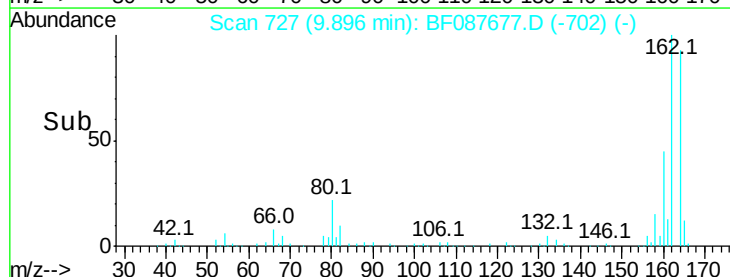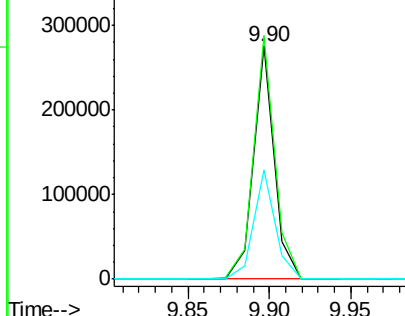


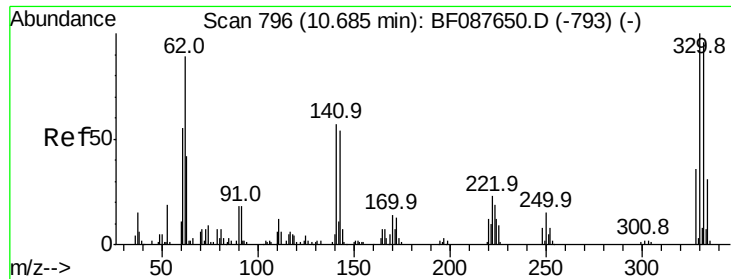




#41
 2,4,6-Tribromophenol
 Concen: 93.22 ng
 RT: 10.68 min Scan# 796
 Delta R.T. -0.00 min
 Lab File: BF087677.D
 Acq: 4 Jun 2016 20:48

Instrument :
 BNA_F
 ClientSampleId :
 OM-SPS-002-160531

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	0.0	0.0#
141	39.0	0.0	0.0#

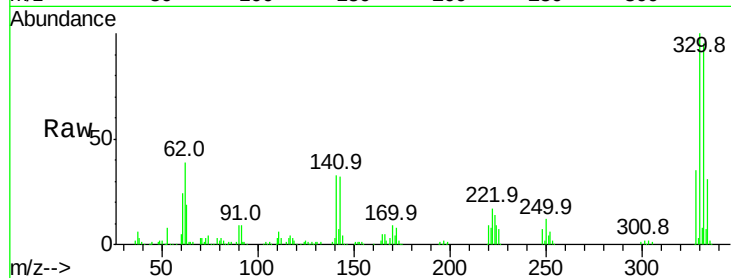


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

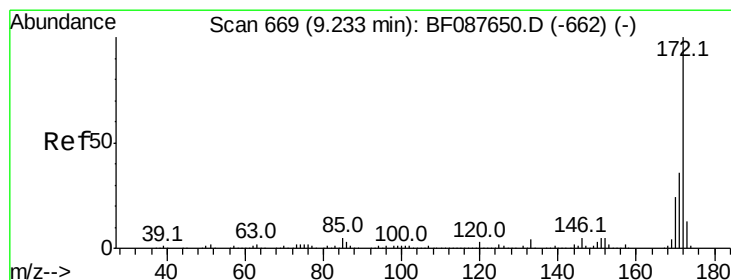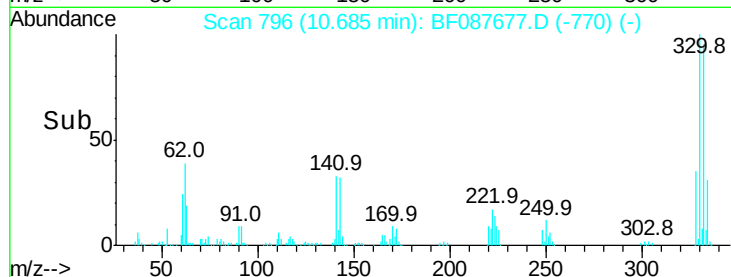
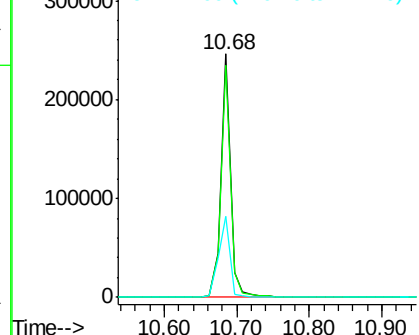



#44
 2-Fluorobiphenyl
 Concen: 50.01 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087677.D
 Acq: 4 Jun 2016 20:48

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.6	43.0
170	24.3	19.2	28.8

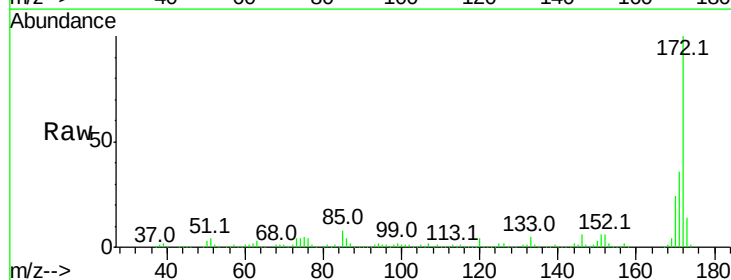

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

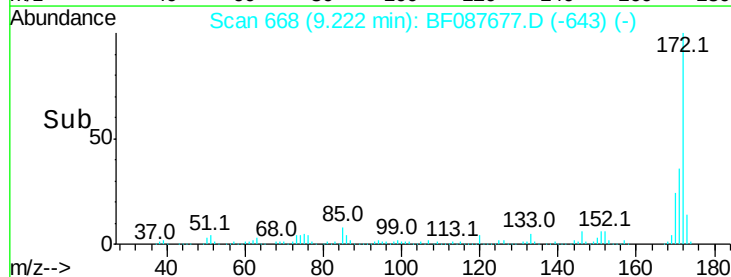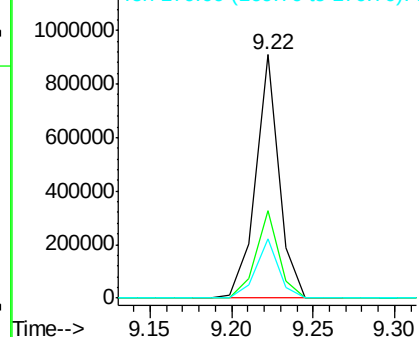


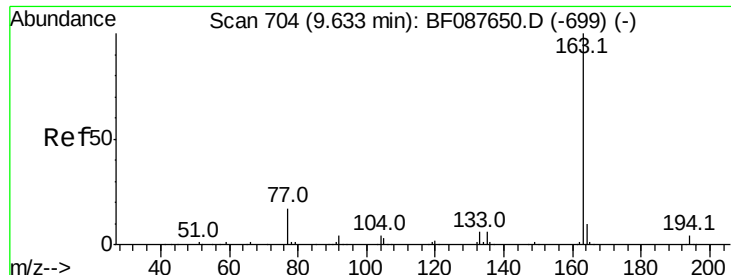




#49
Dimethylphthalate
Concen: 7.31 ng
RT: 9.61 min Scan# 702
Delta R.T. -0.02 min
Lab File: BF087677.D
Acq: 4 Jun 2016 20:48

Instrument :
BNA_F
ClientSampleId :
OM-SPS-002-160531

Tot Ion:163 Resp: 129613
Ion Ratio Lower Upper
163 100
194 2.8 2.8 4.2
164 10.4 8.3 12.5

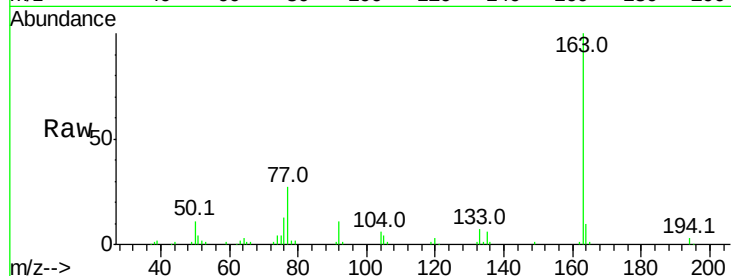


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

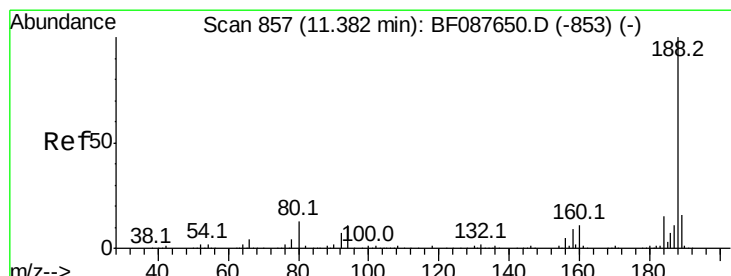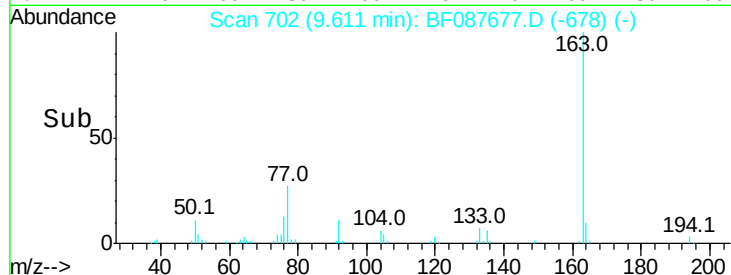
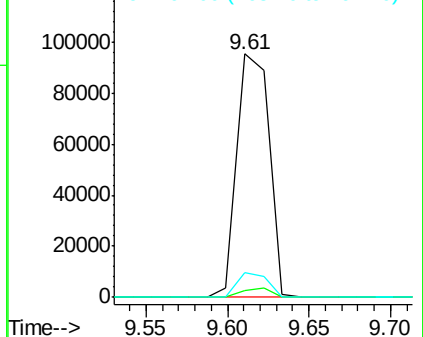



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.38 min Scan# 857
Delta R.T. -0.00 min
Lab File: BF087677.D
Acq: 4 Jun 2016 20:48

Tgt Ion:188 Resp: 489115
Ion Ratio Lower Upper
188 100
94 8.3 9.0 13.6#
80 8.3 10.0 15.0#

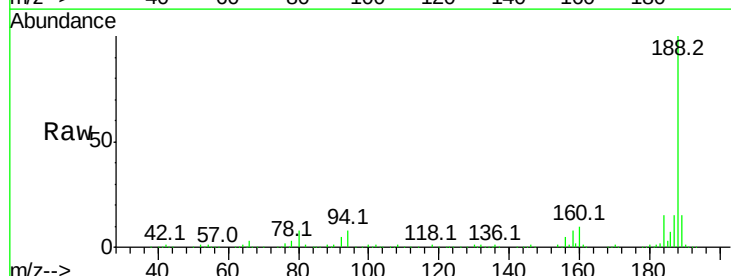

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

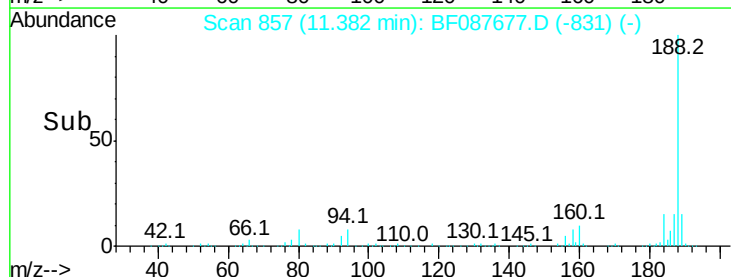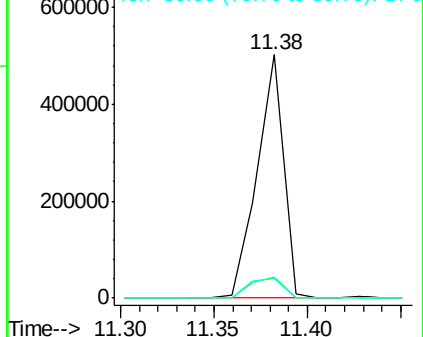

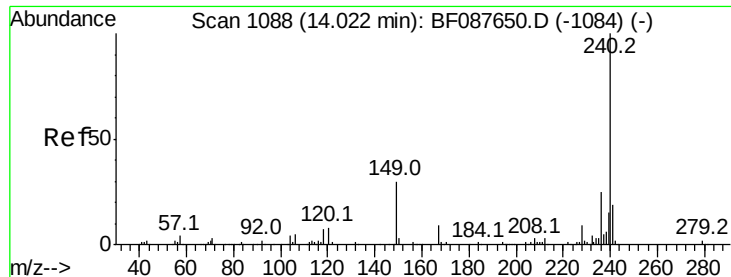

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1087

Delta R.T. -0.01 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48

Instrument :

BNA_F

ClientSampleId :

OM-SPS-002-160531


Tot Ion:240 Resp: 395060

Ion Ratio Lower Upper

240 100

120 12.5 6.8 10.2#




236 25.8 20.2 30.2

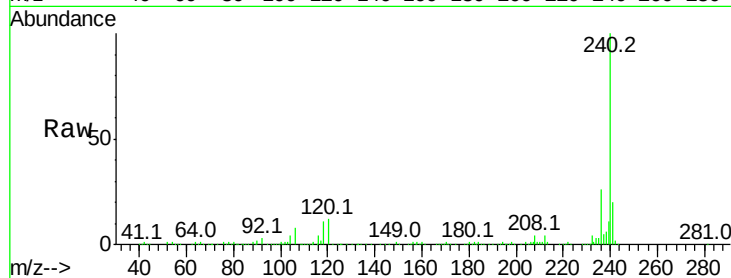

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

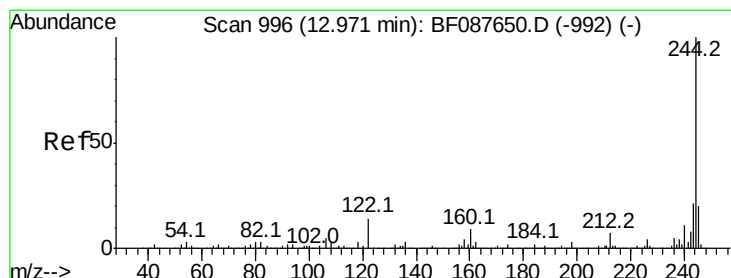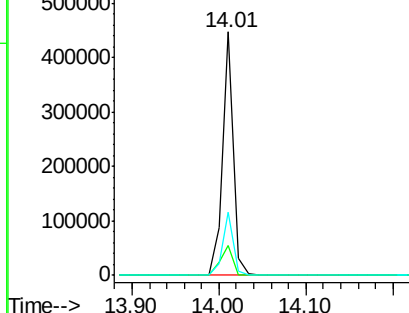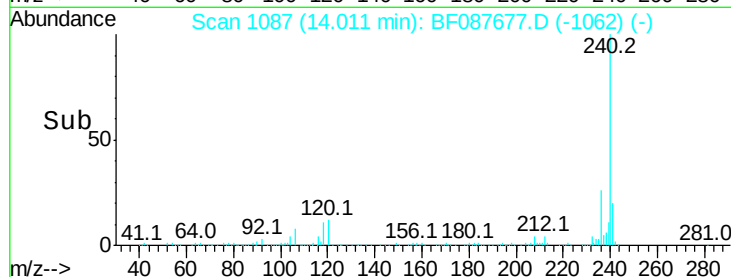

#78

Terphenyl-d14

Concen: 56.44 ng

RT: 12.97 min Scan# 996

Delta R.T. 0.00 min

Lab File: BF087677.D

Acq: 4 Jun 2016 20:48


Tgt Ion:244 Resp: 913739

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0



122 10.8 11.2 16.8#

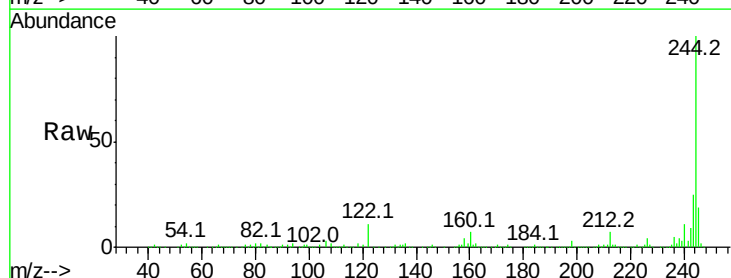


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

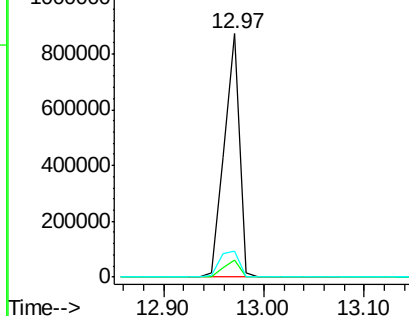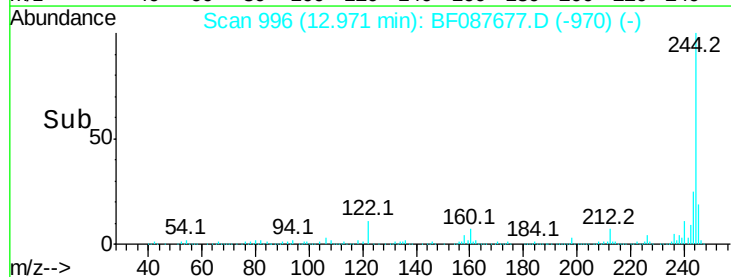


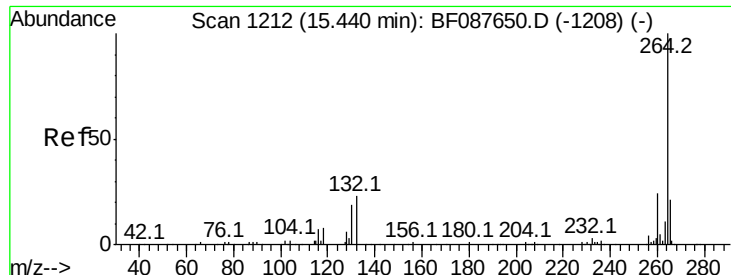

#86
Pervlène-d12
Concen: 20.00 ng
RT: 15.44 min Scan# 1212
Delta R.T. -0.00 min
Lab File: BF087677.D
Acq: 4 Jun 2016 20:48

Instrument :
BNA_F
ClientSampleId :
OM-SPS-002-160531

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.2	28.8
265	21.4	16.9	25.3

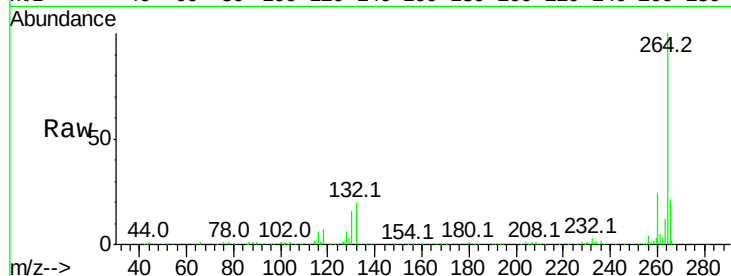

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

