


Data Path : Z:\HPCHEM1\BNA F\Data\BF060416\
 Data File : BF087646.D
 Acq On : 4 Jun 2016 2:22
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jun 04 11:07:28 2016

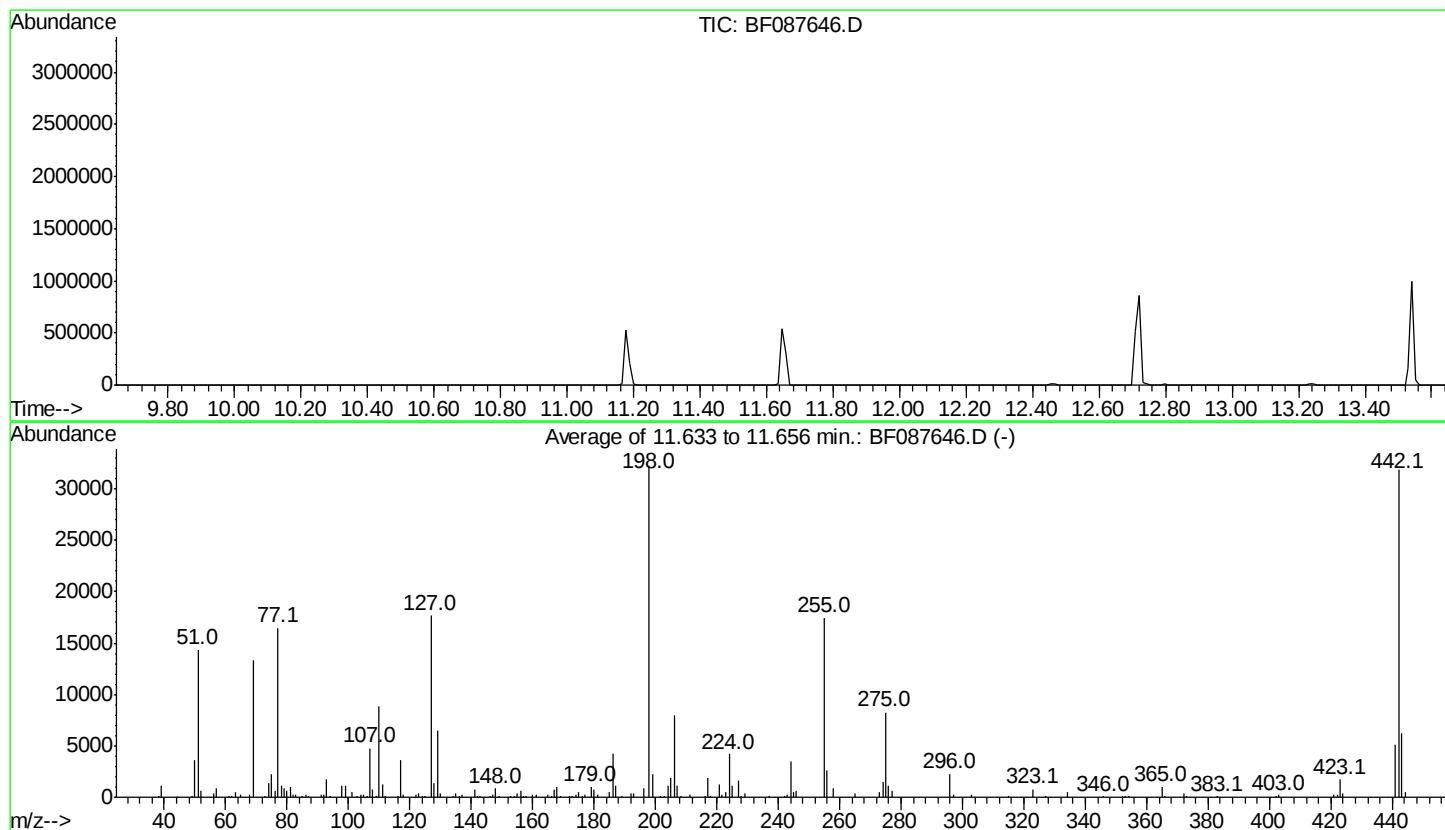

AutoFind: Scans 879, 880, 881; Background Corrected with Scan 876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	14323	PASS
68	69	0.00	2	1.6	211	PASS
69	198	0.00	100	41.4	13355	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.8	17676	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32248	PASS
199	198	5	9	7.0	2255	PASS
275	198	10	60	25.5	8235	PASS
365	198	1	100	3.3	1063	PASS
441	442	0.01	24	16.0	5104	PASS
442	198	50	100	98.8	31852	PASS
443	442	15	24	19.5	6213	PASS