
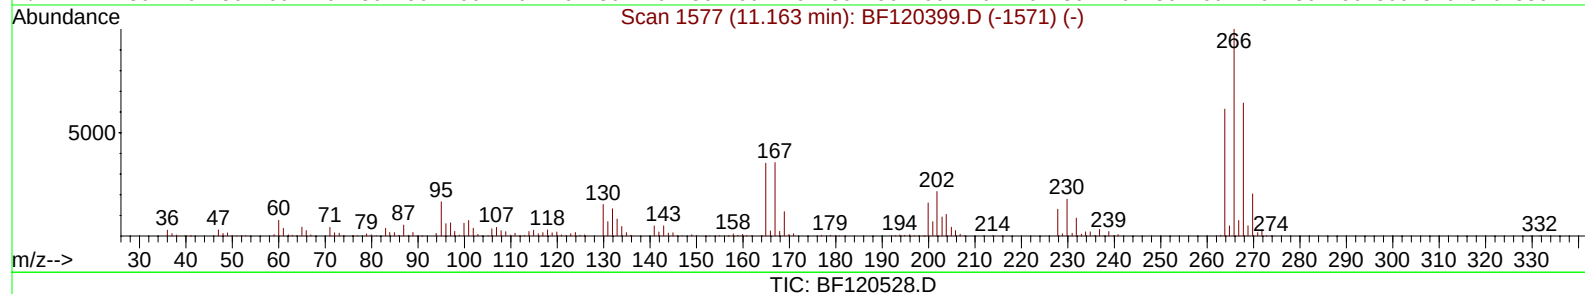
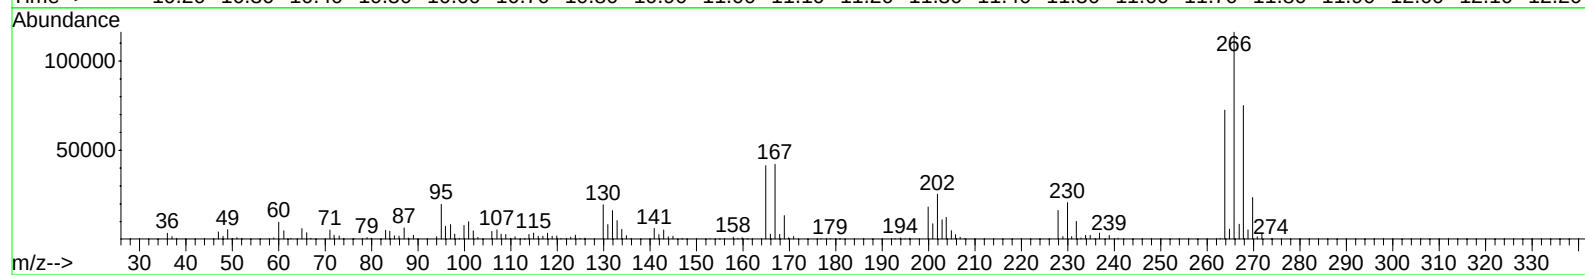


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF060420\  
 Data File : BF120528.D  
 Acq On : 4 Jun 2020 12:41  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 14:36:45 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jun 03 14:26:17 2020  
 Response via : Initial Calibration

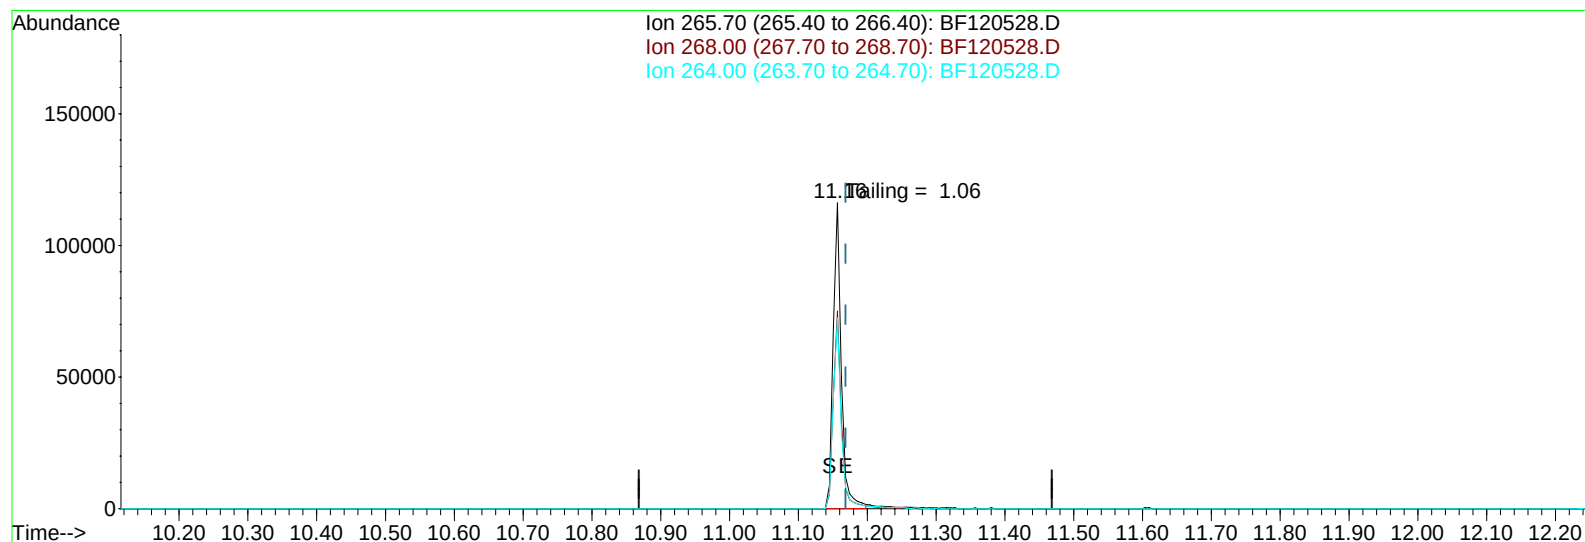

(70) Pentachlorophenol (C)




11.157min (-0.012) 37798.57ng

response 98627

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.80 | 64.63 |
| 264.00 | 63.80 | 62.44 |
| 0.00   | 0.00  | 0.00  |

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF060420\  
Data File   : BF120528.D  
Acq On      : 4 Jun 2020 12:41  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jun 04 14:36:45 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 03 14:26:17 2020  
Response via : Initial Calibration

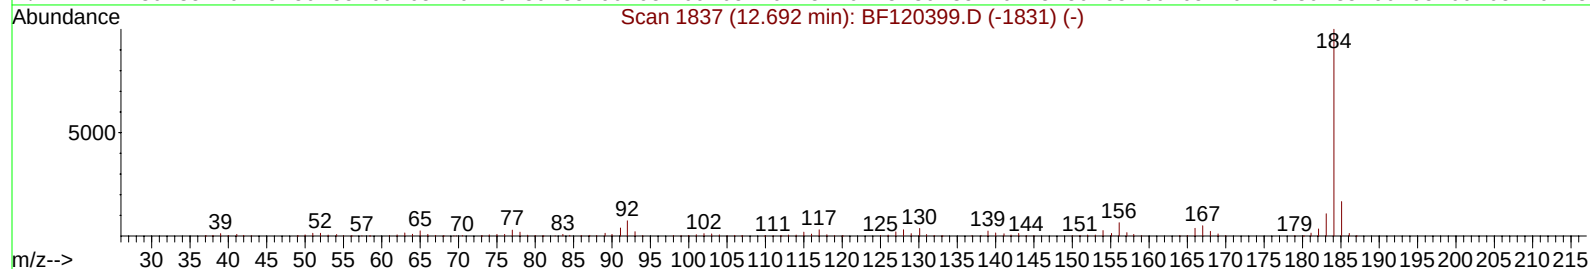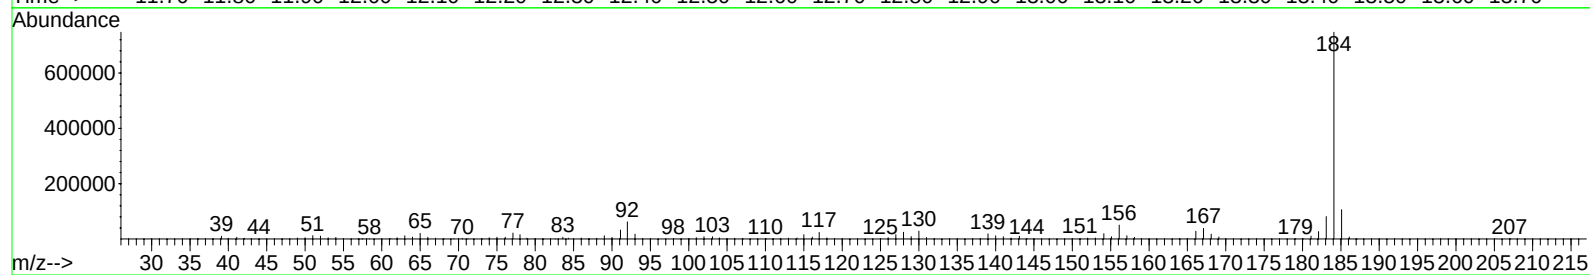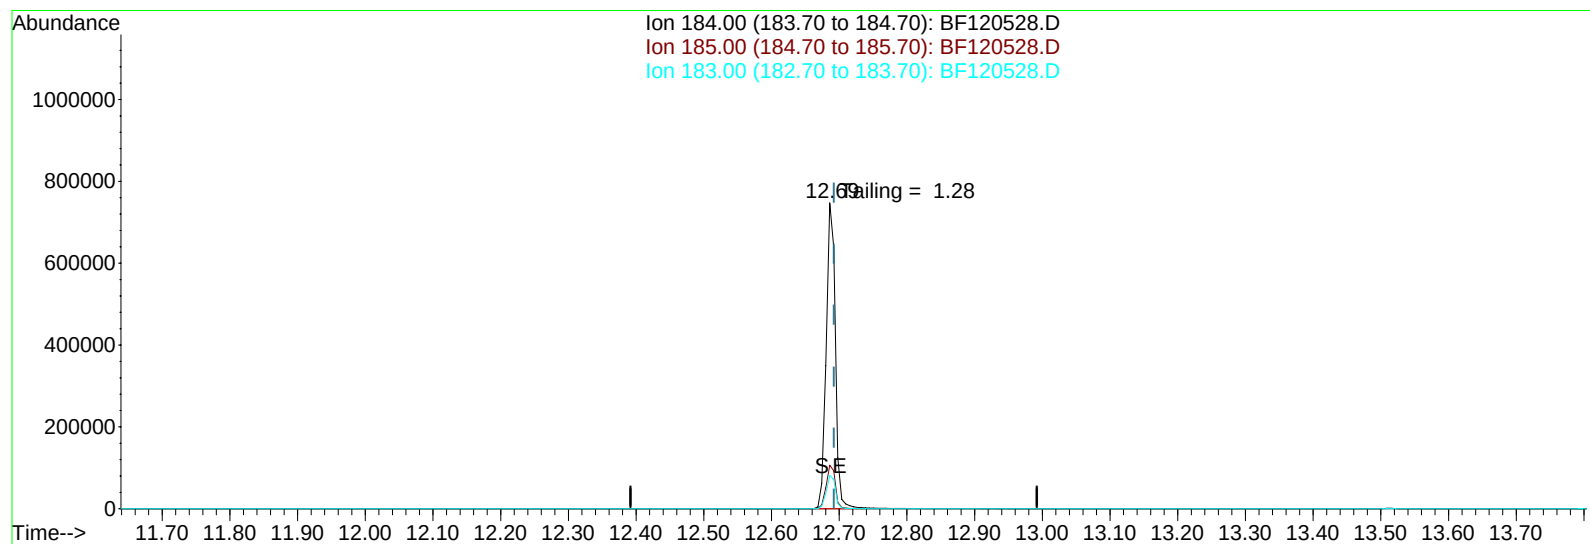

TIC: BF120528.D

(77) Benzidine

12.686min (-0.006) 0.00ng

response 703690

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.50 | 14.21 |
| 183.00 | 11.40 | 10.85 |
| 0.00   | 0.00  | 0.00  |