
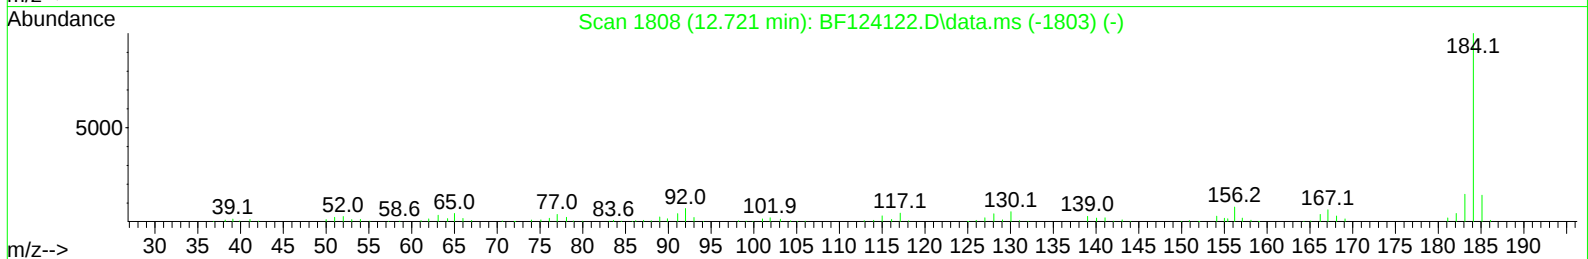
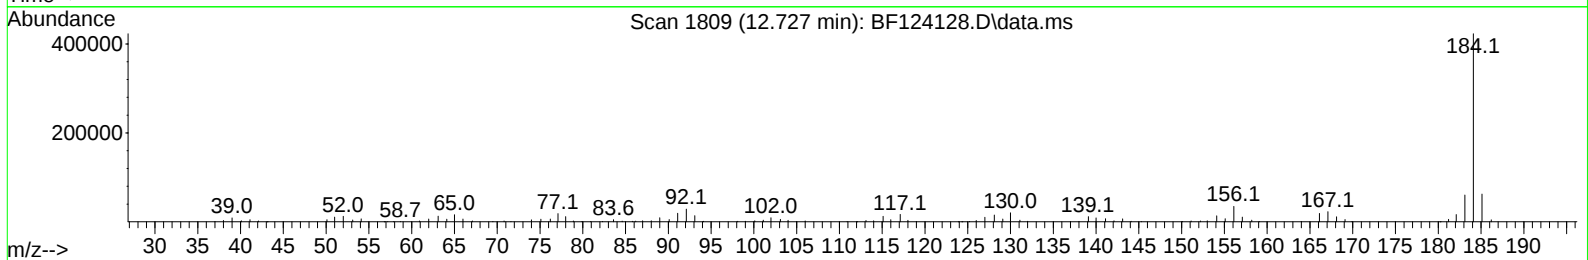


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
 Data File : BF124128.D
 Acq On : 4 Jun 2021 8:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 10:48:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 04 09:56:24 2021
 Response via : Initial Calibration

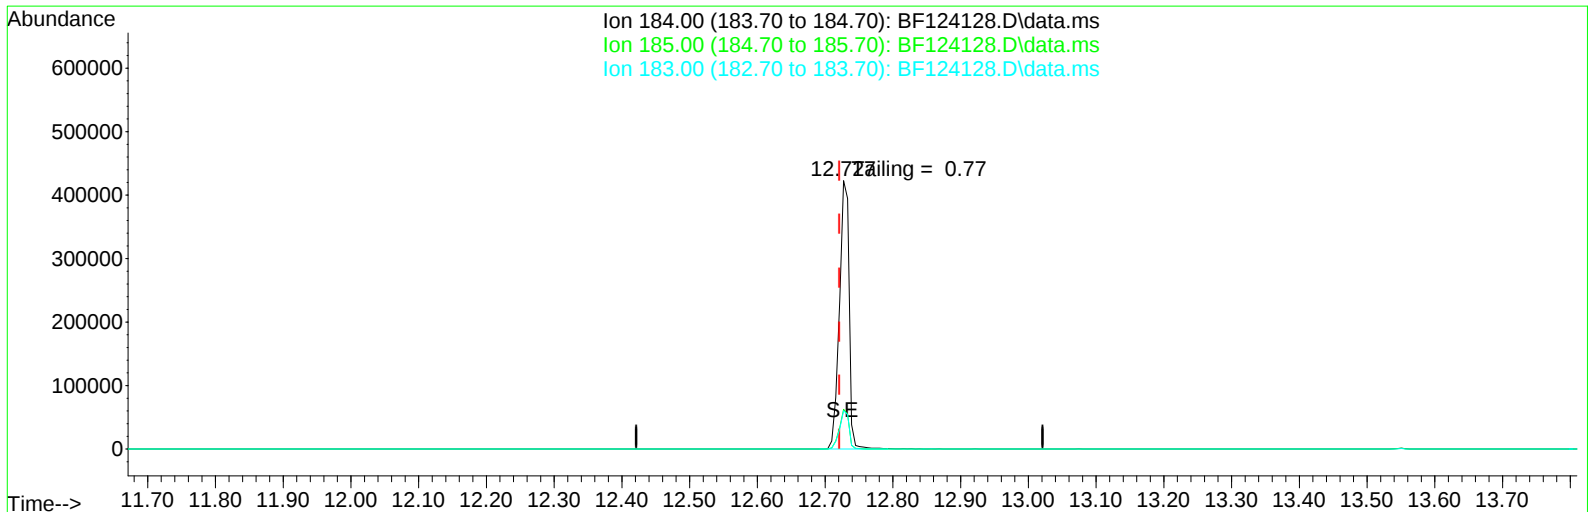

TIC: BF124128.D\data.ms

(77) Benzidine




12.727min (+ 0.006) 0.00 ng

response 425362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.82
183.00	9.80	14.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124128.D
Acq On : 4 Jun 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 04 10:48:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 04 09:56:24 2021
Response via : Initial Calibration

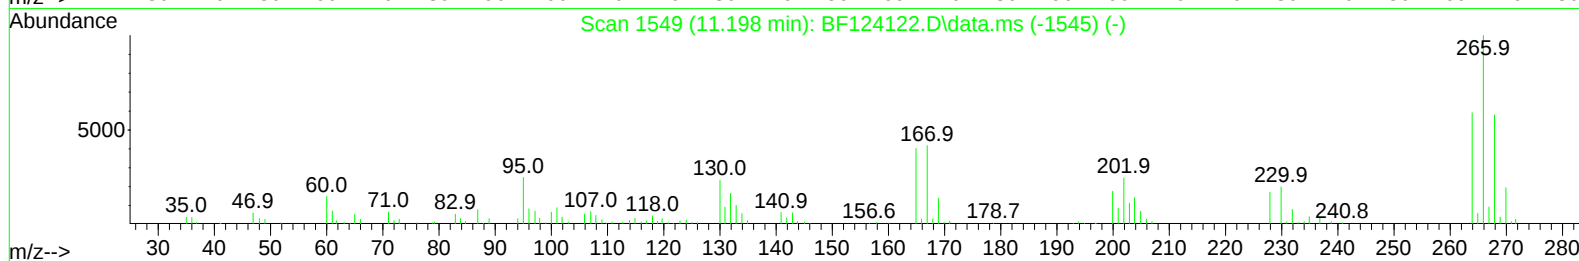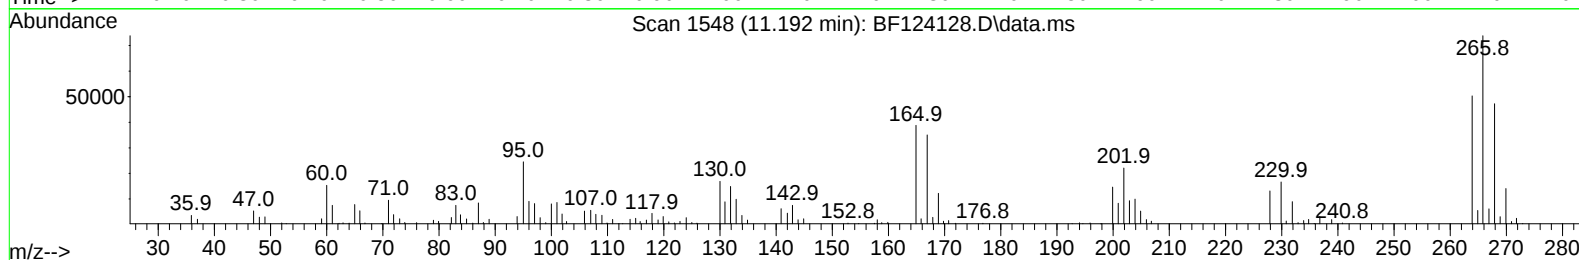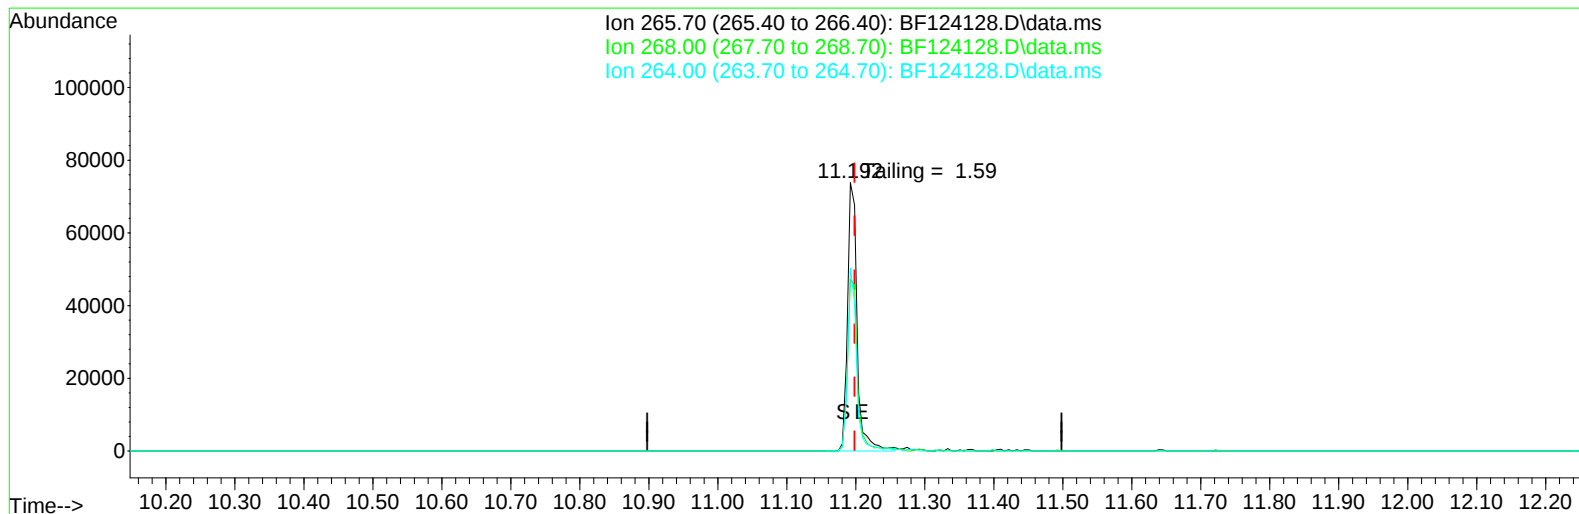

TIC: BF124128.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 16930.58 ng

response 70974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.99
264.00	65.70	68.14
0.00	0.00	0.00