

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
 Data File : BF124144.D
 Acq On : 4 Jun 2021 17:33
 Operator : JU/CG
 Sample : M2597-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 124042

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	3	10	15	rBB	468412	596389	68.37%	7.437%
2	5.493	575	579	583	rBV	964628	872326	100.00%	10.878%
3	6.504	746	751	754	rBV	943558	815181	93.45%	10.165%
4	6.692	781	783	790	rBB	13753	12555	1.44%	0.157%
5	6.863	809	812	816	rBV	239987	211026	24.19%	2.631%
6	7.428	903	908	911	rBV	663580	524514	60.13%	6.541%
7	8.051	1010	1014	1025	rBV	391123	322713	36.99%	4.024%
8	8.145	1027	1030	1033	rBV	281760	240119	27.53%	2.994%
9	9.222	1209	1213	1216	rBV	1062758	808701	92.71%	10.084%
10	9.339	1228	1233	1236	rBV	43897	36421	4.18%	0.454%
11	9.904	1325	1329	1332	rBV	316467	238838	27.38%	2.978%
12	10.451	1419	1422	1425	rBV	14890	11376	1.30%	0.142%
13	10.692	1459	1463	1466	rBV	630870	506971	58.12%	6.322%
14	11.392	1578	1582	1584	rBV	262895	232078	26.60%	2.894%
15	11.416	1584	1586	1589	rVV	113026	90454	10.37%	1.128%
16	11.463	1592	1594	1597	rVB	25500	19576	2.24%	0.244%
17	11.622	1615	1621	1625	rBV3	8424	14964	1.72%	0.187%
18	11.780	1644	1648	1650	rBV	37855	30580	3.51%	0.381%
19	11.892	1663	1667	1668	rBV2	14870	12371	1.42%	0.154%
20	11.916	1668	1671	1676	rVB2	94765	83754	9.60%	1.044%
21	12.004	1682	1686	1688	rBV3	18937	20708	2.37%	0.258%
22	12.022	1688	1689	1694	rVB2	11437	10468	1.20%	0.131%
23	12.439	1758	1760	1762	rBV2	10908	11301	1.30%	0.141%
24	12.469	1762	1765	1766	rVV	24164	23995	2.75%	0.299%
25	12.486	1766	1768	1773	rVB	126410	105077	12.05%	1.310%
26	12.574	1780	1783	1785	rBV	23290	19266	2.21%	0.240%
27	12.604	1785	1788	1793	rVB	154929	127416	14.61%	1.589%
28	12.698	1802	1804	1808	rBV2	35519	38959	4.47%	0.486%
29	12.833	1821	1827	1833	rBV	131759	131365	15.06%	1.638%
30	12.974	1847	1851	1856	rVB	929747	784508	89.93%	9.783%
31	13.051	1859	1864	1867	rBV6	14414	21357	2.45%	0.266%
32	13.163	1881	1883	1886	rVB2	17718	11513	1.32%	0.144%
33	13.227	1891	1894	1896	rBV4	16787	13119	1.50%	0.164%
34	13.263	1896	1900	1904	rVB6	13237	14833	1.70%	0.185%
35	13.357	1914	1916	1919	rBV4	9836	10829	1.24%	0.135%
36	13.780	1986	1988	1990	rBV3	11616	12290	1.41%	0.153%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
 Data File : BF124144.D
 Acq On : 4 Jun 2021 17:33
 Operator : JU/CG
 Sample : M2597-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 124042

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	13.833	1995	1997	2001	rBV5	13494	17277	1.98%	0.215%
38	13.880	2002	2005	2013	rVB9	33031	59106	6.78%	0.737%
39	14.033	2022	2031	2034	rBV3	277723	382449	43.84%	4.769%
40	14.057	2034	2035	2039	rVB	50818	35122	4.03%	0.438%
41	14.257	2066	2069	2073	rBV6	10812	14730	1.69%	0.184%
42	14.321	2076	2080	2082	rBV5	15663	21500	2.46%	0.268%
43	15.080	2206	2209	2217	rVB2	46084	83215	9.54%	1.038%
44	15.386	2259	2261	2264	rVB4	17785	16158	1.85%	0.201%
45	15.451	2269	2272	2278	rVB2	39865	55561	6.37%	0.693%
46	15.515	2278	2283	2287	rBV	142444	193018	22.13%	2.407%
47	15.968	2356	2360	2361	rBV4	16587	13617	1.56%	0.170%
48	15.980	2361	2362	2367	rVB5	14324	14058	1.61%	0.175%
49	16.433	2435	2439	2441	rBV5	14305	16816	1.93%	0.210%
50	16.998	2532	2535	2541	rVB8	20330	31518	3.61%	0.393%
51	17.251	2576	2578	2579	rBV2	14683	11419	1.31%	0.142%
52	18.715	2825	2827	2831	rBV5	11414	15894	1.82%	0.198%




Sum of corrected areas: 8019369

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124144.D
Acq On : 4 Jun 2021 17:33
Operator : JU/CG
Sample : M2597-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
124042

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

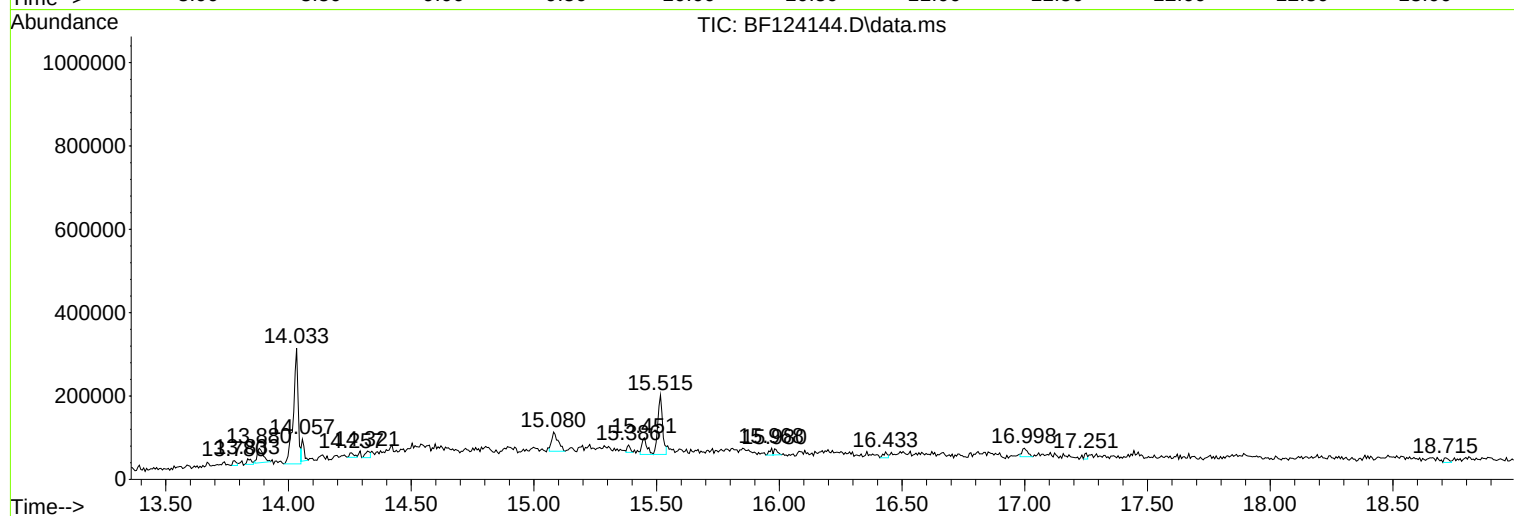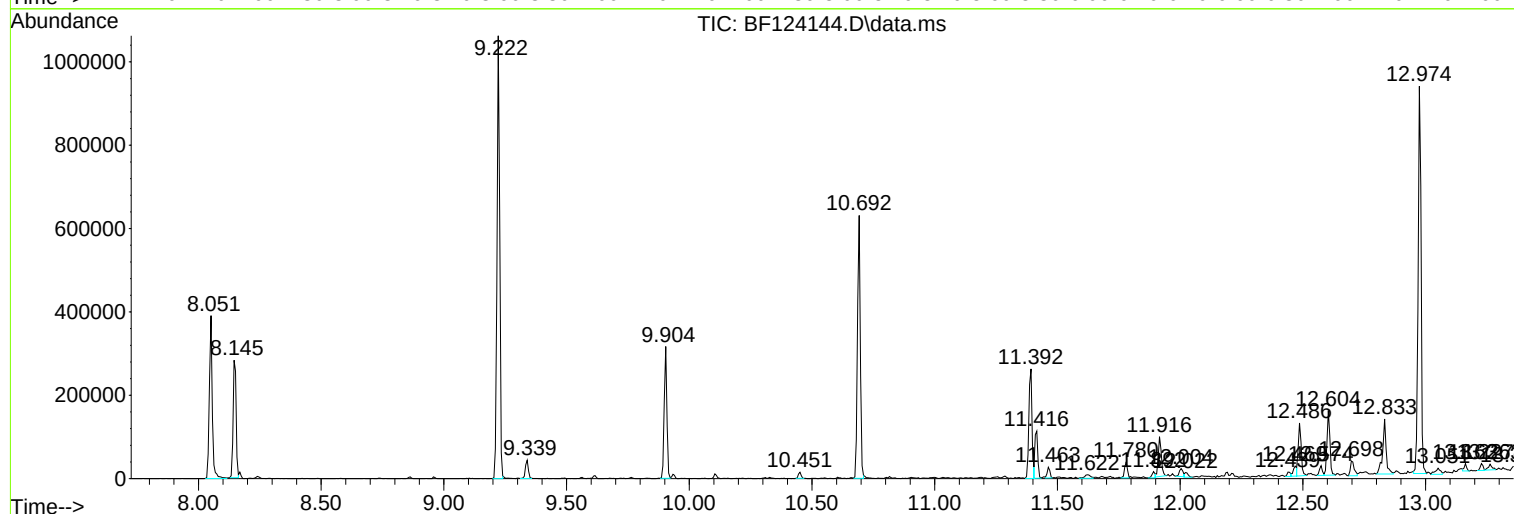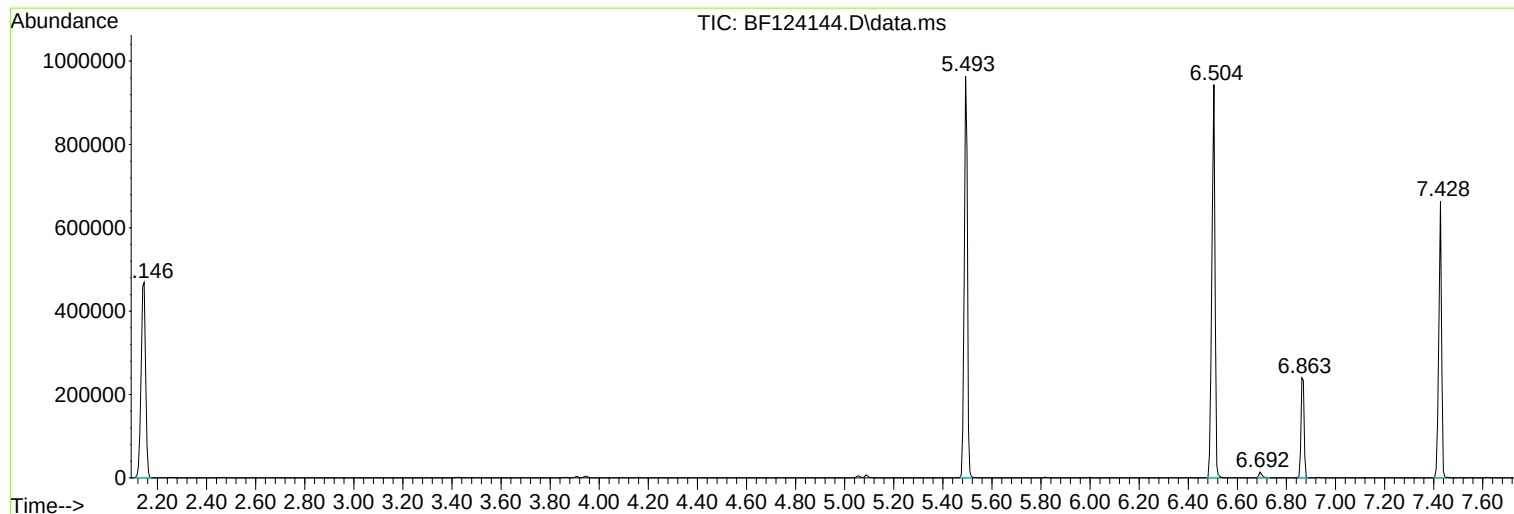

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124144.D
Acq On : 4 Jun 2021 17:33
Operator : JU/CG
Sample : M2597-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
124042

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124144.D
Acq On : 4 Jun 2021 17:33
Operator : JU/CG
Sample : M2597-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
124042

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
