


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
 Data File : BF124128.D
 Acq On : 4 Jun 2021 8:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 04 09:56:24 2021

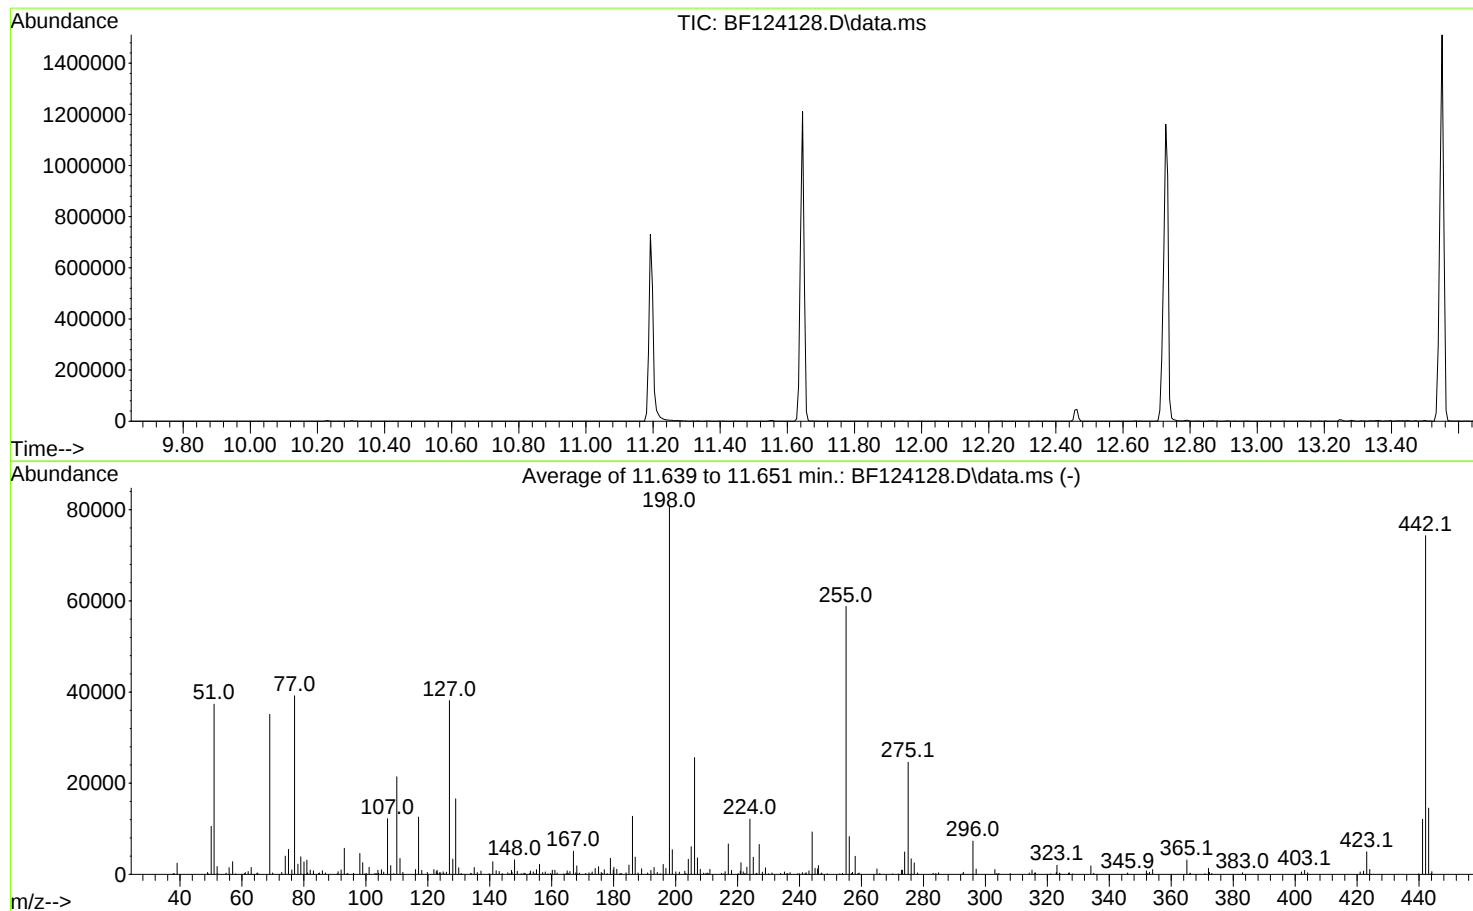

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	37349	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	35097	PASS
70	69	0.00	2	0.9	311	PASS
127	198	10	80	47.2	38133	PASS
197	198	0.00	2	1.6	1300	PASS
198	198	100	100	100.0	80717	PASS
199	198	5	9	6.7	5412	PASS
275	198	10	60	30.5	24624	PASS
365	198	1	100	3.9	3153	PASS
441	198	0.01	100	14.9	12066	PASS
442	442	50	100	100.0	74336	PASS
443	442	15	24	19.6	14547	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/4/2021	BNA_F	<u>BF124128.D</u>
Compound Name	Response	Retention Time
DDT	224555	13.55
DDD	1939	13.24
DDE	463	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2402	226957	1.06

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124128.D
Acq On : 4 Jun 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 10:48:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 04 09:56:24 2021
Response via : Initial Calibration

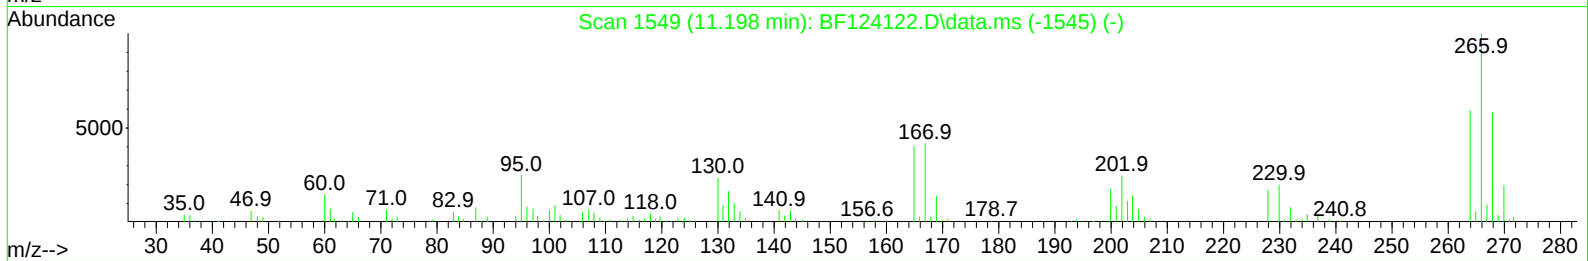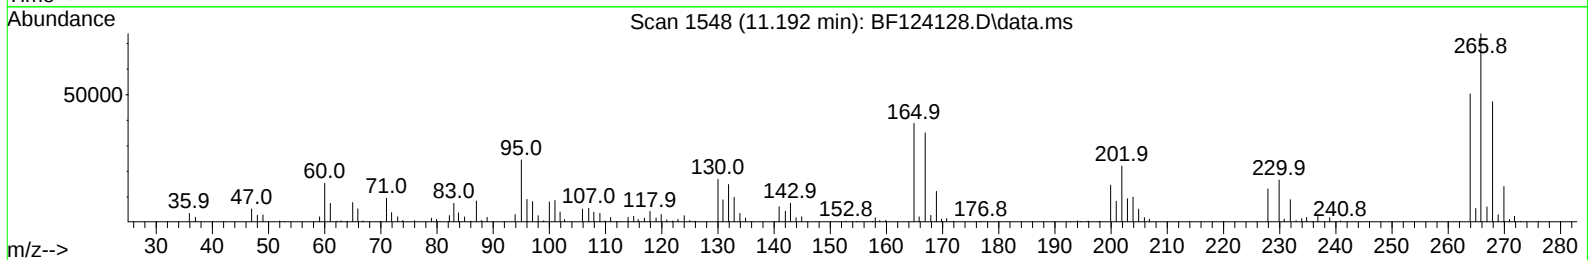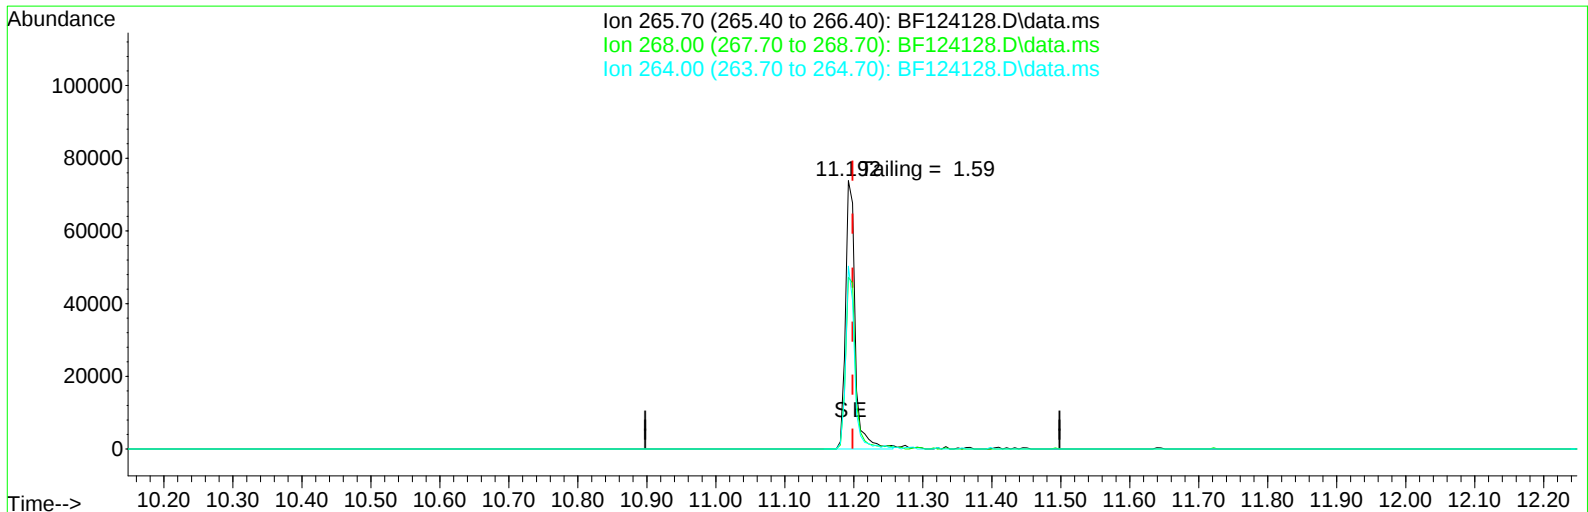

TIC: BF124128.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.006) 16930.58 ng




response 70974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.99
264.00	65.70	68.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060421\
Data File : BF124128.D
Acq On : 4 Jun 2021 8:48
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 10:48:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 04 09:56:24 2021
Response via : Initial Calibration

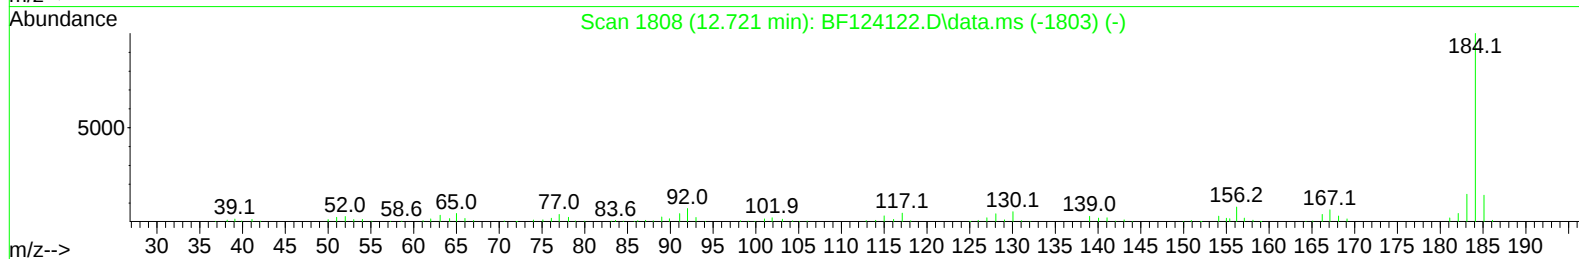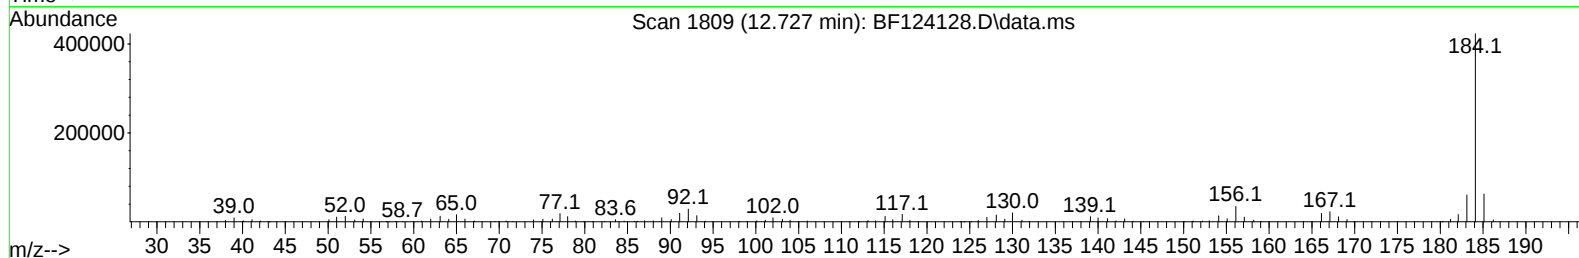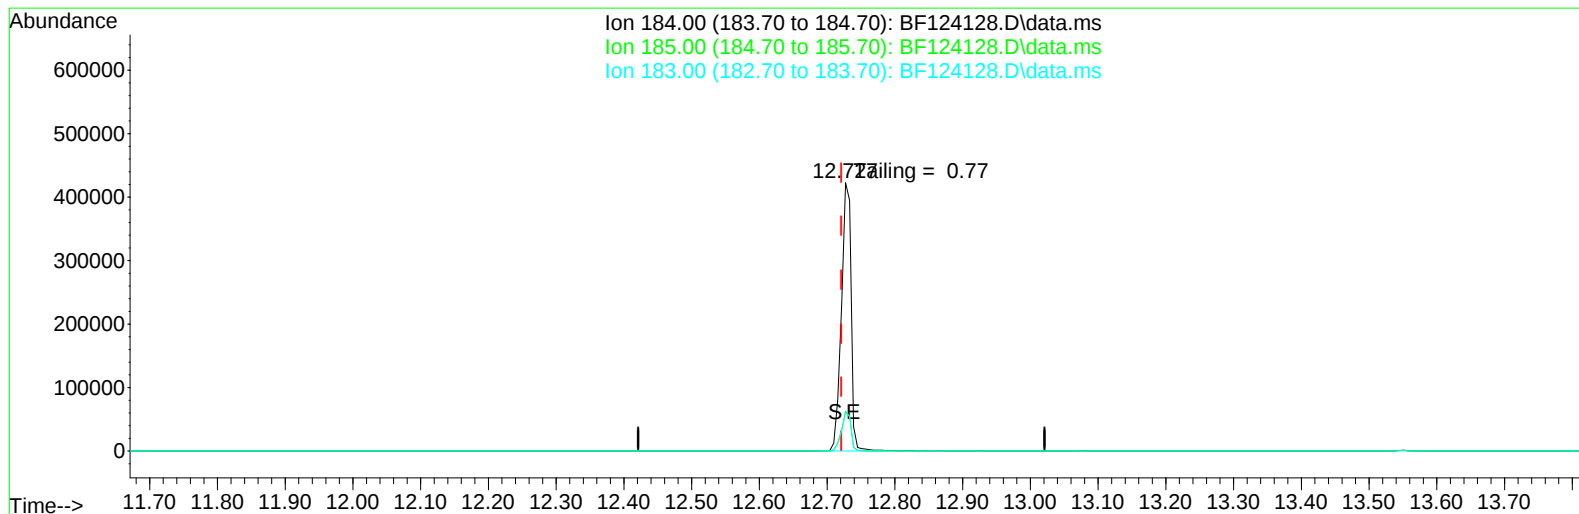

TIC: BF124128.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 425362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.82
183.00	9.80	14.25#
0.00	0.00	0.00