

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
 Data File : BF142617.D
 Acq On : 04 Jun 2025 20:17
 Operator : RC/JU
 Sample : Q2173-13 5X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-400-CF-402B-COMP-25

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	487	494	501	rBV	27137	39246	4.02%	0.496%
2	5.504	557	563	576	rBV	274530	359485	36.82%	4.548%
3	6.516	729	735	752	rBV	266173	364065	37.29%	4.606%
4	6.892	794	799	804	rBV	600945	738453	75.64%	9.342%
5	7.451	888	894	899	rBV	181199	228625	23.42%	2.892%
6	8.181	1012	1018	1032	rBV	709256	938862	96.17%	11.877%
7	9.251	1195	1200	1212	rBV	374556	462938	47.42%	5.856%
8	9.933	1311	1316	1321	rBV	771847	943609	96.66%	11.937%
9	10.645	1433	1437	1445	rVB	14289	18641	1.91%	0.236%
10	10.722	1445	1450	1459	rBV	141200	183962	18.84%	2.327%
11	11.422	1564	1569	1577	rBV	601169	784567	80.36%	9.925%
12	11.939	1649	1657	1663	rBV4	28183	61147	6.26%	0.774%
13	12.033	1670	1673	1681	rVB	11329	23991	2.46%	0.304%
14	12.633	1770	1775	1781	rBV	88656	112495	11.52%	1.423%
15	12.863	1807	1814	1827	rBV	82886	144854	14.84%	1.832%
16	13.004	1833	1838	1844	rVB	242371	309744	31.73%	3.918%
17	13.080	1847	1851	1858	rBV5	7782	13366	1.37%	0.169%
18	13.192	1863	1870	1873	rBV2	13638	23334	2.39%	0.295%
19	13.298	1884	1888	1892	rBV2	8623	11772	1.21%	0.149%
20	13.698	1950	1956	1961	rBV2	14323	28681	2.94%	0.363%
21	13.810	1972	1975	1978	rBV3	9082	13165	1.35%	0.167%
22	13.845	1978	1981	1988	rVV4	12837	26828	2.75%	0.339%
23	13.904	1988	1991	2000	rVB2	18041	31450	3.22%	0.398%
24	14.063	2010	2018	2029	rBV	617220	976265	100.00%	12.350%
25	14.721	2126	2130	2135	rBV	55431	79919	8.19%	1.011%
26	15.115	2192	2197	2205	rBV	74113	167824	17.19%	2.123%
27	15.427	2246	2250	2256	rVB	37155	58572	6.00%	0.741%
28	15.492	2257	2261	2266	rVV	38482	58435	5.99%	0.739%
29	15.557	2266	2272	2284	rVB	421010	700466	71.75%	8.861%




Sum of corrected areas: 7904761

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142617.D
Acq On : 04 Jun 2025 20:17
Operator : RC/JU
Sample : Q2173-13 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-400-CF-402B-COMP-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

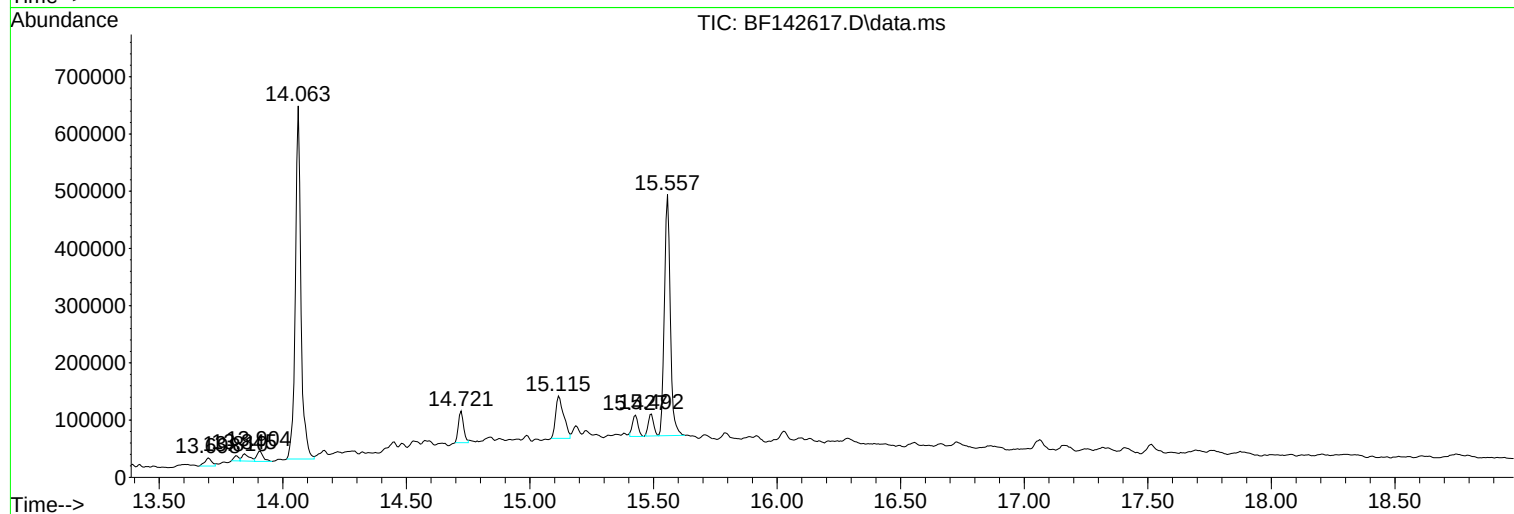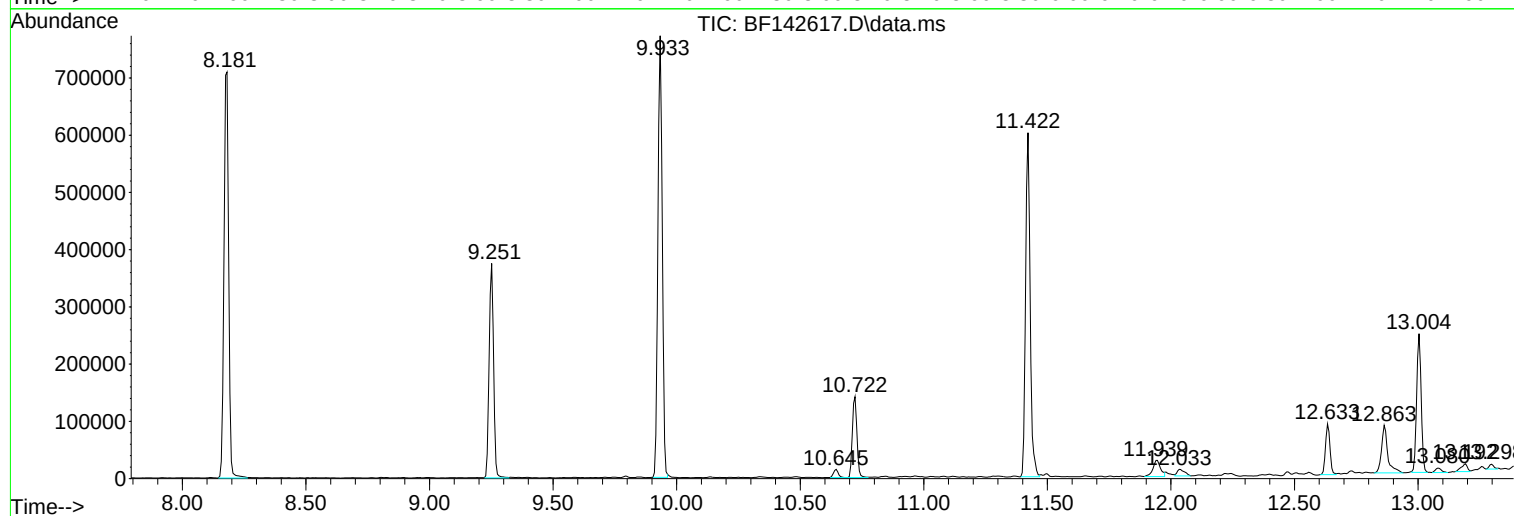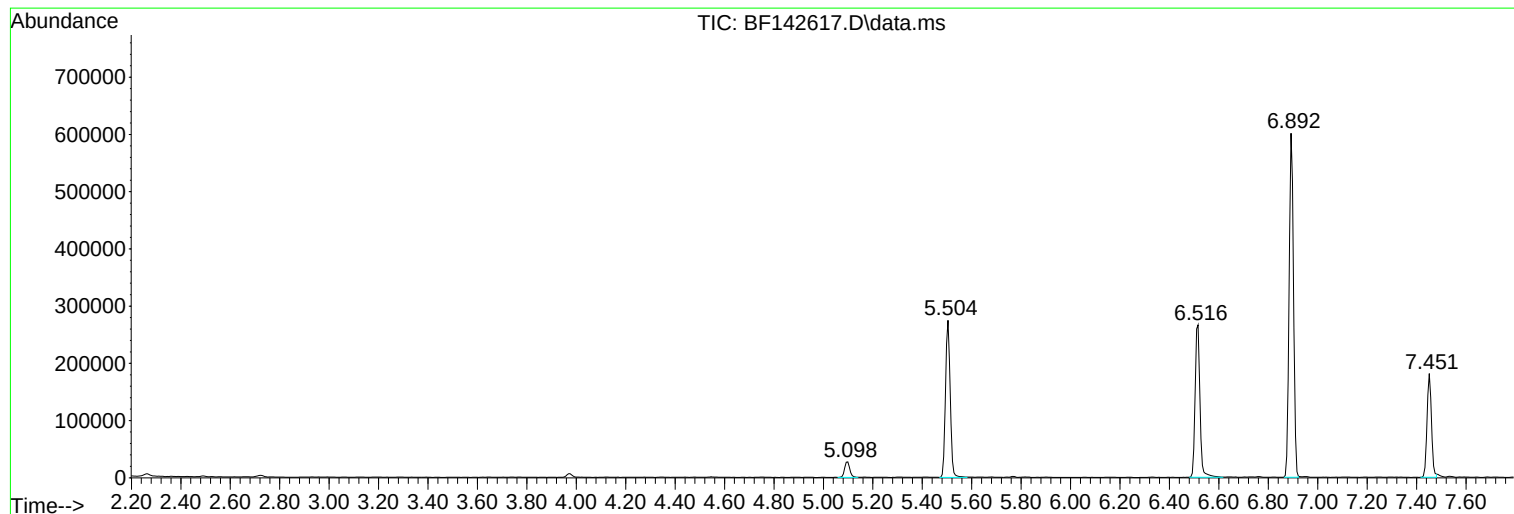

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142617.D
Acq On : 04 Jun 2025 20:17
Operator : RC/JU
Sample : Q2173-13 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-400-CF-402B-COMP-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142617.D
Acq On : 04 Jun 2025 20:17
Operator : RC/JU
Sample : Q2173-13 5X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-400-CF-402B-COMP-25

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------