
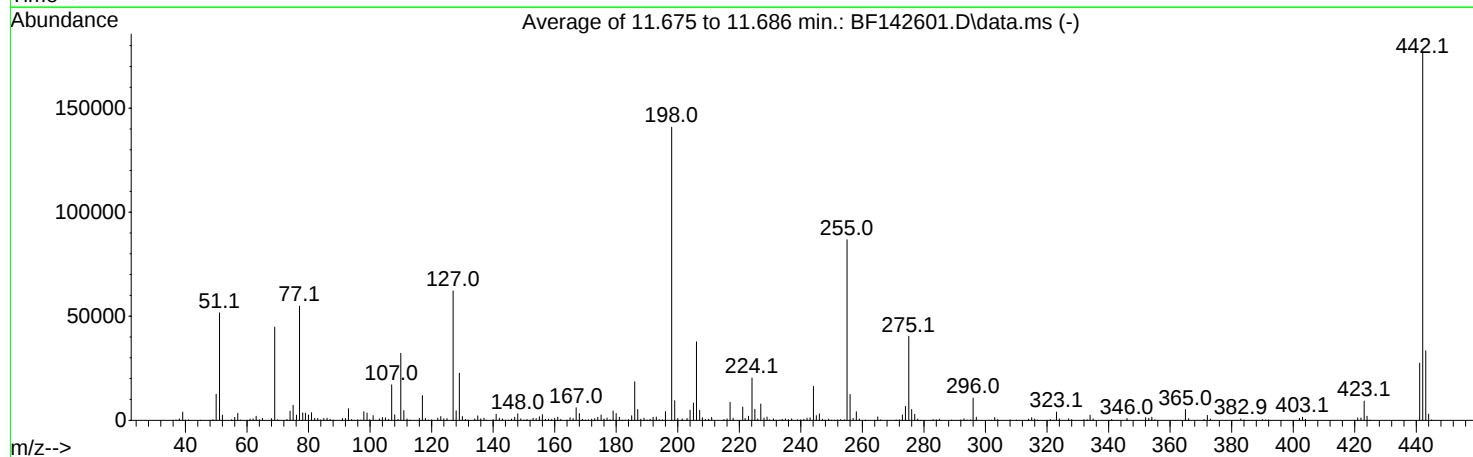


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142601.D
Acq On : 04 Jun 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

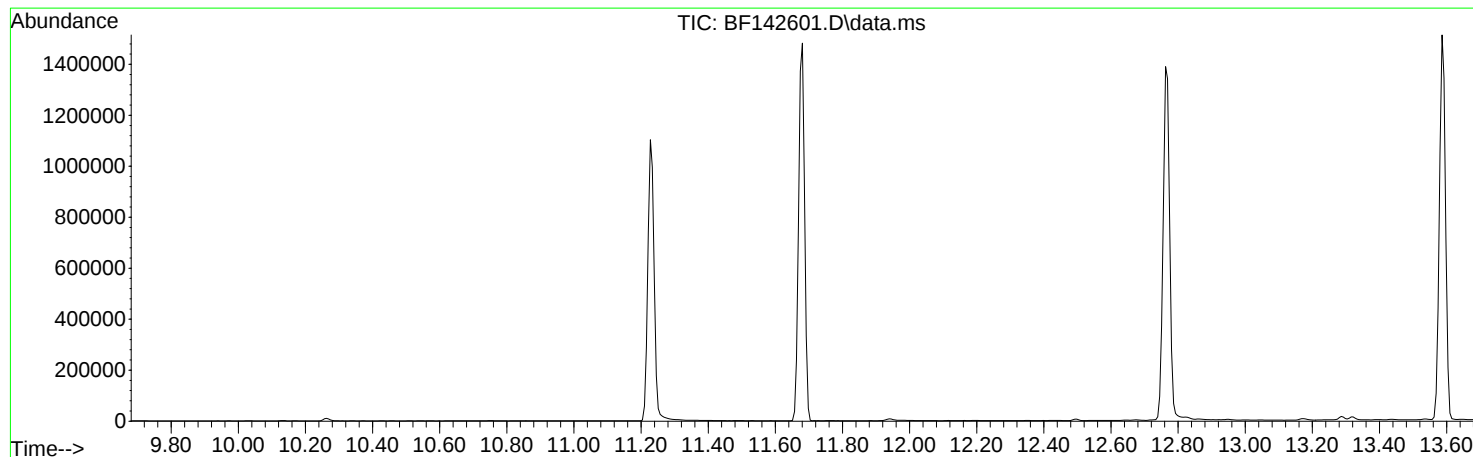




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	51635	PASS
68	69	0.00	2	1.8	804	PASS
69	198	0.00	100	31.8	44819	PASS
70	69	0.00	2	0.7	301	PASS
127	198	10	80	44.2	62200	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140824	PASS
199	198	5	9	6.7	9404	PASS
275	198	10	60	28.6	40309	PASS
365	198	1	100	3.7	5164	PASS
441	198	0.01	100	19.5	27475	PASS
442	442	50	100	100.0	176768	PASS
443	442	15	24	18.9	33427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142601.D
Acq On : 04 Jun 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 13:03:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

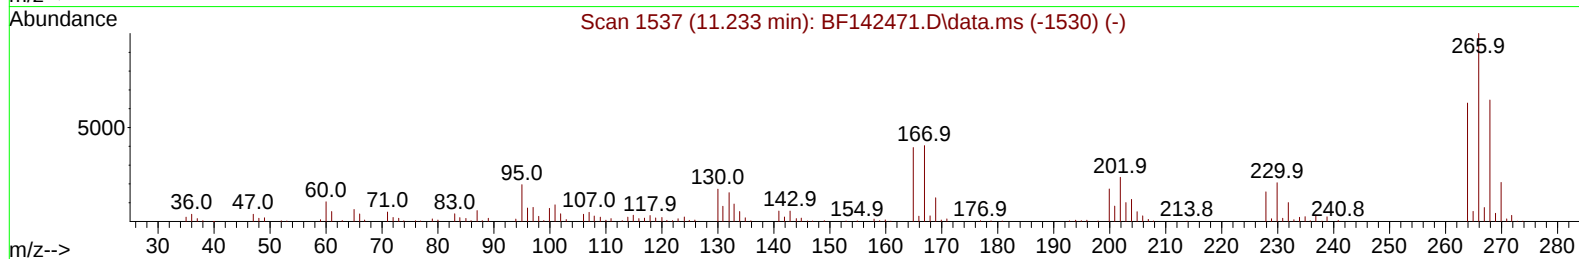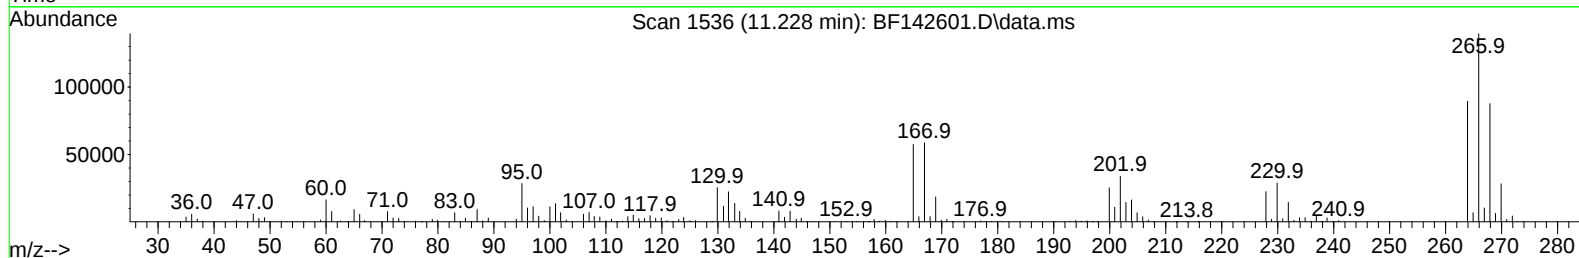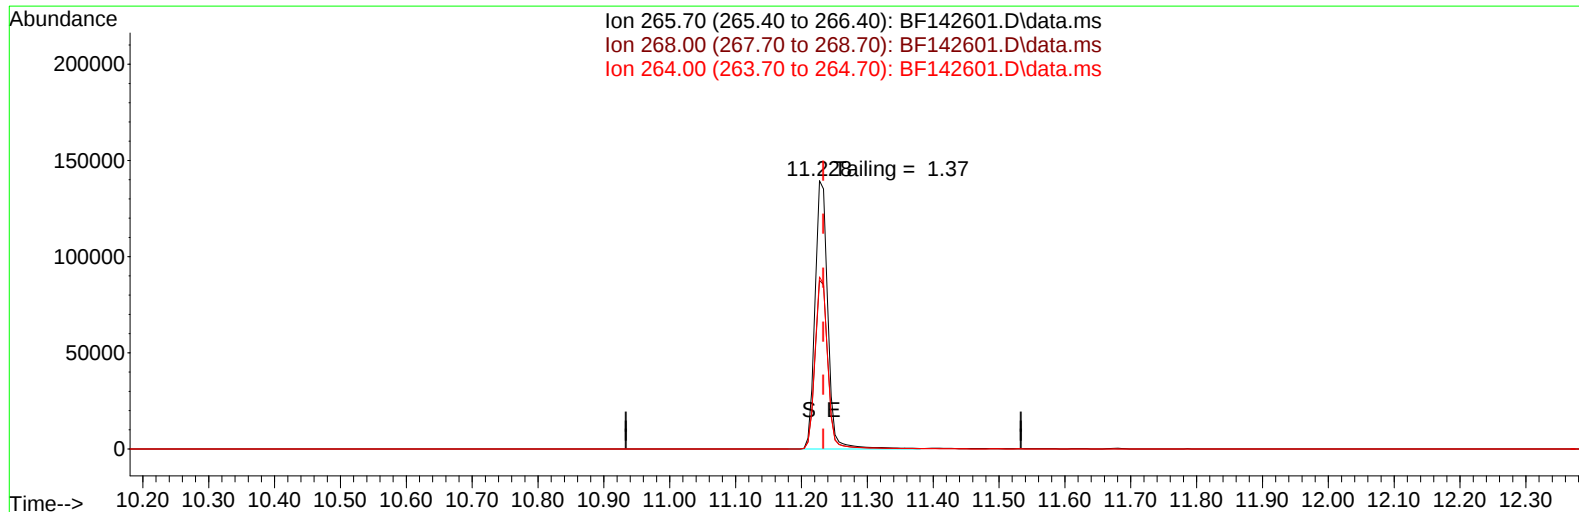

TIC: BF142601.D\data.ms

(70) Pentachlorophenol (C)

11.228min (-0.006) 34098.66 ng




response 188828

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	62.83
264.00	63.00	64.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060425\
Data File : BF142601.D
Acq On : 04 Jun 2025 11:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 04 13:03:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

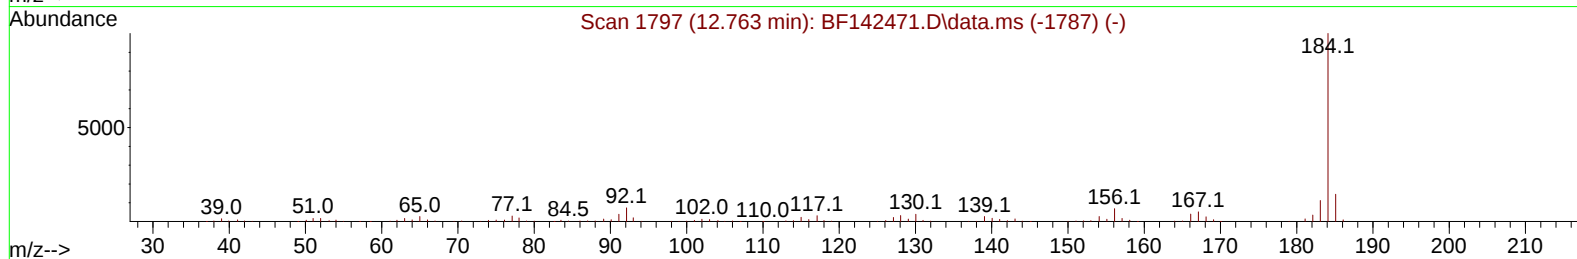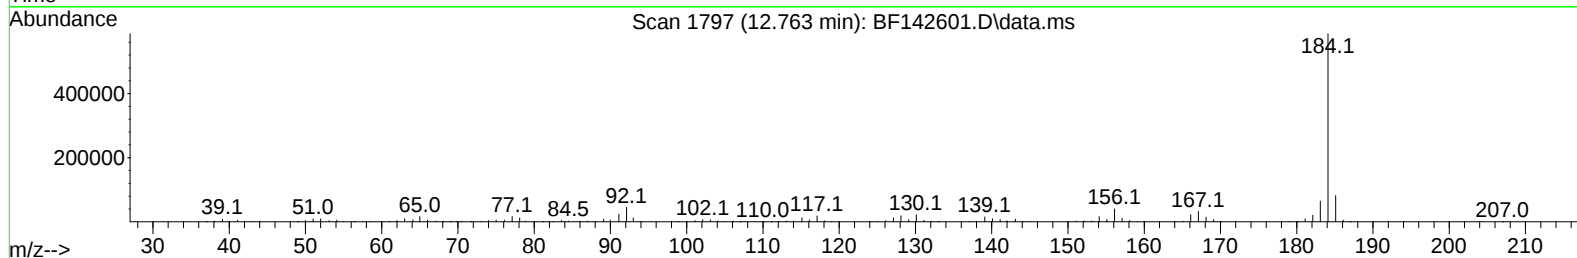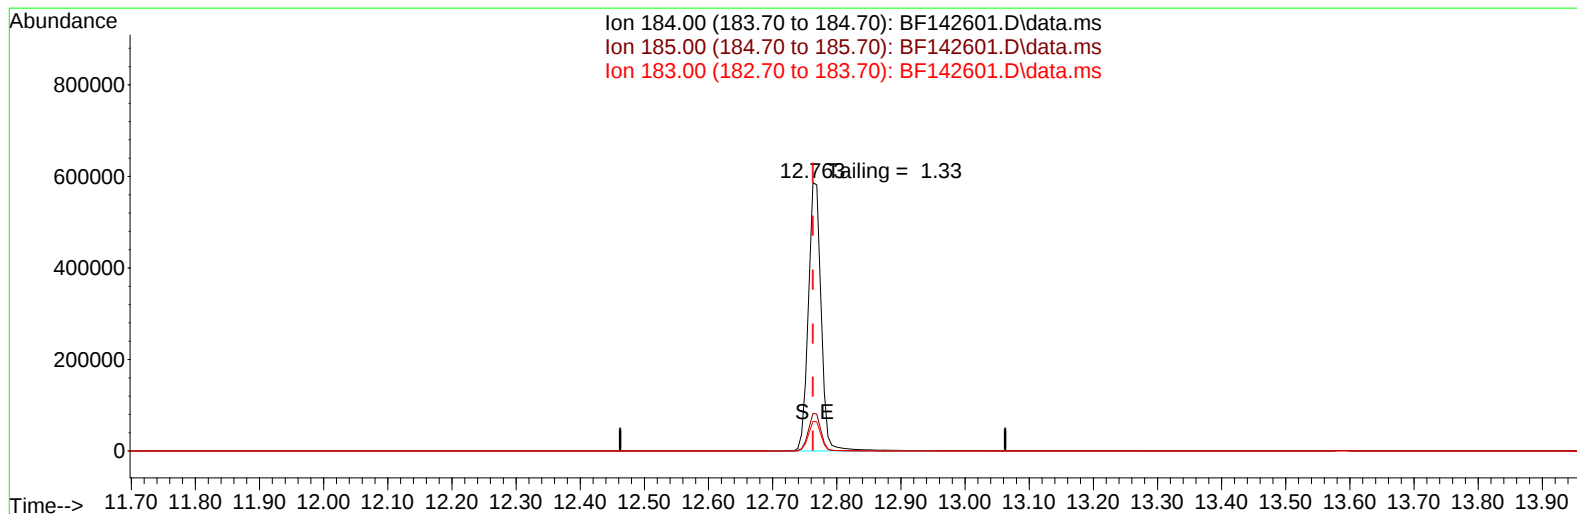

TIC: BF142601.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 822752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.00
183.00	11.20	11.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2025	BNA_F	<u>BF142601.D</u>
Compound Name	Response	Retention Time
DDT	393008	13.586
DDD	8243	13.286
DDE	865	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9108	402116	2.27

Instrument :
BNA_F
ClientSampleId :
DFTPP