

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060515\
 Data File : BF079762.D
 Acq On : 6 Jun 2015 8:22
 Operator : TP/IZ
 Sample : G2443-06 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FD-04

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.461	22	24	26	rVB	184201	179824	13.87%	1.743%
2	2.433	106	109	123	rVB	361668	594860	45.87%	5.764%
3	6.102	428	430	433	rBV	684067	692151	53.37%	6.707%
4	7.085	514	516	518	rBV	845322	754064	58.15%	7.307%
5	7.256	529	531	533	rBV	982171	797310	61.48%	7.726%
6	7.496	549	552	553	rBV	254659	317634	24.49%	3.078%
7	7.645	563	565	568	rVB	417125	572969	44.18%	5.552%
8	8.045	598	600	602	rBV	491480	405803	31.29%	3.932%
9	8.788	662	665	667	rBV	475861	453411	34.96%	4.394%
10	9.862	756	759	761	rVB	1037965	1000946	77.19%	9.699%
11	10.559	818	820	822	rVB	662991	570166	43.97%	5.525%
12	11.359	887	890	892	rBV2	440722	553765	42.70%	5.366%
13	12.079	951	953	955	rBV	667057	647781	49.95%	6.277%
14	13.794	1100	1103	1105	rBV	1322994	1296771	100.00%	12.566%
15	15.097	1214	1217	1220	rBV	596474	816841	62.99%	7.915%
16	17.086	1387	1391	1393	rBV	377675	665400	51.31%	6.448%


Sum of corrected areas: 10319696

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060515\
Data File : BF079762.D
Acq On : 6 Jun 2015 8:22
Operator : TP/IZ
Sample : G2443-06 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD-04

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

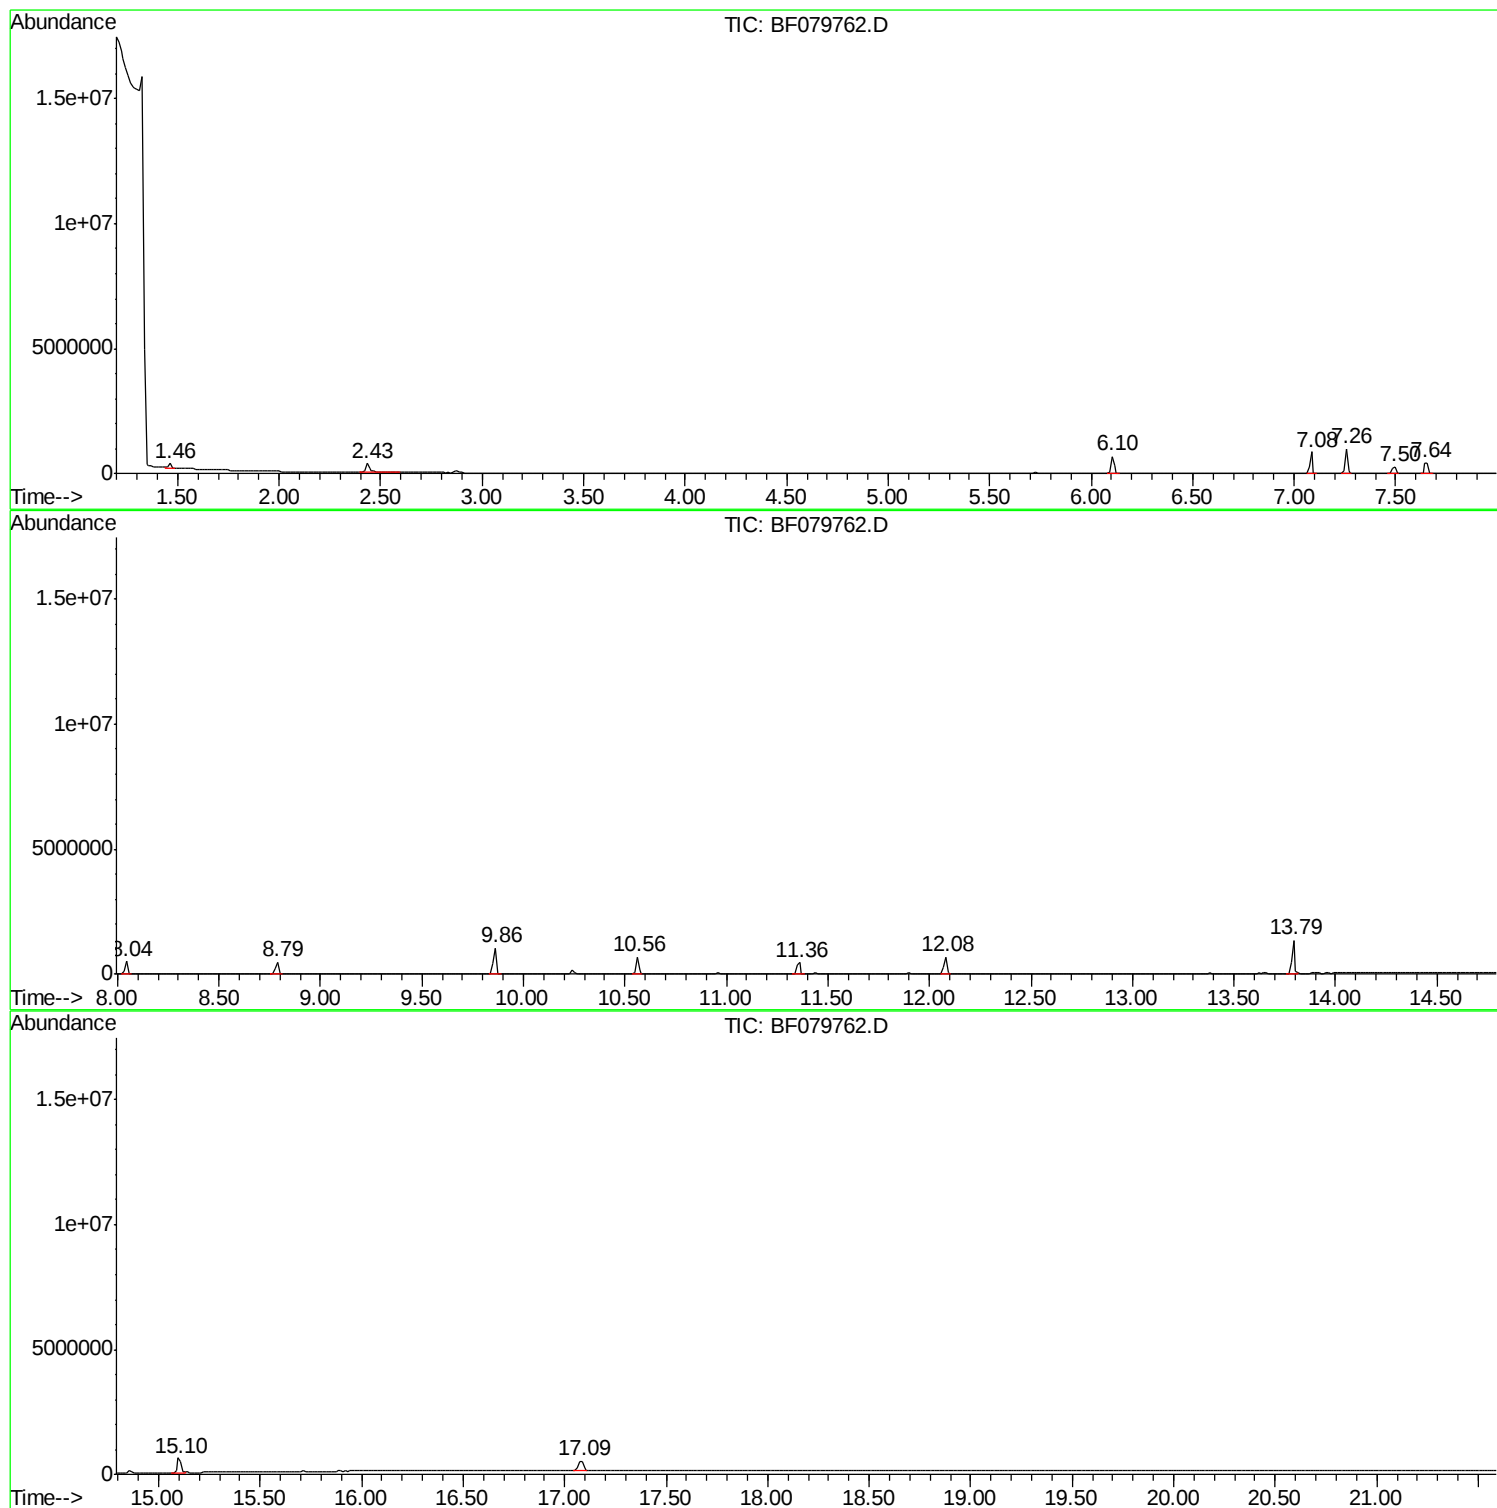

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060515\
Data File : BF079762.D
Acq On : 6 Jun 2015 8:22
Operator : TP/IZ
Sample : G2443-06 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD-04










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, 1,2-dichloro-, (Z)- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.46	11.32 ng	179824	1,4-Dichlorobenzene-d4	7.50

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Ethene, 1,2-dichloro-, (Z)-	96	C2H2Cl2	000156-59-2	97
2		Ethene, 1,2-dichloro-, (E)-	96	C2H2Cl2	000156-60-5	95
3		Ethene, 1,1-dichloro-	96	C2H2Cl2	000075-35-4	91
4		1,2-Dichloroethylene	96	C2H2Cl2	000540-59-0	91
5		Dihydro-4,5-dichloro-2(3H)furanone	154	C4H4Cl2O2	114434-99-0	64

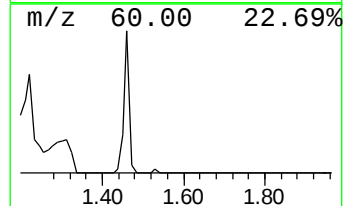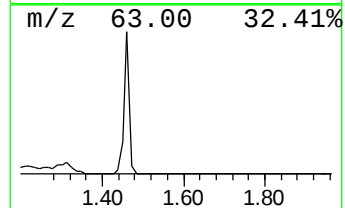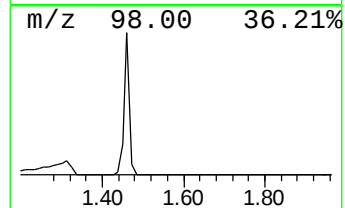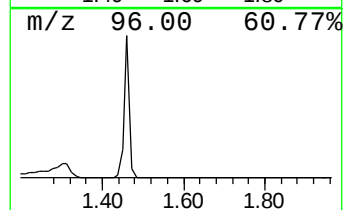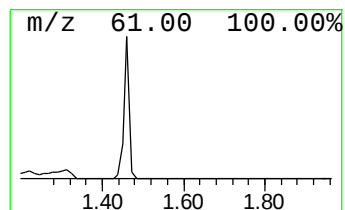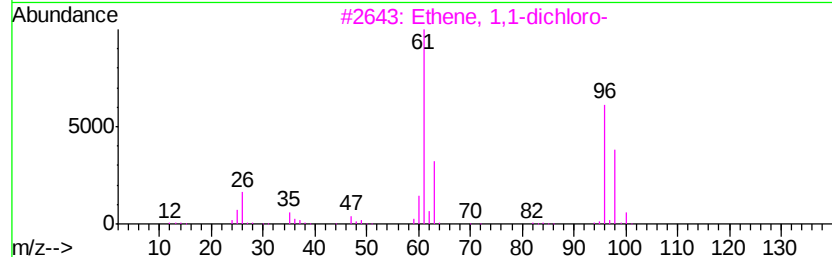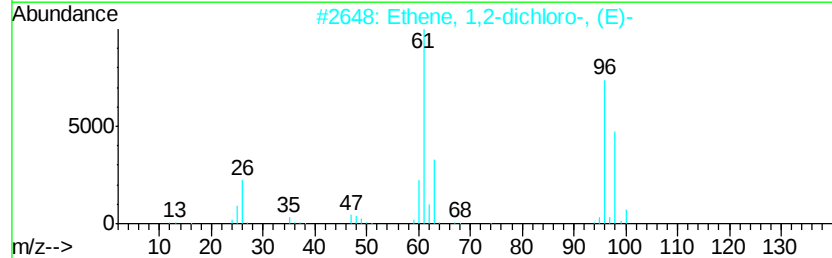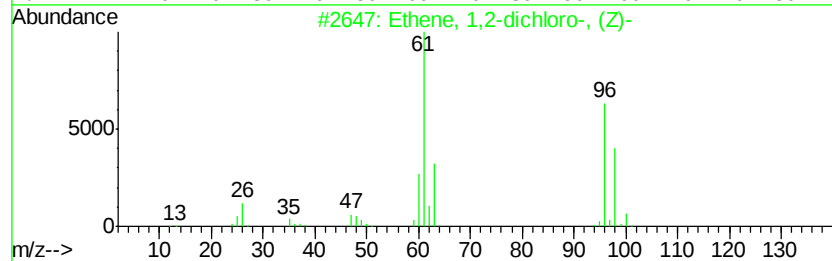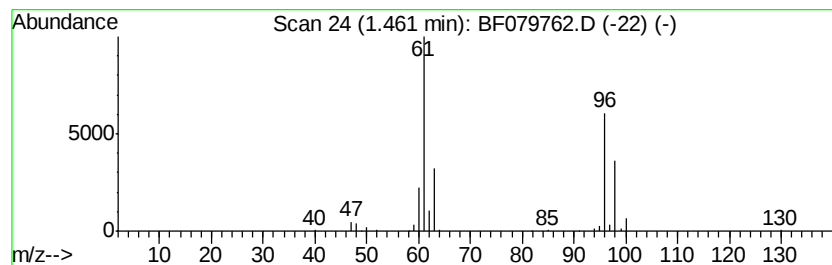

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060515\
Data File : BF079762.D
Acq On : 6 Jun 2015 8:22
Operator : TP/IZ
Sample : G2443-06 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD-04







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown7.26 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.26	50.20 ng	797310	1,4-Dichlorobenzene-d4	7.50

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4			Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

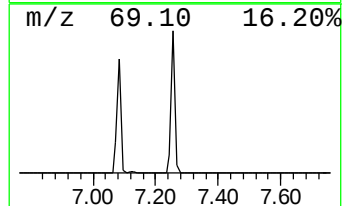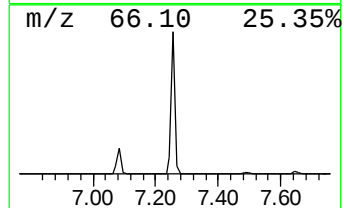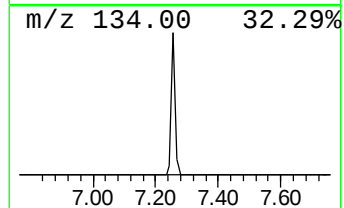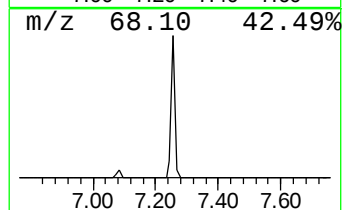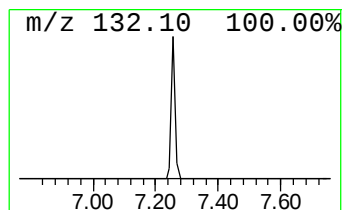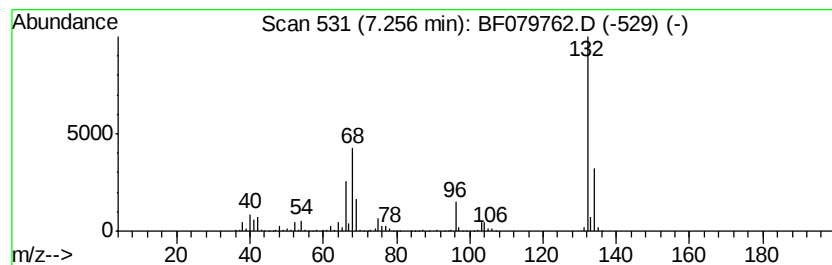

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060515\
Data File : BF079762.D
Acq On : 6 Jun 2015 8:22
Operator : TP/IZ
Sample : G2443-06 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FD-04

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, 1,2-dichl...	1.46	11.3	ng	179824	1	7.50	317634	20.0
unknown7.26	7.26	50.2	ng	797310	1	7.50	317634	20.0