


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060515\
 Data File : BF079737.D
 Acq On : 5 Jun 2015 19:23
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:33:51 2015

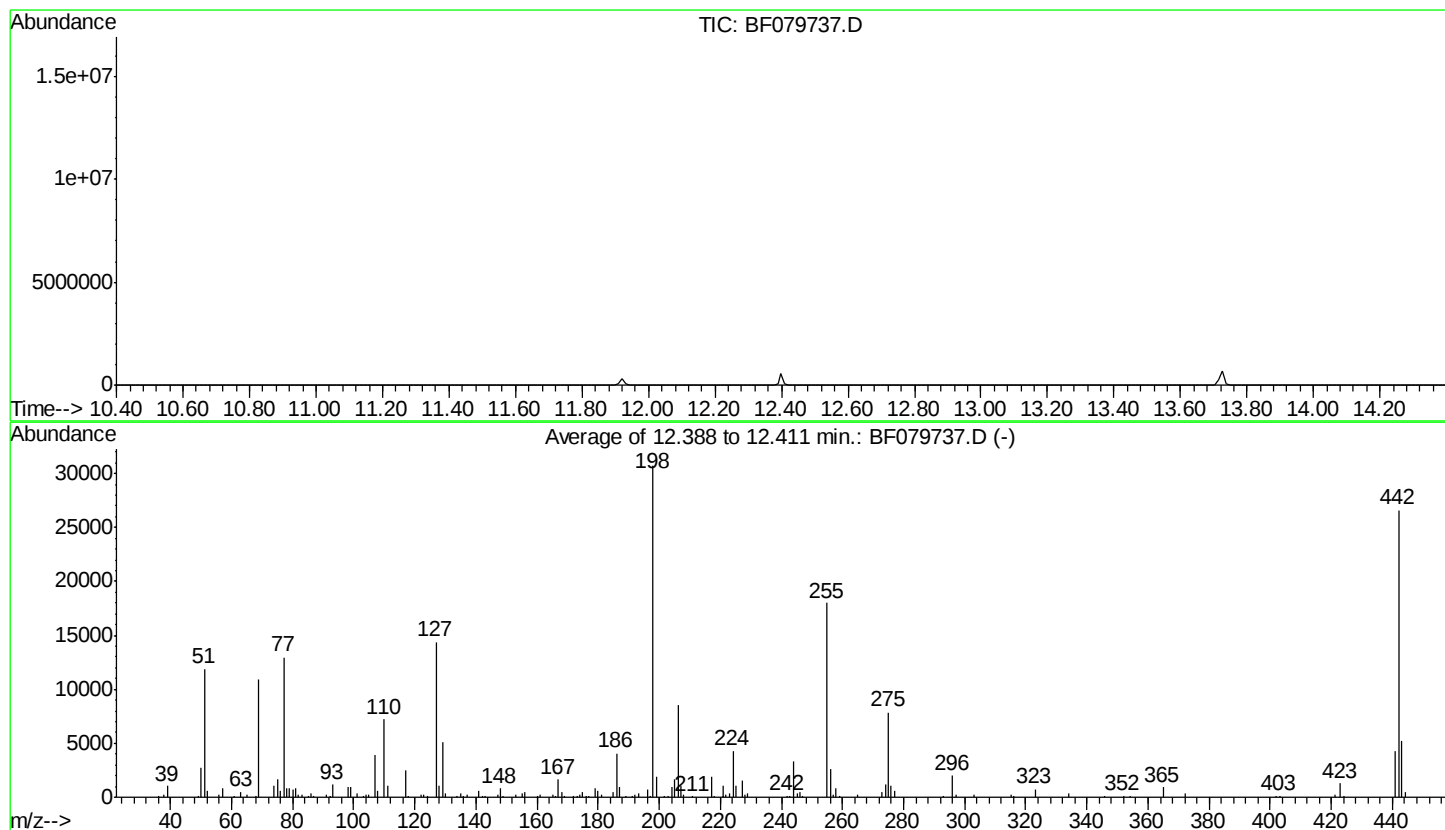

AutoFind: Scans 980, 981, 982; Background Corrected with Scan 977

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	11879	PASS
68	69	0.00	2	1.2	130	PASS
69	198	0.00	100	35.5	10913	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	14367	PASS
197	198	0.00	2	0.4	112	PASS
198	198	100	100	100.0	30729	PASS
199	198	5	9	6.2	1901	PASS
275	198	10	60	25.6	7873	PASS
365	198	1	100	3.1	945	PASS
441	442	0.01	24	16.2	4307	PASS
442	198	50	100	86.6	26596	PASS
443	442	15	24	19.6	5218	PASS