


Data Path : Z:\HPCHEM1\BNA_F\Data\BF060515\
 Data File : BF079746.D
 Acq On : 6 Jun 2015 00:11
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 08 18:33:51 2015

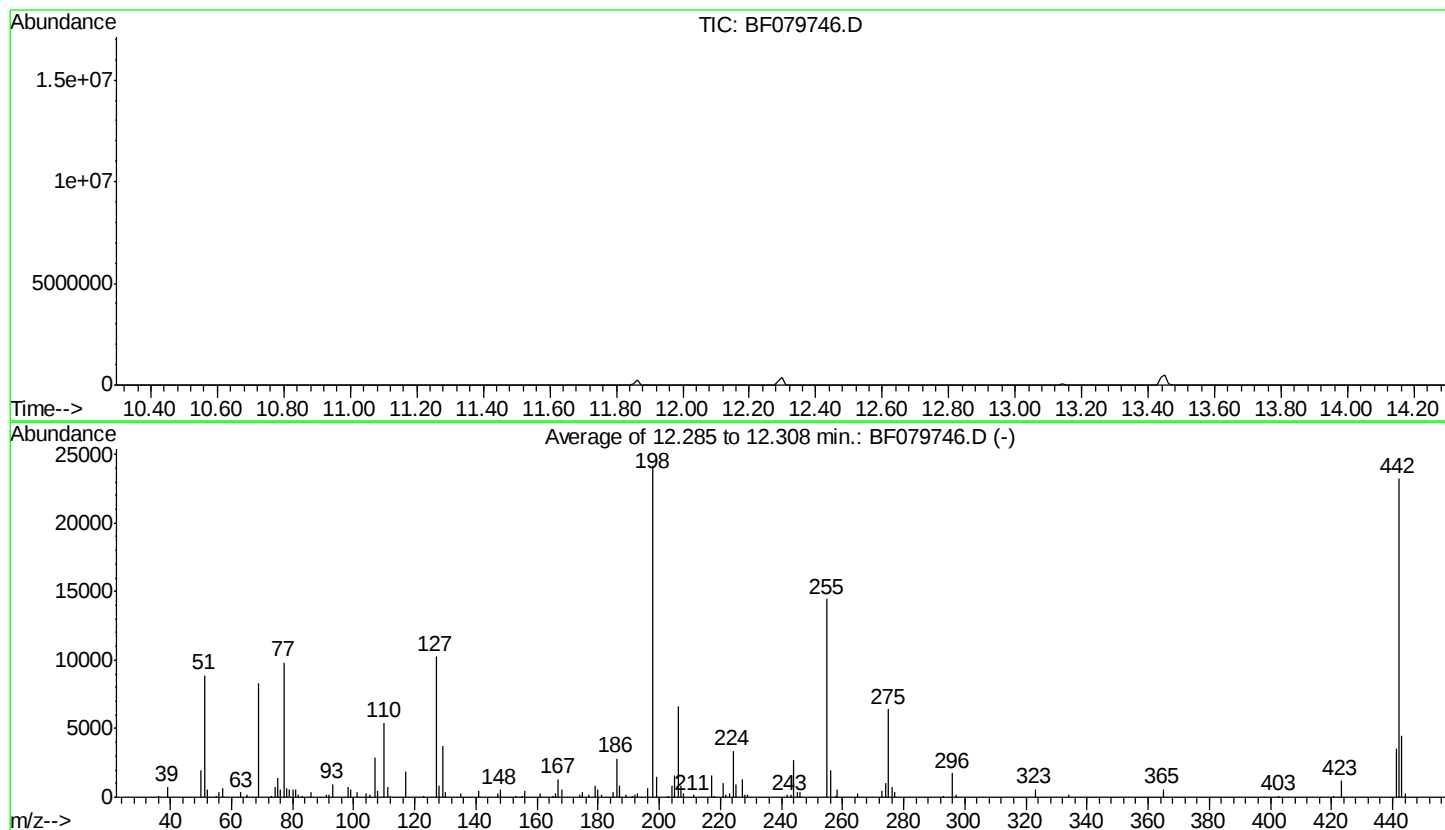

AutoFind: Scans 971, 972, 973; Background Corrected with Scan 968

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	8873	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.5	8340	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	10229	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	24177	PASS
199	198	5	9	6.3	1514	PASS
275	198	10	60	26.5	6397	PASS
365	198	1	100	2.5	600	PASS
441	442	0.01	24	15.4	3581	PASS
442	198	50	100	96.1	23230	PASS
443	442	15	24	19.5	4527	PASS