
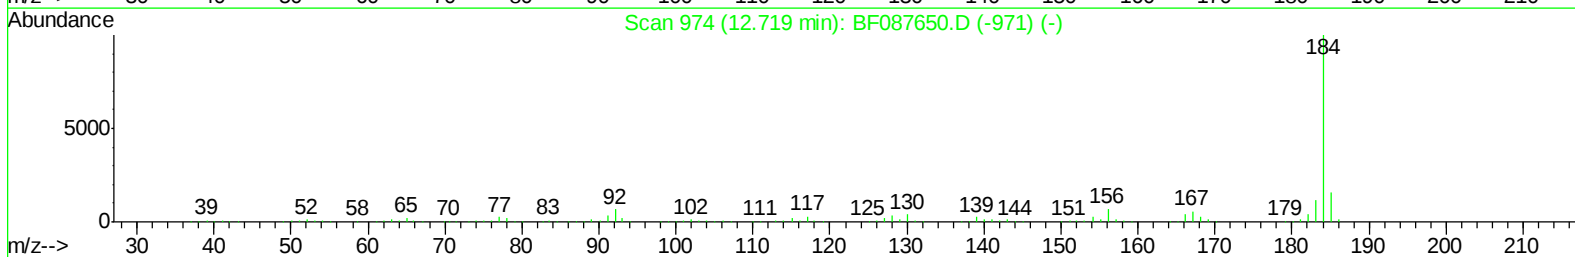
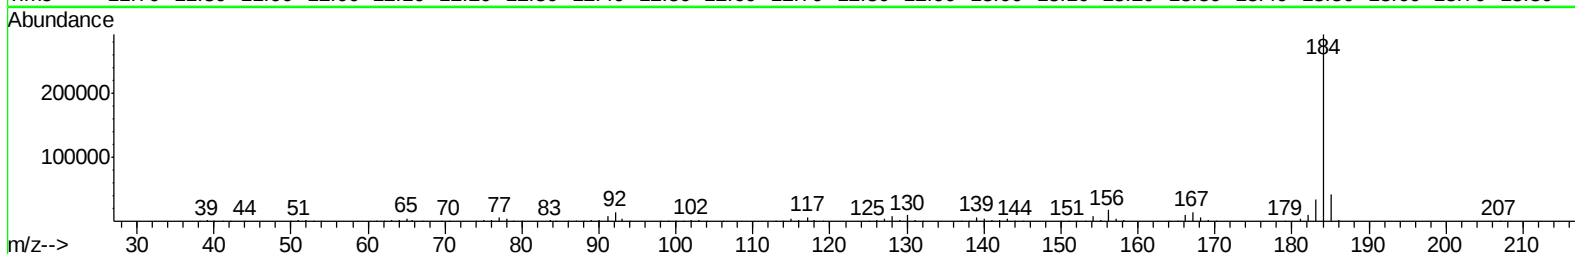


Data Path : Z:\HPCHEM1\BNA_F\Data\bf060516\
Data File : BF087704.D
Acq On : 5 Jun 2016 13:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 06:10:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

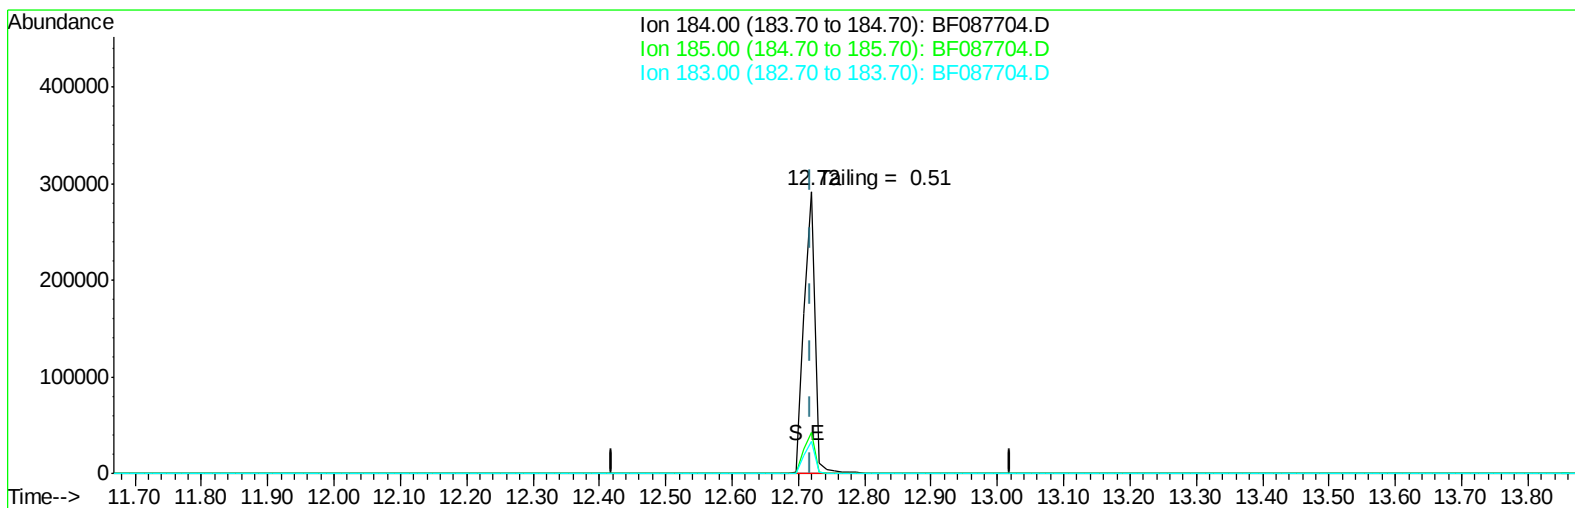

TIC: BF087704.D

(76) Benzidine




12.719min (+0.000) 0.00ng

response 330279

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.71
183.00	11.60	11.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\bf060516\
Data File : BF087704.D
Acq On : 5 Jun 2016 13:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 06:10:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

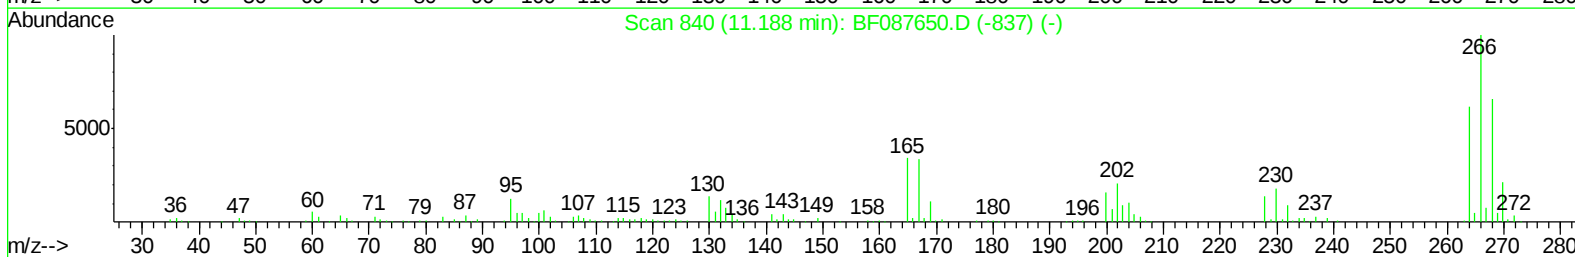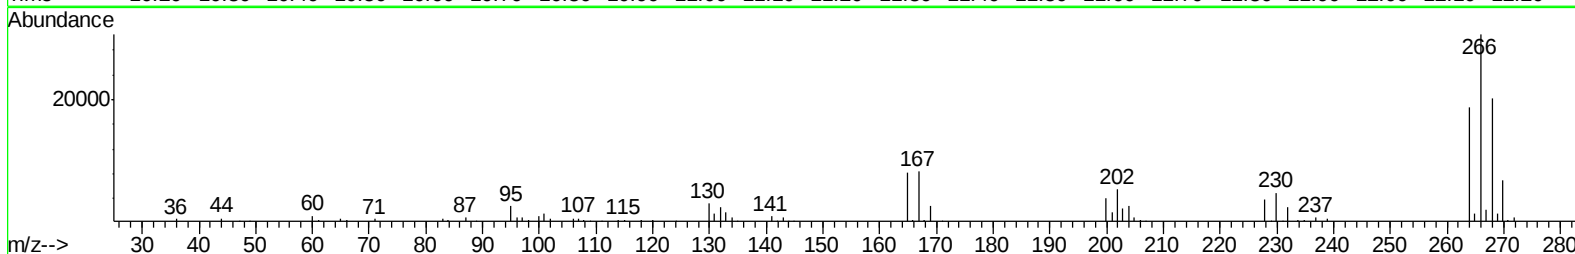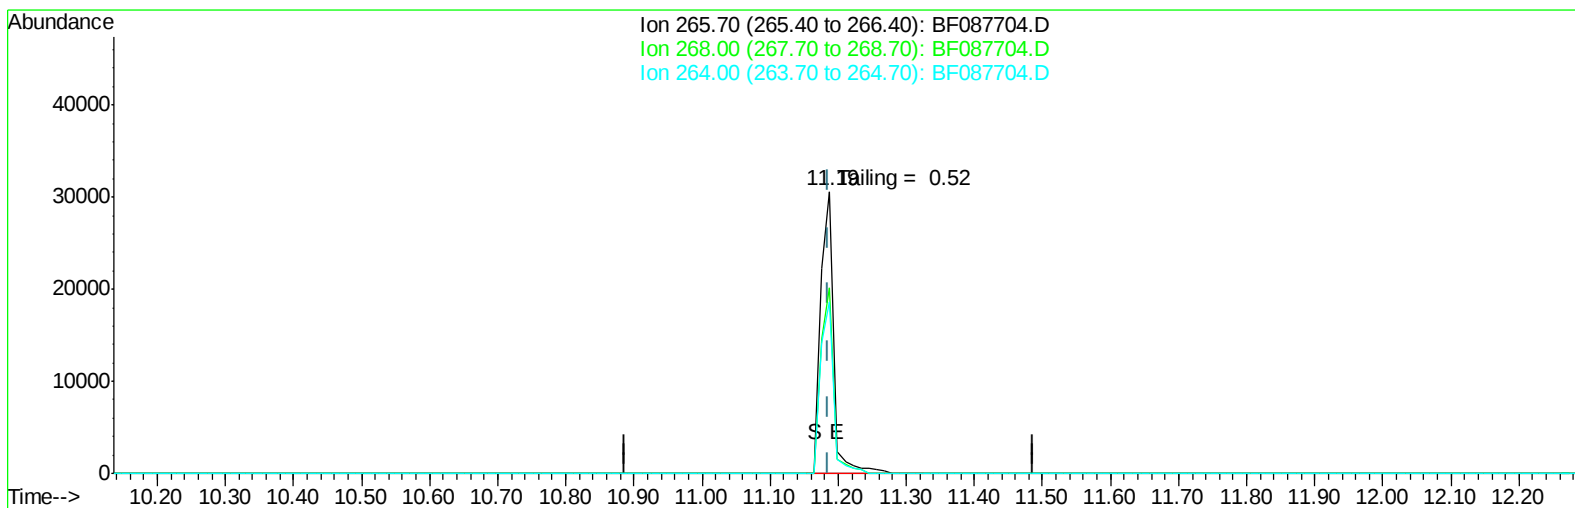

TIC: BF087704.D

(69) Pentachlorophenol (C)

11.188min (+0.001) 22455.73ng

response 40539

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	65.93
264.00	62.00	61.07
0.00	0.00	0.00