
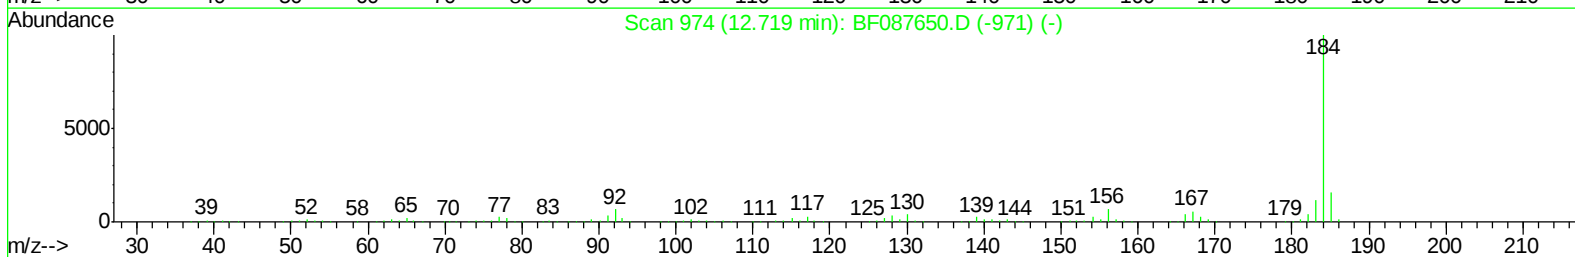
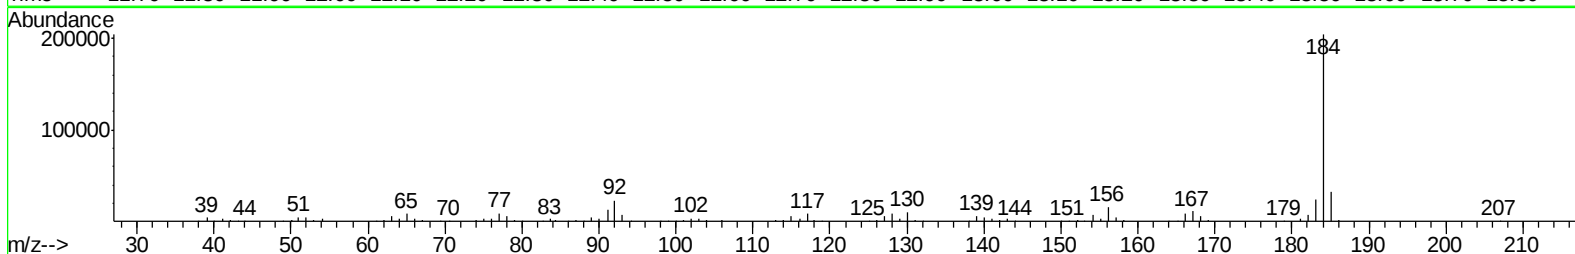


Data Path : Z:\HPCHEM1\BNA_F\Data\bf060516\
Data File : BF087729.D
Acq On : 6 Jun 2016 1:52
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 06:38:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

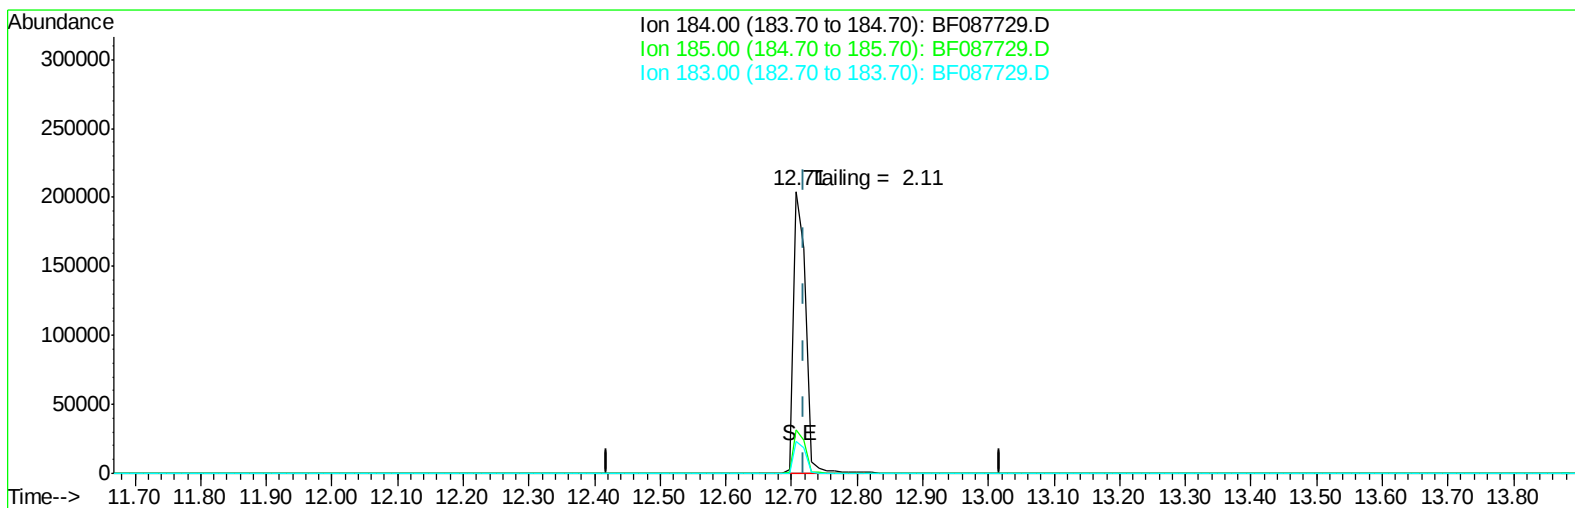

TIC: BF087729.D

(76) Benzidine




12.708min (-0.011) 0.00ng

response 268252

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	15.59
183.00	11.60	11.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\bf060516\
Data File : BF087729.D
Acq On : 6 Jun 2016 1:52
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 06:38:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

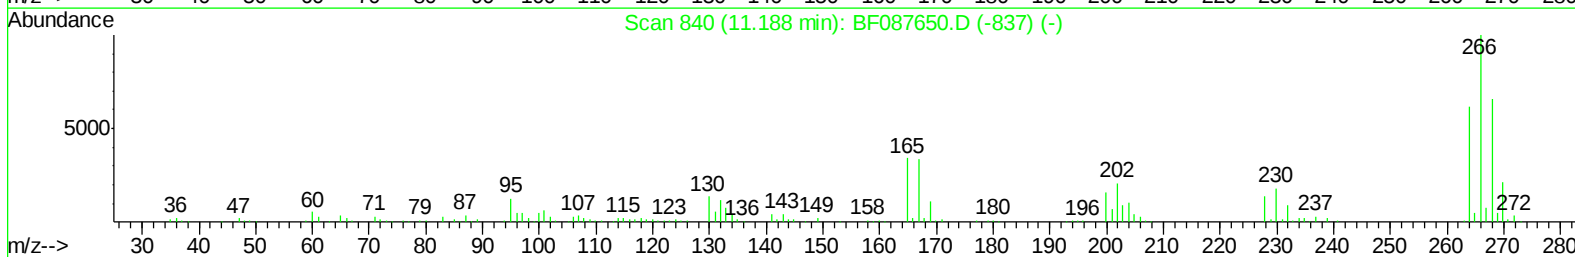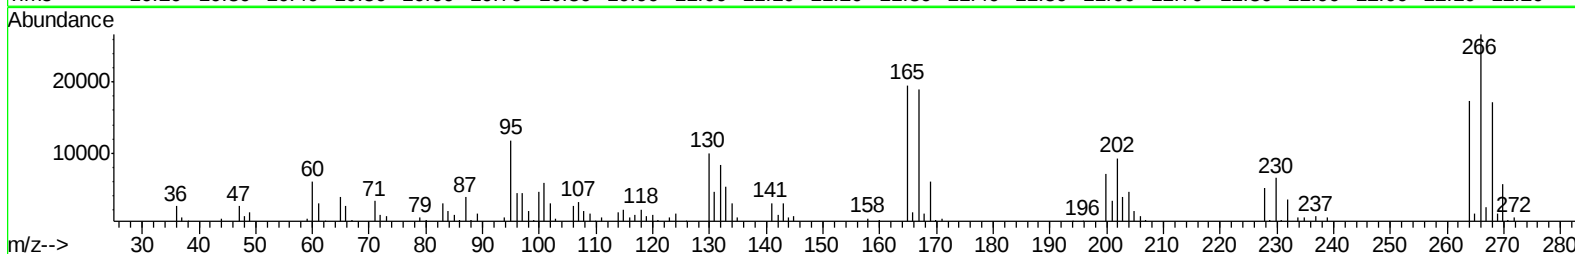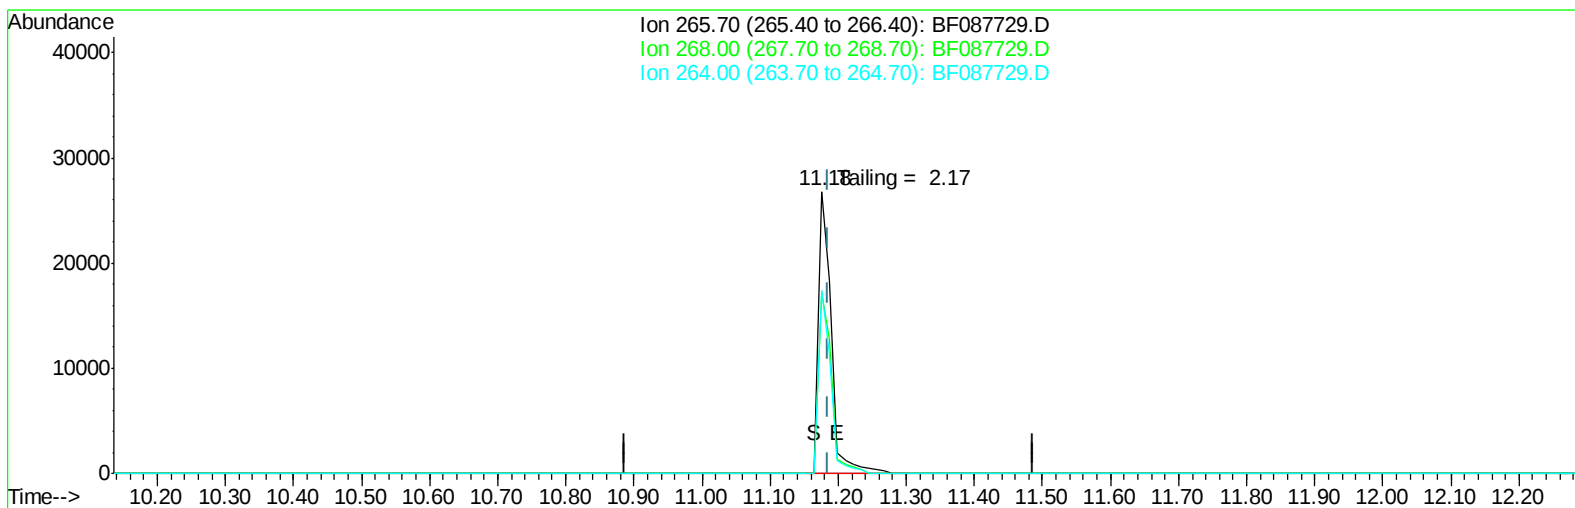

TIC: BF087729.D

(69) Pentachlorophenol (C)

11.176min (-0.011) 0.00ng

response 34908

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	64.22
264.00	62.00	64.81
0.00	0.00	0.00