

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060516\
 Data File : BF087733.D
 Acq On : 6 Jun 2016 3:51
 Operator : UM/SJ
 Sample : H3378-16
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-10

Quant Time: Jun 06 05:07:33 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	122612	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	481379	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	229181	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	443447	20.00	ng	0.00
75) Chrysene-d12	14.01	240	318727	20.00	ng	-0.01
86) Perylene-d12	15.44	264	249192	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	859401	113.29	ng	0.01
7) Phenol-d6	6.49	99	1055284	110.92	ng	0.00
23) Nitrobenzene-d5	7.43	82	762884	91.69	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	267661	116.35	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1207341	79.07	ng	-0.01
78) Terphenyl-d14	12.97	244	1038087	79.47	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.61	163	104028	6.24	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060516\
Data File : BF087733.D
Acq On : 6 Jun 2016 3:51
Operator : UM/SJ
Sample : H3378-16
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-10

Quant Time: Jun 06 05:07:33 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

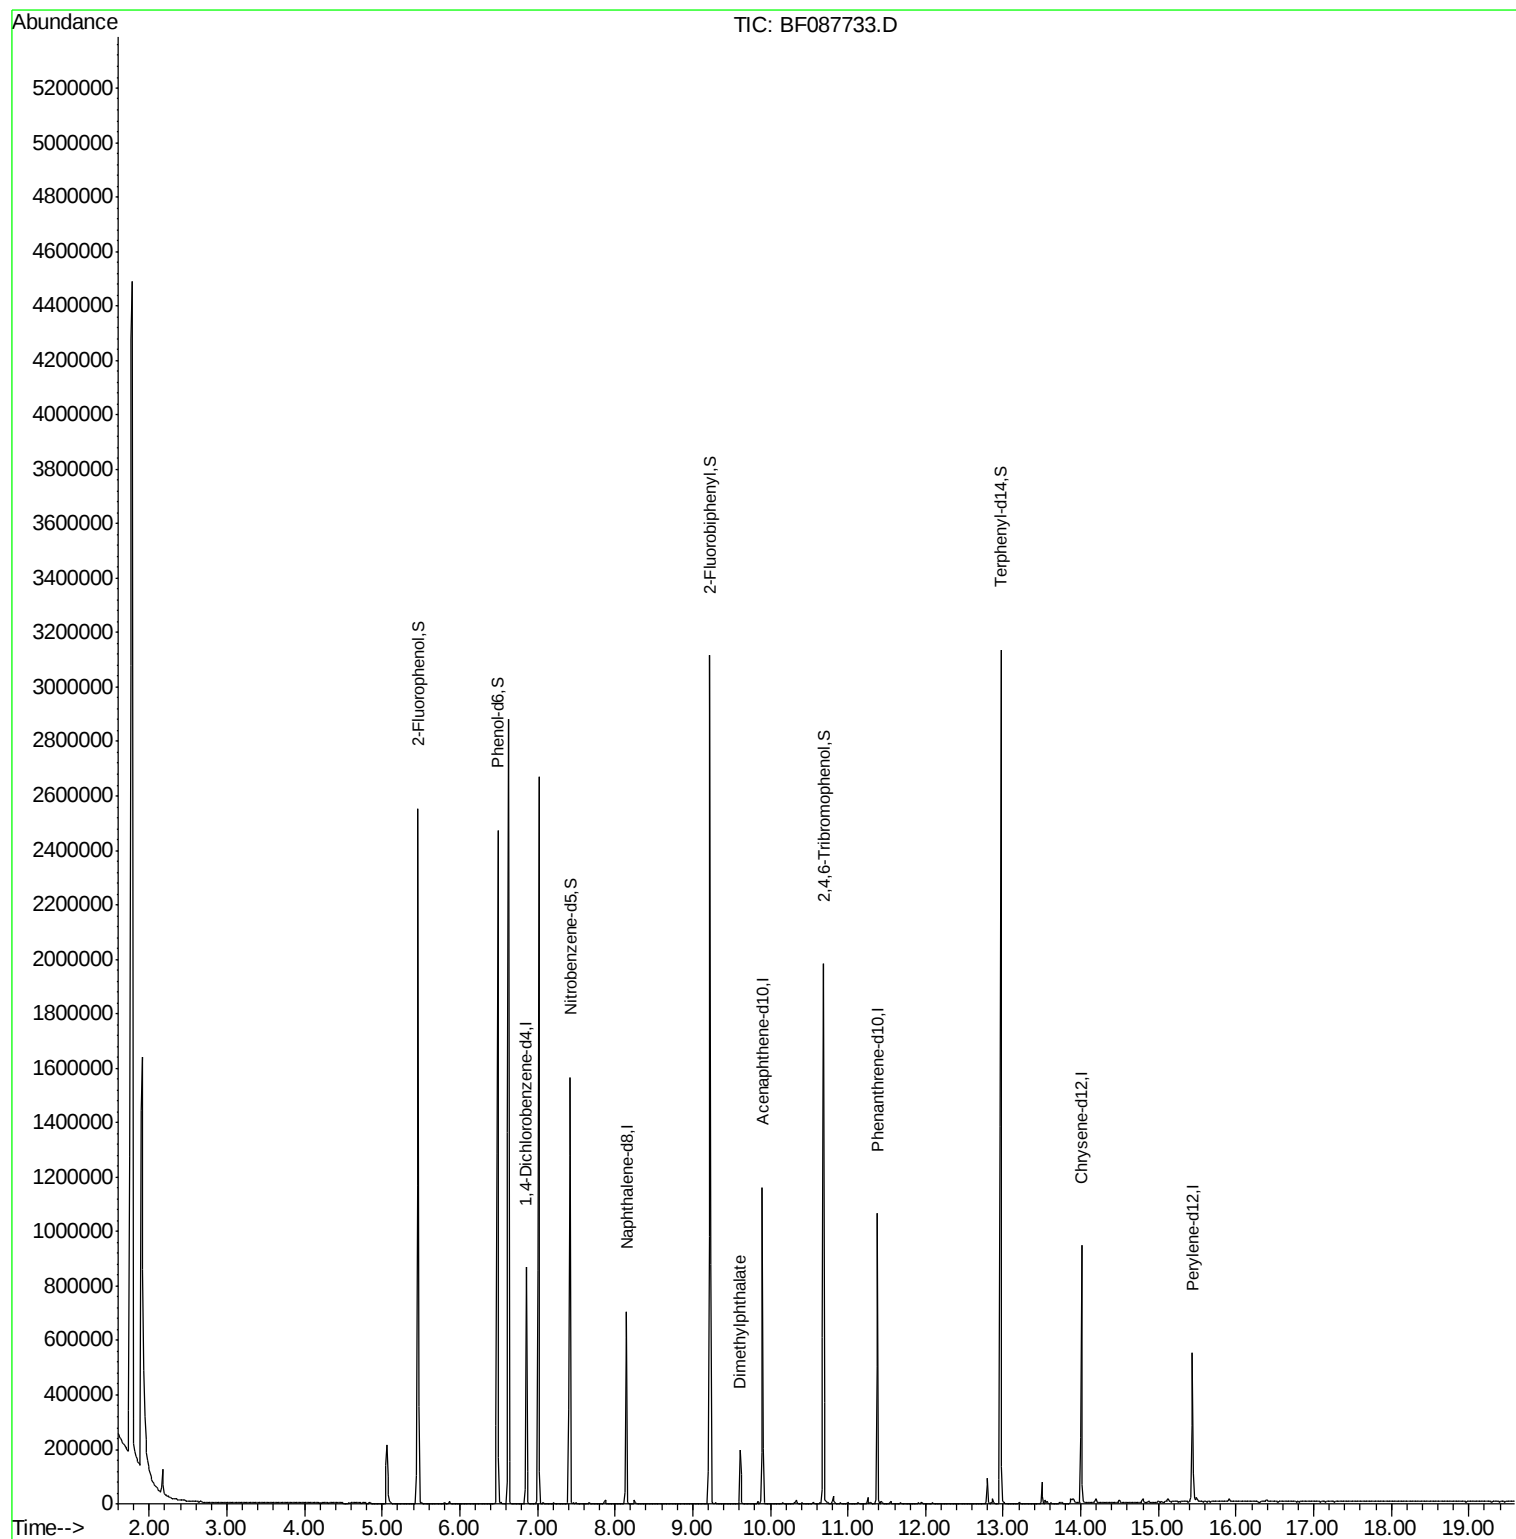

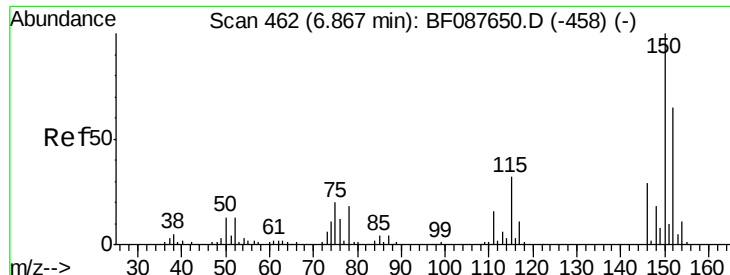

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 461

Delta R.T. -0.01 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51

Instrument :

BNA_F

ClientSampleId :

SB-10


Tot Ion:152 Resp: 122612

Ion Ratio Lower Upper

152 100

150 155.8 123.8 185.6




115 62.5 39.6 59.4#

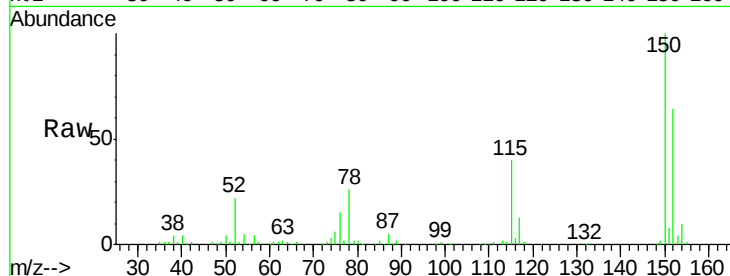

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

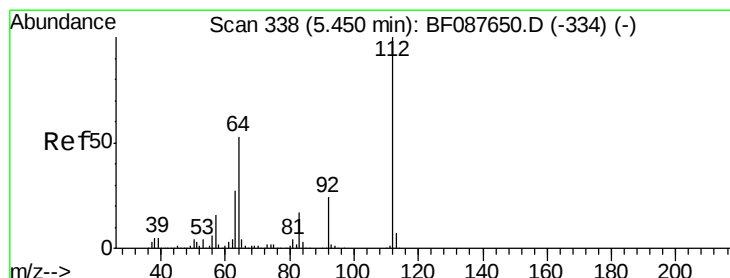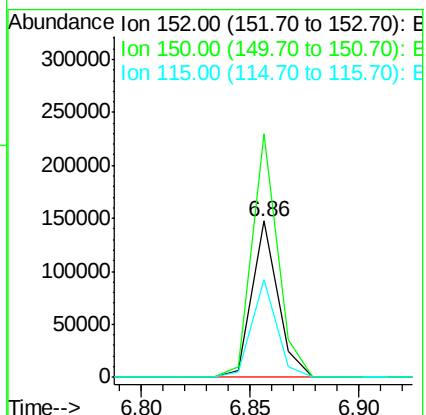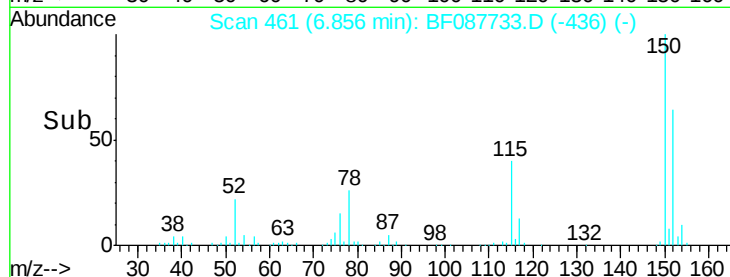

#5

2-Fluorophenol

Concen: 113.29 ng

RT: 5.46 min Scan# 339

Delta R.T. 0.01 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51


Tgt Ion:112 Resp: 859401

Ion Ratio Lower Upper

112 100

64 57.9 42.2 63.2



63 30.5 21.8 32.8

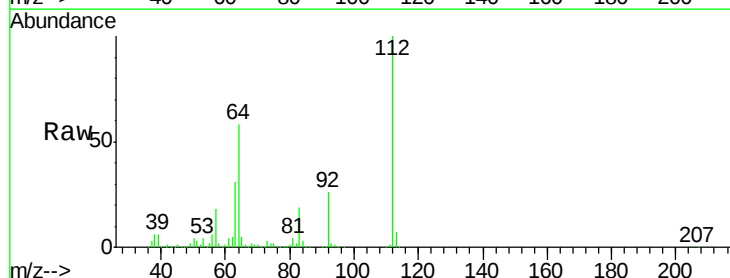


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

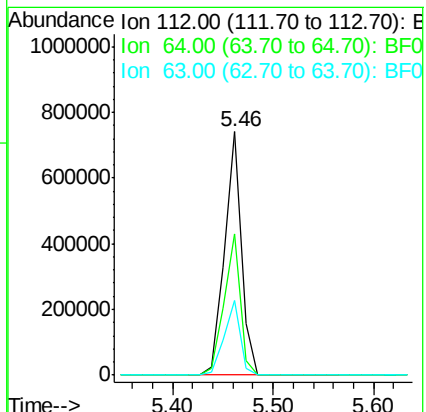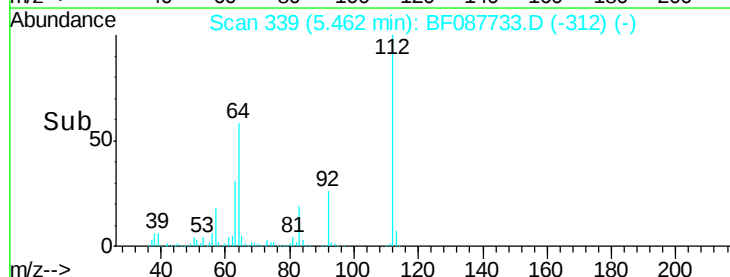



#7

Phenol-d6

Concen: 110.92 ng

RT: 6.49 min Scan# 429

Delta R.T. 0.00 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51

Instrument :

BNA_F

ClientSampleId :

SB-10


Tot Ion: 99 Resp: 1055284

Ion Ratio Lower Upper

99 100

42 17.8 12.2 18.2




71 34.2 23.4 35.0

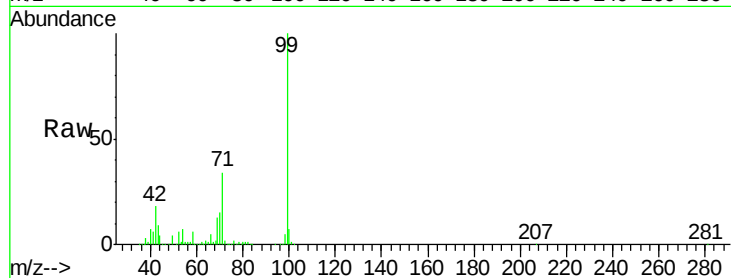

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

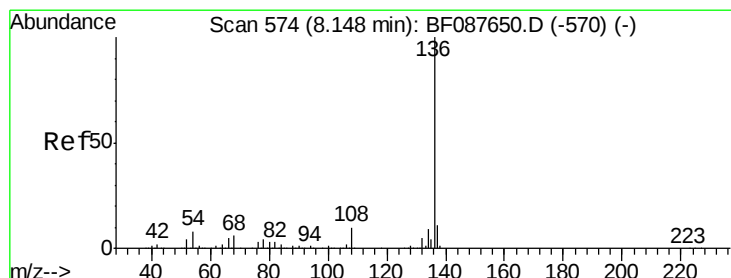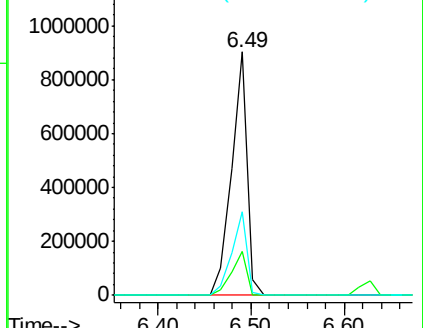

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 574

Delta R.T. 0.00 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51

Tgt Ion: 136 Resp: 481379


Ion Ratio Lower Upper

136 100

137 10.5 9.1 13.7

54 5.4 6.6 10.0#

68 4.5 5.1 7.7#


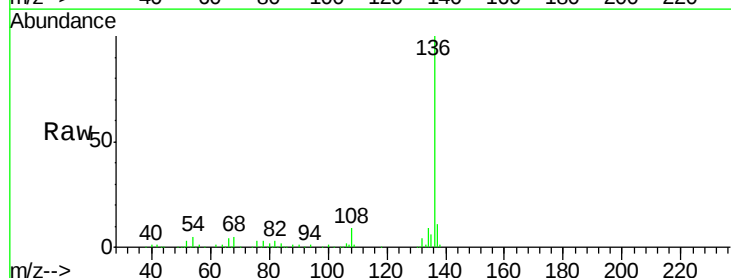



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

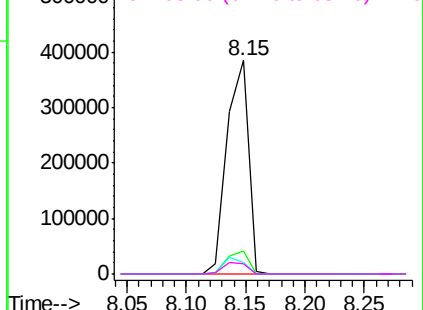







#23
 Nitrobenzene-d5
 Concen: 91.69 ng
 RT: 7.43 min Scan# 511
 Delta R.T. 0.00 min
 Lab File: BF087733.D
 Acq: 6 Jun 2016 3:51

Instrument :
 BNA_F
 ClientSampleID :
 SB-10

Tot Ion: 82 Resp: 762884
 Ion Ratio Lower Upper
 82 100
 128 55.3 35.9 53.9#
 54 44.2 40.9 61.3

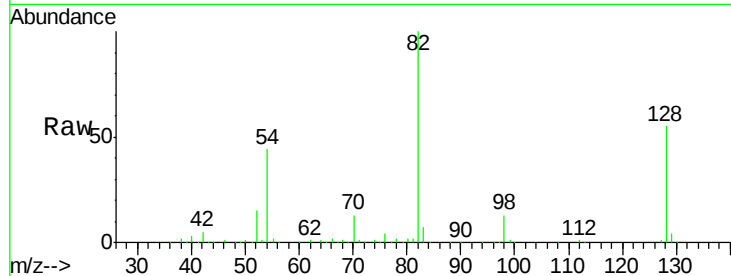


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

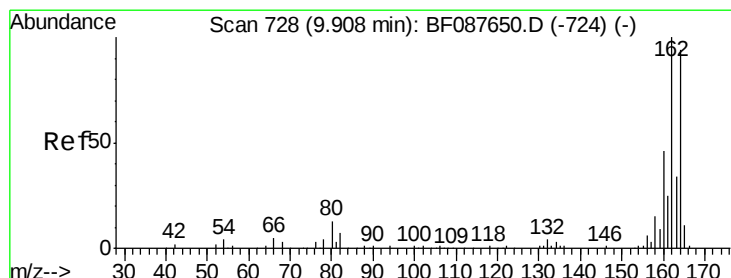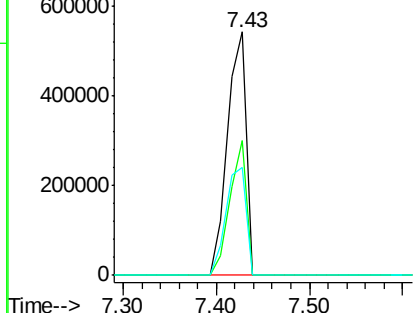




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 727
 Delta R.T. -0.01 min
 Lab File: BF087733.D
 Acq: 6 Jun 2016 3:51

Tgt Ion:164 Resp: 229181
 Ion Ratio Lower Upper
 164 100
 162 103.3 85.4 128.2
 160 46.5 39.5 59.3

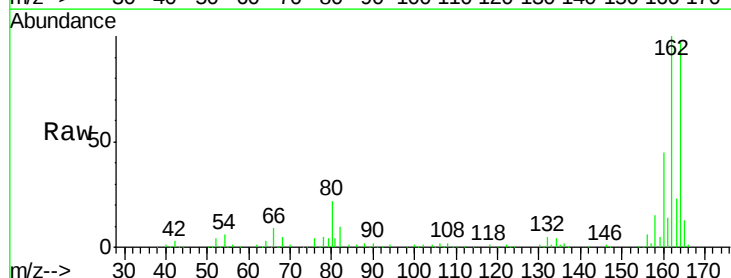

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

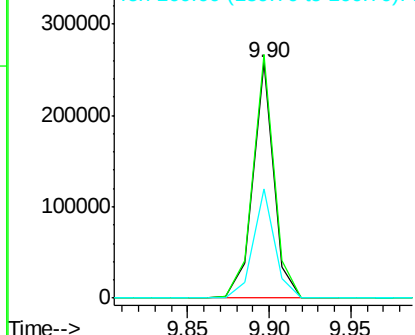


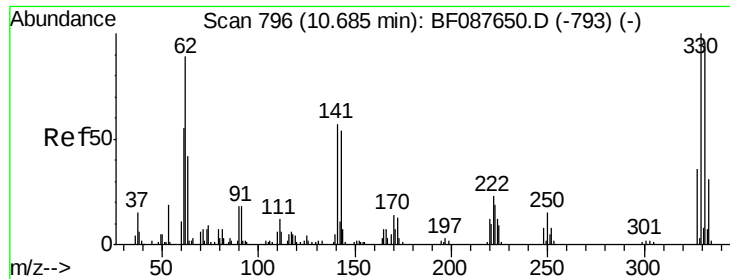




#41
 2,4,6-Tribromophenol
 Concen: 116.35 ng
 RT: 10.69 min Scan# 796
 Delta R.T. 0.00 min
 Lab File: BF087733.D
 Acq: 6 Jun 2016 3:51

Instrument :
 BNA_F
 ClientSampleId :
 SB-10

Tot Ion:330 Resp: 267661
 Ion Ratio Lower Upper
 330 100
 332 95.6 0.0 0.0#
 141 35.4 0.0 0.0#

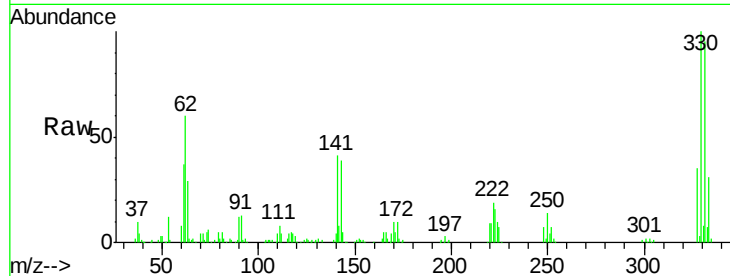


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

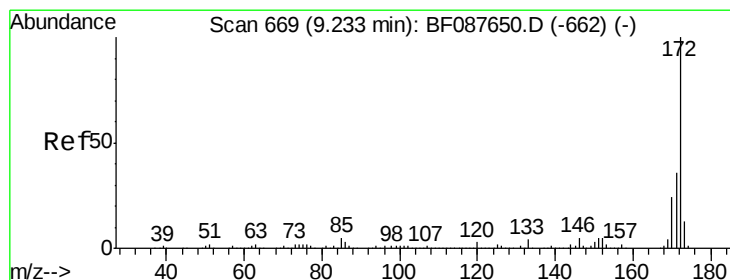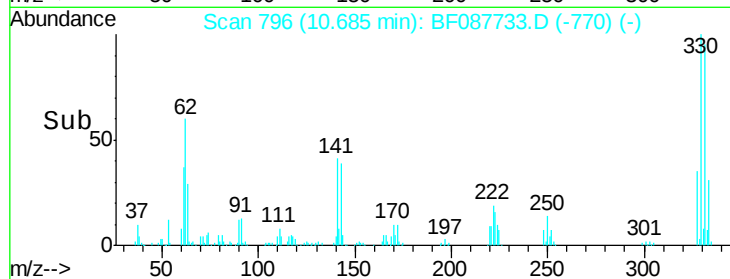
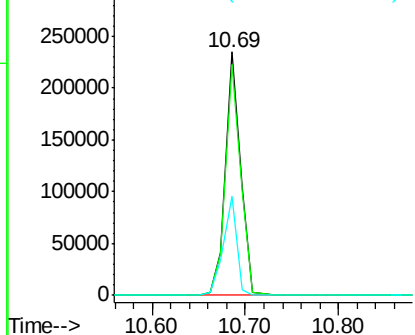



#44
 2-Fluorobiphenyl
 Concen: 79.07 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087733.D
 Acq: 6 Jun 2016 3:51

Tgt Ion:172 Resp: 1207341
 Ion Ratio Lower Upper
 172 100
 171 36.2 28.6 43.0
 170 24.5 19.2 28.8

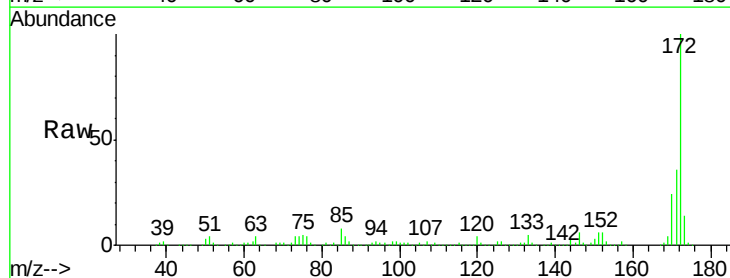

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

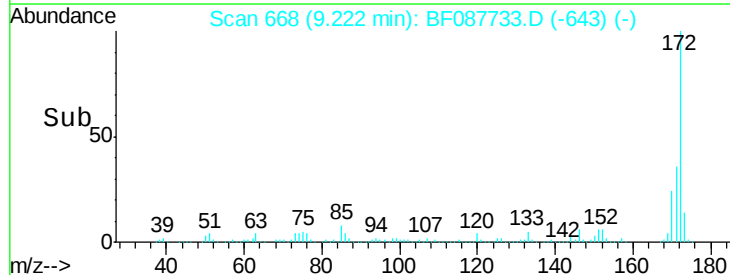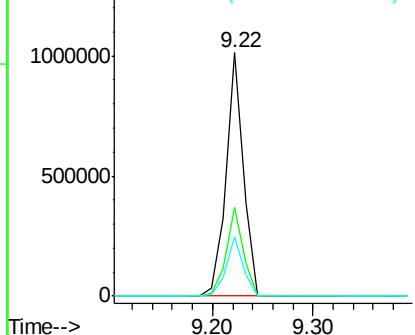



#49

Dimethylphthalate

Concen: 6.24 ng

RT: 9.61 min Scan# 702

Delta R.T. -0.02 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51

Instrument :

BNA_F

ClientSampleId :

SB-10


Tot Ion:163 Resp: 104028

Ion Ratio Lower Upper

163 100

194 2.9 2.8 4.2




164 10.7 8.3 12.5

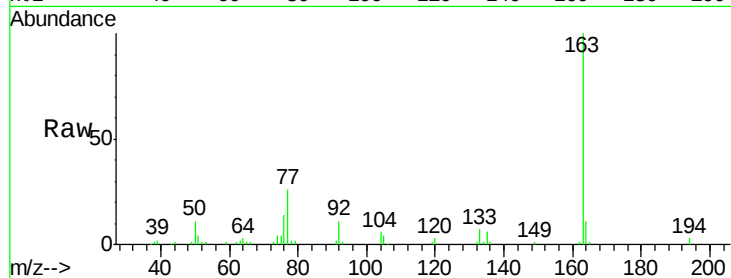

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

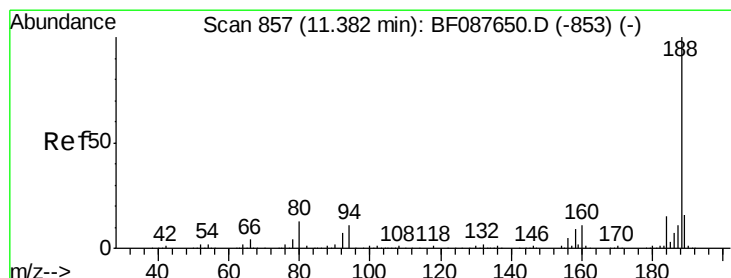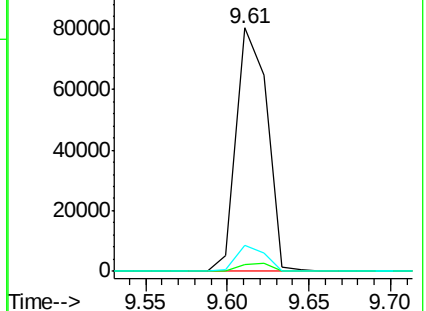

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.38 min Scan# 857

Delta R.T. 0.00 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51


Tgt Ion:188 Resp: 443447

Ion Ratio Lower Upper

188 100

94 7.7 9.0 13.6#



80 7.9 10.0 15.0#

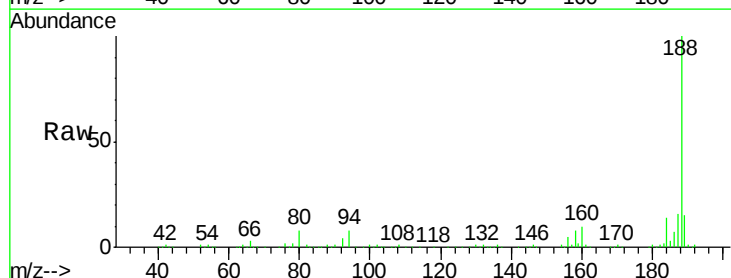


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

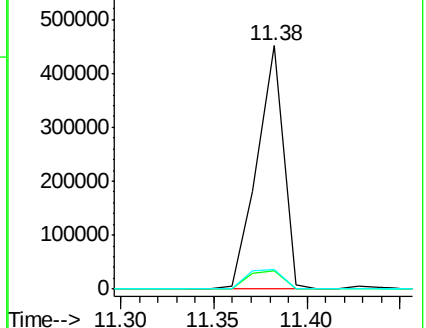

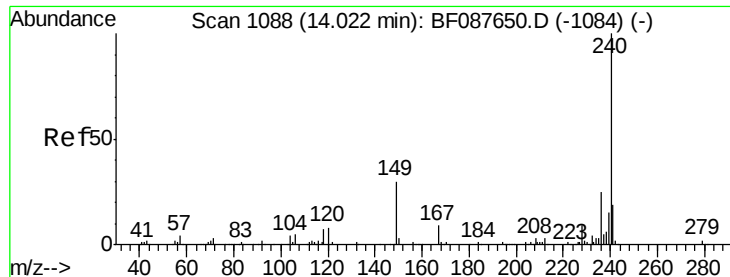

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1087

Delta R.T. -0.01 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51

Instrument :

BNA_F

ClientSampleId :

SB-10


Tot Ion:240 Resp: 318727

Ion Ratio Lower Upper

240 100

120 12.3 6.8 10.2#




236 25.4 20.2 30.2

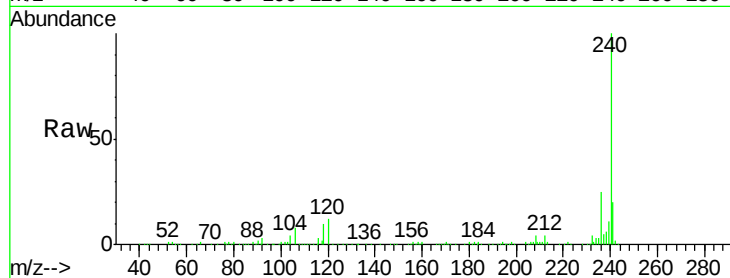

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

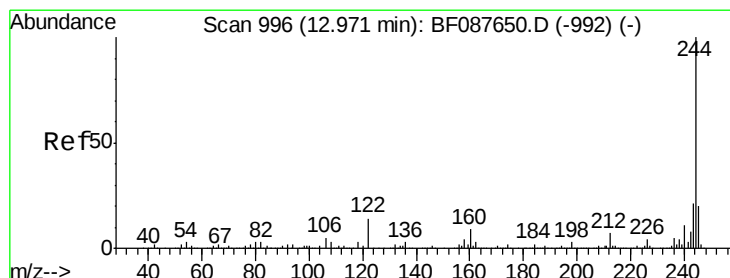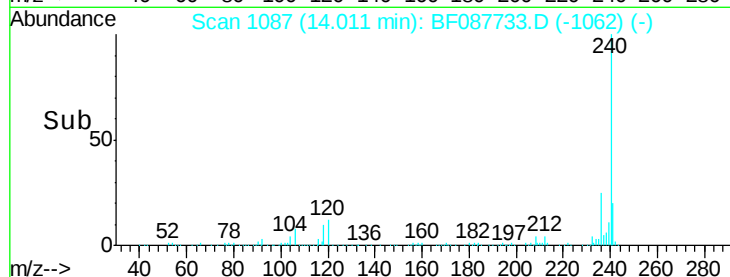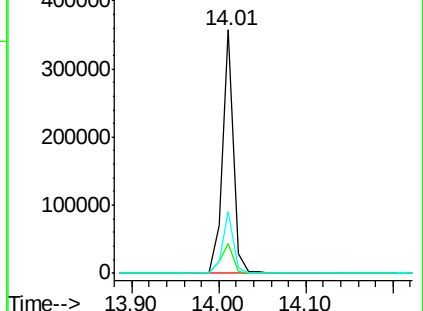

#78

Terphenyl-d14

Concen: 79.47 ng

RT: 12.97 min Scan# 996

Delta R.T. 0.00 min

Lab File: BF087733.D

Acq: 6 Jun 2016 3:51


Tgt Ion:244 Resp: 1038087

Ion Ratio Lower Upper

244 100

212 7.6 6.0 9.0



122 13.1 11.2 16.8

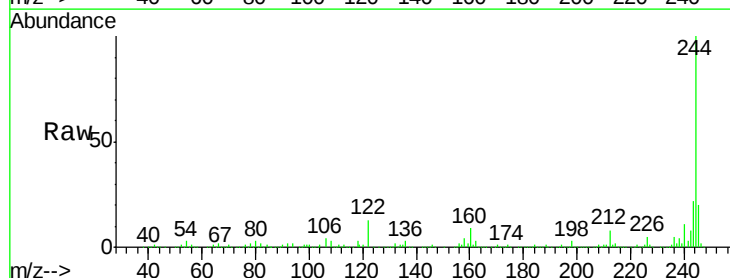


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

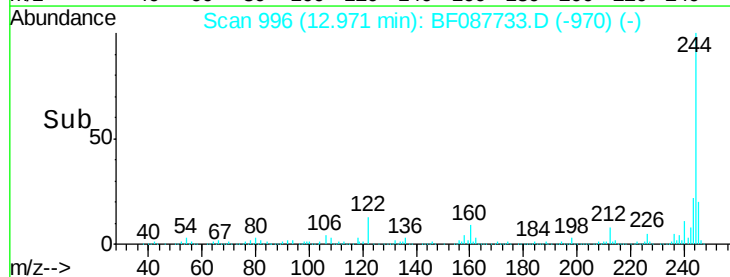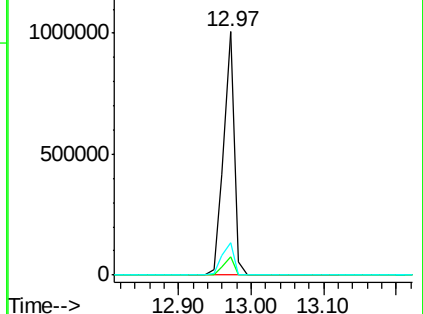



#86
Pervlène-d12
Concen: 20.00 ng
RT: 15.44 min Scan# 1212
Delta R.T. 0.00 min
Lab File: BF087733.D
Acq: 6 Jun 2016 3:51

Instrument :
BNA_F
ClientSampleId :
SB-10

Tot Ion: 264 Resp: 249192

Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.6	16.9	25.3

