

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060516\
 Data File : BF087737.D
 Acq On : 6 Jun 2016 5:50
 Operator : UM/SJ
 Sample : H3190-13RE
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1672(0-4)RE

Manual Integrations
 APPROVED

SOHIL
 6/6/2016 7:25:30 PM

Quant Time: Jun 06 12:27:54 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 04 11:07:28 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	162411	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	706783	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	298106	20.00	ng	-0.01
63) Phenanthrene-d10	11.38	188	522507	20.00	ng	0.00
75) Chrysene-d12	14.02	240	344581	20.00	ng	0.00
86) Perylene-d12	15.45	264	346711	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	499468	49.71	ng	0.00
7) Phenol-d6	6.49	99	773962	61.42	ng	0.00
23) Nitrobenzene-d5	7.43	82	491479	40.23	ng	0.00
41) 2,4,6-Tribromophenol	10.70	330	348360	116.42	ng	0.01
44) 2-Fluorobiphenyl	9.22	172	1010927	45.26	ng	-0.01
78) Terphenyl-d14	12.97	244	1141874	80.86	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	9.62	163	516814	23.85	ng	100
70) Phenanthrene	11.41	178	162572	5.74	ng	98
71) Anthracene	11.45	178	64737	2.28	ng	98
74) Fluoranthene	12.59	202	485069	17.40	ng	97
77) Pyrene	12.82	202	460435	18.76	ng	99
80) Benzo(a)anthracene	14.01	228	248373	12.49	ng	95
82) Chrysene	14.05	228	225898	11.41	ng	97
85) Indeno(1,2,3-cd)pyrene	16.83	276	139672	8.54	ng	# 100
87) Benzo(b)fluoranthene	15.04	252	370755m	16.44	ng	
88) Benzo(k)fluoranthene	15.06	252	114138m	6.08	ng	
89) Benzo(a)pyrene	15.38	252	187760	9.90	ng	97
90) Dibenzo(a,h)anthracene	16.85	278	34845m	2.16	ng	
91) Benzo(a,h,i)perylene	17.26	276	120000	7.37	ng	# 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060516\
Data File : BF087737.D
Acq On : 6 Jun 2016 5:50
Operator : UM/SJ
Sample : H3190-13RE
Misc :
ALS Vial : 73 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
CHS-STA-1672(0-4)RE

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

Quant Time: Jun 06 12:27:54 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 04 11:07:28 2016
Response via : Initial Calibration

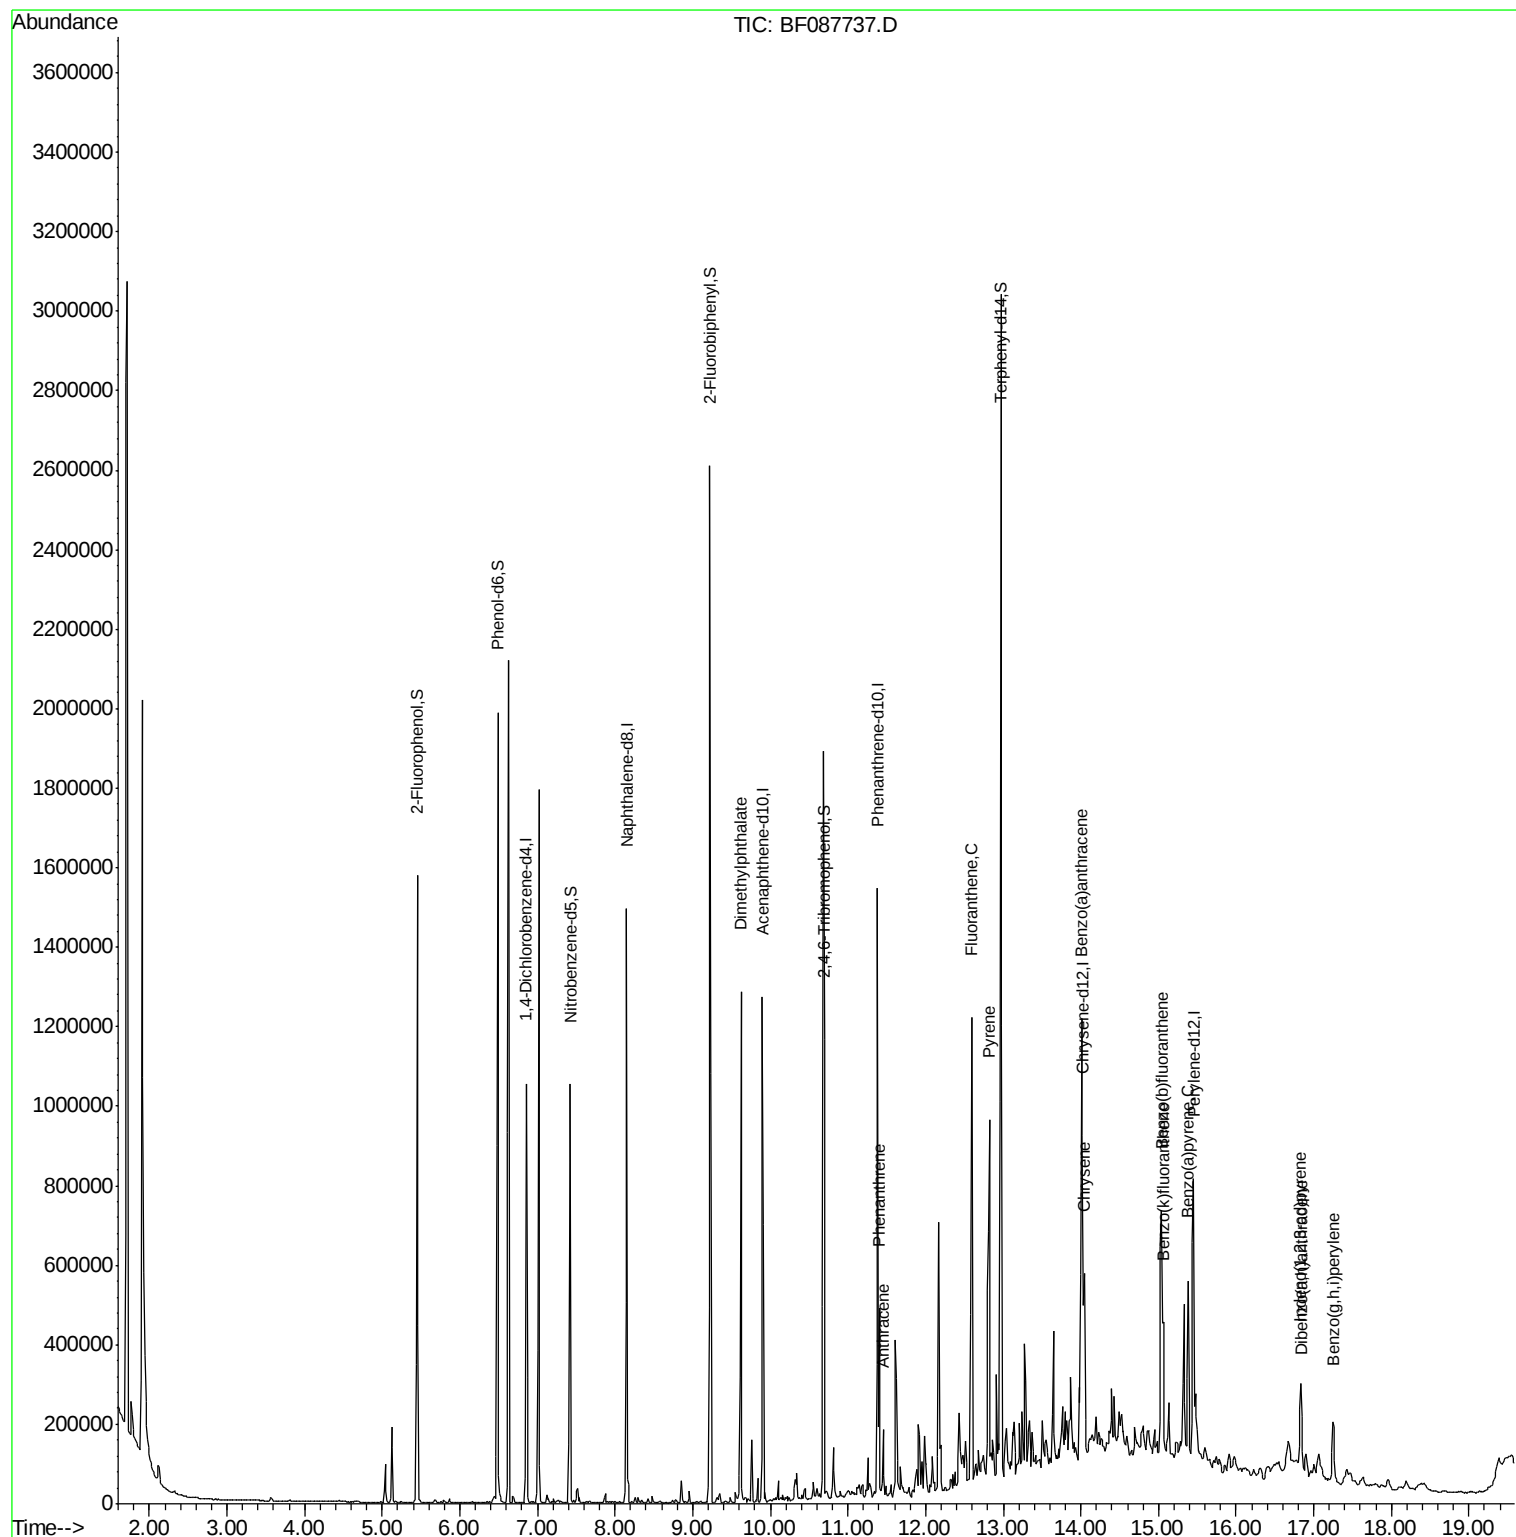

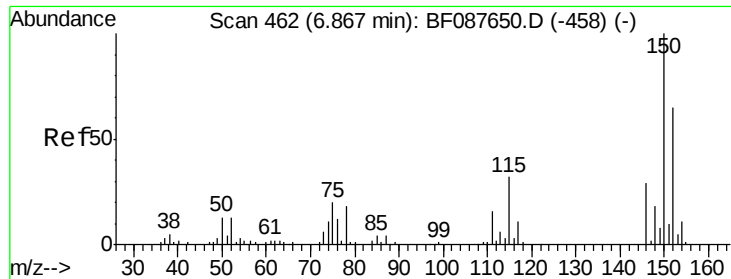

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 461

Delta R.T. -0.01 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Instrument :

BNA_F





ClientSampleId :

CHS-STA-1672(0-4)RE

Tot Ion:	152	Resp:	162411
Ion Ratio	Lower	Upper	
152	100		
150	159.3	123.8	185.6
115	67.4	39.6	59.4

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

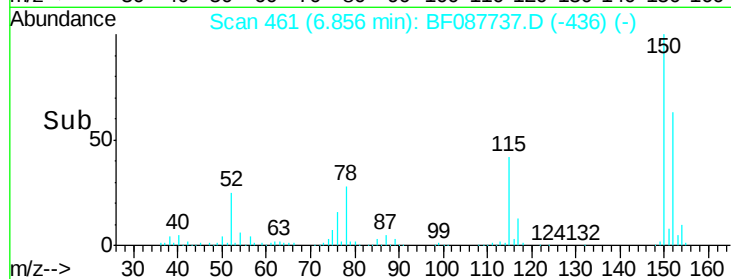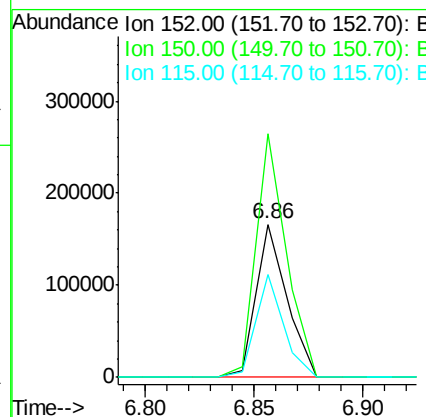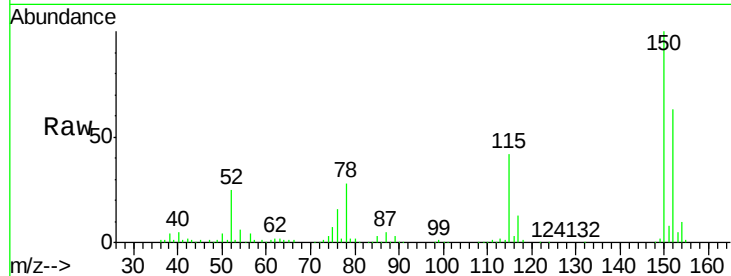

#5

2-Fluorophenol

Concen: 49.71 ng




RT: 5.45 min Scan# 338




Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion:	112	Resp:	499468
Ion Ratio	Lower	Upper	
112	100		
64	59.2	42.2	63.2
63	30.5	21.8	32.8

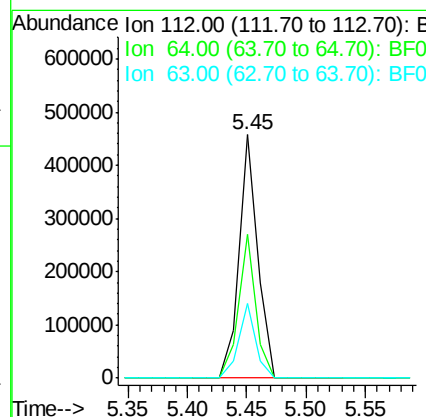

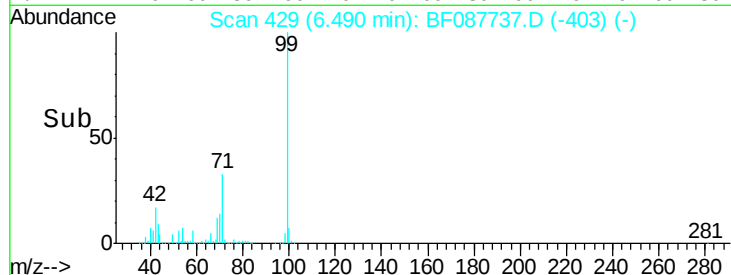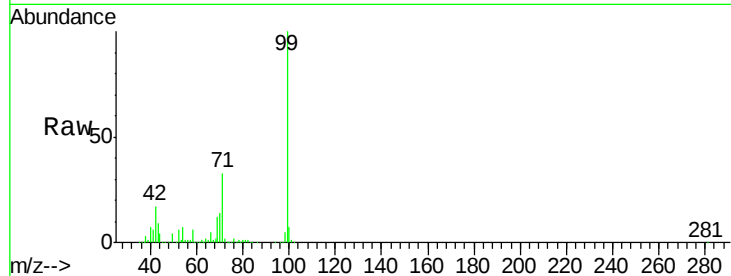

#7

Phenol-d6

Concen: 61.42 ng

RT: 6.49 min Scan# 429

Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tot Ion	Ion	Ratio	Resp	Lower	Upper
99	100		773962		
42	17.0	12.2	18.2		
71	33.3	23.4	35.0		

Instrument :





BNA_F

ClientSampleId :

CHS-STA-1672(0-4)RE

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

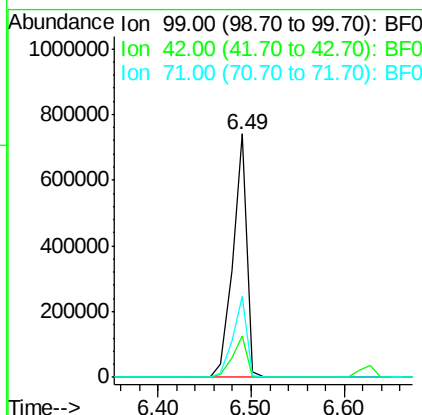

#21

Naphthalene-d8

Concen: 20.00 ng


RT: 8.15 min Scan# 574


Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
136	100		706783		
137	11.1	9.1	13.7		
54	6.7	6.6	10.0		
68	5.4	5.1	7.7		

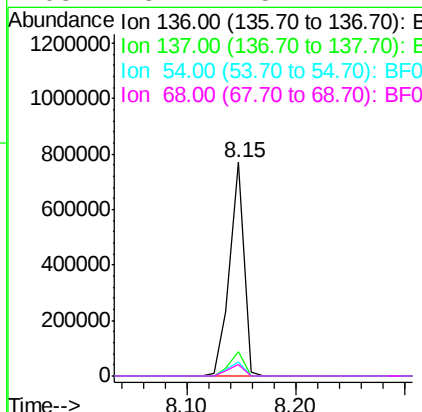




#23
 Nitrobenzene-d5
 Concen: 40.23 ng
 RT: 7.43 min Scan# 511
 Delta R.T. 0.00 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1672(0-4)RE




Tot Ion	Ratio	Resp	Lower	Upper
82	100	491479		
128	56.4	35.9	53.9#	
54	42.6	40.9	61.3	

Manual Integrations
 APPROVED

SOHIL
 6/6/2016 7:25:30 PM

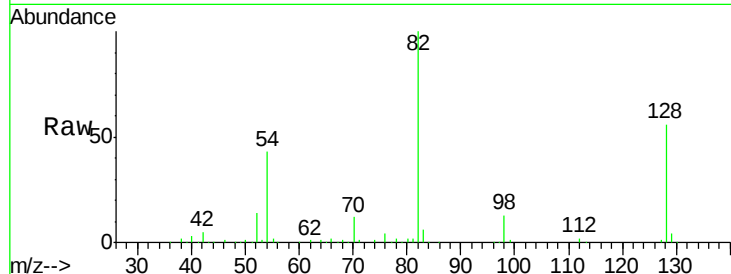


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

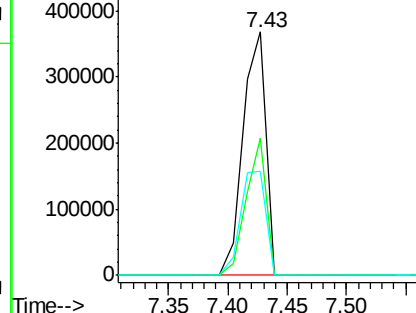




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 727
 Delta R.T. -0.01 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Resp	Lower	Upper
164	100	298106		
162	104.4	85.4	128.2	
160	46.5	39.5	59.3	



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

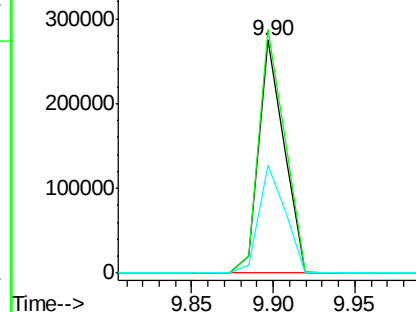

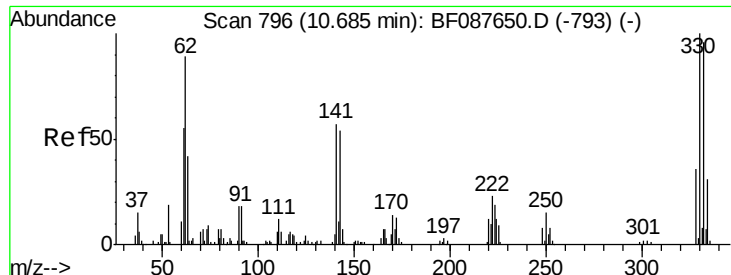





#41
 2,4,6-Tribromophenol
 Concen: 116.42 ng
 RT: 10.70 min Scan# 797
 Delta R.T. 0.01 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1672(0-4)RE

Tot Ion	Ratio	Resp Lower	Upper
330	100		
332	96.8	0.0	0.0#
141	29.9	0.0	0.0#




Manual Integrations
 APPROVED


SOHIL
 6/6/2016 7:25:30 PM

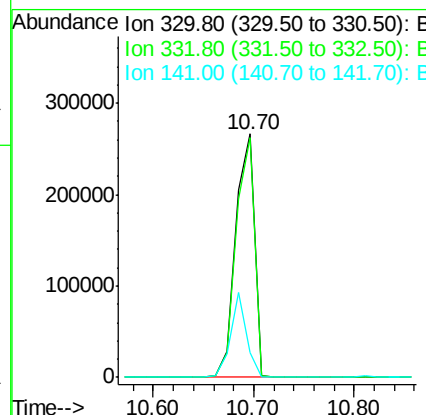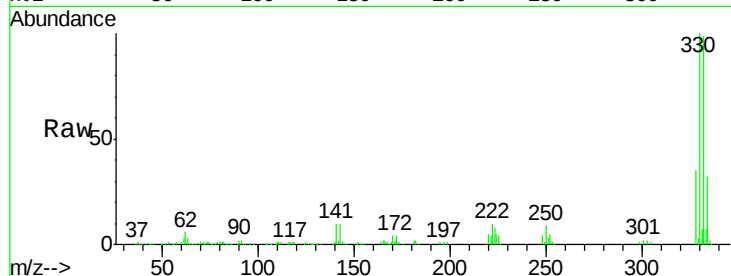

#44
 2-Fluorobiphenyl
 Concen: 45.26 ng
 RT: 9.22 min Scan# 668
 Delta R.T. -0.01 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Resp Lower	Upper
172	100		
171	35.9	28.6	43.0
170	23.9	19.2	28.8

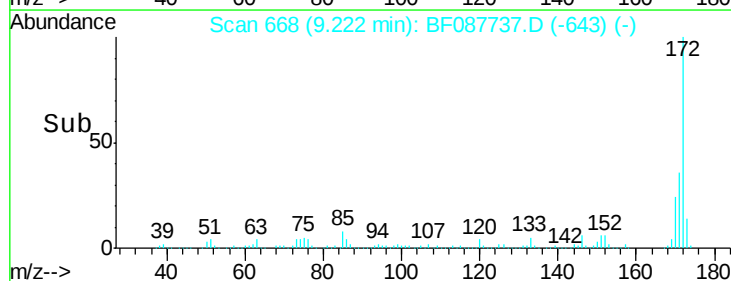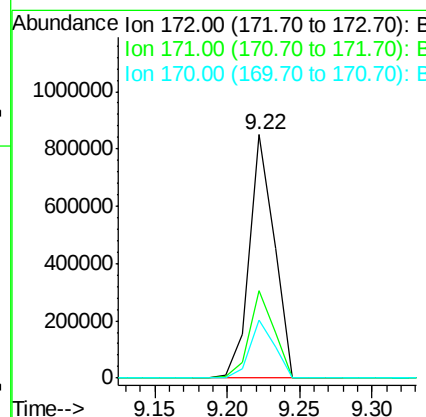

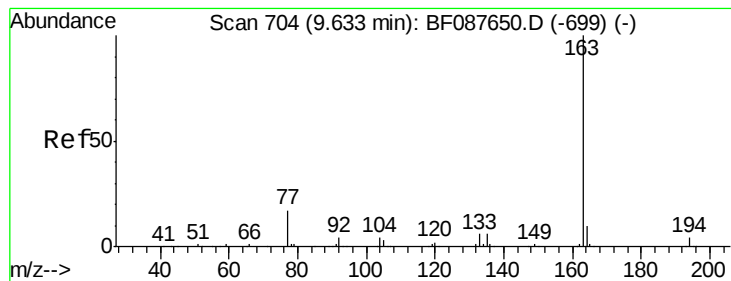

#49

Dimethylphthalate

Concen: 23.85 ng

RT: 9.62 min Scan# 703

Delta R.T. -0.01 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Instrument :

BNA_F





ClientSampleId :

CHS-STA-1672(0-4)RE

Tot Ion:	163	Resp:	516814
Ion Ratio	Lower	Upper	
163	100		
194	3.4	2.8	4.2
164	10.2	8.3	12.5

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

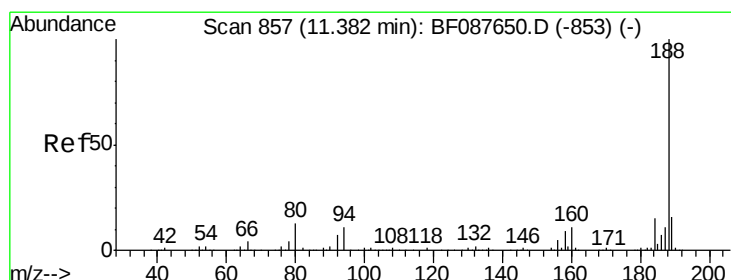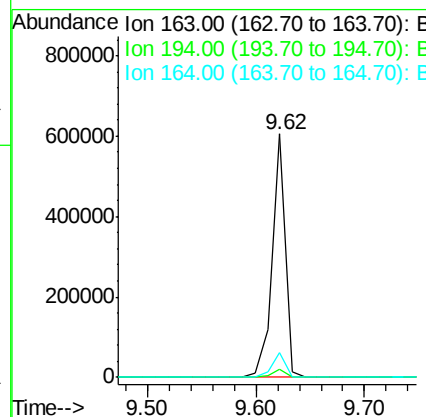

#63

Phenanthrene-d10

Concen: 20.00 ng




RT: 11.38 min Scan# 857


Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion:	188	Resp:	522507
Ion Ratio	Lower	Upper	
188	100		
94	10.7	9.0	13.6
80	11.2	10.0	15.0

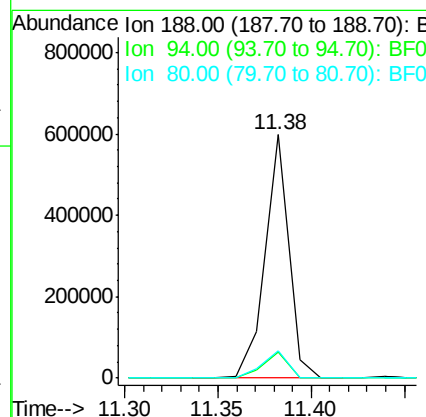



#70

Phenanthrene

Concen: 5.74 ng

RT: 11.41 min Scan# 859

Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Instrument :

BNA_F





ClientSampleId :

CHS-STA-1672(0-4)RE

Tot Ion:178	Resp:	162572
Ion Ratio	Lower	Upper
178	100	
176	19.0	15.8 23.6
179	15.2	13.0 19.4

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

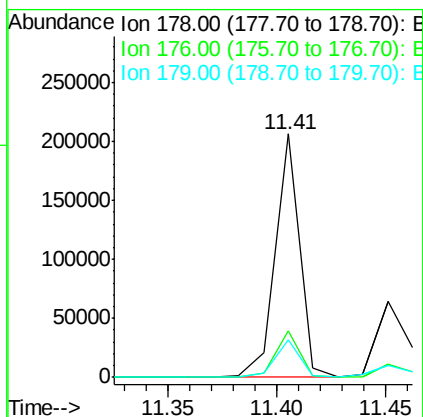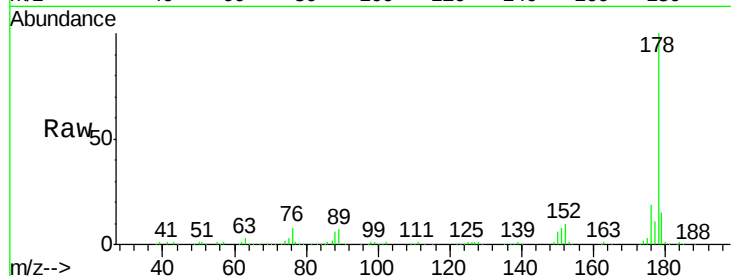

#71

Anthracene

Concen: 2.28 ng




RT: 11.45 min Scan# 863


Delta R.T. -0.01 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion:178	Resp:	64737
Ion Ratio	Lower	Upper
178	100	
176	17.9	15.6 23.4
179	15.6	12.8 19.2

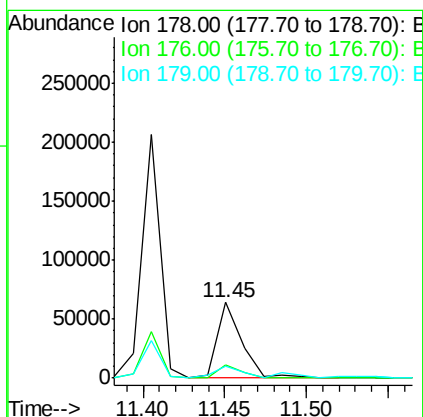

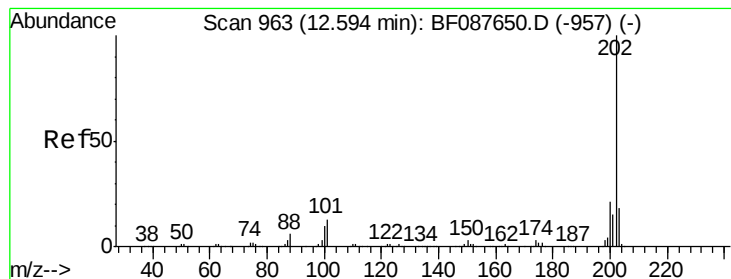





#74
 Fluoranthene
 Concen: 17.40 ng
 RT: 12.59 min Scan# 963
 Delta R.T. 0.00 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1672(0-4)RE

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	10.3	0.0	33.1
203	17.9	0.0	38.1




Manual Integrations
 APPROVED


SOHIL
 6/6/2016 7:25:30 PM

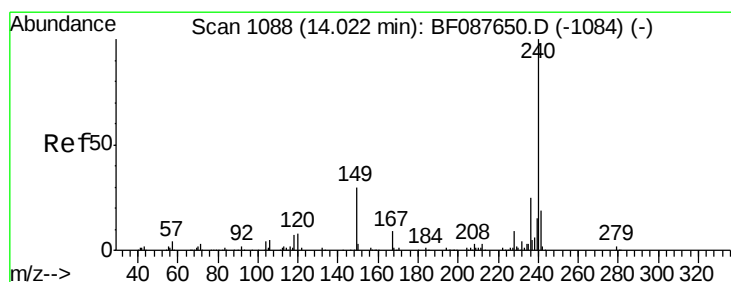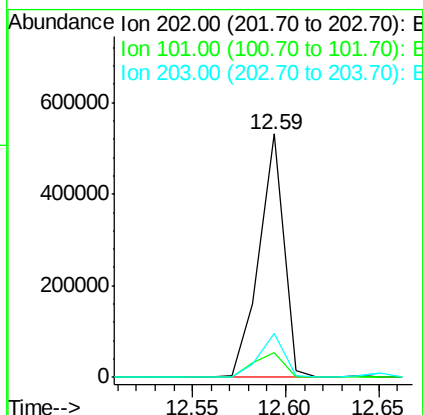

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 14.02 min Scan# 1088
 Delta R.T. 0.00 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Resp Lower	Upper
240	100		
120	7.2	6.8	10.2
236	25.1	20.2	30.2

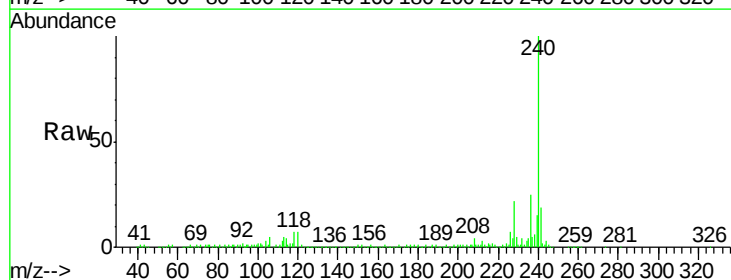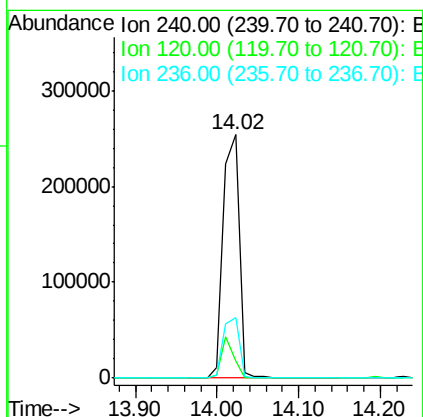







#77
Pvrene
Concen: 18.76 ng
RT: 12.82 min Scan# 983
Delta R.T. 0.00 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Instrument :
BNA_F
ClientSampleId :
CHS-STA-1672(0-4)RE

Tot Ion	Ratio	Lower	Upper
202	100		
200	21.0	17.4	26.2
203	17.7	14.5	21.7




Manual Integrations
APPROVED


SOHIL
6/6/2016 7:25:30 PM

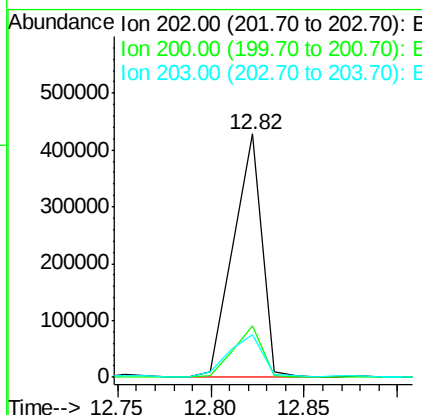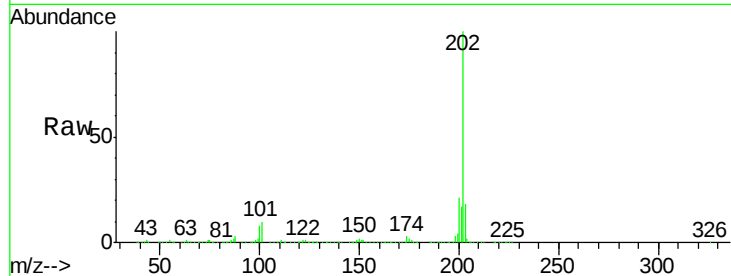

#78
Terphenyl-d14
Concen: 80.86 ng
RT: 12.97 min Scan# 996
Delta R.T. 0.00 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.7	6.0	9.0
122	14.2	11.2	16.8

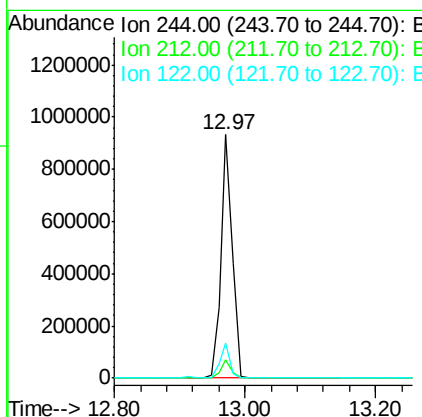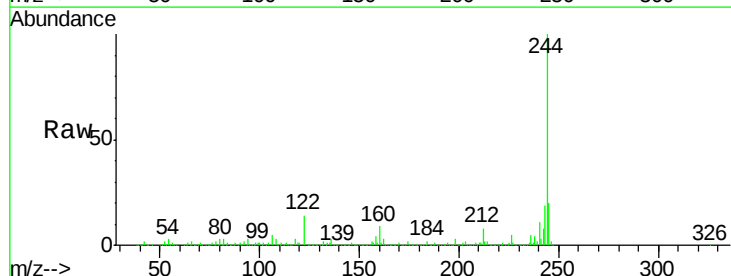

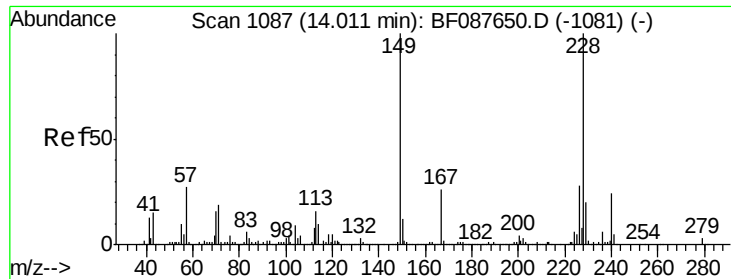





#80
Benzo(a)anthracene
Concen: 12.49 ng
RT: 14.01 min Scan# 1087
Delta R.T. 0.00 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Instrument :
BNA_F
ClientSampleId :
CHS-STA-1672(0-4)RE

Tot Ion	Ratio	Lower	Upper
228	100		
226	31.6	22.3	33.5
229	21.2	16.0	24.0




Manual Integrations
APPROVED


SOHIL
6/6/2016 7:25:30 PM

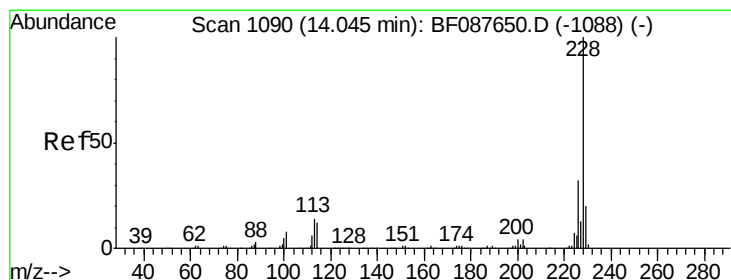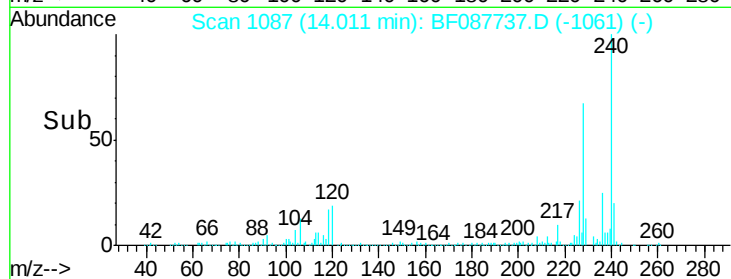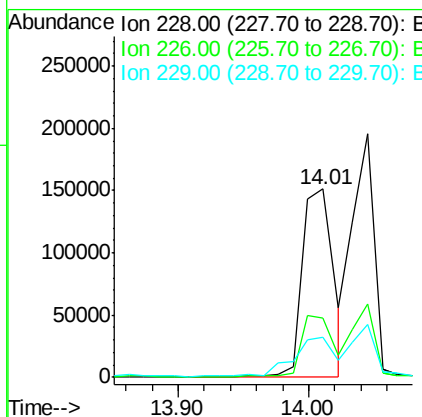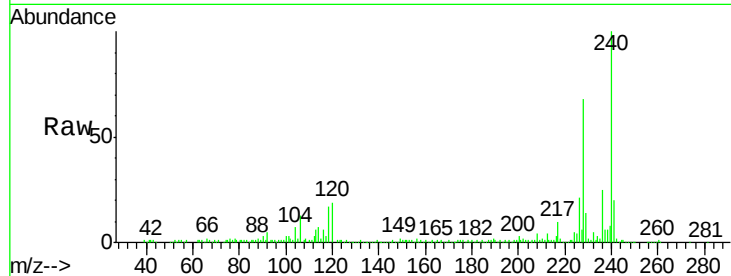

#82
Chrysene
Concen: 11.41 ng
RT: 14.05 min Scan# 1090
Delta R.T. 0.00 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	25.4	38.2
229	21.5	16.3	24.5

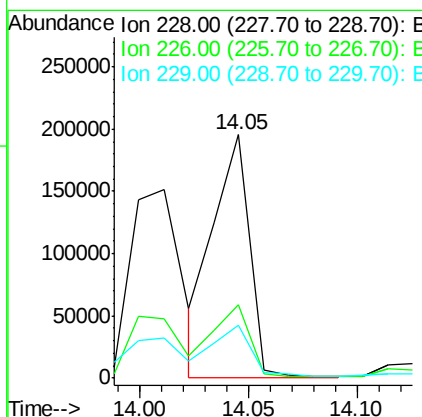

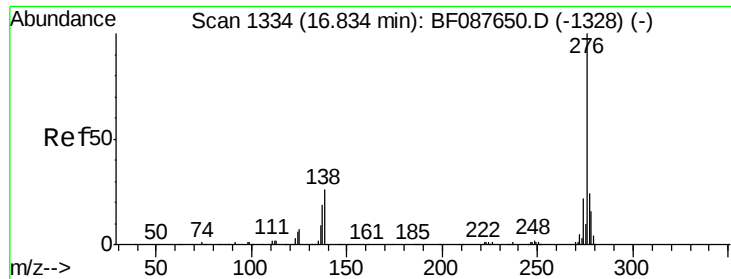


#85
Indeno(1,2,3-cd)pyrene
Concen: 8.54 ng
RT: 16.83 min Scan# 1334
Delta R.T. 0.00 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Instrument :
BNA_F
ClientSampleId :
CHS-STA-1672(0-4)RE




Tot Ion	Ratio	Resp Lower	Upper
276	100		
138	25.0	0.0	0.0#
277	25.3	0.0	0.0#

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM




Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E


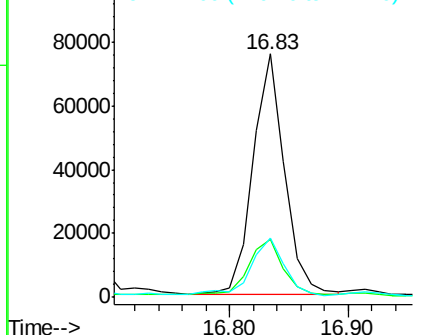



#86
Perylene-d12
Concen: 20.00 ng
RT: 15.45 min Scan# 1213
Delta R.T. 0.01 min
Lab File: BF087737.D
Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Resp Lower	Upper
264	100		
260	23.4	19.2	28.8
265	21.9	16.9	25.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

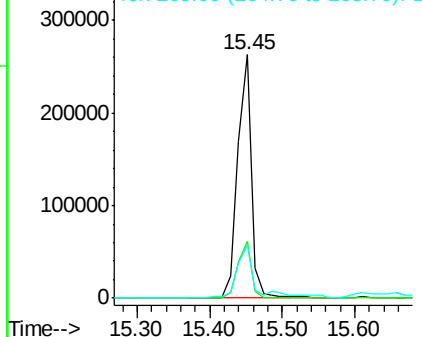

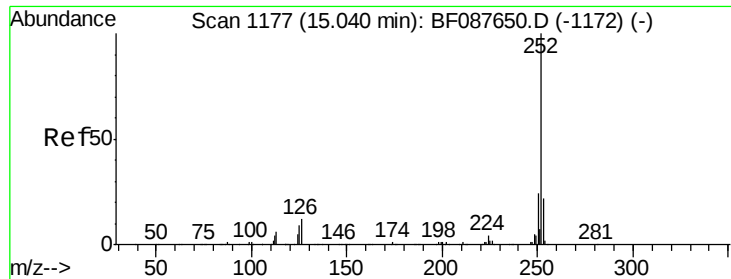

#87

Benzo(b)fluoranthene

Concen: 16.44 ng m

RT: 15.04 min Scan# 1177

Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Instrument :

BNA_F


ClientSampleId :

CHS-STA-1672(0-4)RE




Tot Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.4	26.2
125	12.7	7.1	10.7

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

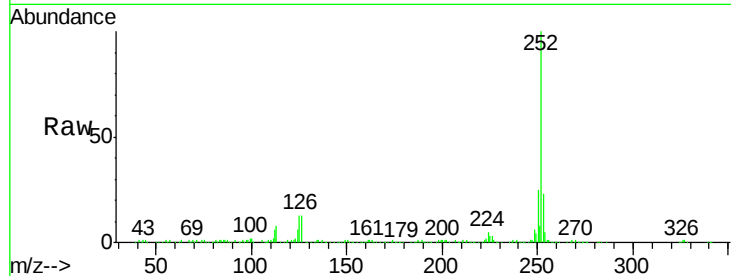

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

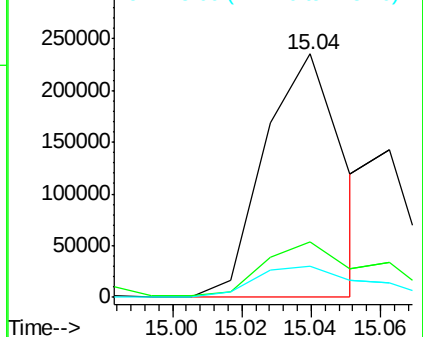

#88

Benzo(k)fluoranthene

Concen: 6.08 ng m

RT: 15.06 min Scan# 1179




Delta R.T. 0.00 min


Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.0	27.0
125	10.1	11.2	16.8

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

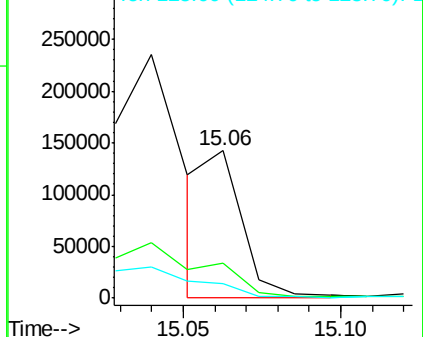

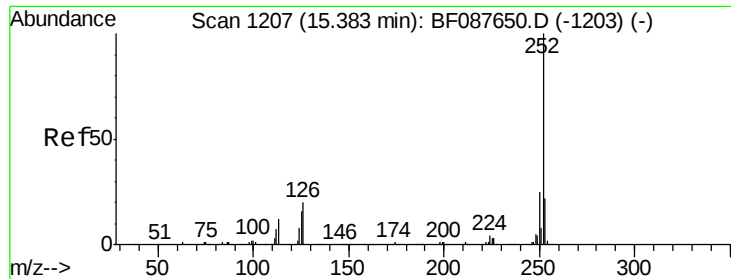

#89

Benzo(a)pyrene

Concen: 9.90 ng

RT: 15.38 min Scan# 1207

Delta R.T. 0.00 min

Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Instrument :

BNA_F


ClientSampleId :

CHS-STA-1672(0-4)RE




Tot Ion	Ratio	Lower	Upper
252	100		
253	23.5	17.9	26.9
125	14.1	12.5	18.7

Manual Integrations
APPROVED

SOHIL
6/6/2016 7:25:30 PM

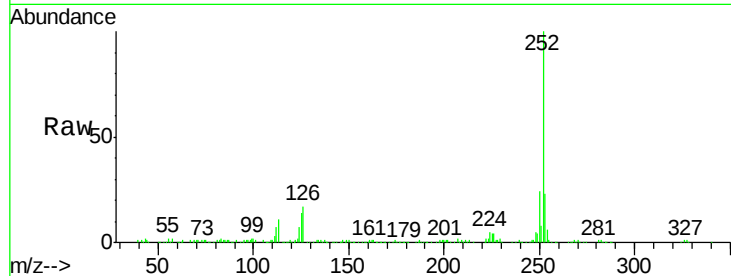

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

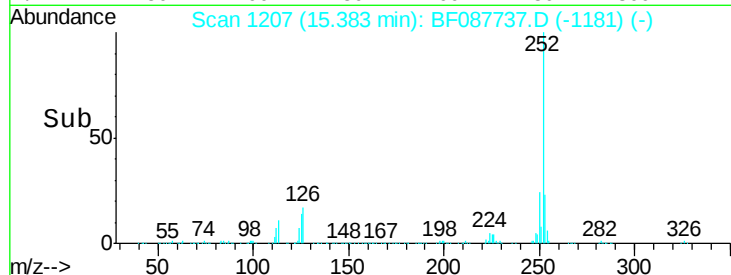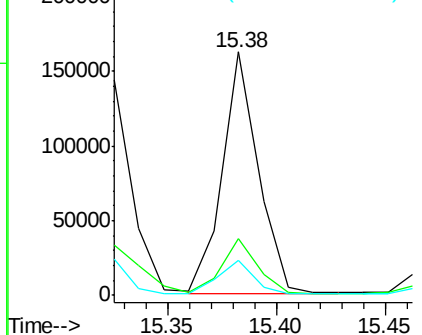

#90

Dibenzo(a,h)anthracene

Concen: 2.16 ng m

RT: 16.85 min Scan# 1335




Delta R.T. -0.01 min


Lab File: BF087737.D

Acq: 6 Jun 2016 5:50

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.7	15.7	23.5
279	29.3	19.4	29.2#

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

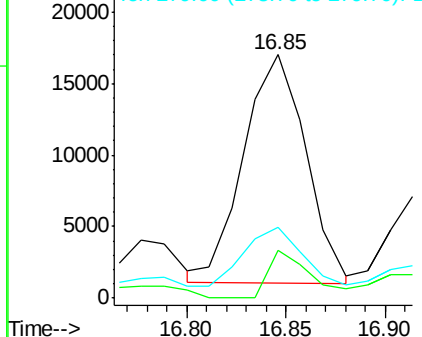

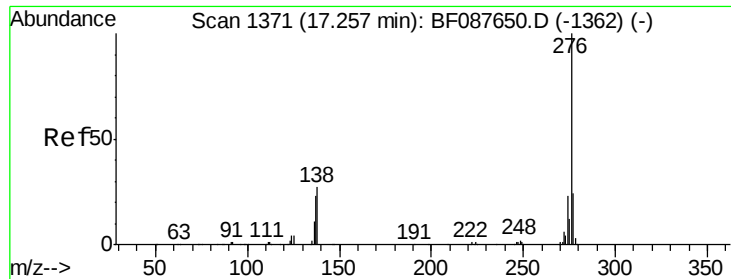

#91
 Benzo(a,h,i)perylene
 Concen: 7.37 ng
 RT: 17.26 min Scan# 1371
 Delta R.T. 0.00 min
 Lab File: BF087737.D
 Acq: 6 Jun 2016 5:50

Instrument :
 BNA_F
 ClientSampleId :
 CHS-STA-1672(0-4)RE

Tot Ion	Ratio	Lower	Upper
276	100		
277	24.6	18.9	28.3
138	21.4	21.4	32.2

Manual Integrations
 APPROVED

SOHIL
 6/6/2016 7:25:30 PM

