
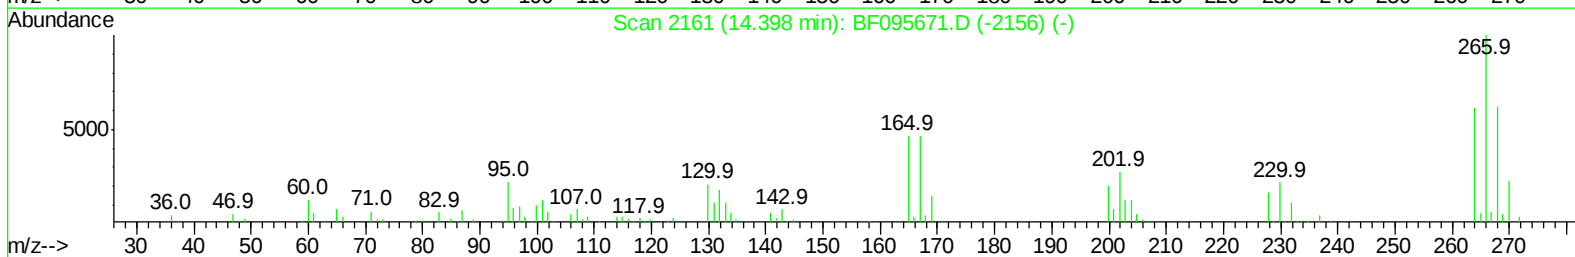
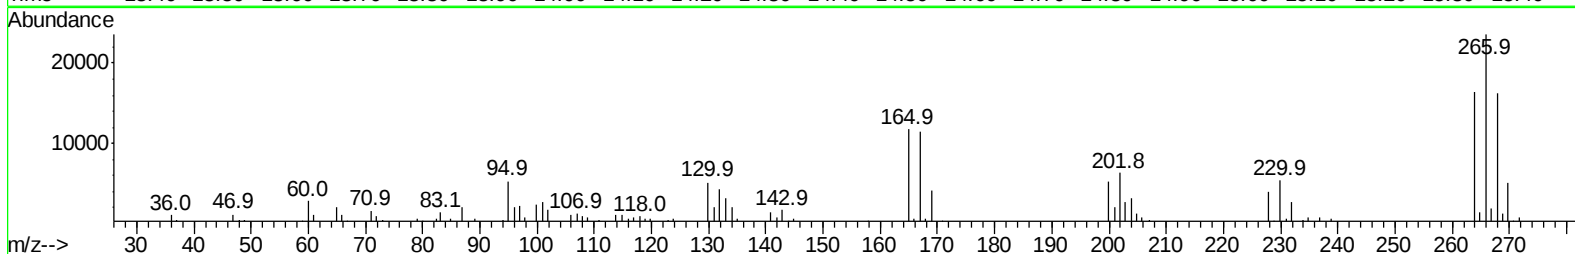


Data Path : Z:\HPCHEM1\BNA F\Data\BF060517\
Data File : BF095667.D
Acq On : 5 Jun 2017 11:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 15:25:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

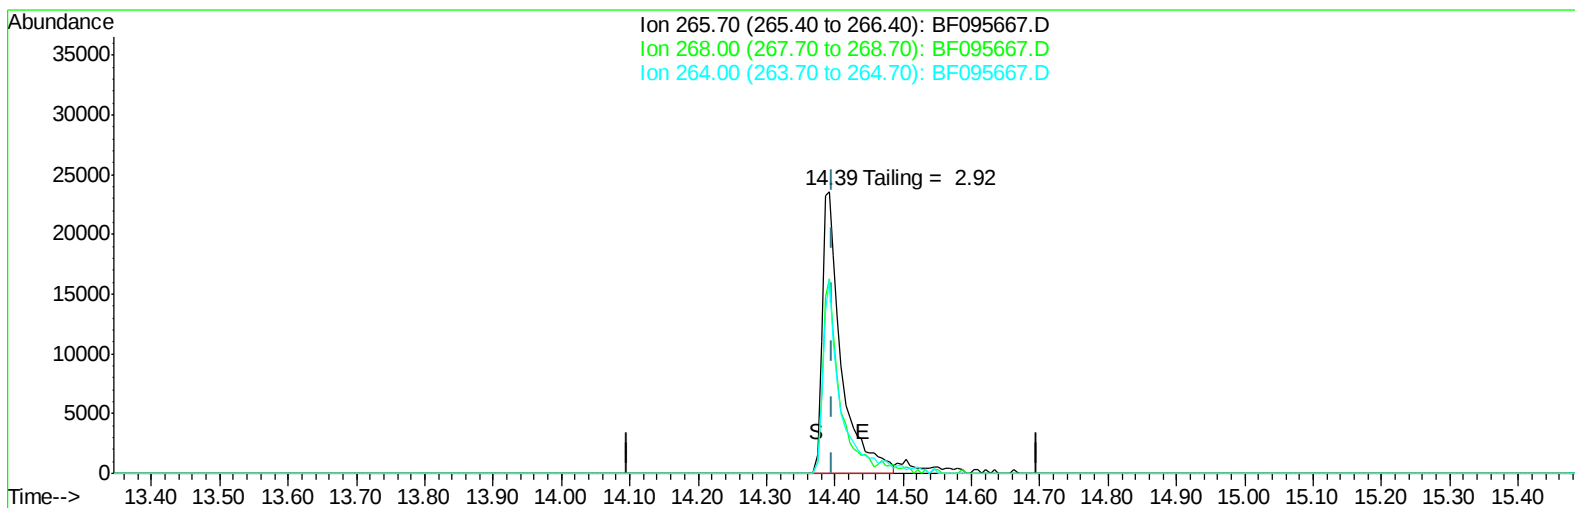

TIC: BF095667.D

(69) Pentachlorophenol (C)




14.392min (-0.005) 0.00ng

response 46113

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.02
264.00	64.60	69.27
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF060517\
Data File : BF095667.D
Acq On : 5 Jun 2017 11:52
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 15:25:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

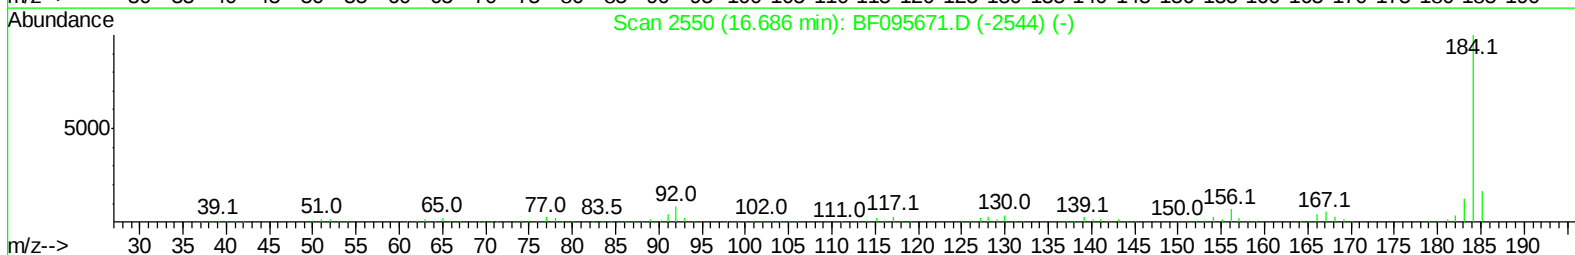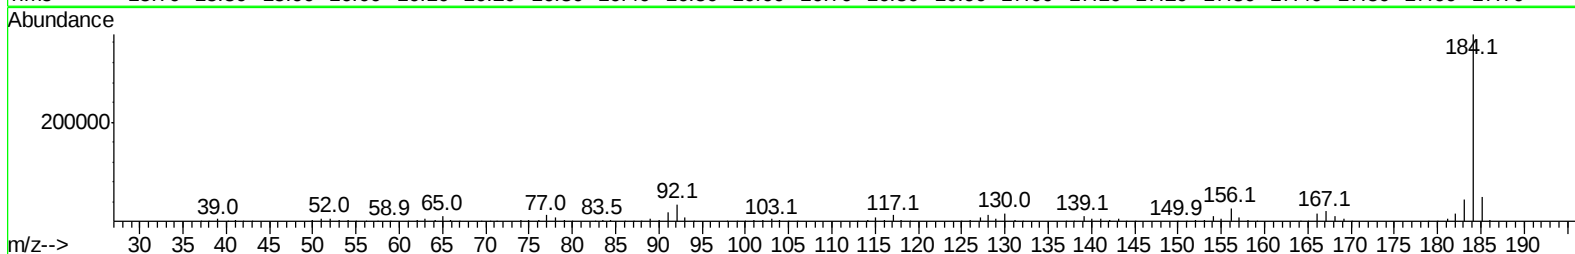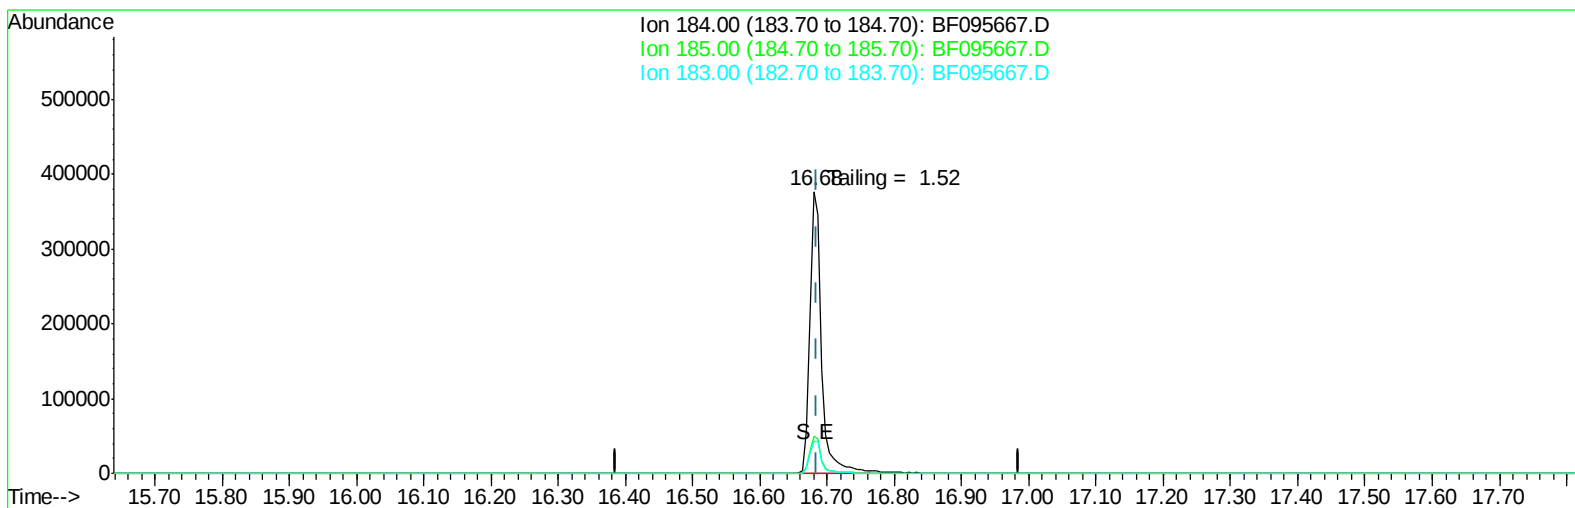

TIC: BF095667.D

(76) Benzidine

16.680min (-0.006) 0.00ng

response 466759

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.39#
183.00	12.20	11.60
0.00	0.00	0.00