
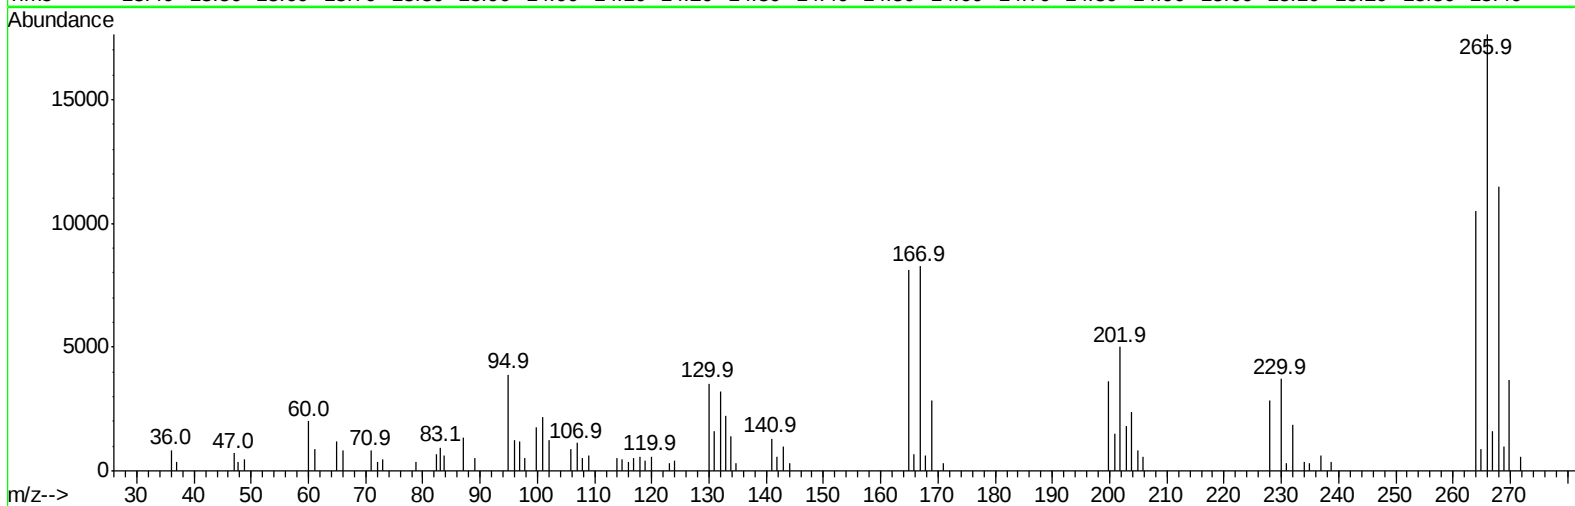


Data Path : Z:\HPCHEM1\BNA F\DATA\BF060517\
Data File : BF095676.D
Acq On : 5 Jun 2017 16:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 09:01:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

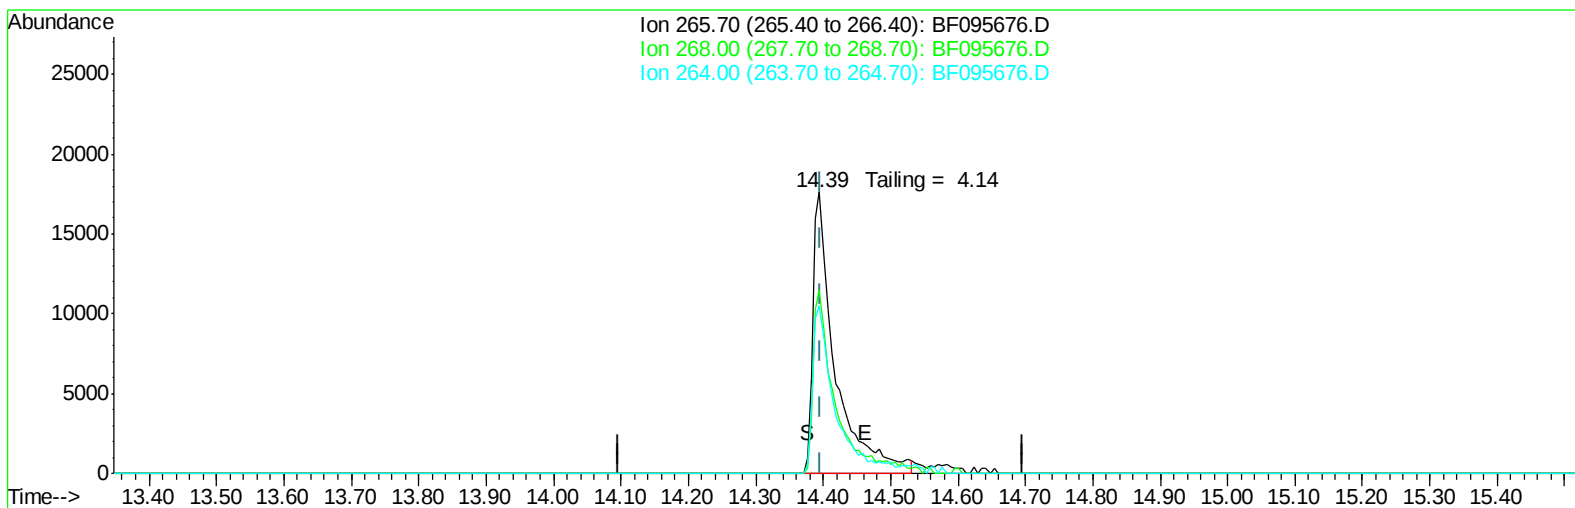

TIC: BF095676.D

(69) Pentachlorophenol (C)



14.395min (-0.002) 0.00ng

response 38927

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.01
264.00	64.60	59.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF060517\
Data File : BF095676.D
Acq On : 5 Jun 2017 16:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 06 09:01:42 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

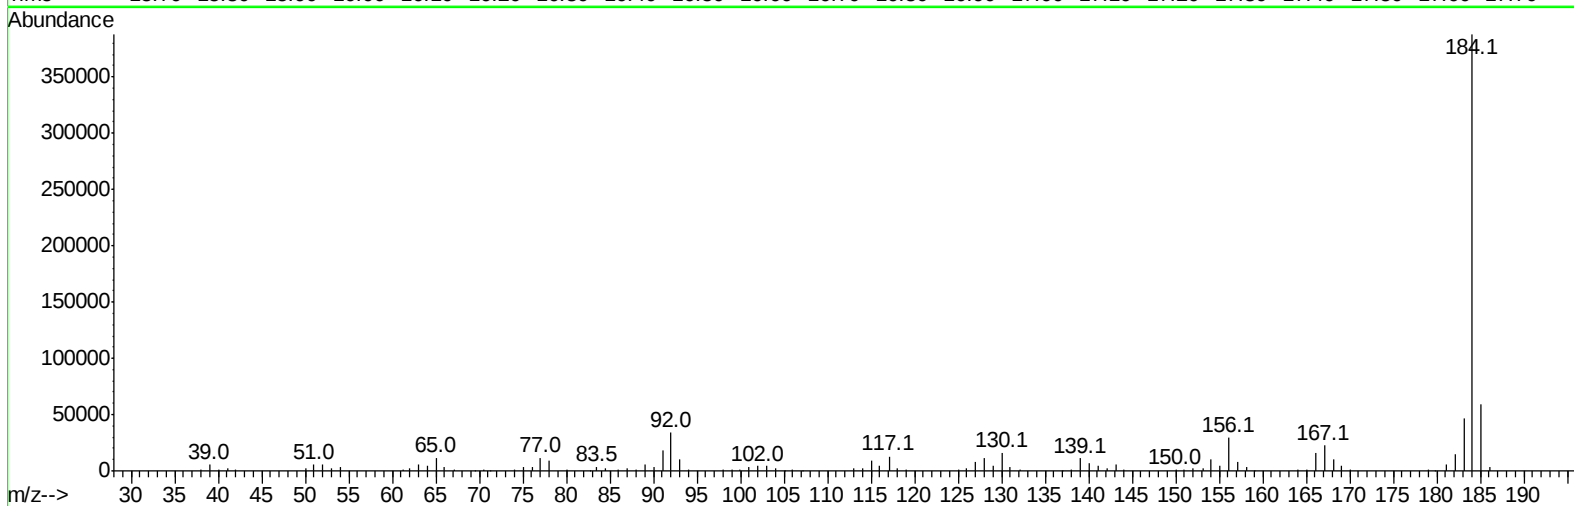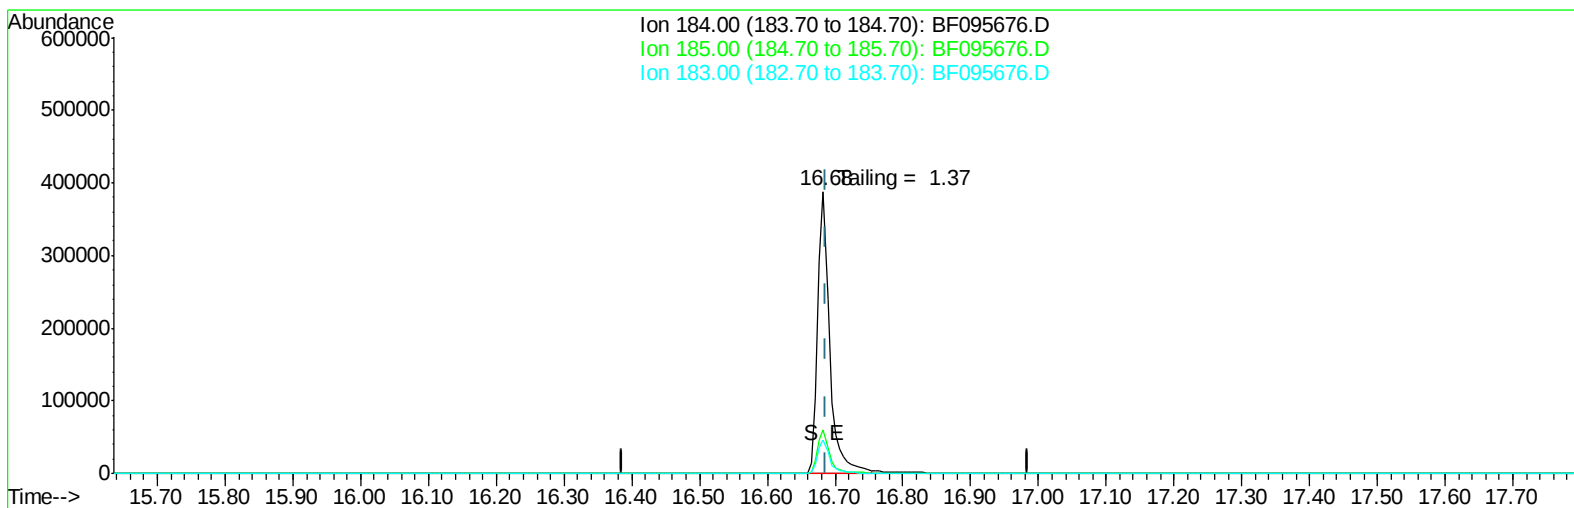

TIC: BF095676.D

(76) Benzidine

16.683min (-0.003) 0.00ng

response 466828

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.35#
183.00	12.20	11.99
0.00	0.00	0.00