

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
 Data File : BF095683.D
 Acq On : 5 Jun 2017 20:32
 Operator : SJ/MA
 Sample : I3441-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-141-060117

Quant Time: Jun 06 02:01:52 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 05 16:15:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	108655	20.00	ng	0.00
21) Naphthalene-d8	9.42	136	413805	20.00	ng	0.00
38) Acenaphthene-d10	12.25	164	215004	20.00	ng	0.00
63) Phenanthrene-d10	14.64	188	346594	20.00	ng	0.00
75) Chrysene-d12	18.35	240	308359	20.00	ng	0.00
86) Perylene-d12	20.02	264	210345	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	847203	124.24	ng	0.03
7) Phenol-d6	6.96	99	1020943	125.06	ng	0.00
23) Nitrobenzene-d5	8.31	82	699799	105.03	ng	0.00
41) 2,4,6-Tribromophenol	13.55	330	254221	133.64	ng	0.00
44) 2-Fluorobiphenyl	11.21	172	1304736	84.45	ng	0.00
78) Terphenyl-d14	17.02	244	1091569	87.85	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
Data File : BF095683.D
Acq On : 5 Jun 2017 20:32
Operator : SJ/MA
Sample : I3441-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-RO-141-060117

Quant Time: Jun 06 02:01:52 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration




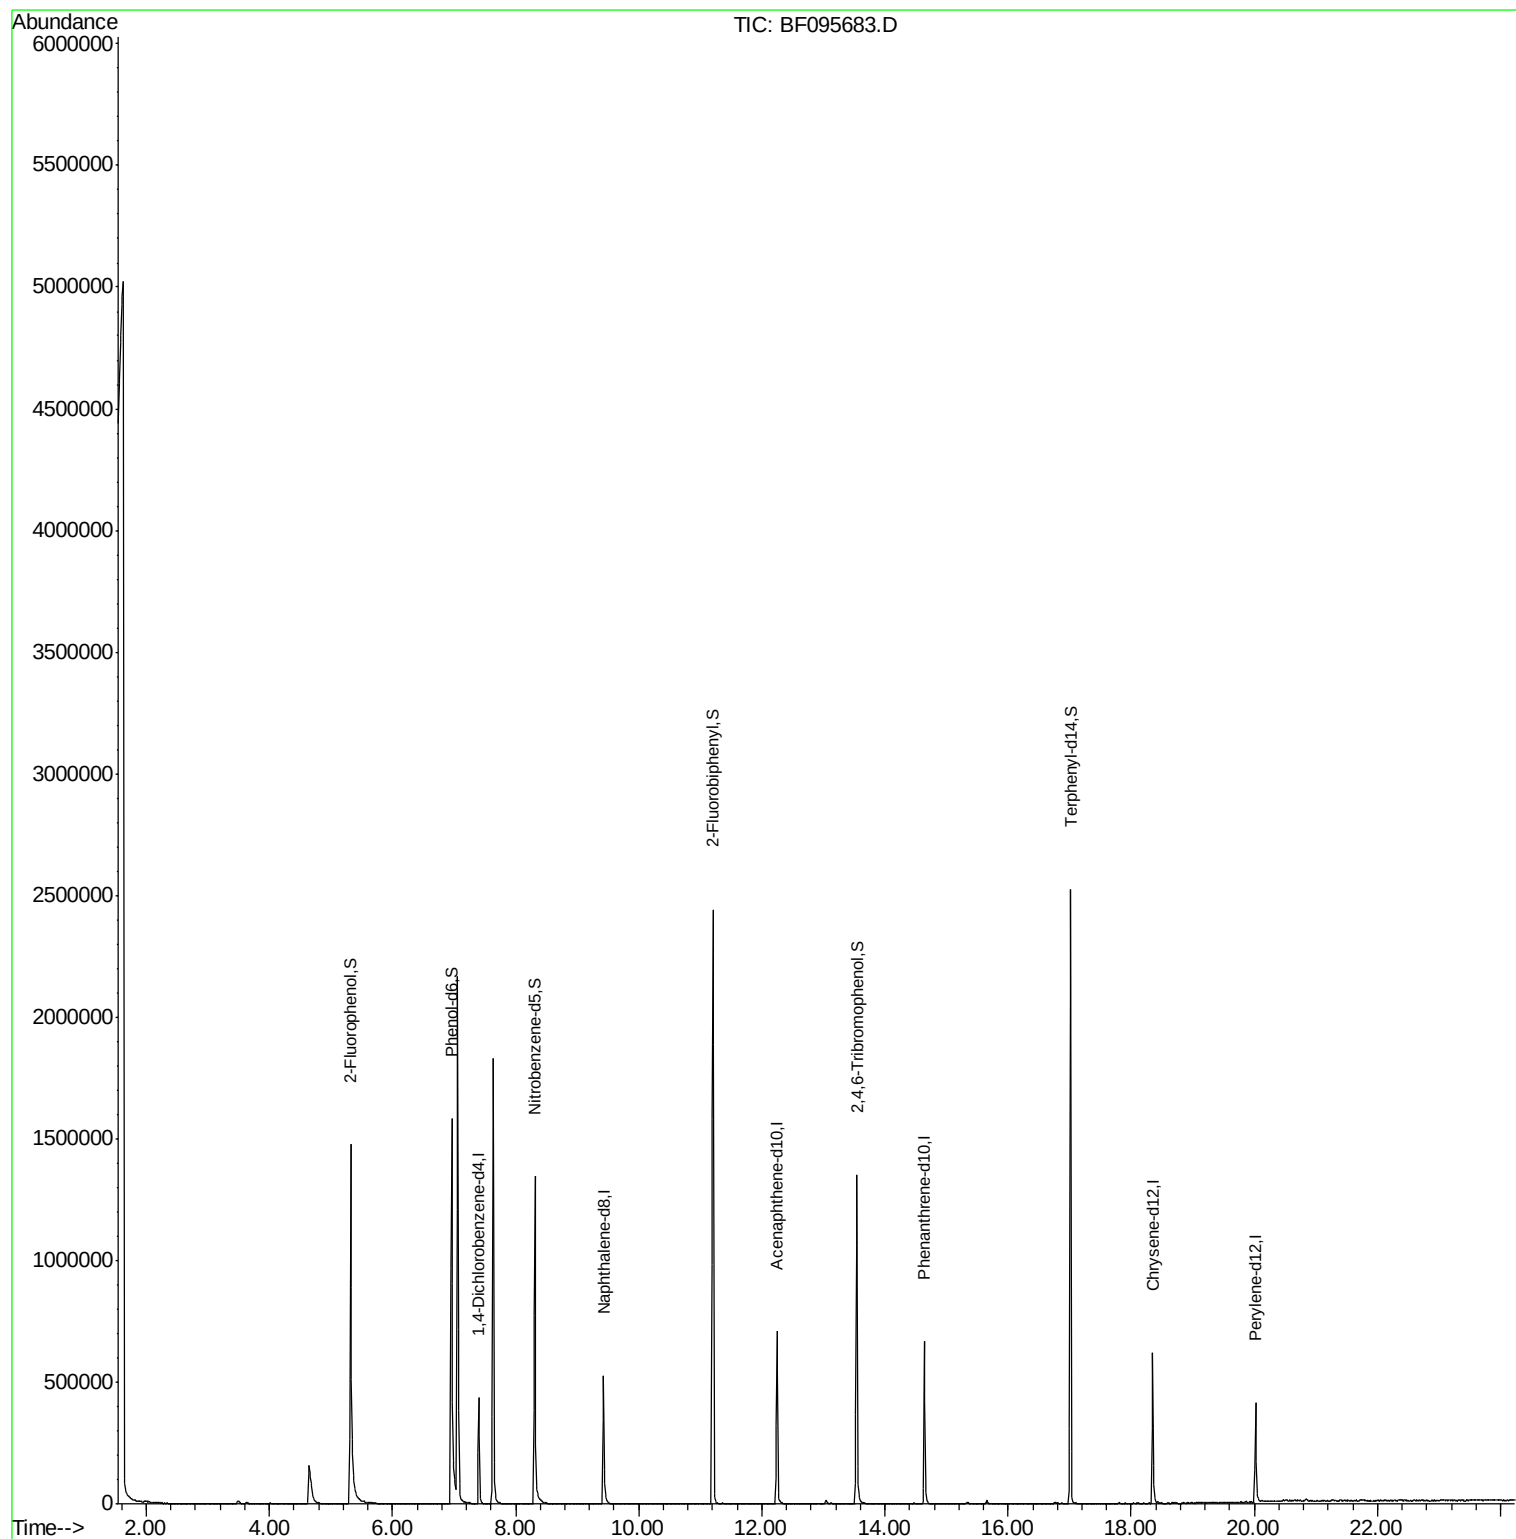


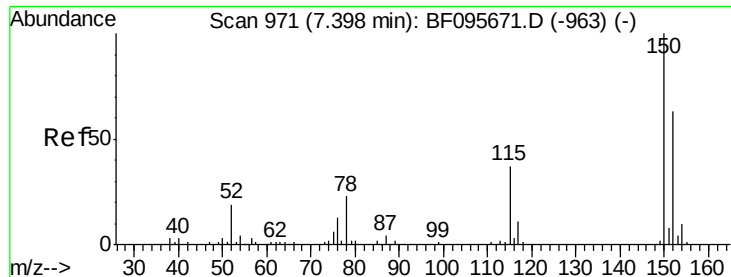

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.40 min Scan# 997
 Delta R.T. 0.00 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32




Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-141-060117


Tgt Ion:152 Resp: 108655
 Ion Ratio Lower Upper
 152 100
 150 155.0 126.2 189.2
 115 59.0 52.2 78.2

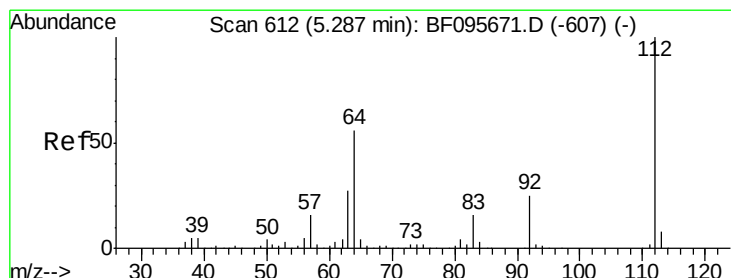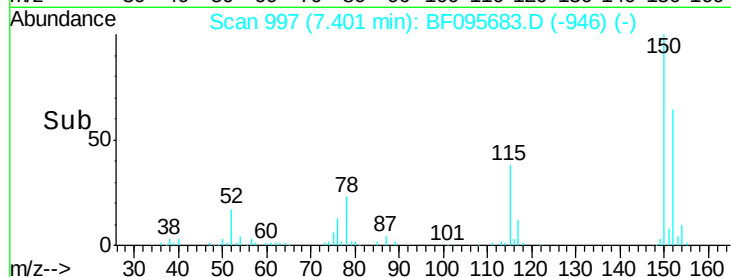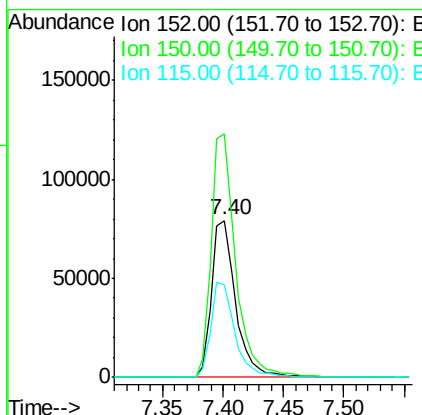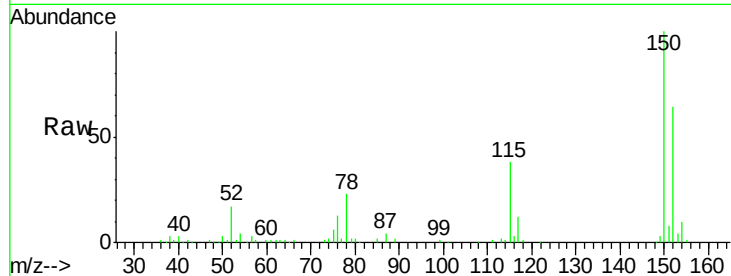

#5
 2-Fluorophenol
 Concen: 124.244 ng
 RT: 5.32 min Scan# 643
 Delta R.T. 0.03 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32

Tgt Ion:112 Resp: 847203
 Ion Ratio Lower Upper
 112 100
 64 54.1 46.0 69.0
 63 26.2 23.4 35.0

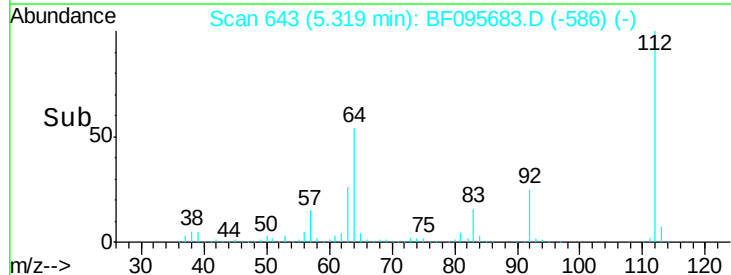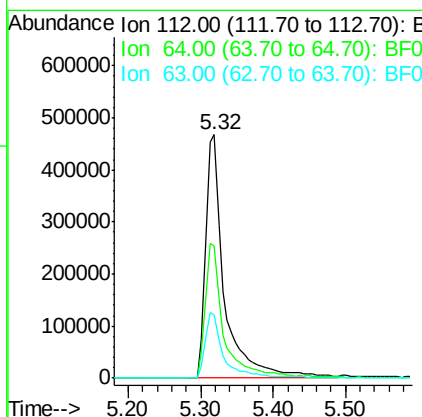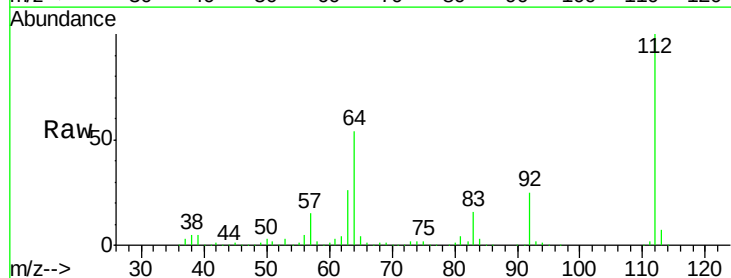

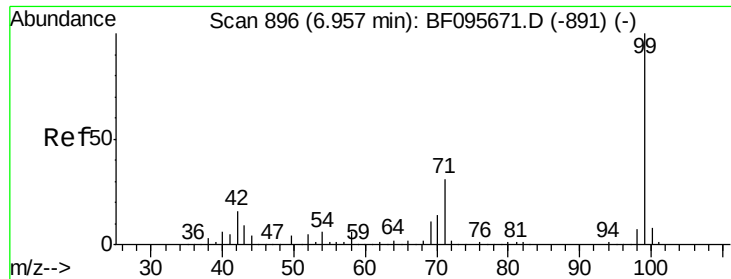

#7

Phenol-d6

Concen: 125.065 ng

RT: 6.96 min Scan# 922

Delta R.T. 0.00 min

Lab File: BF095683.D

Acq: 5 Jun 2017 20:32

Instrument :

BNA_F

ClientSampleId :

OR-RO-141-060117


Tgt Ion: 99 Resp: 1020943

Ion Ratio Lower Upper

99 100

42 16.0 13.5 20.3




71 32.1 24.5 36.7

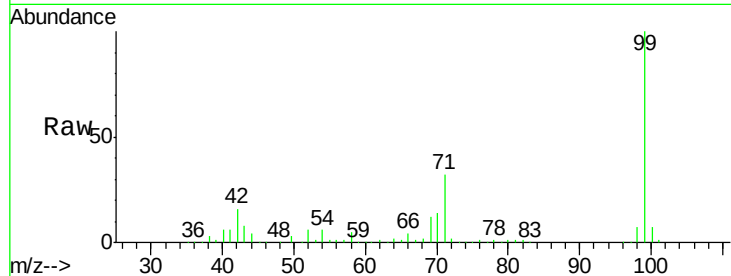

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

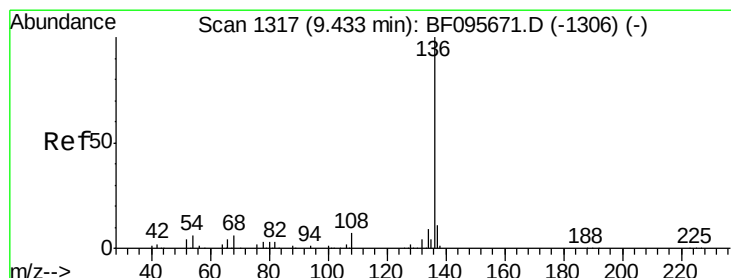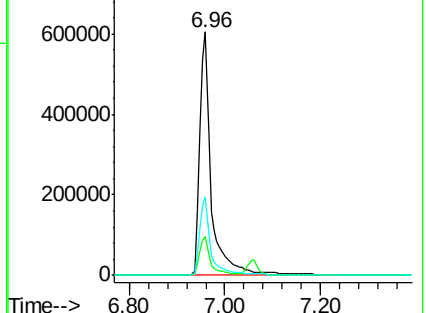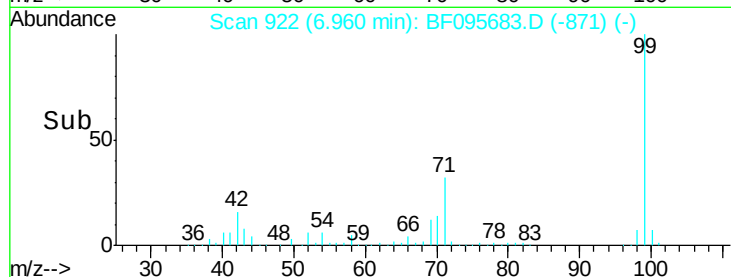

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 9.42 min Scan# 1341

Delta R.T. -0.01 min

Lab File: BF095683.D

Acq: 5 Jun 2017 20:32

Tgt Ion: 136 Resp: 413805


Ion Ratio Lower Upper

136 100

137 10.2 8.5 12.7

54 6.9 4.9 7.3

68 5.6 4.1 6.1


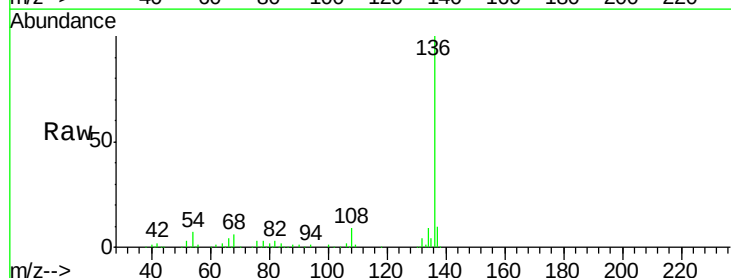



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



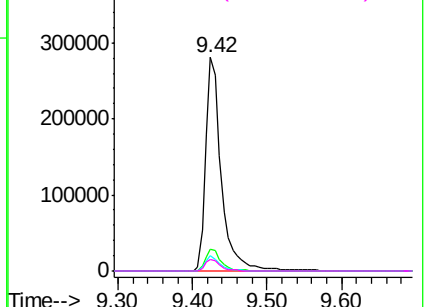
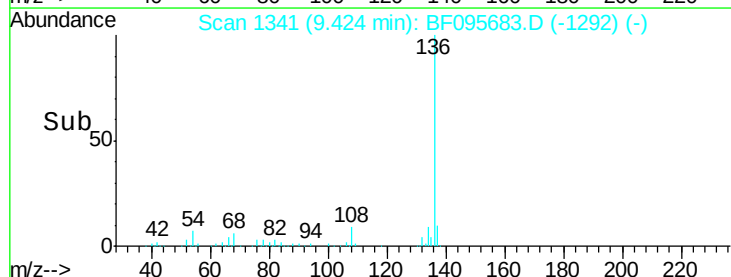


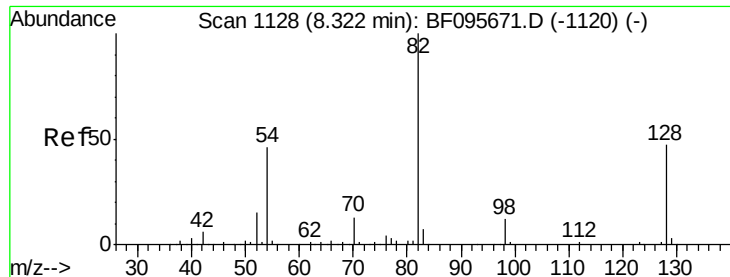

#23
 Nitrobenzene-d5
 Concen: 105.027 ng
 RT: 8.31 min Scan# 1152
 Delta R.T. -0.01 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32




Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-141-060117


Tgt Ion: 82 Resp: 699799
 Ion Ratio Lower Upper
 82 100
 128 47.5 34.0 51.0
 54 47.4 42.2 63.2

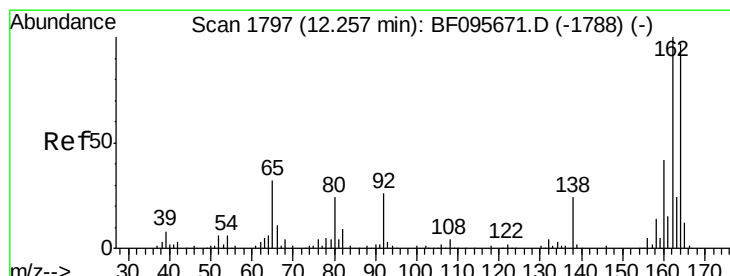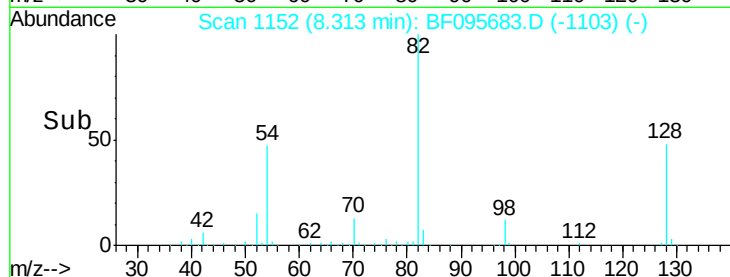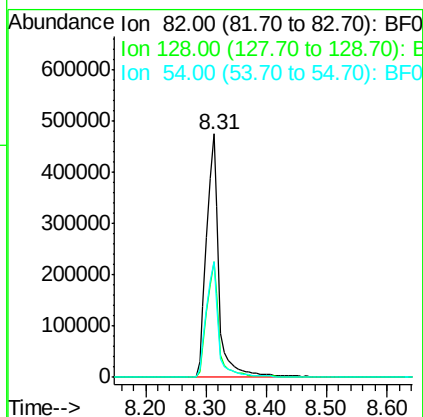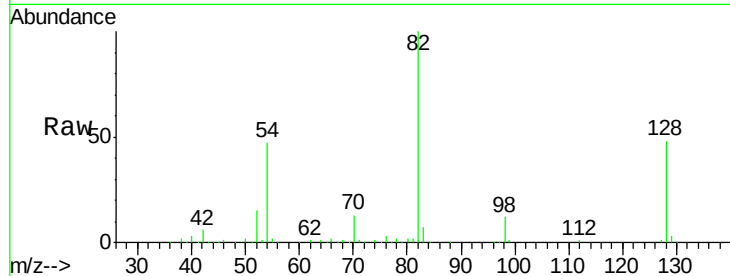

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 12.25 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32

Tgt Ion: 164 Resp: 215004
 Ion Ratio Lower Upper
 164 100
 162 106.0 82.6 123.8
 160 45.1 36.2 54.2

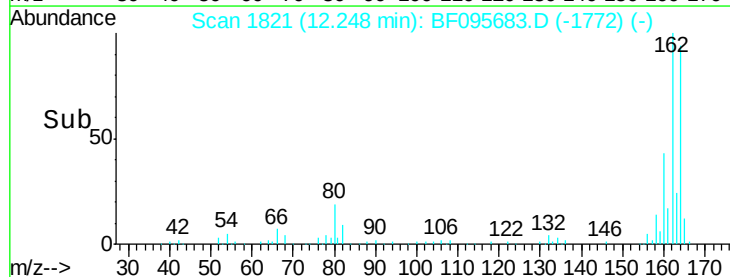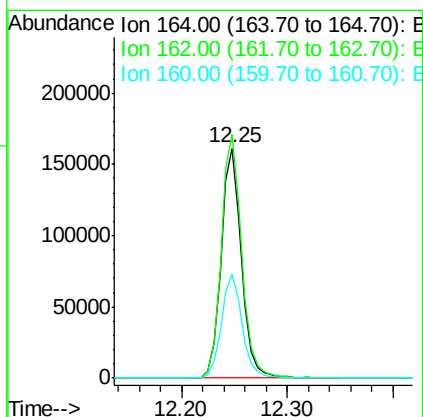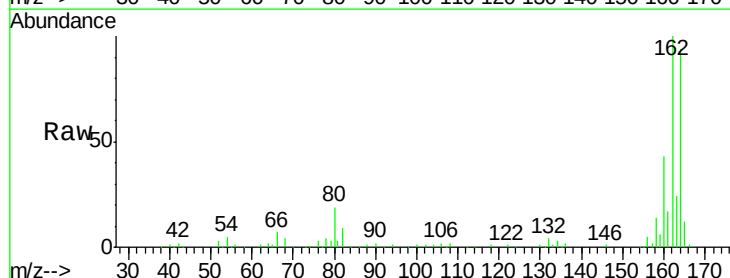


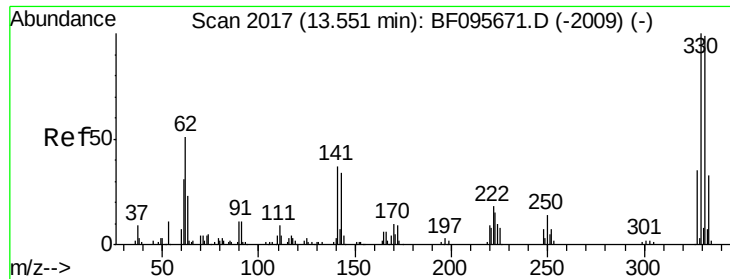




#41
 2,4,6-Tribromophenol
 Concen: 133.640 ng
 RT: 13.55 min Scan# 2042
 Delta R.T. -0.00 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32

Instrument :
 BNA_F
 ClientSampleId :
 OR-RO-141-060117

Tgt Ion:330 Resp: 254221
 Ion Ratio Lower Upper
 330 100
 332 95.7 76.6 115.0
 141 38.9 31.4 47.2

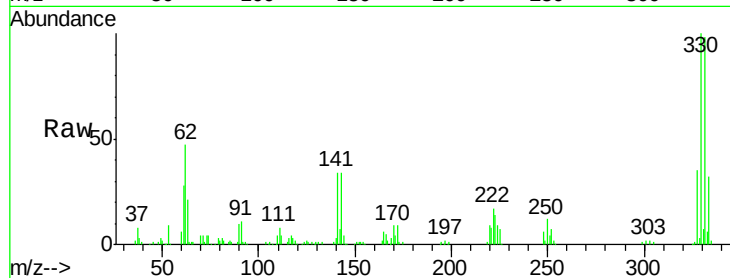


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

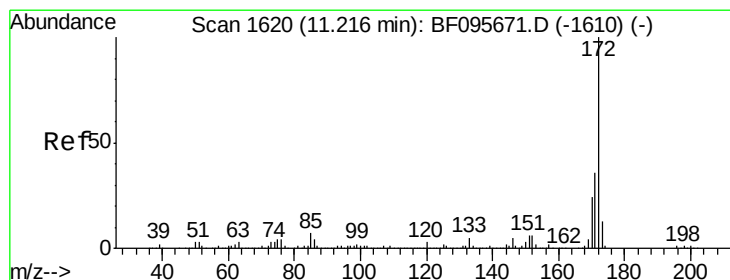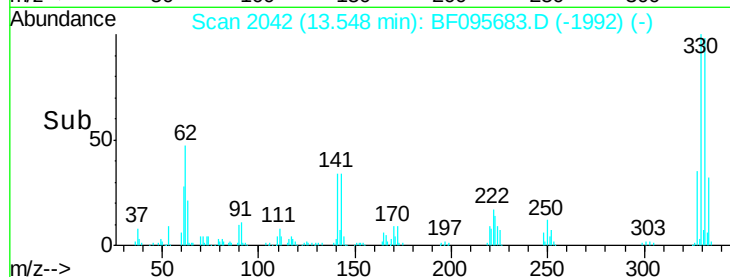
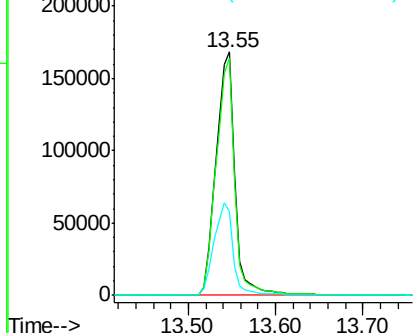



#44
 2-Fluorobiphenyl
 Concen: 84.447 ng
 RT: 11.21 min Scan# 1644
 Delta R.T. -0.01 min
 Lab File: BF095683.D
 Acq: 5 Jun 2017 20:32

Tgt Ion:172 Resp: 1304736
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.6 44.4
 170 24.1 19.8 29.8

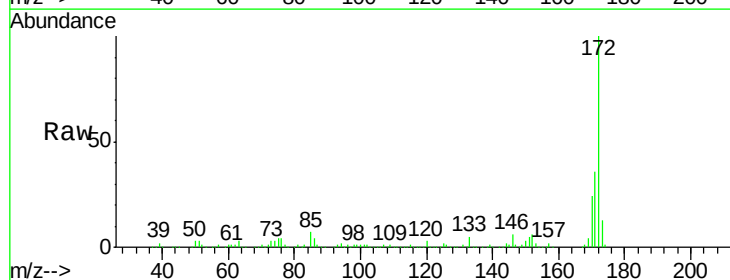

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



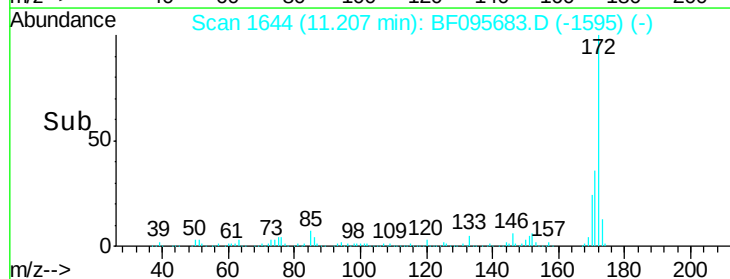
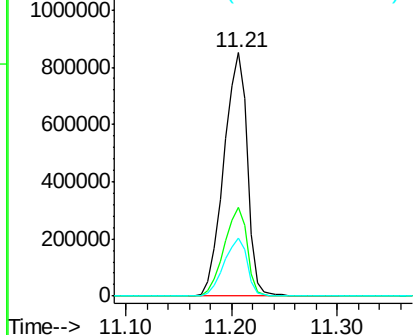


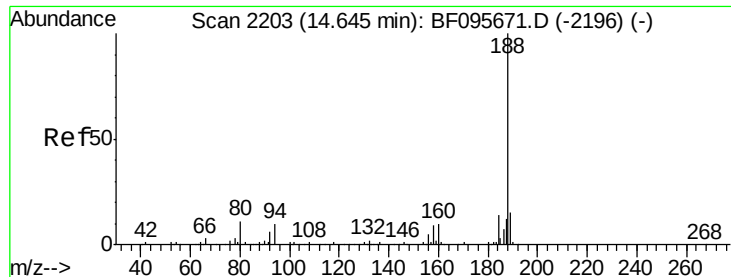

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 14.64 min Scan# 2228
Delta R.T. -0.00 min
Lab File: BF095683.D
Acq: 5 Jun 2017 20:32




Instrument :
BNA_F
ClientSampleId :
OR-RO-141-060117


Tgt Ion:188 Resp: 346594
Ion Ratio Lower Upper
188 100
94 10.2 9.4 14.2
80 10.6 10.2 15.2

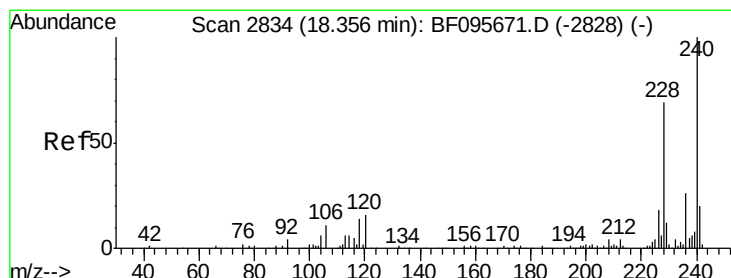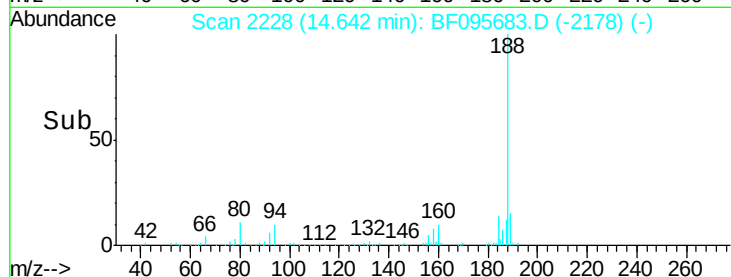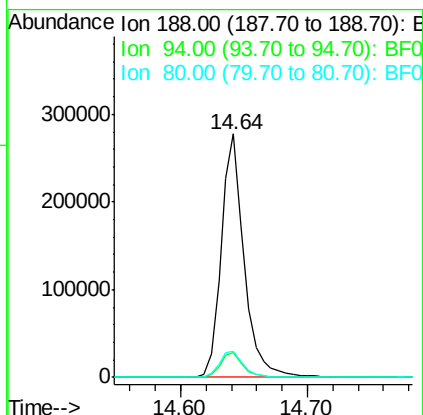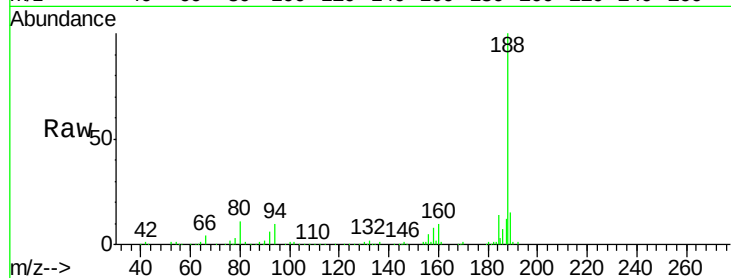

#75
Chrysene-d12
Concen: 20.000 ng
RT: 18.35 min Scan# 2859
Delta R.T. -0.00 min
Lab File: BF095683.D
Acq: 5 Jun 2017 20:32

Tgt Ion:240 Resp: 308359
Ion Ratio Lower Upper
240 100
120 12.8 5.8 8.8#
236 25.3 20.5 30.7

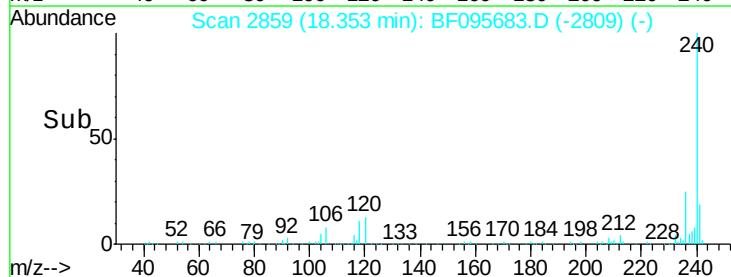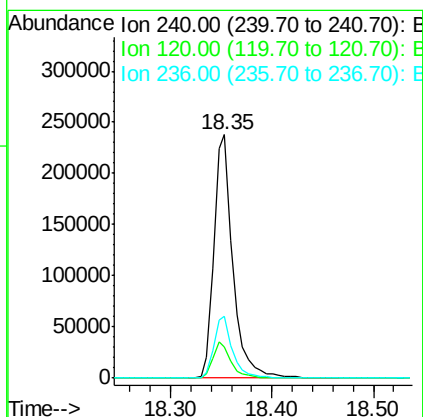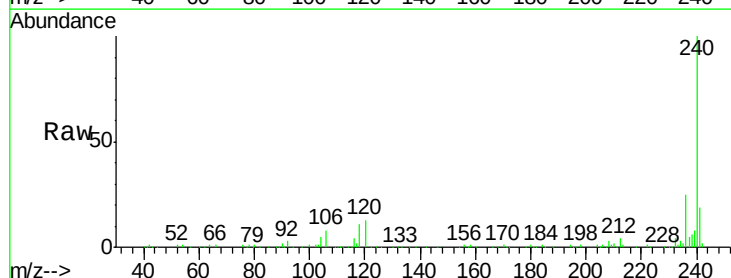

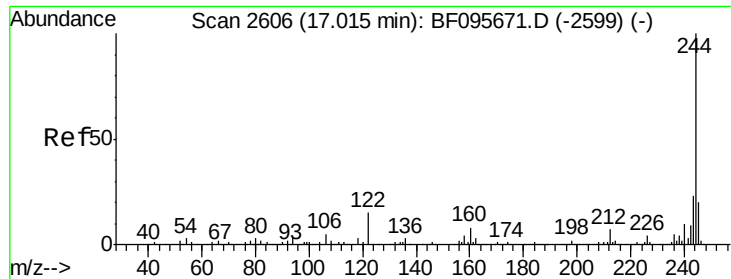

#78

Terphenyl-d14

Concen: 87.852 ng

RT: 17.02 min Scan# 2632

Delta R.T. 0.00 min

Lab File: BF095683.D

Acq: 5 Jun 2017 20:32

Instrument :

BNA_F

ClientSampleId :

OR-RO-141-060117


Tgt Ion:244 Resp: 1091569

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0




122 14.5 10.3 15.5

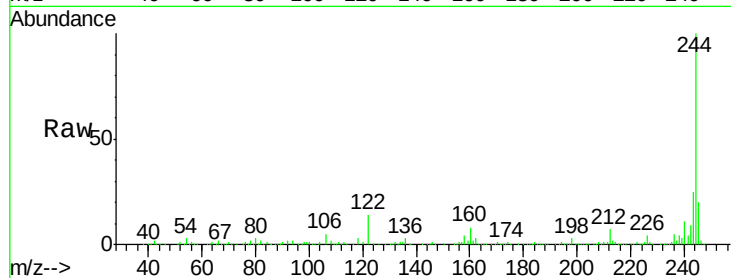

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

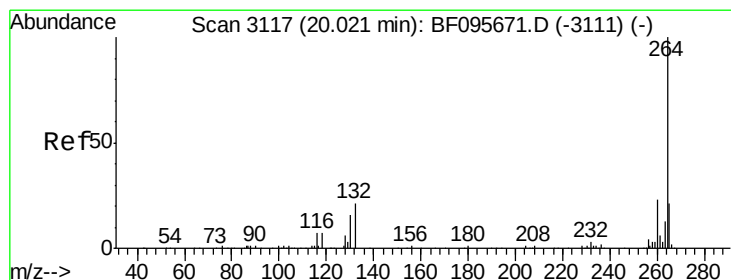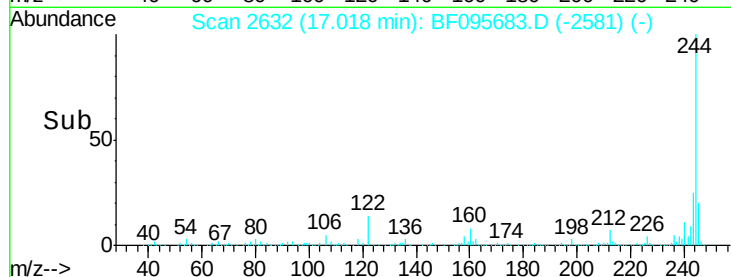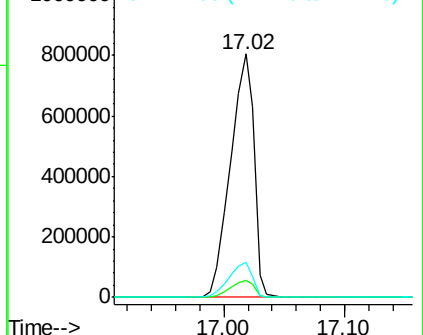

#86

Perylene-d12

Concen: 20.000 ng

RT: 20.02 min Scan# 3142

Delta R.T. -0.00 min

Lab File: BF095683.D

Acq: 5 Jun 2017 20:32


Tgt Ion:264 Resp: 210345

Ion Ratio Lower Upper

264 100

260 22.4 19.5 29.3

265 21.0 17.2 25.8

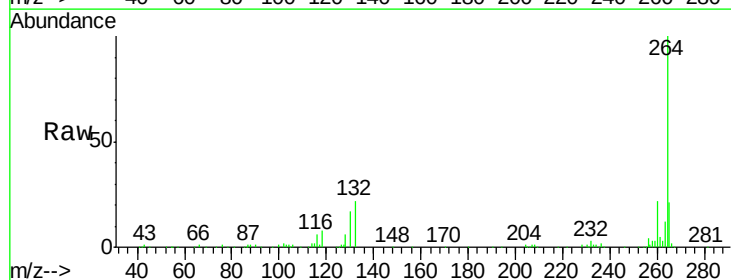

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

