

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
Data File : BF095697.D
Acq On : 6 Jun 2017 4:02
Operator : SJ/MA
Sample : I3444-05 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-RO-286-060117

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.602	8	11	35	rBV	782635	1495869	100.00%	23.191%
2	5.319	640	643	655	rBV2	52351	140178	9.37%	2.173%
3	6.978	922	925	937	rBV	68939	173318	11.59%	2.687%
4	7.066	937	940	957	rVB	127416	280037	18.72%	4.341%
5	7.395	992	996	1012	rBV	406166	560763	37.49%	8.694%
6	7.637	1033	1037	1053	rBV	141834	199665	13.35%	3.095%
7	8.319	1150	1153	1170	rBV	52501	113115	7.56%	1.754%
8	9.431	1337	1342	1356	rBV	562931	690524	46.16%	10.705%
9	11.207	1640	1644	1656	rBV	274867	309284	20.68%	4.795%
10	11.907	1758	1763	1768	rBV	21322	28002	1.87%	0.434%
11	12.254	1816	1822	1828	rBV2	574899	729759	48.78%	11.314%
12	13.548	2038	2042	2049	rBV	58443	84786	5.67%	1.314%
13	14.642	2224	2228	2241	rVB	406955	526918	35.22%	8.169%
14	17.012	2626	2631	2637	rVB	191216	211588	14.14%	3.280%
15	18.353	2855	2859	2867	rBV	448753	536041	35.83%	8.310%
16	20.024	3139	3143	3152	rBV	294612	370462	24.77%	5.743%


Sum of corrected areas: 6450309

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
Data File : BF095697.D
Acq On : 6 Jun 2017 4:02
Operator : SJ/MA
Sample : I3444-05 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-RO-286-060117

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

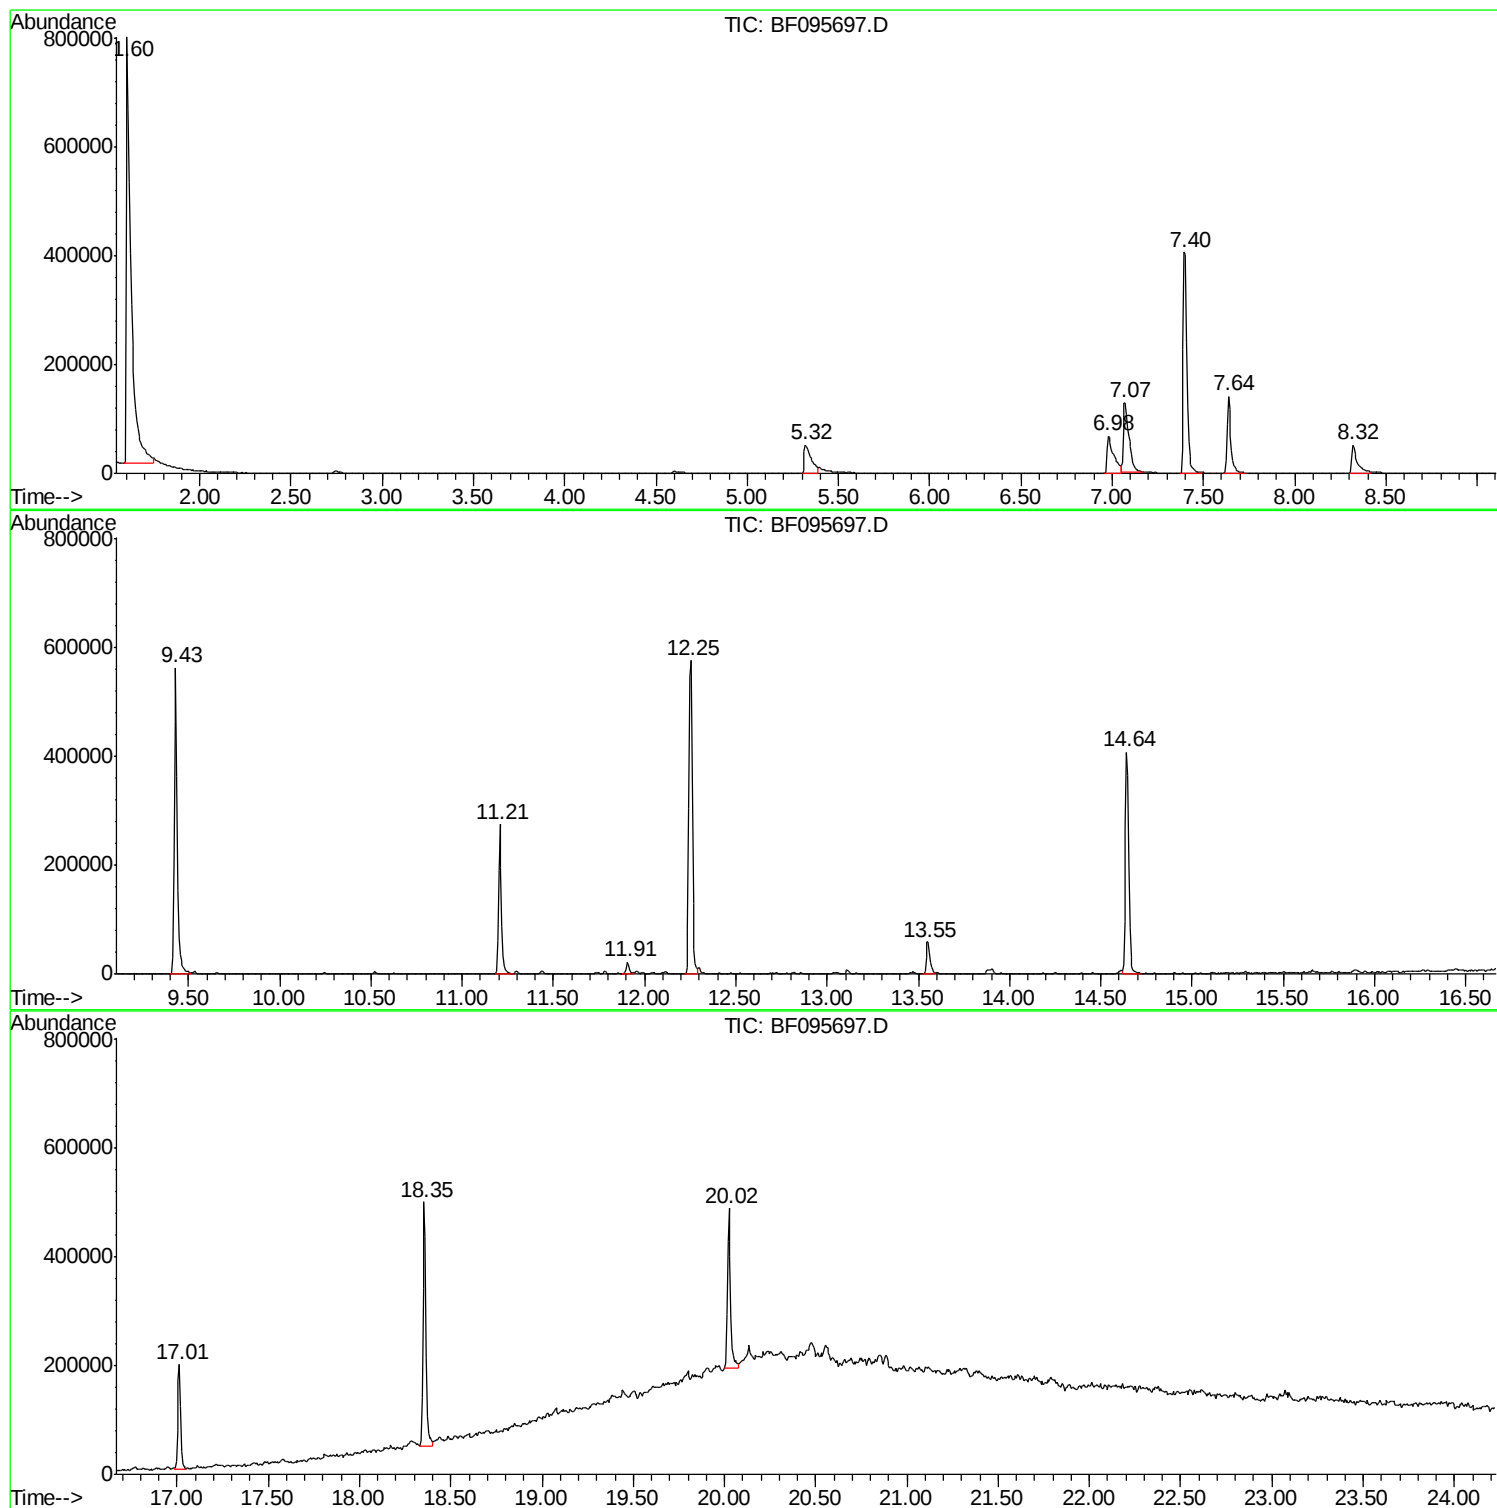

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
Data File : BF095697.D
Acq On : 6 Jun 2017 4:02
Operator : SJ/MA
Sample : I3444-05 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-RO-286-060117










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.07 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.07	9.99 ng	280037	1,4-Dichlorobenzene-d4	7.40

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2			N-(-phenylisopropyl)benzalimine	223	C16H17N	1000379-01-3	12
3			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5			1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

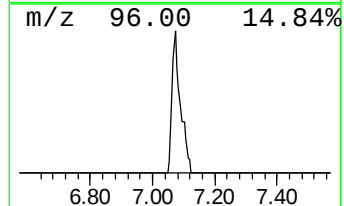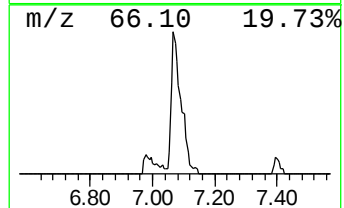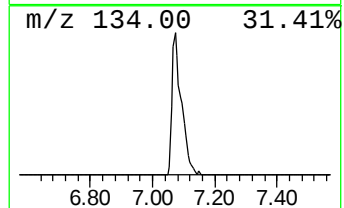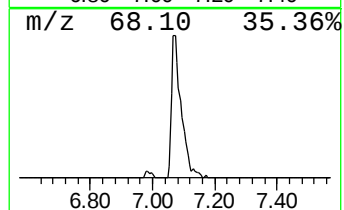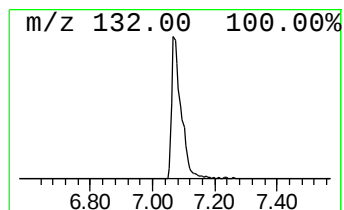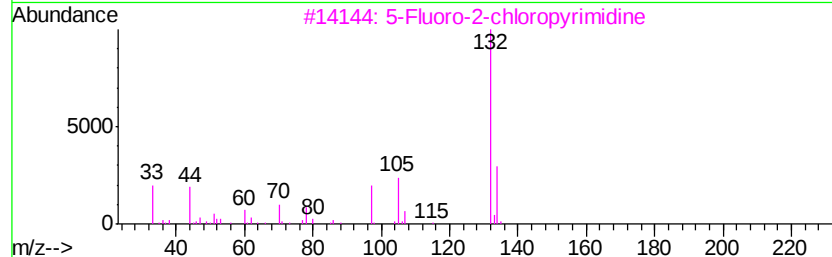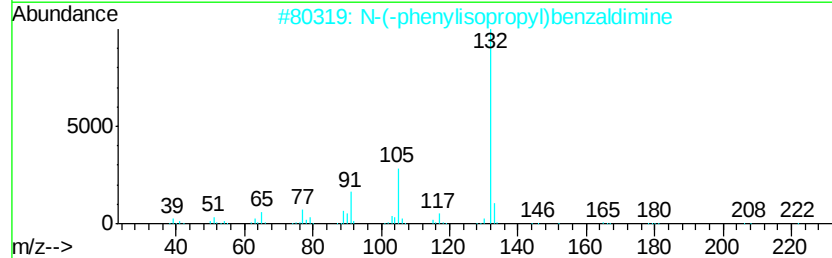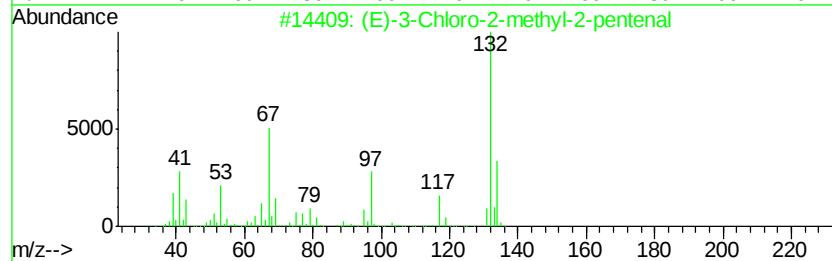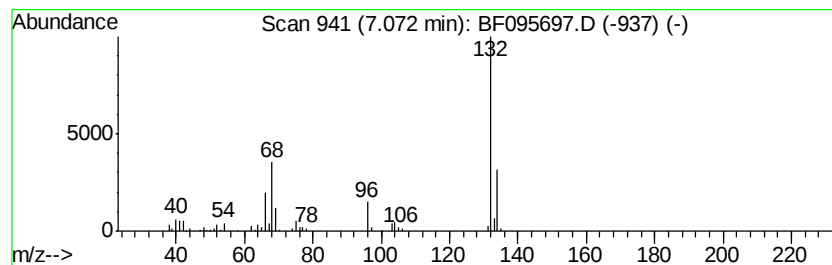

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
Data File : BF095697.D
Acq On : 6 Jun 2017 4:02
Operator : SJ/MA
Sample : I3444-05 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-RO-286-060117

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.07	7.07	10.0	ng	280037	1	7.40	560763	20.0