


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
 Data File : BF095667.D
 Acq On : 5 Jun 2017 11:52
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

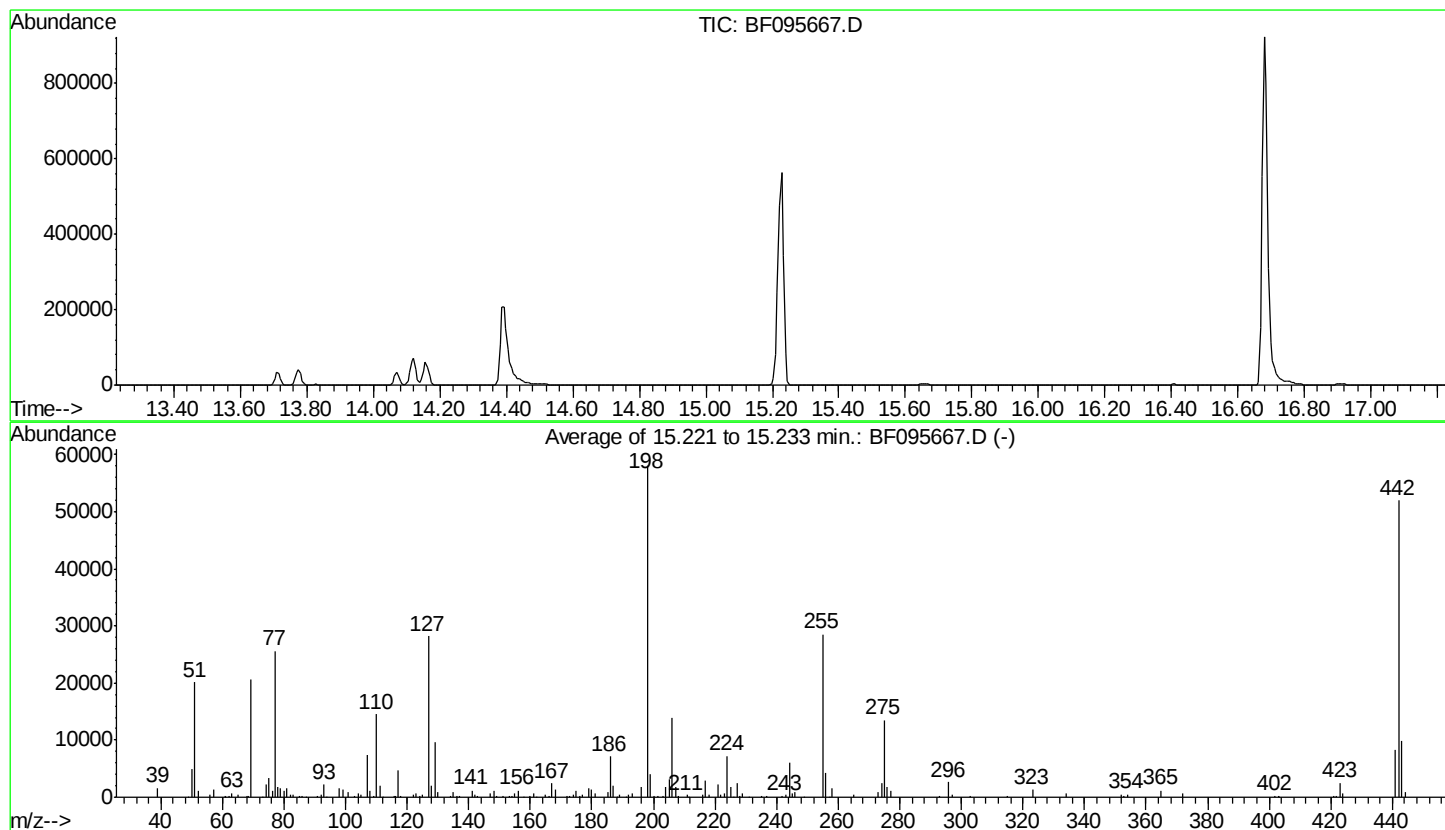

AutoFind: Scans 2301, 2302, 2303; Background Corrected with Scan 2294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	20148	PASS
68	69	0.00	2	1.0	199	PASS
69	198	0.00	100	35.5	20580	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	28205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58050	PASS
199	198	5	9	6.9	4030	PASS
275	198	10	60	23.3	13507	PASS
365	198	1	100	2.0	1190	PASS
441	442	0.01	24	15.8	8230	PASS
442	198	50	100	89.5	51952	PASS
443	442	15	24	18.9	9827	PASS