


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF060517\
 Data File : BF095676.D
 Acq On : 5 Jun 2017 16:41
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 05 16:15:31 2017

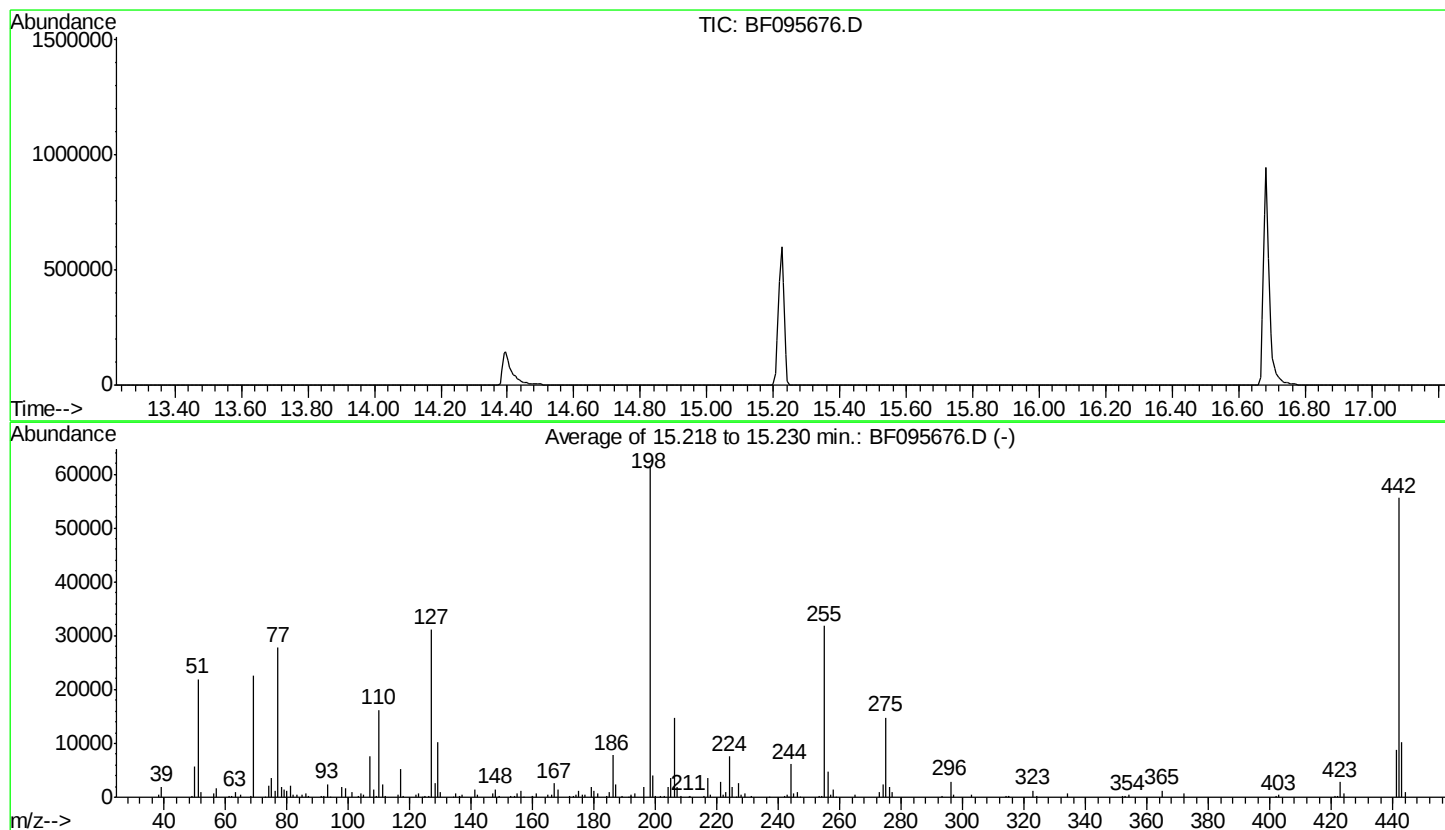

AutoFind: Scans 2326, 2327, 2328; Background Corrected with Scan 2319

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	21906	PASS
68	69	0.00	2	1.2	269	PASS
69	198	0.00	100	36.9	22690	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.5	31101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61560	PASS
199	198	5	9	6.5	4024	PASS
275	198	10	60	24.0	14755	PASS
365	198	1	100	2.1	1276	PASS
441	442	0.01	24	16.0	8861	PASS
442	198	50	100	90.2	55504	PASS
443	442	15	24	18.6	10344	PASS