
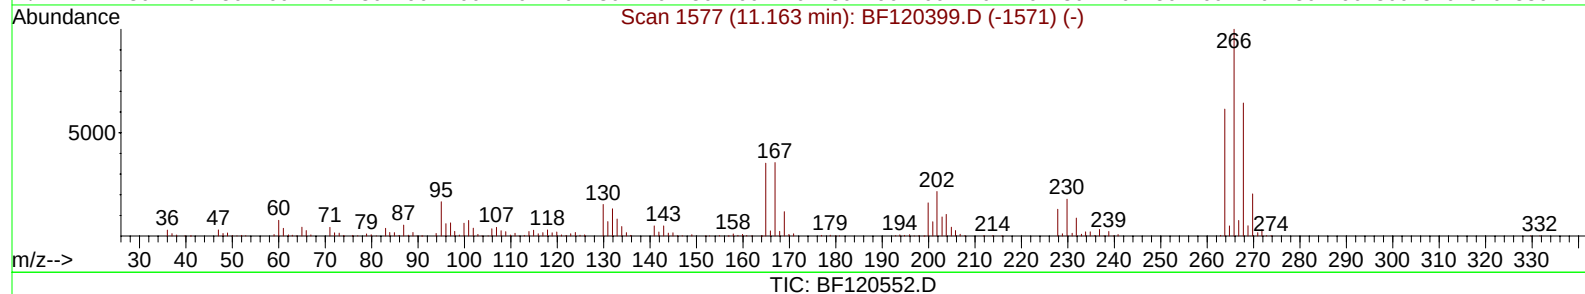
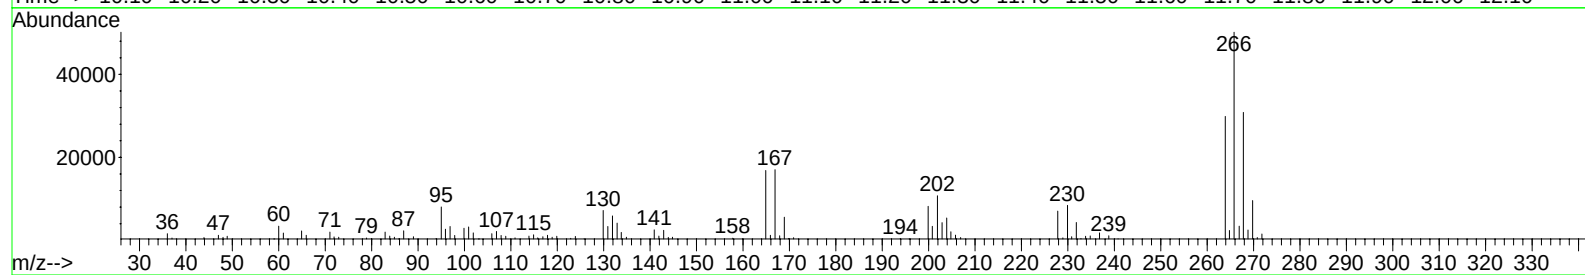


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
Data File : BF120552.D
Acq On : 5 Jun 2020 10:53
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 17:44:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 05 15:36:20 2020
Response via : Initial Calibration

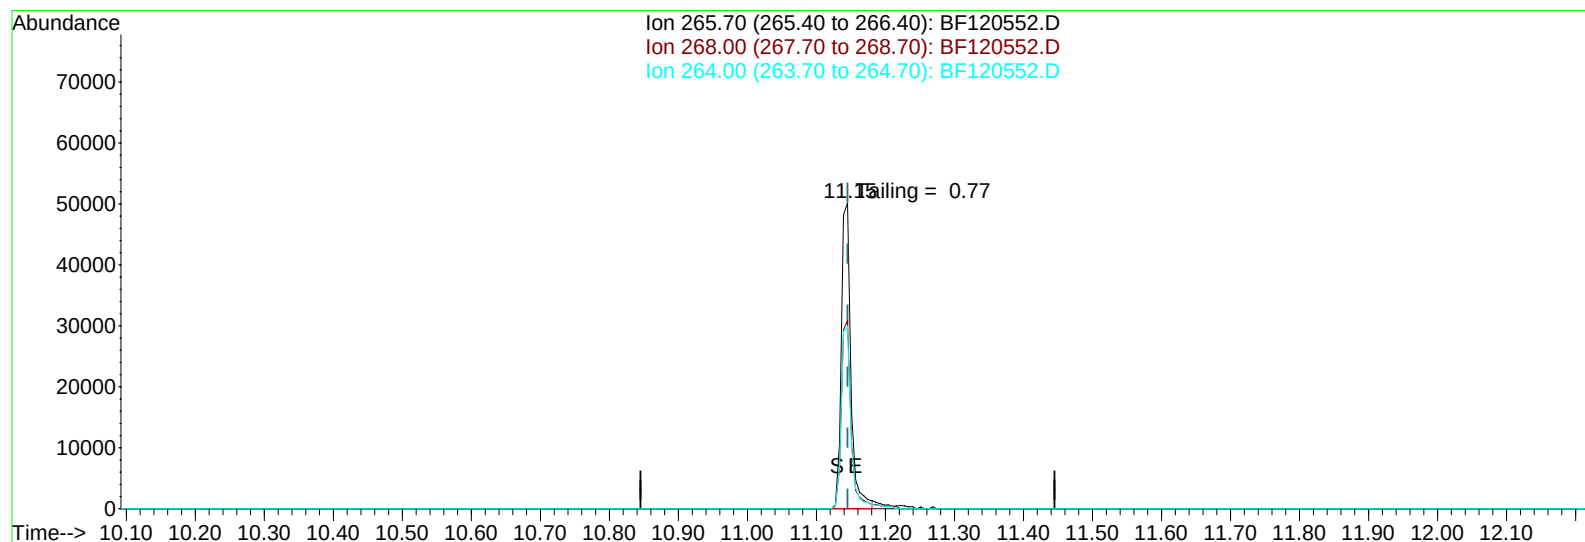

(70) Pentachlorophenol (C)




11.145min (-0.000) 67854.52ng

response 49949

Ion	Exp%	Act%
265.70	100	100
268.00	63.00	61.50
264.00	64.20	59.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
 Data File : BF120552.D
 Acq On : 5 Jun 2020 10:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 17:44:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 05 15:36:20 2020
 Response via : Initial Calibration

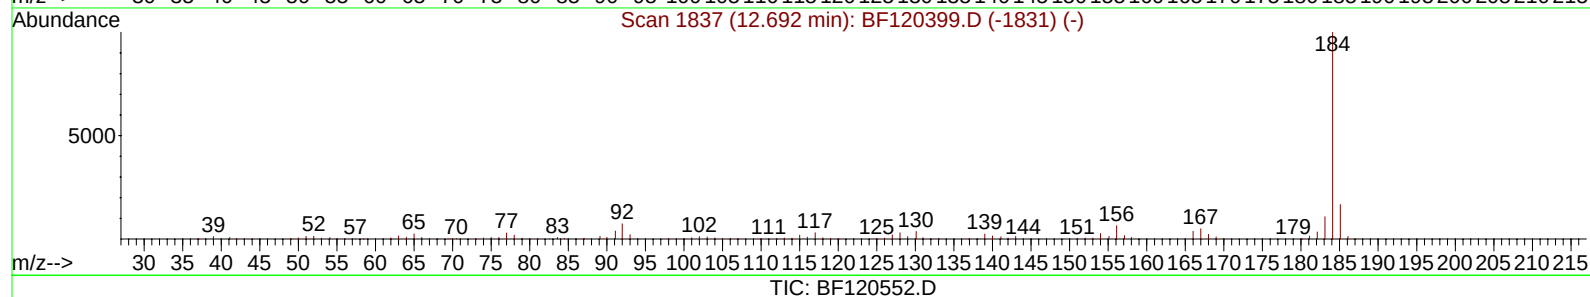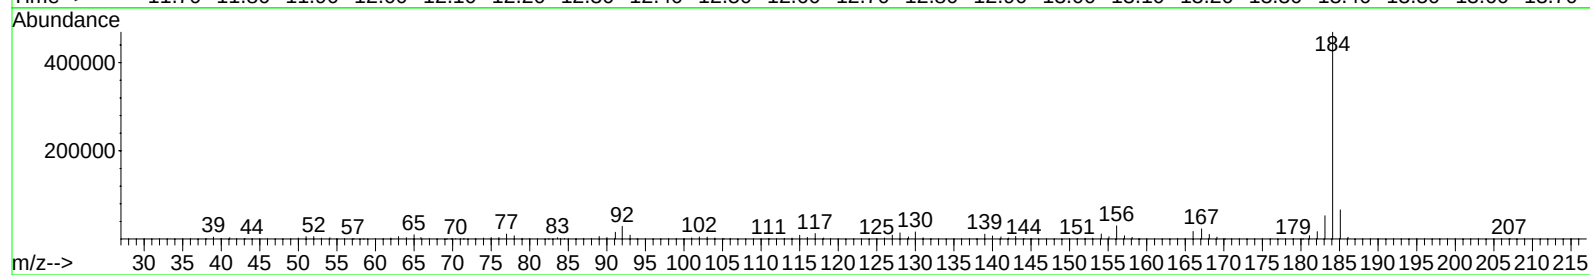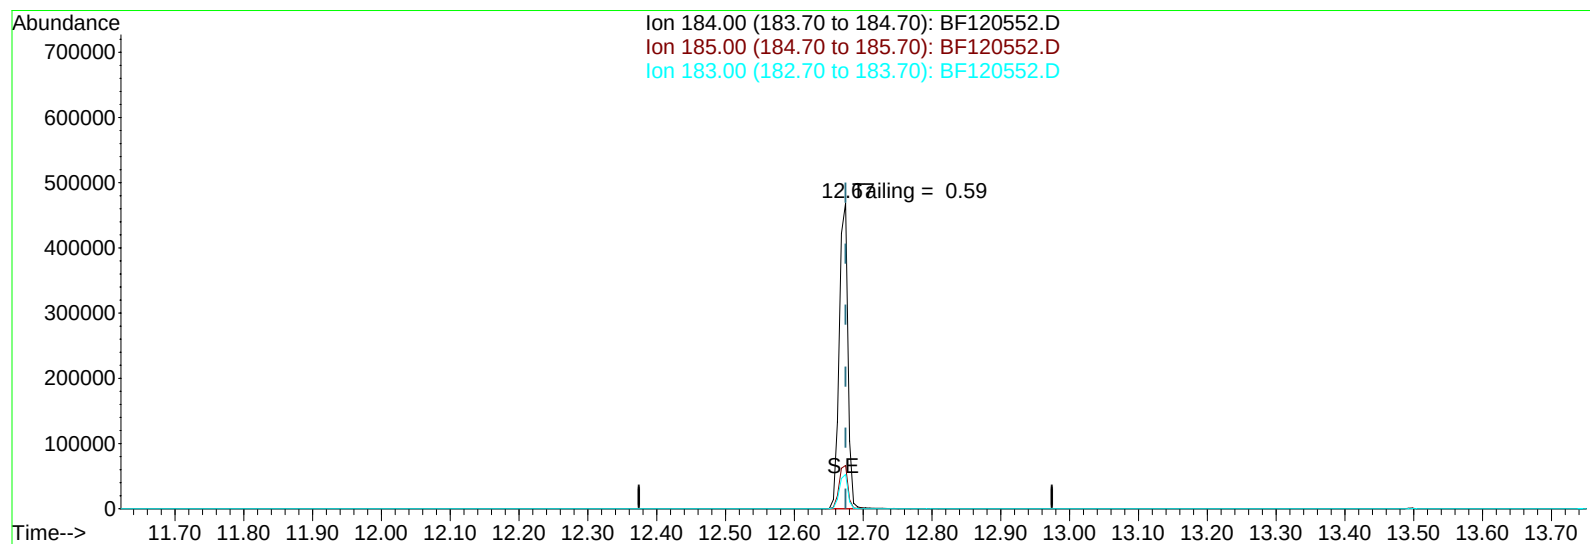

(77) Benzidine

12.674min (-0.000) 0.00ng

response 409802

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.16
183.00	10.70	11.28
0.00	0.00	0.00