

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
 Data File : BF120559.D
 Acq On : 5 Jun 2020 15:01
 Operator : JU/CG
 Sample : L2886-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLAB-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.940	7	9	23	rBV	886755	1251277	32.39%	2.754%
2	2.051	23	28	34	rVB	894707	1112728	28.81%	2.449%
3	5.434	599	603	607	rBV	2538561	2495112	64.60%	5.492%
4	6.457	772	777	780	rBV	2932773	2928363	75.81%	6.445%
5	6.645	806	809	815	rBV	329100	277183	7.18%	0.610%
6	6.816	834	838	842	rBV	1229821	977390	25.30%	2.151%
7	6.975	860	865	868	rBV	3146986	2710258	70.17%	5.965%
8	7.380	928	934	937	rBV	2281868	2107286	54.56%	4.638%
9	8.098	1052	1056	1059	rBV	1588130	1238428	32.06%	2.726%
10	9.174	1234	1239	1242	rBV	4369500	3862570	100.00%	8.501%
11	9.298	1254	1260	1263	rBV	1949604	1918457	49.67%	4.222%
12	9.569	1302	1306	1309	rVB	586287	485204	12.56%	1.068%
13	9.663	1318	1322	1327	rBV3	29162	41879	1.08%	0.092%
14	9.780	1334	1342	1345	rBV4	26878	48881	1.27%	0.108%
15	9.851	1350	1354	1358	rVB	1681593	1386857	35.91%	3.052%
16	10.257	1420	1423	1426	rBV2	48731	49713	1.29%	0.109%
17	10.433	1449	1453	1467	rBV	952919	881838	22.83%	1.941%
18	10.639	1484	1488	1491	rBV	997799	807663	20.91%	1.778%
19	11.339	1603	1607	1610	rBV	1569745	1356574	35.12%	2.986%
20	11.516	1633	1637	1642	rBV2	157865	179907	4.66%	0.396%
21	11.568	1642	1646	1651	rVB	50061	66479	1.72%	0.146%
22	11.727	1670	1673	1678	rBV2	42027	44733	1.16%	0.098%
23	11.868	1693	1697	1700	rBV	350414	318213	8.24%	0.700%
24	11.898	1700	1702	1705	rVB	52999	45410	1.18%	0.100%
25	12.386	1781	1785	1789	rBV	333553	371631	9.62%	0.818%
26	12.427	1789	1792	1796	rVB	57395	52621	1.36%	0.116%
27	12.580	1815	1818	1821	rVB	294229	262479	6.80%	0.578%
28	12.651	1827	1830	1835	rBV2	84603	97439	2.52%	0.214%
29	12.798	1853	1855	1863	rVB	180741	166345	4.31%	0.366%
30	12.880	1867	1869	1872	rVB	53804	42474	1.10%	0.093%
31	12.927	1872	1877	1880	rBV	3569195	3402762	88.10%	7.489%
32	13.157	1909	1916	1919	rBV	525969	519636	13.45%	1.144%
33	13.398	1954	1957	1961	rVB2	124321	120297	3.11%	0.265%
34	13.498	1969	1974	1978	rBV	1104106	949150	24.57%	2.089%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
Data File : BF120559.D
Acq On : 5 Jun 2020 15:01
Operator : JU/CG
Sample : L2886-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.827	2026	2030	2037	rVB	1636707	1547886	40.07%	3.407%
36	13.974	2049	2055	2059	rVB2	1153131	1401032	36.27%	3.084%
37	14.145	2080	2084	2087	rBV	1369302	1234531	31.96%	2.717%
38	14.339	2114	2117	2119	rVB	61871	57699	1.49%	0.127%
39	14.451	2132	2136	2147	rVB	1388752	1455228	37.68%	3.203%
40	14.604	2159	2162	2165	rBV	327149	275757	7.14%	0.607%
41	14.633	2165	2167	2170	rVB	78192	74387	1.93%	0.164%
42	14.751	2183	2187	2191	rBV	1119476	1036822	26.84%	2.282%
43	14.827	2197	2200	2206	rVB	106303	110594	2.86%	0.243%
44	14.892	2208	2211	2214	rBV2	79734	79239	2.05%	0.174%
45	15.086	2239	2244	2247	rBV	983802	1189859	30.80%	2.619%
46	15.427	2297	2302	2304	rBV	726632	859395	22.25%	1.892%
47	15.456	2304	2307	2318	rVB	680670	943736	24.43%	2.077%
48	15.651	2337	2340	2344	rBV2	68648	91738	2.38%	0.202%
49	15.886	2374	2380	2384	rBV	624037	929469	24.06%	2.046%
50	15.939	2385	2389	2394	rVB2	127702	223617	5.79%	0.492%
51	16.380	2458	2464	2470	rVB	324343	557375	14.43%	1.227%
52	16.956	2556	2562	2569	rVB	263871	536032	13.88%	1.180%
53	17.645	2673	2679	2687	rVB	105861	252764	6.54%	0.556%


Sum of corrected areas: 45434397

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
Data File : BF120559.D
Acq On : 5 Jun 2020 15:01
Operator : JU/CG
Sample : L2886-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

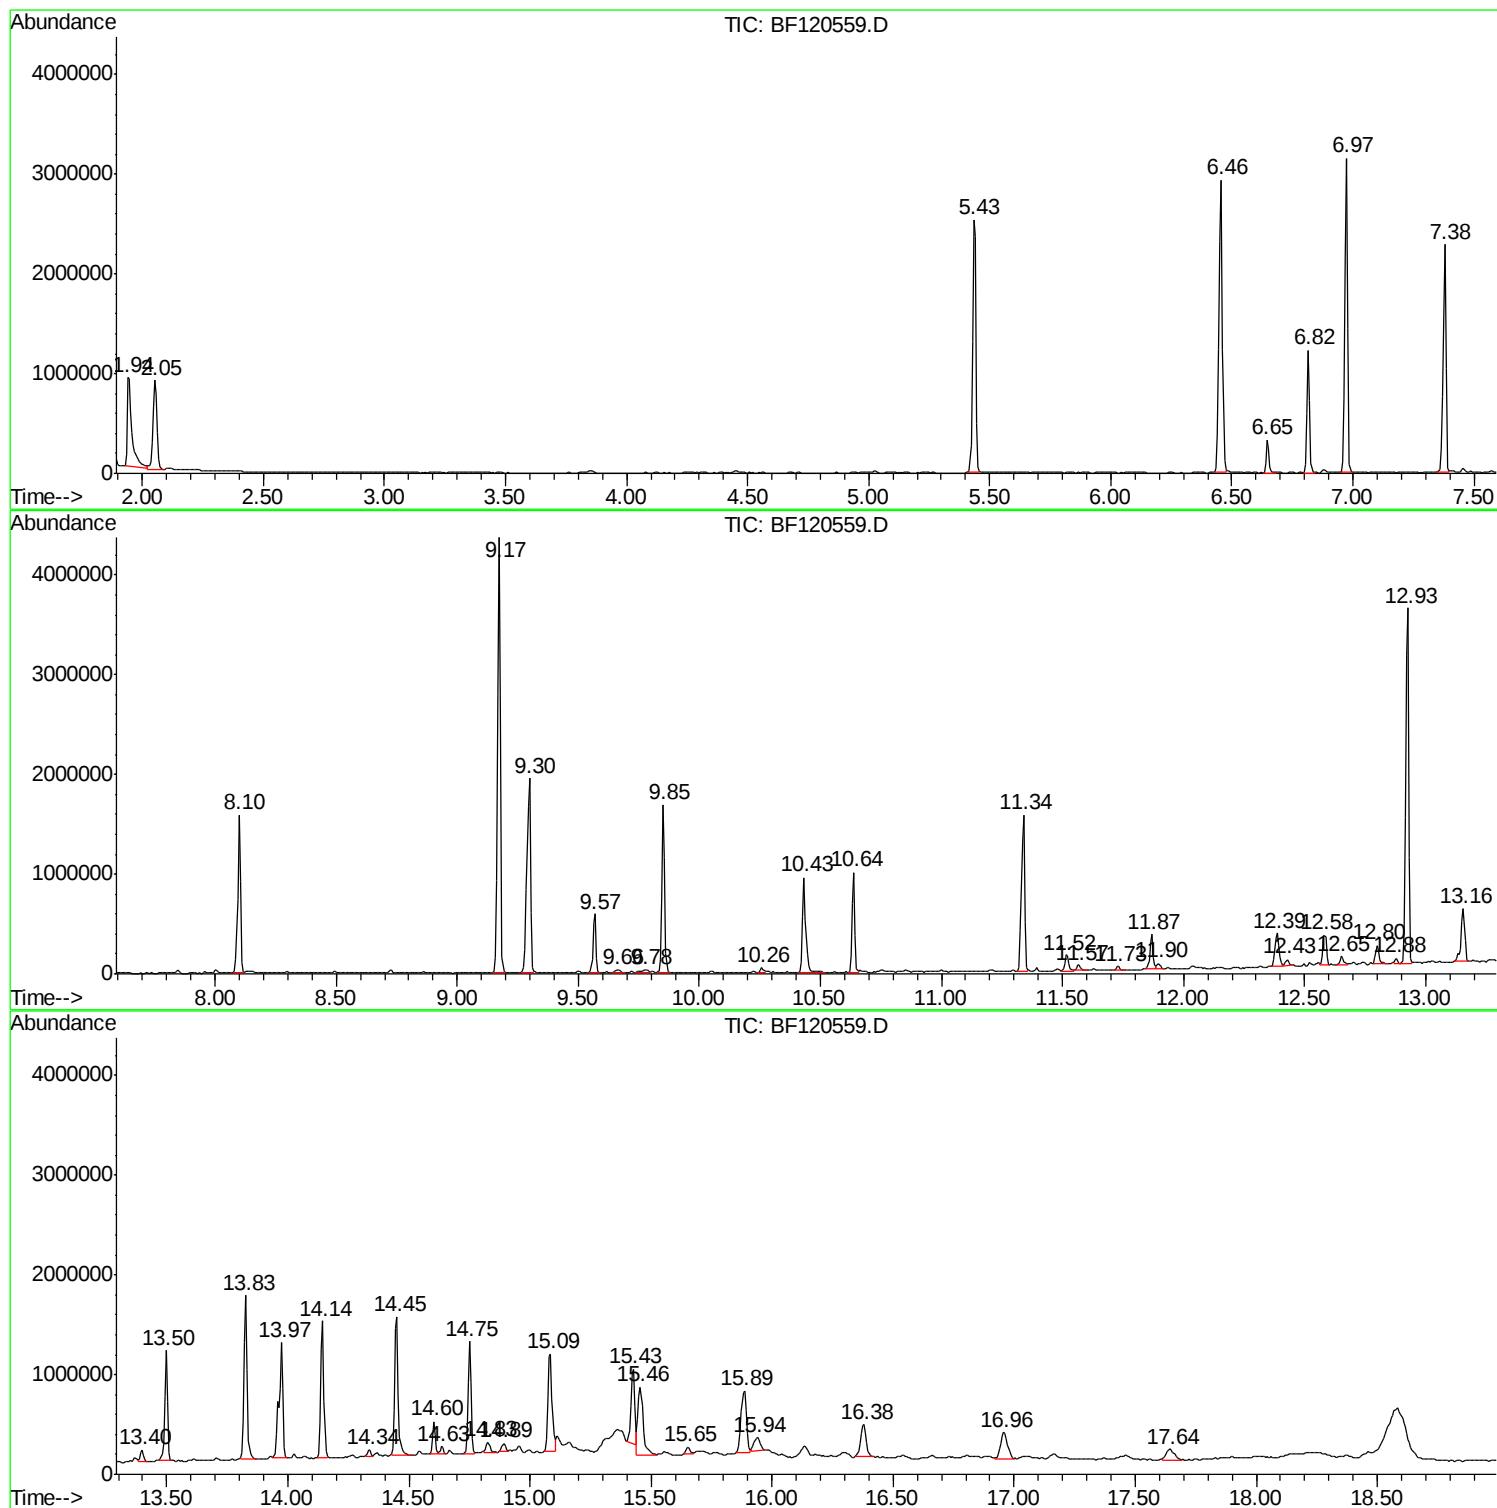

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060520\
Data File : BF120559.D
Acq On : 5 Jun 2020 15:01
Operator : JU/CG
Sample : L2886-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060520\
Data File : BF120559.D
Acq On : 5 Jun 2020 15:01
Operator : JU/CG
Sample : L2886-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc