

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
 Data File : BF120560.D
 Acq On : 5 Jun 2020 15:30
 Operator : JU/CG
 Sample : L2886-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLAB-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.946	7	10	20	rBV	447647	594036	13.30%	1.566%
2	2.028	20	24	31	rVB	730347	907688	20.32%	2.392%
3	5.434	599	603	609	rVB	1976159	1736373	38.87%	4.576%
4	5.681	642	645	650	rBV	142731	141464	3.17%	0.373%
5	6.451	772	776	786	rVB	1841874	1806226	40.44%	4.760%
6	6.816	834	838	841	rBV	1066520	825467	18.48%	2.175%
7	6.975	861	865	868	rBV	2159672	1879562	42.08%	4.953%
8	7.381	930	934	937	rVB	1732511	1590205	35.60%	4.191%
9	8.098	1051	1056	1059	rBV	1575066	1247292	27.92%	3.287%
10	9.175	1235	1239	1242	rBV	3624547	2991211	66.97%	7.883%
11	9.275	1254	1256	1262	rVB2	80328	73672	1.65%	0.194%
12	9.545	1298	1302	1303	rBV2	69843	76092	1.70%	0.201%
13	9.563	1303	1305	1310	rVB	433247	385220	8.62%	1.015%
14	9.851	1349	1354	1358	rBV	1646459	1381861	30.94%	3.642%
15	10.057	1386	1389	1392	rBV	94857	77538	1.74%	0.204%
16	10.280	1425	1427	1430	rVB3	73985	67525	1.51%	0.178%
17	10.639	1484	1488	1491	rBV	999005	827742	18.53%	2.181%
18	10.757	1505	1508	1512	rBV	159843	167702	3.75%	0.442%
19	11.139	1571	1573	1577	rVB	88677	70683	1.58%	0.186%
20	11.204	1581	1584	1587	rVV2	145001	174618	3.91%	0.460%
21	11.233	1587	1589	1595	rVB	125144	132958	2.98%	0.350%
22	11.339	1603	1607	1610	rBV	1384271	1238036	27.72%	3.263%
23	11.392	1613	1616	1619	rVV	234540	222980	4.99%	0.588%
24	11.586	1647	1649	1651	rVB	108366	78756	1.76%	0.208%
25	11.633	1654	1657	1662	rVV2	434054	432275	9.68%	1.139%
26	11.680	1662	1665	1668	rVV2	99174	116834	2.62%	0.308%
27	11.727	1671	1673	1676	rBV	73243	73515	1.65%	0.194%
28	11.798	1682	1685	1686	rBV	147544	146019	3.27%	0.385%
29	11.868	1694	1697	1699	rBV	500684	429745	9.62%	1.133%
30	11.892	1699	1701	1704	rVB2	162926	141097	3.16%	0.372%
31	11.927	1705	1707	1709	rBV	137934	158666	3.55%	0.418%
32	12.016	1719	1722	1724	rBV	120435	121996	2.73%	0.322%
33	12.039	1724	1726	1729	rBV	851262	777243	17.40%	2.048%
34	12.104	1735	1737	1740	rBV2	180976	168918	3.78%	0.445%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060520\
 Data File : BF120560.D
 Acq On : 5 Jun 2020 15:30
 Operator : JU/CG
 Sample : L2886-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLAB-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.192	1750	1752	1754	rBV	252473	260334	5.83%	0.686%
36	12.327	1772	1775	1777	rBV	676854	646113	14.46%	1.703%
37	12.386	1783	1785	1790	rVB2	357034	389501	8.72%	1.027%
38	12.433	1790	1793	1796	rBV	1182923	1052854	23.57%	2.775%
39	12.539	1808	1811	1814	rBV3	543019	698807	15.64%	1.842%
40	12.574	1814	1817	1820	rBV	631901	750200	16.80%	1.977%
41	12.651	1827	1830	1832	rBV2	621749	767368	17.18%	2.022%
42	12.786	1850	1853	1854	rBV	657539	640043	14.33%	1.687%
43	12.810	1854	1857	1859	rVV	816143	733882	16.43%	1.934%
44	12.927	1873	1877	1886	rBV2	2600234	4466801	100.00%	11.772%
45	13.015	1890	1892	1894	rBV2	540893	516541	11.56%	1.361%
46	13.163	1914	1917	1921	rBV2	1033576	1223880	27.40%	3.225%
47	13.292	1937	1939	1943	rBV	951179	1153379	25.82%	3.040%
48	13.374	1950	1953	1959	rBV4	830838	1847852	41.37%	4.870%
49	14.862	2203	2206	2208	rVB	1430347	1535508	34.38%	4.047%


Sum of corrected areas: 37944278

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF060520\
Data File : BF120560.D
Acq On : 5 Jun 2020 15:30
Operator : JU/CG
Sample : L2886-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

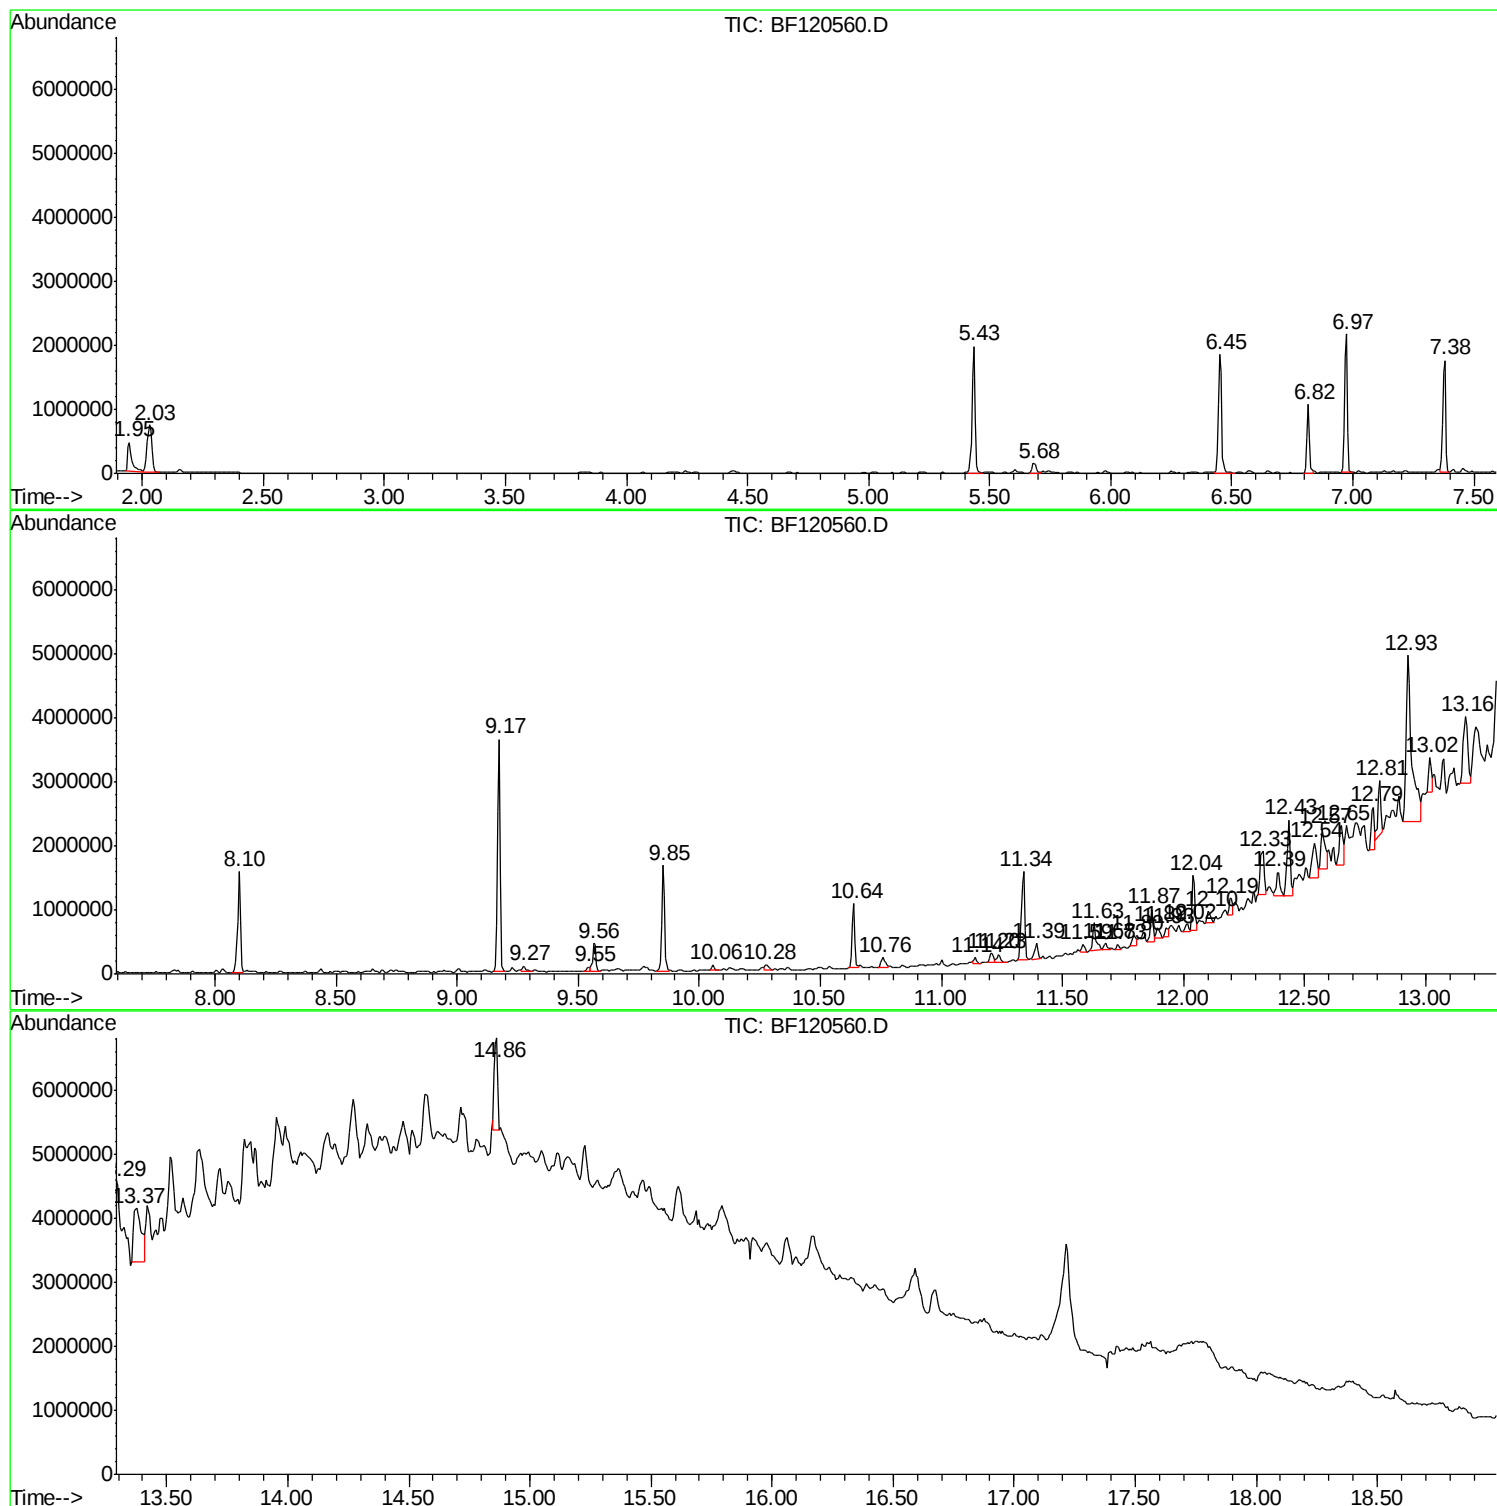

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060520\
Data File : BF120560.D
Acq On : 5 Jun 2020 15:30
Operator : JU/CG
Sample : L2886-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060520\
Data File : BF120560.D
Acq On : 5 Jun 2020 15:30
Operator : JU/CG
Sample : L2886-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLAB-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc