


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060520\
 Data File : BF120552.D
 Acq On : 5 Jun 2020 10:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 05 15:36:20 2020

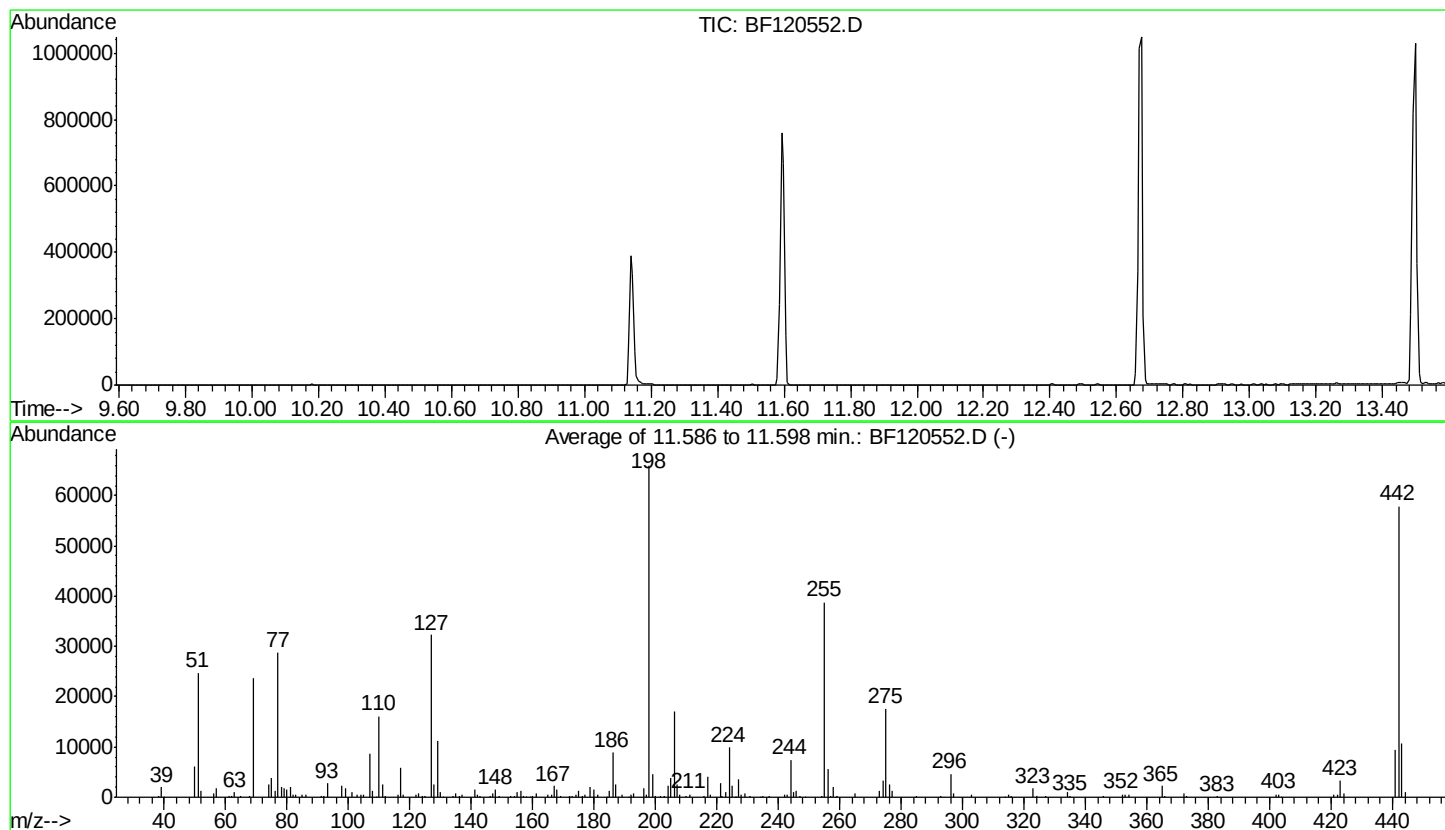

AutoFind: Scans 1649, 1650, 1651; Background Corrected with Scan 1645

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	24746	PASS
68	69	0.00	2	1.3	320	PASS
69	198	0.00	100	35.9	23707	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	32325	PASS
197	198	0.00	2	0.7	436	PASS
198	198	100	100	100.0	65952	PASS
199	198	5	9	7.0	4594	PASS
275	198	10	60	26.8	17680	PASS
365	198	1	100	3.4	2254	PASS
441	198	0.01	100	14.4	9480	PASS
442	198	50	100	87.7	57808	PASS
443	442	15	24	18.7	10807	PASS