
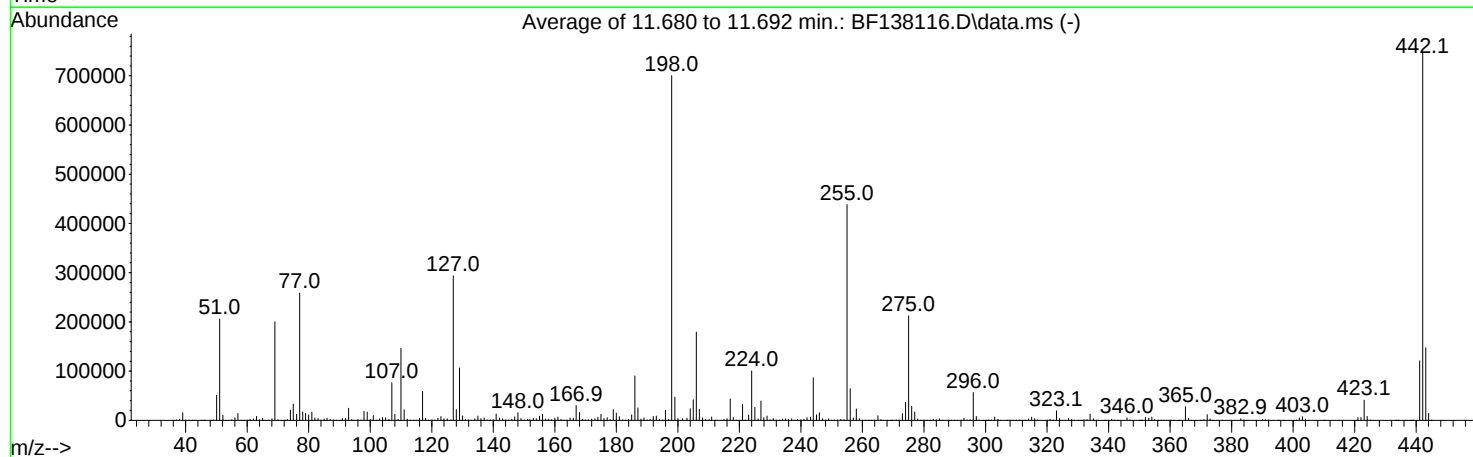


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060524\
Data File : BF138116.D
Acq On : 05 Jun 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 06 05:19:29 2024

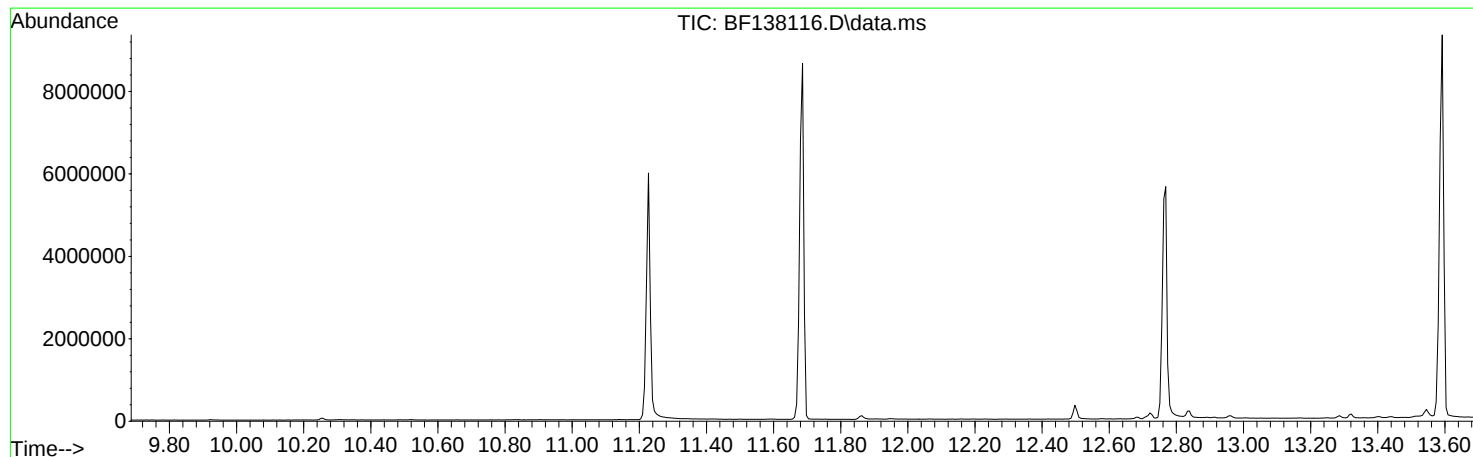




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	206013	PASS
68	69	0.00	2	1.6	3223	PASS
69	198	0.00	100	28.6	200359	PASS
70	69	0.00	2	0.6	1254	PASS
127	198	10	80	41.9	293403	PASS
197	198	0.00	2	0.3	2126	PASS
198	198	100	100	100.0	700053	PASS
199	198	5	9	6.8	47441	PASS
275	198	10	60	30.3	212344	PASS
365	198	1	100	3.9	27520	PASS
441	198	0.01	100	17.3	121011	PASS
442	442	50	100	100.0	747264	PASS
443	442	15	24	19.8	147672	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060524\
Data File : BF138116.D
Acq On : 05 Jun 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 11:59:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

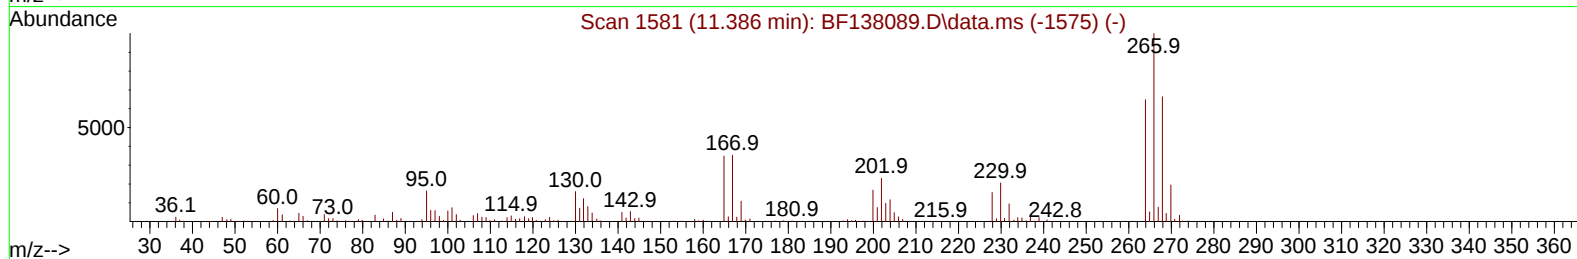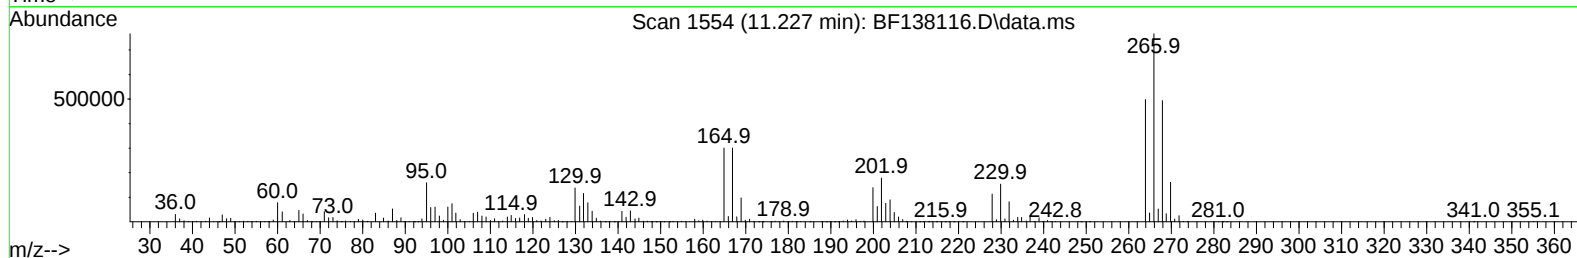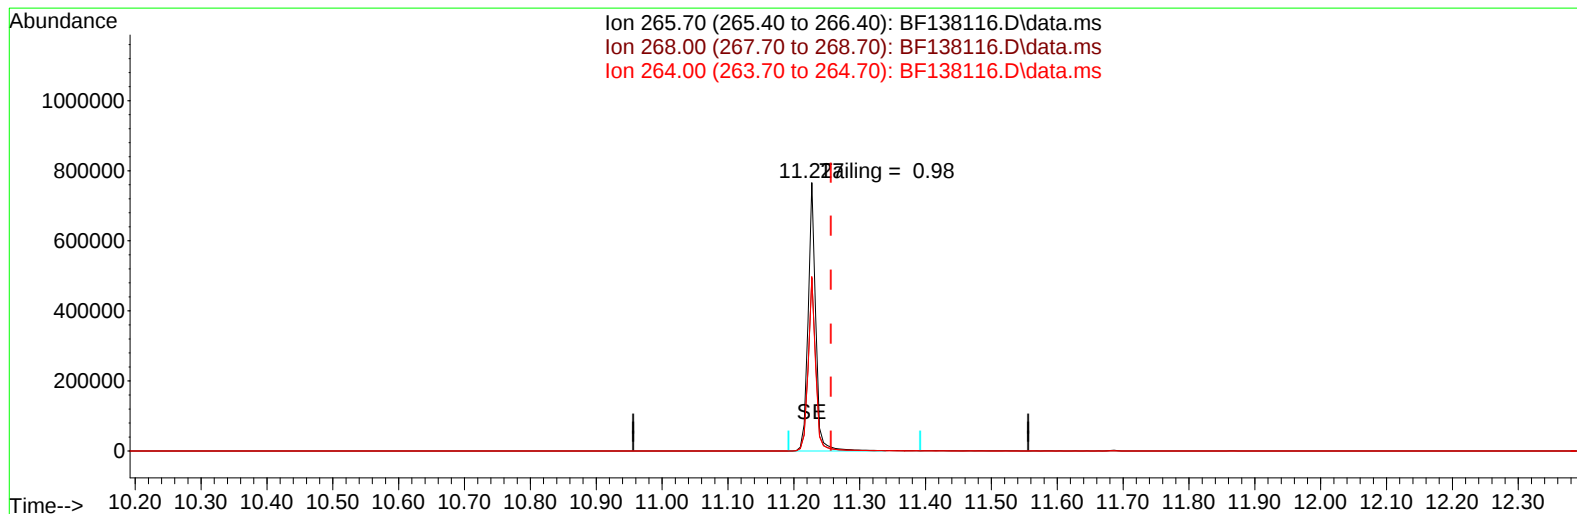

TIC: BF138116.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.029) 74480.86 ng




response 627757

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	64.41
264.00	64.80	65.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060524\
Data File : BF138116.D
Acq On : 05 Jun 2024 10:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jun 05 11:59:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF060524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 01 01:21:05 2024
Response via : Initial Calibration

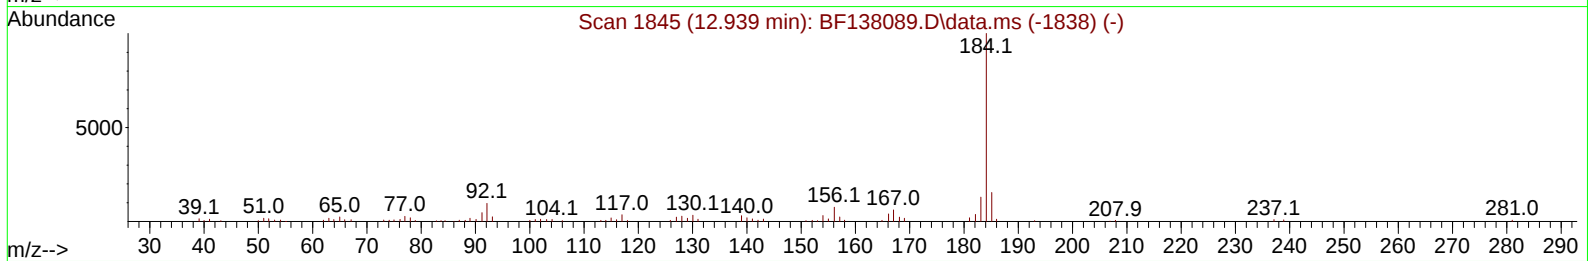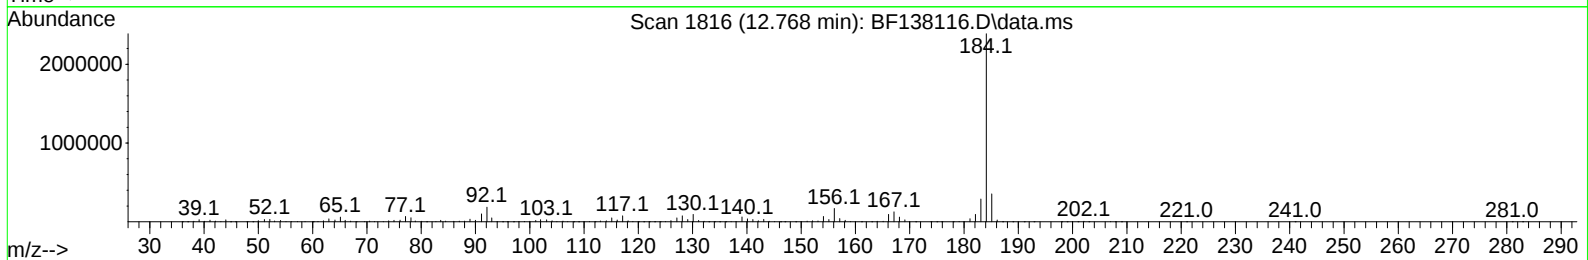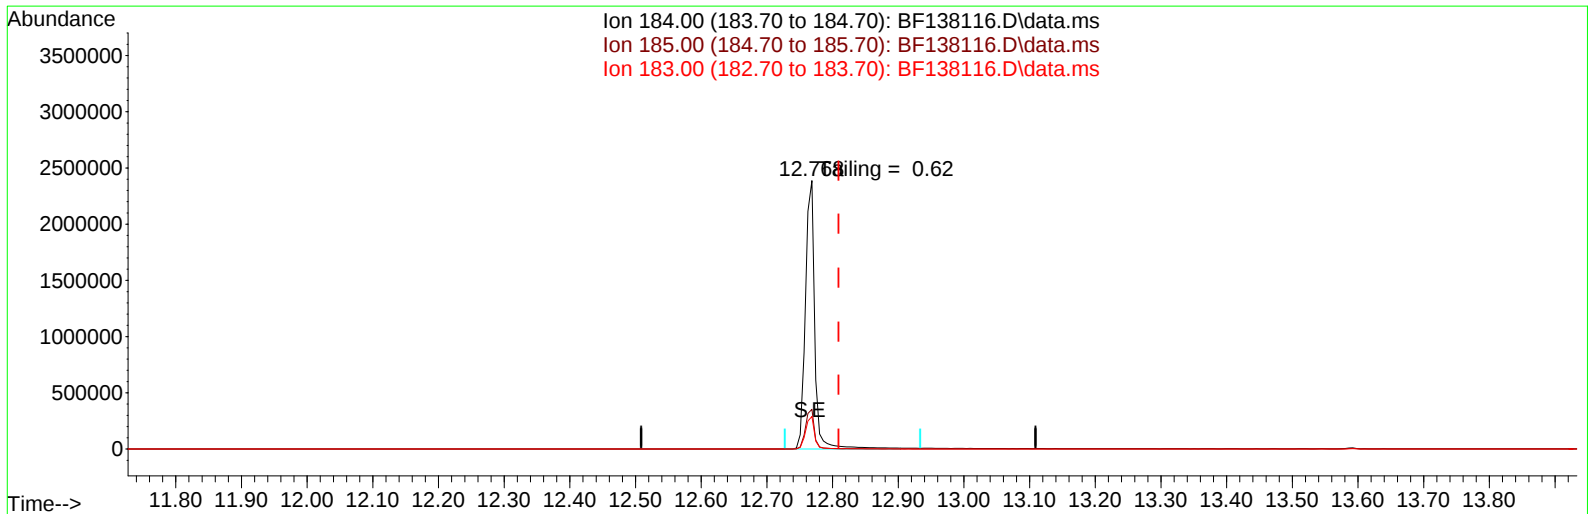

TIC: BF138116.D\data.ms

(77) Benzidine

12.768min (-0.041) -20.00 ng

response 2365623

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.83
183.00	12.80	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/5/2024	BNA_F	<u>BF138116.D</u>
Compound Name	Response	Retention Time
DDT	1415665	13.592
DDD	18360	13.321
DDE	664	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19024	1434689	1.33

Instrument :
BNA_F
ClientSampleId :
DFTPP