
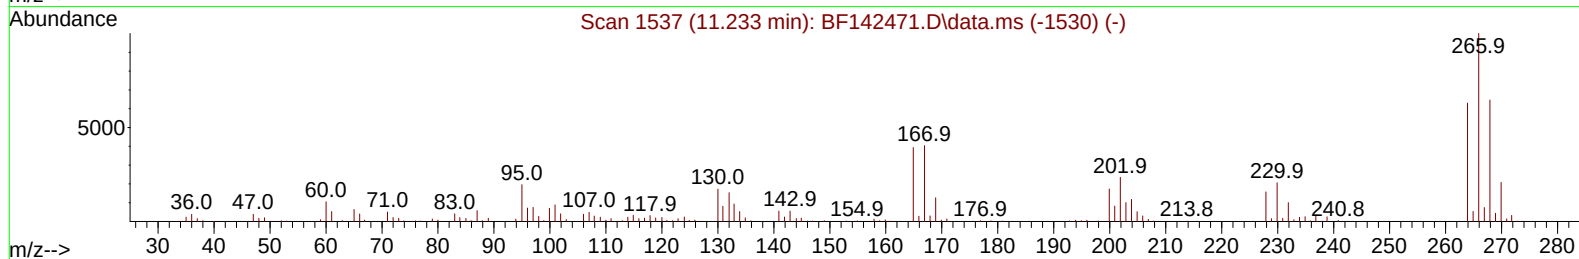
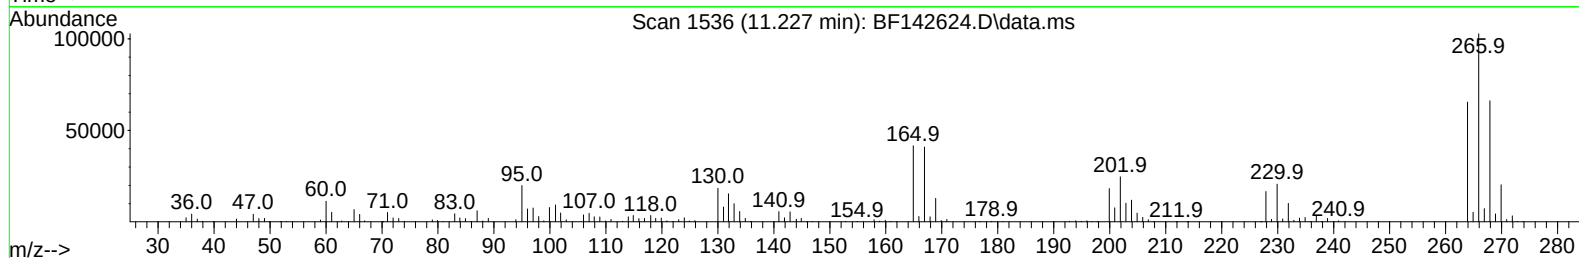


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060525\
Data File : BF142624.D
Acq On : 05 Jun 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 12:57:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

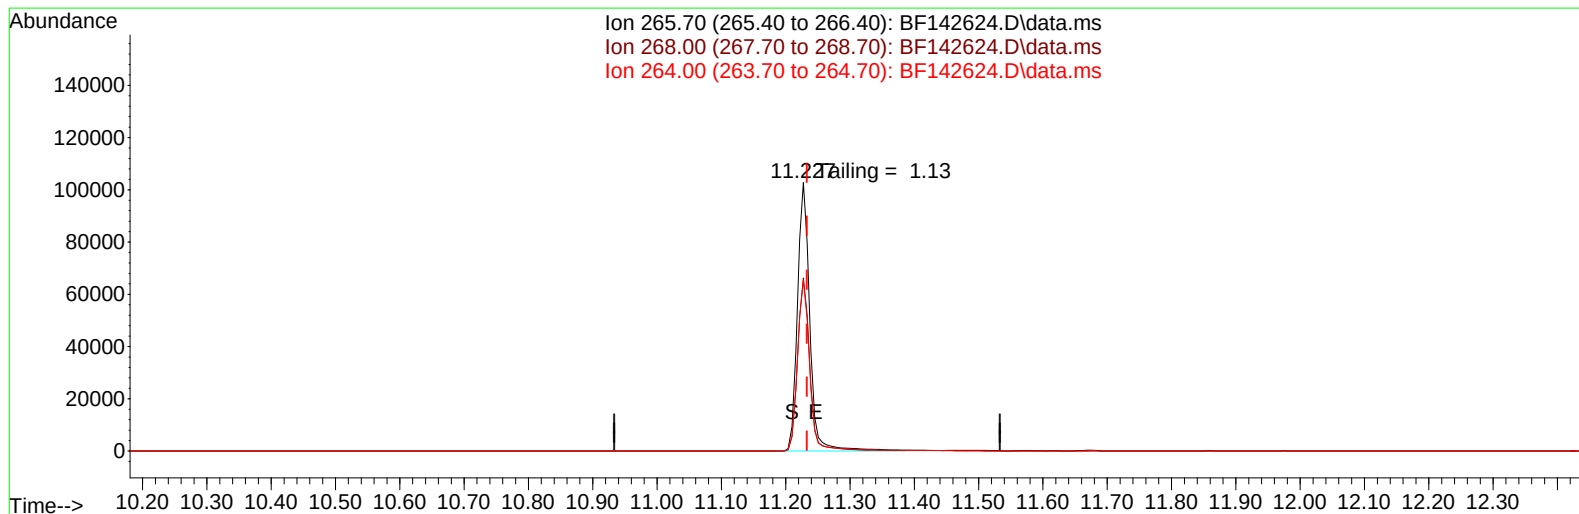

TIC: BF142624.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.006) 0.00 ng

response 138743

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.43
264.00	63.00	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF060525\
Data File : BF142624.D
Acq On : 05 Jun 2025 09:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 05 12:57:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

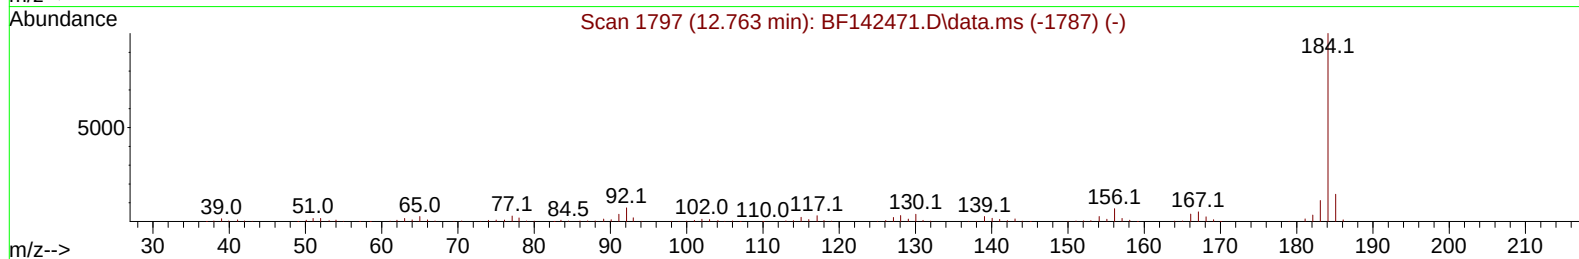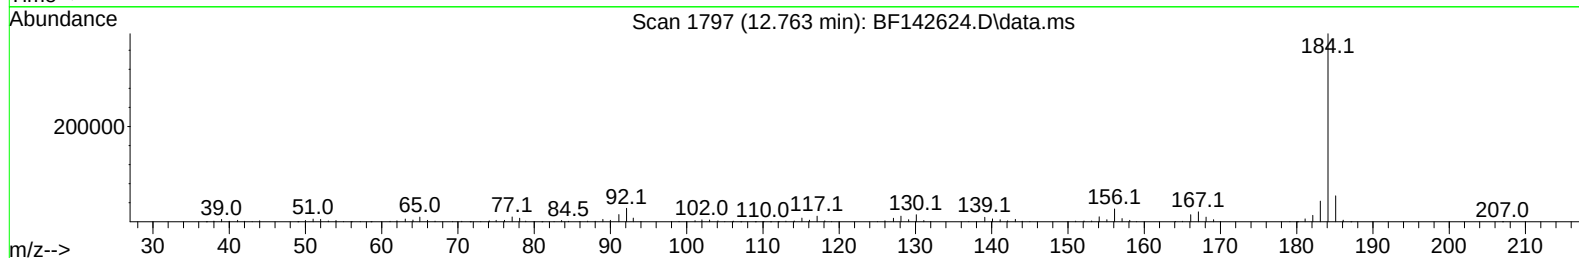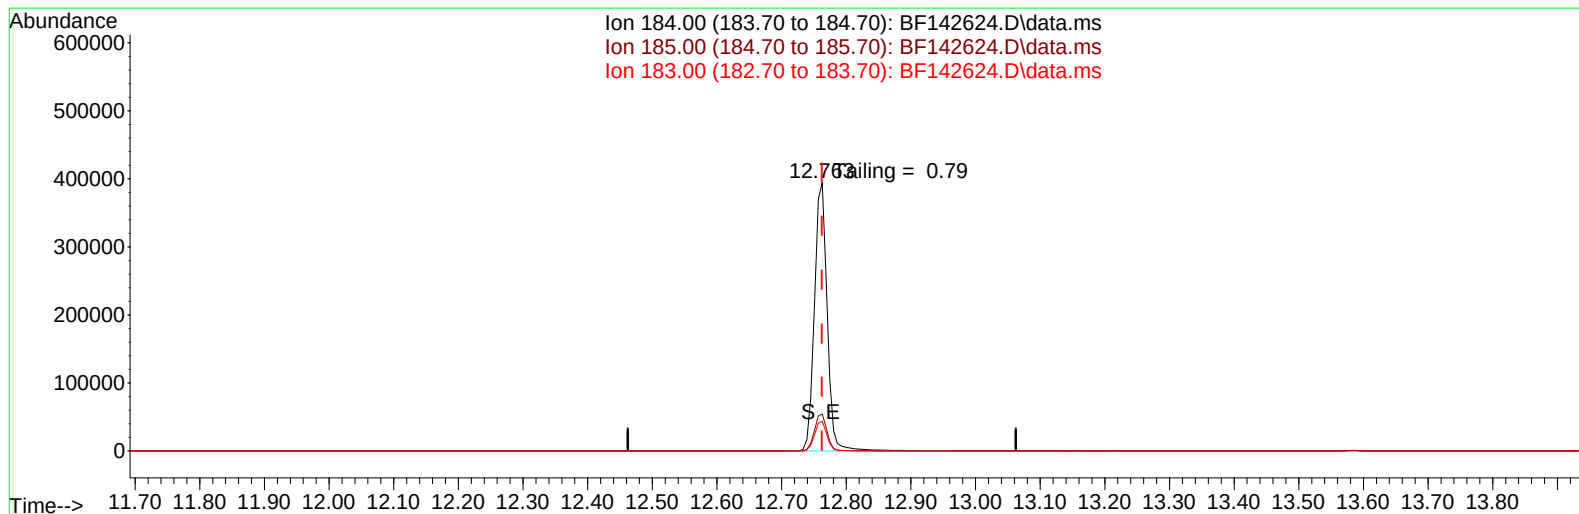

TIC: BF142624.D\data.ms

(77) Benzidine

12.763min (+ 0.000) 0.00 ng

response 543002

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.80
183.00	11.20	11.04
0.00	0.00	0.00